

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047641.D
 Acq On : 24 Mar 2022 18:52
 Operator : SY/MD
 Sample : VU0324WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	100	rVB	130214	156261	14.23%	1.687%
2	1.919	172	180	198	rBV	101694	138651	12.62%	1.497%
3	2.482	352	355	359	rVB3	359	230	0.02%	0.002%
4	2.572	370	383	419	rBV	235038	397140	36.16%	4.288%
5	2.716	426	428	433	rVB2	547	432	0.04%	0.005%
6	2.800	446	454	463	rBV2	1959	3030	0.28%	0.033%
7	2.880	475	479	482	rBV2	244	231	0.02%	0.002%
8	3.051	525	532	534	rBV4	990	1070	0.10%	0.012%
9	3.234	585	589	595	rVB3	286	322	0.03%	0.003%
10	3.273	595	601	603	rBV2	275	234	0.02%	0.003%
11	3.356	623	627	628	rBV2	465	345	0.03%	0.004%
12	3.488	666	668	671	rVB	329	198	0.02%	0.002%
13	3.697	730	733	735	rBV2	306	272	0.02%	0.003%
14	3.822	767	772	776	rBV3	387	442	0.04%	0.005%
15	4.134	863	869	873	rVB3	214	236	0.02%	0.003%
16	4.192	884	887	892	rVB3	245	216	0.02%	0.002%
17	4.301	918	921	927	rBV2	216	262	0.02%	0.003%
18	4.327	927	929	933	rVB2	324	265	0.02%	0.003%
19	4.363	933	940	942	rBV2	270	286	0.03%	0.003%
20	4.642	1012	1027	1063	rBV	100738	325304	29.62%	3.512%
21	4.861	1092	1095	1097	rBV3	307	233	0.02%	0.003%
22	4.980	1130	1132	1136	rVB	427	275	0.03%	0.003%
23	5.067	1142	1159	1186	rBV	202658	438803	39.95%	4.737%
24	5.295	1227	1230	1237	rVB4	640	677	0.06%	0.007%
25	5.382	1249	1257	1260	rBV4	331	359	0.03%	0.004%
26	5.526	1297	1302	1307	rBV2	425	315	0.03%	0.003%
27	5.729	1340	1365	1397	rBV2	410862	1098385	100.00%	11.859%
28	6.047	1459	1464	1466	rBV3	414	318	0.03%	0.003%
29	6.115	1482	1485	1492	rVB3	390	499	0.05%	0.005%
30	6.195	1505	1510	1513	rBV2	255	233	0.02%	0.003%
31	6.250	1513	1527	1548	rBV	354002	672511	61.23%	7.261%
32	6.491	1599	1602	1607	rVB2	371	326	0.03%	0.004%
33	6.530	1607	1614	1617	rBV5	1589	2155	0.20%	0.023%
34	6.604	1634	1637	1641	rVB4	718	561	0.05%	0.006%
35	6.694	1651	1665	1683	rBV	245715	485341	44.19%	5.240%
36	6.806	1694	1700	1707	rVB6	512	529	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047641.D
 Acq On : 24 Mar 2022 18:52
 Operator : SY/MD
 Sample : VU0324WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.858	1713	1716	1719	rVB	431	234	0.02%	0.003%
38	6.906	1728	1731	1736	rVB2	300	268	0.02%	0.003%
39	6.983	1752	1755	1760	rVB3	249	205	0.02%	0.002%
40	7.015	1760	1765	1769	rVB2	208	242	0.02%	0.003%
41	7.044	1769	1774	1777	rBV2	528	552	0.05%	0.006%
42	7.186	1810	1818	1821	rBV2	965	1081	0.10%	0.012%
43	7.227	1827	1831	1834	rBV4	385	336	0.03%	0.004%
44	7.250	1834	1838	1843	rVV4	306	281	0.03%	0.003%
45	7.491	1911	1913	1919	rBV2	226	281	0.03%	0.003%
46	7.568	1924	1937	1956	rBV	140736	252276	22.97%	2.724%
47	7.803	1999	2010	2019	rBV5	1931	3247	0.30%	0.035%
48	7.899	2026	2040	2055	rBV	523123	902689	82.18%	9.746%
49	8.182	2115	2128	2151	rBV	100630	177245	16.14%	1.914%
50	8.369	2184	2186	2189	rVB3	514	308	0.03%	0.003%
51	8.555	2238	2244	2249	rBV6	660	881	0.08%	0.010%
52	8.578	2249	2251	2257	rVB4	344	307	0.03%	0.003%
53	8.639	2257	2270	2304	rBV	373733	723372	65.86%	7.810%
54	8.922	2355	2358	2362	rVB2	378	268	0.02%	0.003%
55	9.025	2387	2390	2395	rVB3	231	226	0.02%	0.002%
56	9.224	2450	2452	2458	rVB2	317	271	0.02%	0.003%
57	9.266	2460	2465	2467	rBV2	274	282	0.03%	0.003%
58	9.417	2499	2512	2539	rBV	523874	897816	81.74%	9.693%
59	9.571	2556	2560	2566	rVB2	1113	1150	0.10%	0.012%
60	9.700	2590	2600	2607	rBV5	1639	2908	0.26%	0.031%
61	9.761	2615	2619	2622	rBV	254	224	0.02%	0.002%
62	9.890	2656	2659	2663	rVB2	304	228	0.02%	0.002%
63	10.063	2706	2713	2718	rBV3	377	455	0.04%	0.005%
64	10.108	2718	2727	2742	rVB4	1752	3374	0.31%	0.036%
65	10.166	2742	2745	2748	rVB	376	243	0.02%	0.003%
66	10.192	2748	2753	2757	rVB3	271	269	0.02%	0.003%
67	10.349	2796	2802	2803	rBV2	292	318	0.03%	0.003%
68	10.446	2829	2832	2837	rVV3	264	214	0.02%	0.002%
69	10.481	2837	2843	2852	rVB3	1146	1658	0.15%	0.018%
70	10.571	2869	2871	2877	rVB3	312	300	0.03%	0.003%
71	10.620	2882	2886	2890	rBV	341	402	0.04%	0.004%
72	10.674	2895	2903	2912	rVB3	3033	4318	0.39%	0.047%
73	10.758	2916	2929	2945	rBV	397480	632547	57.59%	6.829%
74	10.870	2956	2964	2969	rBV4	752	1053	0.10%	0.011%
75	10.899	2969	2973	2975	rVV2	488	398	0.04%	0.004%
76	10.922	2978	2980	2985	rVB3	801	637	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047641.D
 Acq On : 24 Mar 2022 18:52
 Operator : SY/MD
 Sample : VU0324WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.983	2996	2999	3002	rVB2	274	191	0.02%	0.002%
78	11.083	3026	3030	3032	rBV3	822	690	0.06%	0.007%
79	11.128	3039	3044	3049	rBV4	461	617	0.06%	0.007%
80	11.295	3090	3096	3101	rBV2	278	360	0.03%	0.004%
81	11.356	3110	3115	3117	rBV3	308	271	0.02%	0.003%
82	11.468	3140	3150	3164	rVB4	3696	6803	0.62%	0.073%
83	11.581	3178	3185	3189	rBV2	613	799	0.07%	0.009%
84	11.700	3214	3222	3226	rBV3	1414	1840	0.17%	0.020%
85	11.748	3230	3237	3244	rBV5	2451	3478	0.32%	0.038%
86	11.812	3244	3257	3274	rBV	606991	960480	87.44%	10.370%
87	11.938	3292	3296	3297	rBV2	647	422	0.04%	0.005%
88	11.970	3303	3306	3319	rVB3	2538	3091	0.28%	0.033%
89	12.121	3350	3353	3359	rVB3	412	422	0.04%	0.005%
90	12.195	3359	3376	3392	rBV	531993	885902	80.65%	9.565%
91	12.269	3396	3399	3403	rVB3	674	513	0.05%	0.006%
92	12.333	3416	3419	3427	rVB4	1073	997	0.09%	0.011%
93	12.777	3555	3557	3565	rVB2	346	275	0.03%	0.003%
94	12.999	3621	3626	3632	rBV3	967	1304	0.12%	0.014%
95	13.221	3688	3695	3708	rBV3	4256	6279	0.57%	0.068%
96	13.674	3833	3836	3839	rBV2	256	197	0.02%	0.002%
97	13.844	3880	3889	3899	rBV3	6940	10017	0.91%	0.108%
98	14.089	3955	3965	3975	rBV2	16896	26255	2.39%	0.283%
99	14.333	4032	4041	4051	rVB4	6974	10536	0.96%	0.114%
100	15.343	4353	4355	4358	rBV2	553	307	0.03%	0.003%




Sum of corrected areas: 9262357

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047641.D
Acq On : 24 Mar 2022 18:52
Operator : SY/MD
Sample : VU0324WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK070

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

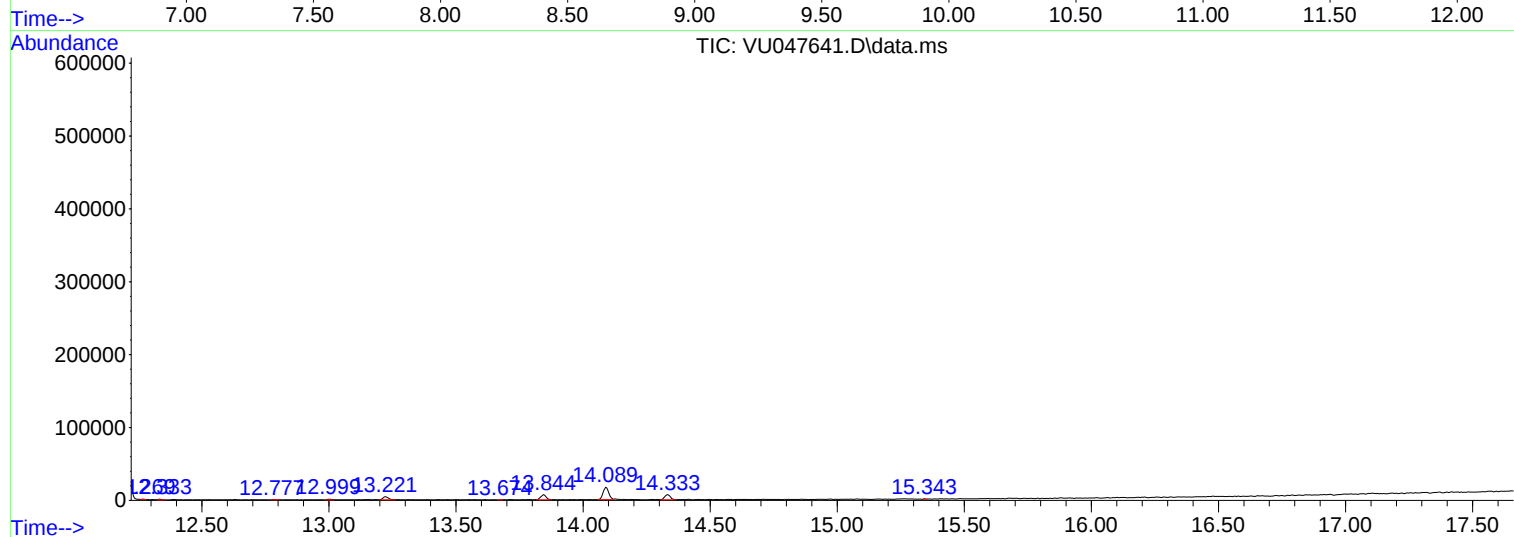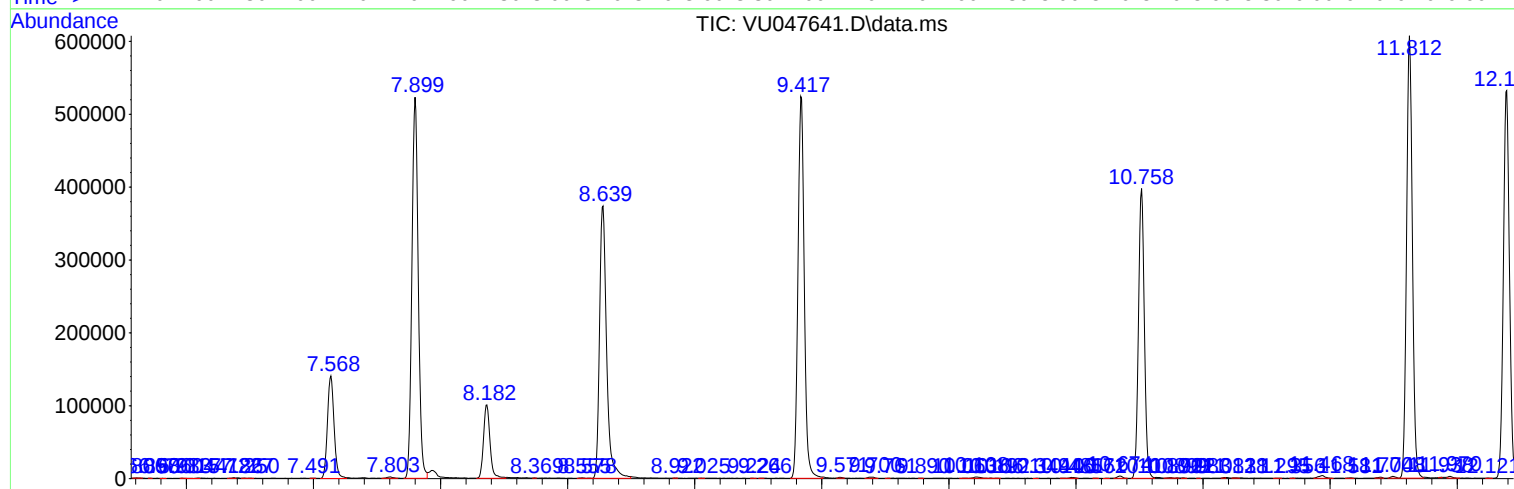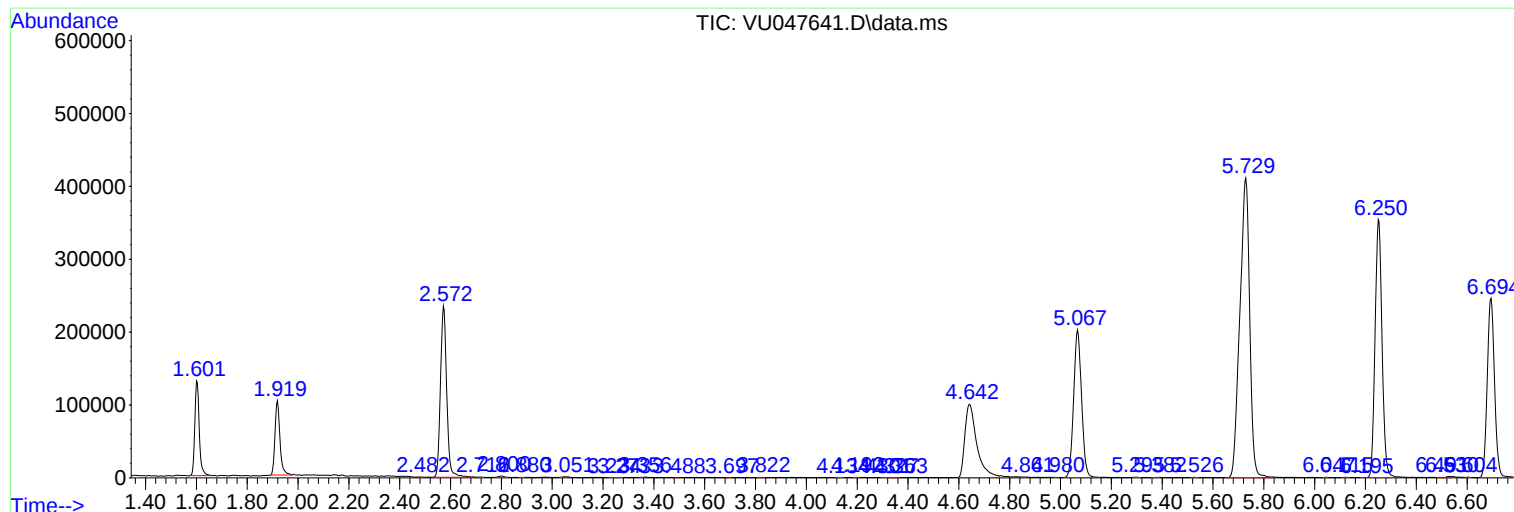

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047641.D
Acq On : 24 Mar 2022 18:52
Operator : SY/MD
Sample : VU0324WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK070

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047641.D
Acq On : 24 Mar 2022 18:52
Operator : SY/MD
Sample : VU0324WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK070

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
