

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047642.D
 Acq On : 24 Mar 2022 19:15
 Operator : SY/MD
 Sample : N2081-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5W6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rVB	114452	139392	14.64%	2.078%
2	1.919	172	180	196	rBV	93101	123373	12.96%	1.839%
3	2.572	371	383	401	rBV	204787	344778	36.21%	5.139%
4	2.707	422	425	430	rVB4	528	416	0.04%	0.006%
5	2.803	446	455	461	rBV3	2159	3404	0.36%	0.051%
6	3.051	528	532	534	rBV3	477	422	0.04%	0.006%
7	3.186	564	574	577	rBV2	2643	3704	0.39%	0.055%
8	3.327	614	618	621	rBV	232	208	0.02%	0.003%
9	3.359	624	628	633	rVV2	592	493	0.05%	0.007%
10	3.649	716	718	722	rVB3	262	190	0.02%	0.003%
11	3.684	726	729	734	rVV2	253	189	0.02%	0.003%
12	3.867	781	786	791	rBV4	544	756	0.08%	0.011%
13	3.948	805	811	814	rBV2	303	328	0.03%	0.005%
14	3.989	818	824	827	rBV2	305	353	0.04%	0.005%
15	4.047	839	842	846	rBV2	439	498	0.05%	0.007%
16	4.076	848	851	855	rVB	264	254	0.03%	0.004%
17	4.218	889	895	901	rVB2	296	341	0.04%	0.005%
18	4.636	1010	1025	1068	rBV	103427	305848	32.13%	4.559%
19	4.903	1104	1108	1110	rBV2	369	313	0.03%	0.005%
20	5.005	1134	1140	1142	rBV2	432	436	0.05%	0.006%
21	5.067	1142	1159	1185	rBV	171396	373991	39.28%	5.575%
22	5.202	1199	1201	1204	rVB3	404	253	0.03%	0.004%
23	5.292	1223	1229	1231	rBV3	476	522	0.05%	0.008%
24	5.395	1256	1261	1263	rBV	421	319	0.03%	0.005%
25	5.642	1332	1338	1342	rBV2	209	242	0.03%	0.004%
26	5.729	1342	1365	1386	rBV2	354776	952046	100.00%	14.191%
27	5.986	1440	1445	1447	rBV2	403	369	0.04%	0.006%
28	6.015	1451	1454	1458	rVV2	304	248	0.03%	0.004%
29	6.050	1462	1465	1469	rVV2	363	279	0.03%	0.004%
30	6.124	1484	1488	1490	rBV2	308	241	0.03%	0.004%
31	6.166	1493	1501	1510	rBV4	915	1426	0.15%	0.021%
32	6.253	1513	1528	1551	rBV	111632	215060	22.59%	3.206%
33	6.536	1610	1616	1622	rBV4	1169	1732	0.18%	0.026%
34	6.587	1629	1632	1638	rVB4	564	498	0.05%	0.007%
35	6.613	1638	1640	1644	rBV2	394	218	0.02%	0.003%
36	6.694	1651	1665	1685	rBV	213177	418667	43.98%	6.241%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047642.D
 Acq On : 24 Mar 2022 19:15
 Operator : SY/MD
 Sample : N2081-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5W6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.002	1754	1761	1762	rBV3	339	328	0.03%	0.005%
38	7.144	1801	1805	1810	rVB3	291	354	0.04%	0.005%
39	7.192	1812	1820	1823	rBV2	601	857	0.09%	0.013%
40	7.240	1832	1835	1844	rVB3	370	400	0.04%	0.006%
41	7.568	1924	1937	1956	rBV	119732	215155	22.60%	3.207%
42	7.690	1972	1975	1977	rBV2	687	450	0.05%	0.007%
43	7.758	1991	1996	1998	rBV2	240	244	0.03%	0.004%
44	7.796	2000	2008	2009	rBV2	2593	2712	0.28%	0.040%
45	7.899	2026	2040	2056	rBV	441404	773169	81.21%	11.525%
46	8.115	2104	2107	2113	rBV4	244	214	0.02%	0.003%
47	8.179	2113	2127	2147	rBV2	91735	171409	18.00%	2.555%
48	8.430	2201	2205	2207	rBV2	314	232	0.02%	0.003%
49	8.472	2207	2218	2233	rVB3	9352	18803	1.98%	0.280%
50	8.542	2233	2240	2241	rBV2	363	442	0.05%	0.007%
51	8.558	2241	2245	2247	rBV3	456	265	0.03%	0.004%
52	8.636	2257	2269	2307	rBV	309640	611343	64.21%	9.113%
53	9.047	2393	2397	2400	rBV2	373	255	0.03%	0.004%
54	9.121	2415	2420	2423	rBV2	401	421	0.04%	0.006%
55	9.263	2460	2464	2467	rBV2	439	331	0.03%	0.005%
56	9.417	2500	2512	2546	rVB	173379	299095	31.42%	4.458%
57	9.568	2552	2559	2561	rBV2	651	660	0.07%	0.010%
58	9.681	2591	2594	2595	rBV	505	245	0.03%	0.004%
59	9.928	2666	2671	2678	rVB3	623	701	0.07%	0.010%
60	10.099	2719	2724	2726	rBV2	840	649	0.07%	0.010%
61	10.115	2726	2729	2731	rVV2	572	401	0.04%	0.006%
62	10.224	2757	2763	2766	rBV3	302	329	0.03%	0.005%
63	10.423	2821	2825	2829	rBV3	263	223	0.02%	0.003%
64	10.481	2840	2843	2851	rBV2	639	751	0.08%	0.011%
65	10.562	2862	2868	2870	rBV2	380	302	0.03%	0.005%
66	10.578	2870	2873	2877	rVB4	443	383	0.04%	0.006%
67	10.671	2893	2902	2910	rBV5	3587	5748	0.60%	0.086%
68	10.758	2916	2929	2945	rBV	329676	532576	55.94%	7.939%
69	10.893	2959	2971	2985	rVB2	14882	26398	2.77%	0.393%
70	11.053	3012	3021	3026	rVB5	1313	1617	0.17%	0.024%
71	11.102	3026	3036	3037	rBV4	1136	1389	0.15%	0.021%
72	11.144	3047	3049	3052	rBV2	571	350	0.04%	0.005%
73	11.246	3079	3081	3085	rVB2	325	193	0.02%	0.003%
74	11.372	3117	3120	3123	rBV2	298	196	0.02%	0.003%
75	11.426	3134	3137	3140	rVV3	623	485	0.05%	0.007%
76	11.459	3140	3147	3159	rVB7	3624	6987	0.73%	0.104%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047642.D
 Acq On : 24 Mar 2022 19:15
 Operator : SY/MD
 Sample : N2081-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5W6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.571	3179	3182	3184	rBV2	800	589	0.06%	0.009%
78	11.693	3210	3220	3228	rBV7	2249	3619	0.38%	0.054%
79	11.751	3231	3238	3245	rVB3	1555	2172	0.23%	0.032%
80	11.812	3245	3257	3272	rBV	209386	338212	35.52%	5.041%
81	11.938	3283	3296	3297	rBV6	1931	2834	0.30%	0.042%
82	12.108	3346	3349	3353	rBV4	500	556	0.06%	0.008%
83	12.192	3359	3375	3398	rBV	462646	754558	79.26%	11.247%
84	12.272	3398	3400	3406	rVB3	677	557	0.06%	0.008%
85	12.324	3411	3416	3417	rBV4	1600	1274	0.13%	0.019%
86	12.372	3428	3431	3435	rBV3	582	539	0.06%	0.008%
87	12.401	3435	3440	3447	rVB6	1147	1355	0.14%	0.020%
88	12.462	3456	3459	3462	rBV3	351	289	0.03%	0.004%
89	12.484	3462	3466	3467	rBV2	592	406	0.04%	0.006%
90	12.635	3509	3513	3517	rVB3	493	429	0.05%	0.006%
91	12.709	3532	3536	3538	rBV2	322	283	0.03%	0.004%
92	12.777	3548	3557	3564	rBV3	1452	2293	0.24%	0.034%
93	12.954	3604	3612	3621	rBV4	1011	1653	0.17%	0.025%
94	12.999	3623	3626	3629	rVB2	565	327	0.03%	0.005%
95	13.127	3663	3666	3669	rBV	308	216	0.02%	0.003%
96	13.221	3688	3695	3704	rVB4	2635	3698	0.39%	0.055%
97	13.529	3785	3791	3799	rBV6	749	1155	0.12%	0.017%
98	13.841	3883	3888	3899	rVB3	3761	4983	0.52%	0.074%
99	14.092	3959	3966	3978	rVB3	7620	11824	1.24%	0.176%
100	14.333	4034	4041	4049	rVB4	4080	6079	0.64%	0.091%




Sum of corrected areas: 6708769

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047642.D
Acq On : 24 Mar 2022 19:15
Operator : SY/MD
Sample : N2081-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5W6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

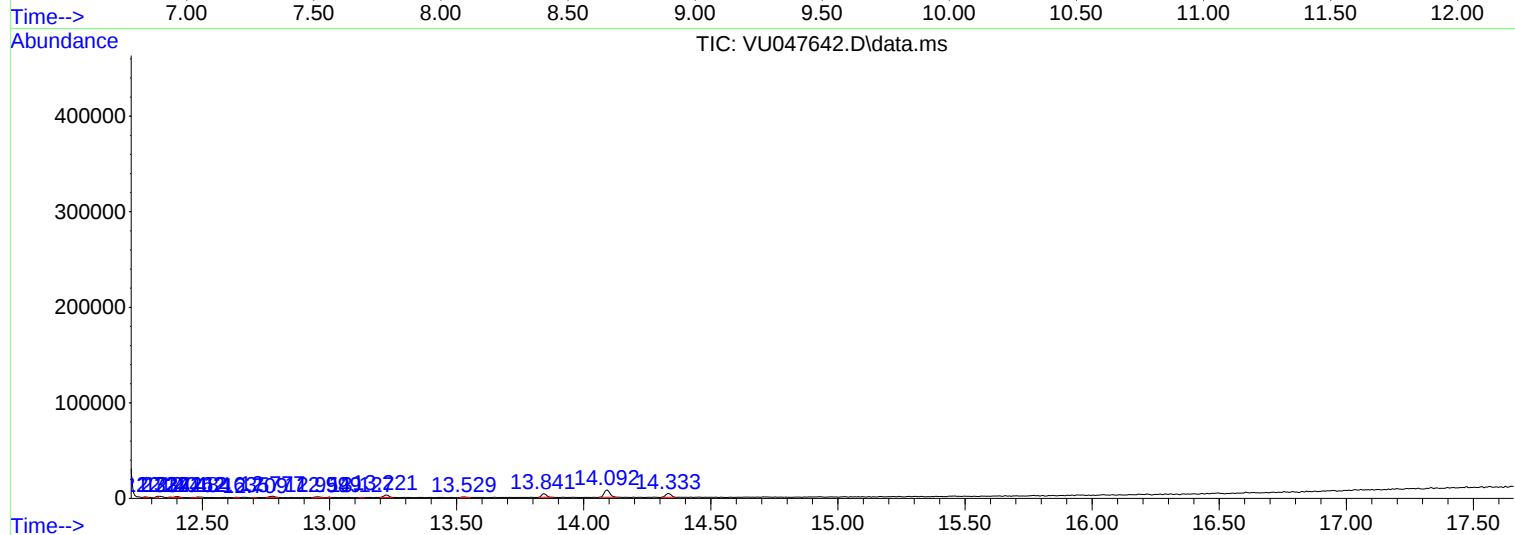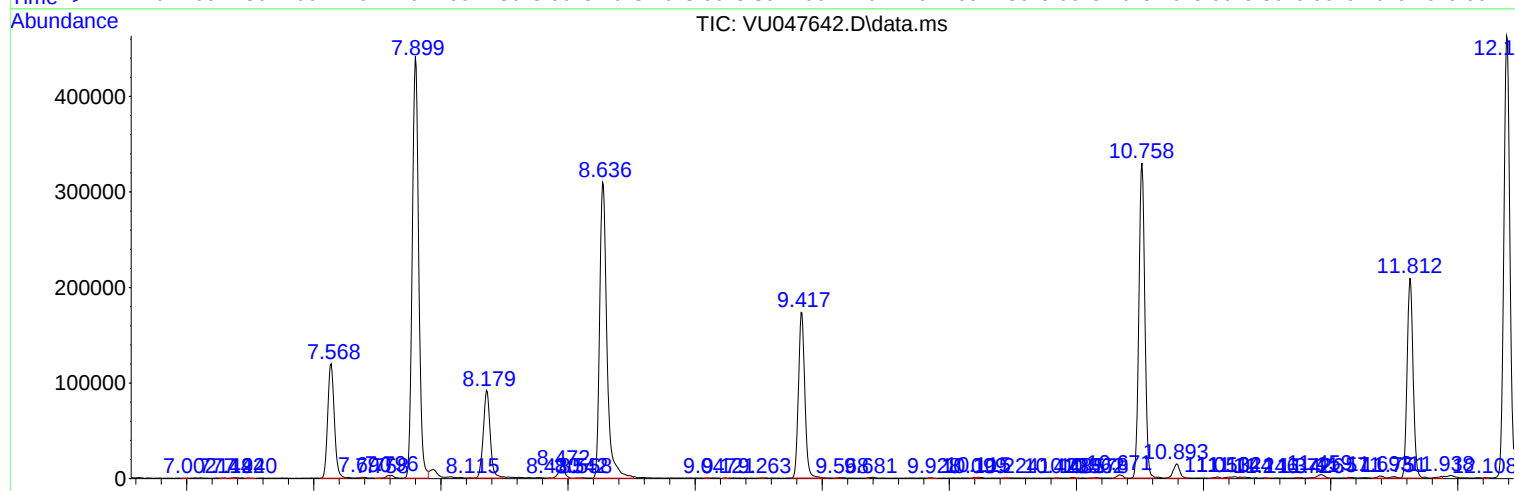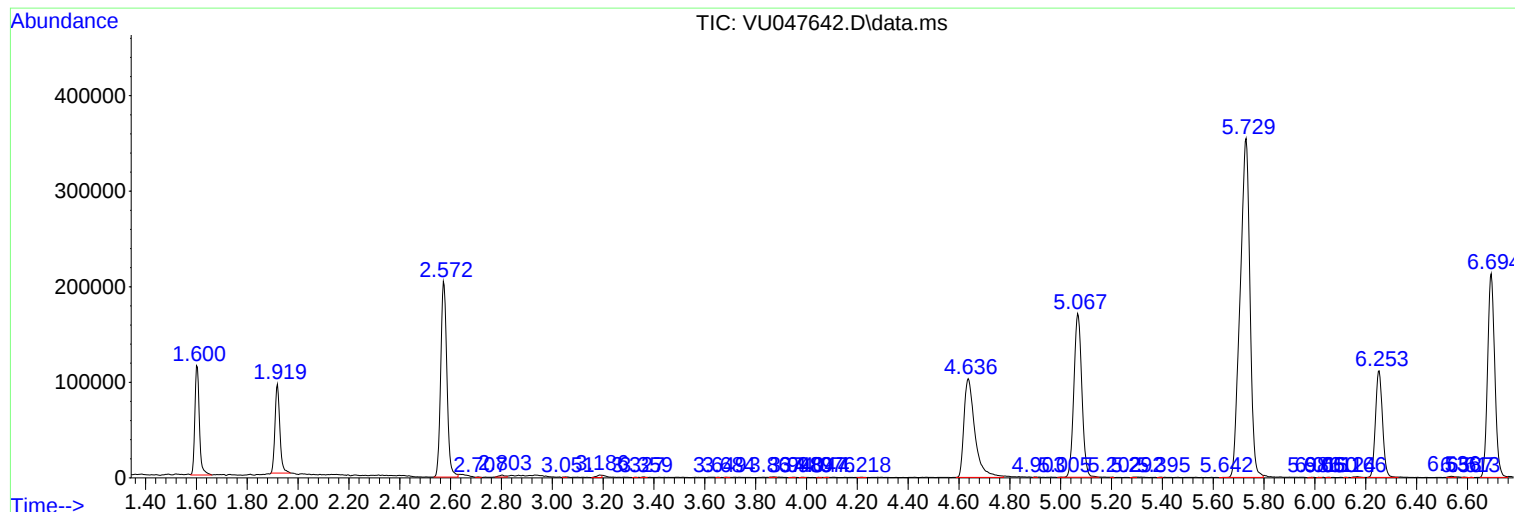

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047642.D
Acq On : 24 Mar 2022 19:15
Operator : SY/MD
Sample : N2081-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5W6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047642.D
Acq On : 24 Mar 2022 19:15
Operator : SY/MD
Sample : N2081-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5W6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc