

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047644.D
 Acq On : 24 Mar 2022 20:00
 Operator : SY/MD
 Sample : N2081-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	71	82	95	rBV3	56298	79327	3.35%	1.142%
2	1.851	154	159	163	rBV7	1336	1603	0.07%	0.023%
3	1.919	173	180	182	rBV	35756	38531	1.63%	0.555%
4	2.575	372	384	400	rBV3	87994	160770	6.79%	2.315%
5	2.800	443	454	463	rBV2	1587	2537	0.11%	0.037%
6	2.951	490	501	510	rBV4	2047	5042	0.21%	0.073%
7	3.189	570	575	578	rBV2	583	509	0.02%	0.007%
8	3.311	608	613	615	rBV2	785	734	0.03%	0.011%
9	3.362	620	629	643	rVB7	6470	13103	0.55%	0.189%
10	3.575	688	695	697	rBV2	301	320	0.01%	0.005%
11	3.874	768	788	812	rBV	182972	437639	18.47%	6.302%
12	4.028	834	836	843	rVB2	568	469	0.02%	0.007%
13	4.215	891	894	902	rBV3	297	344	0.01%	0.005%
14	4.469	968	973	977	rVB3	192	212	0.01%	0.003%
15	4.539	988	995	998	rBV3	350	483	0.02%	0.007%
16	4.562	998	1002	1003	rBV2	766	504	0.02%	0.007%
17	4.671	1013	1036	1067	rBV2	267471	684753	28.90%	9.860%
18	4.935	1114	1118	1121	rVB2	486	304	0.01%	0.004%
19	4.957	1121	1125	1126	rVV2	320	247	0.01%	0.004%
20	4.970	1126	1129	1134	rVB4	294	227	0.01%	0.003%
21	5.067	1143	1159	1192	rBV2	211630	560840	23.67%	8.076%
22	5.321	1220	1238	1270	rBV	1062346	2369325	100.00%	34.118%
23	5.459	1279	1281	1284	rBV3	376	230	0.01%	0.003%
24	5.507	1293	1296	1302	rBV3	601	519	0.02%	0.007%
25	5.729	1345	1365	1388	rBV2	134639	363052	15.32%	5.228%
26	6.250	1514	1527	1547	rBV	80261	154274	6.51%	2.222%
27	6.546	1608	1619	1633	rVB2	16555	30452	1.29%	0.439%
28	6.623	1638	1643	1646	rBV3	404	331	0.01%	0.005%
29	6.642	1646	1649	1652	rVB3	312	215	0.01%	0.003%
30	6.694	1652	1665	1681	rBV	79821	155827	6.58%	2.244%
31	6.761	1681	1686	1699	rVB6	3491	6085	0.26%	0.088%
32	6.864	1713	1718	1721	rBV3	379	382	0.02%	0.006%
33	7.018	1763	1766	1768	rBV	324	213	0.01%	0.003%
34	7.112	1793	1795	1800	rVB3	287	219	0.01%	0.003%
35	7.185	1814	1818	1821	rBV3	352	365	0.02%	0.005%
36	7.288	1848	1850	1856	rVB3	320	226	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047644.D
 Acq On : 24 Mar 2022 20:00
 Operator : SY/MD
 Sample : N2081-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.343	1862	1867	1872	rBV3	236	296	0.01%	0.004%
38	7.394	1879	1883	1887	rBV3	235	260	0.01%	0.004%
39	7.513	1916	1920	1924	rBV2	304	255	0.01%	0.004%
40	7.568	1924	1937	1954	rBV2	45845	79303	3.35%	1.142%
41	7.668	1963	1968	1972	rBV2	481	489	0.02%	0.007%
42	7.755	1990	1995	1997	rBV2	229	230	0.01%	0.003%
43	7.796	2001	2008	2009	rBV2	823	733	0.03%	0.011%
44	7.854	2021	2026	2027	rBV2	358	253	0.01%	0.004%
45	7.899	2028	2040	2055	rBV	156114	274805	11.60%	3.957%
46	8.038	2077	2083	2088	rVB5	1465	1814	0.08%	0.026%
47	8.182	2117	2128	2142	rBV2	31603	54233	2.29%	0.781%
48	8.372	2184	2187	2195	rVB3	542	480	0.02%	0.007%
49	8.478	2208	2220	2232	rVB2	8757	16979	0.72%	0.244%
50	8.555	2232	2244	2258	rBV	100111	169569	7.16%	2.442%
51	8.639	2258	2270	2303	rVV	103737	209122	8.83%	3.011%
52	8.870	2332	2342	2348	rBV5	1479	2528	0.11%	0.036%
53	8.922	2352	2358	2360	rBV3	608	653	0.03%	0.009%
54	9.185	2437	2440	2444	rVV2	301	222	0.01%	0.003%
55	9.417	2498	2512	2535	rBV	124155	214583	9.06%	3.090%
56	9.693	2591	2598	2609	rVB8	1663	3036	0.13%	0.044%
57	9.886	2654	2658	2661	rBV4	570	500	0.02%	0.007%
58	10.041	2701	2706	2710	rBV3	413	439	0.02%	0.006%
59	10.066	2712	2714	2719	rVB4	460	363	0.02%	0.005%
60	10.102	2719	2725	2726	rBV3	801	787	0.03%	0.011%
61	10.201	2752	2756	2761	rVB3	242	229	0.01%	0.003%
62	10.272	2768	2778	2785	rBV6	2808	3888	0.16%	0.056%
63	10.375	2806	2810	2814	rVB3	746	546	0.02%	0.008%
64	10.603	2878	2881	2884	rBV2	268	212	0.01%	0.003%
65	10.645	2889	2894	2898	rBV3	920	1026	0.04%	0.015%
66	10.697	2906	2910	2917	rVB4	1326	1754	0.07%	0.025%
67	10.758	2917	2929	2944	rBV	126212	204159	8.62%	2.940%
68	10.896	2962	2972	2985	rVB2	14563	24551	1.04%	0.354%
69	10.989	2996	3001	3002	rBV3	465	338	0.01%	0.005%
70	11.089	3024	3032	3040	rBV4	1606	2263	0.10%	0.033%
71	11.179	3055	3060	3061	rBV	329	227	0.01%	0.003%
72	11.279	3087	3091	3092	rBV3	620	367	0.02%	0.005%
73	11.301	3092	3098	3102	rVB7	1714	2043	0.09%	0.029%
74	11.468	3139	3150	3157	rBV5	4378	7212	0.30%	0.104%
75	11.584	3181	3186	3187	rBV2	611	428	0.02%	0.006%
76	11.603	3189	3192	3196	rVB4	1048	881	0.04%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047644.D
 Acq On : 24 Mar 2022 20:00
 Operator : SY/MD
 Sample : N2081-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.703	3221	3223	3227	rVV2	539	398	0.02%	0.006%
78	11.748	3230	3237	3245	rVB6	1037	1605	0.07%	0.023%
79	11.812	3245	3257	3273	rBV	153544	248878	10.50%	3.584%
80	11.899	3275	3284	3290	rVB2	3096	4373	0.18%	0.063%
81	11.973	3303	3307	3316	rVB5	787	1169	0.05%	0.017%
82	12.095	3341	3345	3352	rVV6	1416	1873	0.08%	0.027%
83	12.195	3363	3376	3395	rBV	181541	304057	12.83%	4.378%
84	12.291	3400	3406	3408	rBV3	394	360	0.02%	0.005%
85	12.314	3410	3413	3415	rVB2	662	340	0.01%	0.005%
86	12.330	3415	3418	3424	rBV5	878	836	0.04%	0.012%
87	12.369	3427	3430	3432	rBV	455	283	0.01%	0.004%
88	12.491	3463	3468	3476	rVB5	950	1289	0.05%	0.019%
89	12.574	3489	3494	3502	rVB2	1157	1483	0.06%	0.021%
90	12.703	3526	3534	3541	rVB5	1711	2595	0.11%	0.037%
91	12.774	3550	3556	3565	rBV3	1410	1993	0.08%	0.029%
92	12.867	3581	3585	3594	rVB5	1525	2089	0.09%	0.030%
93	13.024	3629	3634	3636	rBV3	515	455	0.02%	0.007%
94	13.227	3692	3697	3706	rVB6	1757	2151	0.09%	0.031%
95	13.629	3820	3822	3824	rBV3	445	214	0.01%	0.003%
96	13.844	3880	3889	3897	rBV7	2157	3399	0.14%	0.049%
97	14.092	3958	3966	3978	rVB2	5635	9054	0.38%	0.130%
98	14.253	4013	4016	4018	rBV	432	319	0.01%	0.005%
99	14.333	4035	4041	4055	rVB5	1758	2829	0.12%	0.041%
100	14.497	4090	4092	4097	rBV2	381	253	0.01%	0.004%




Sum of corrected areas: 6944564

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047644.D
Acq On : 24 Mar 2022 20:00
Operator : SY/MD
Sample : N2081-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

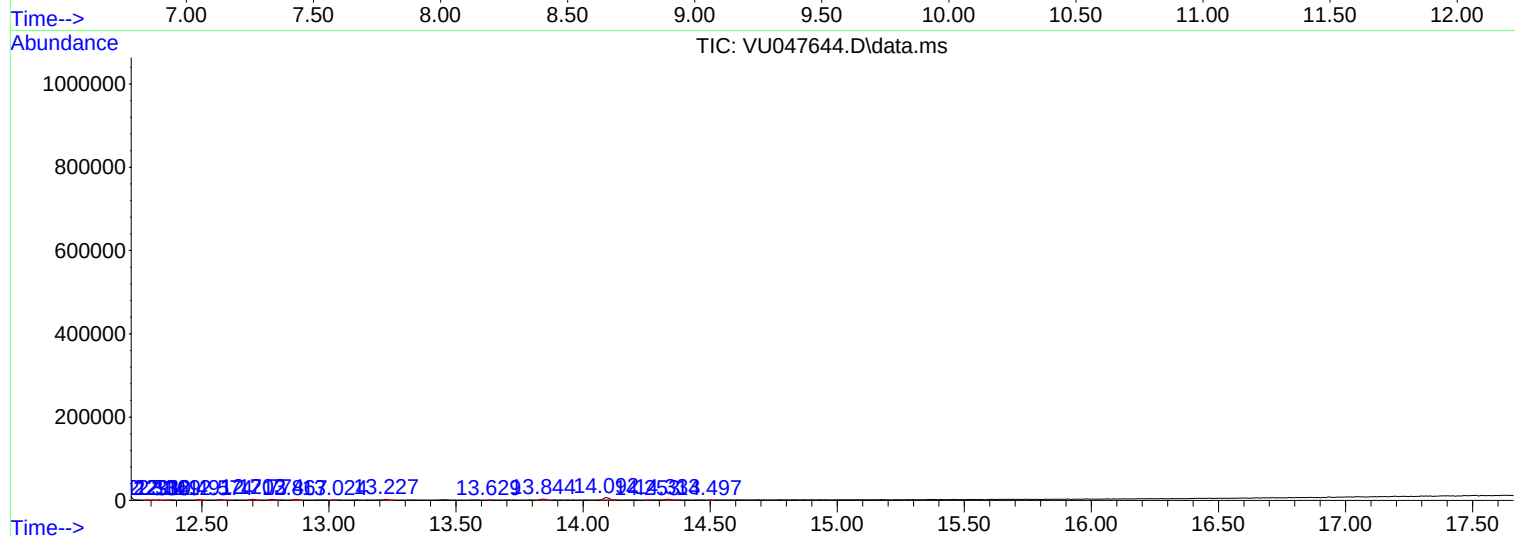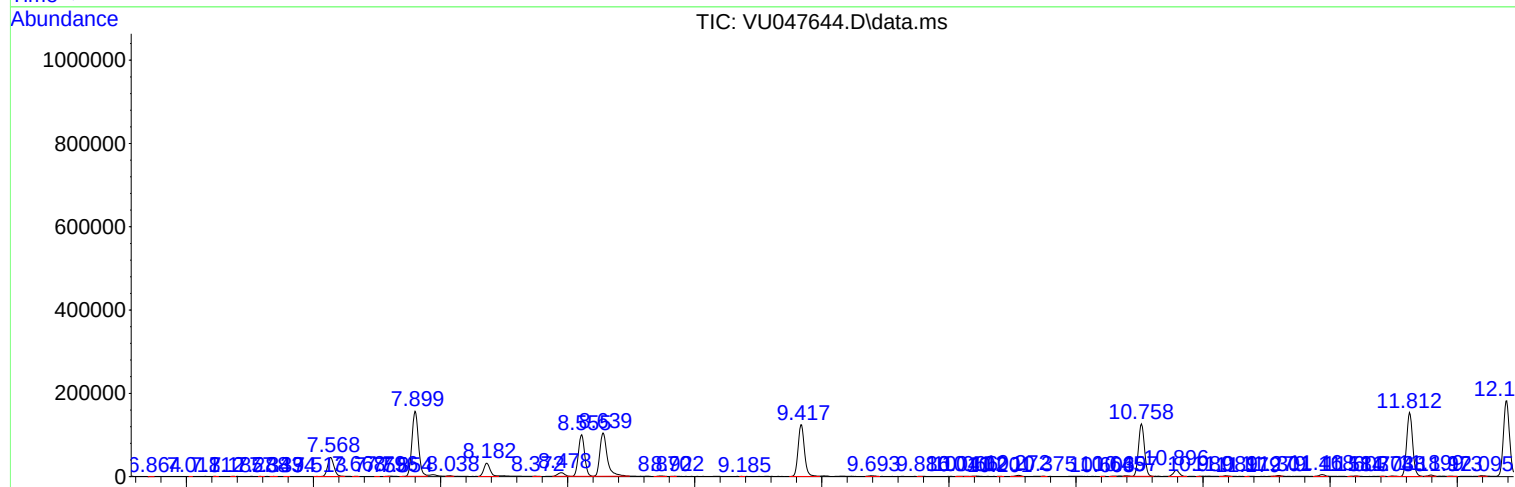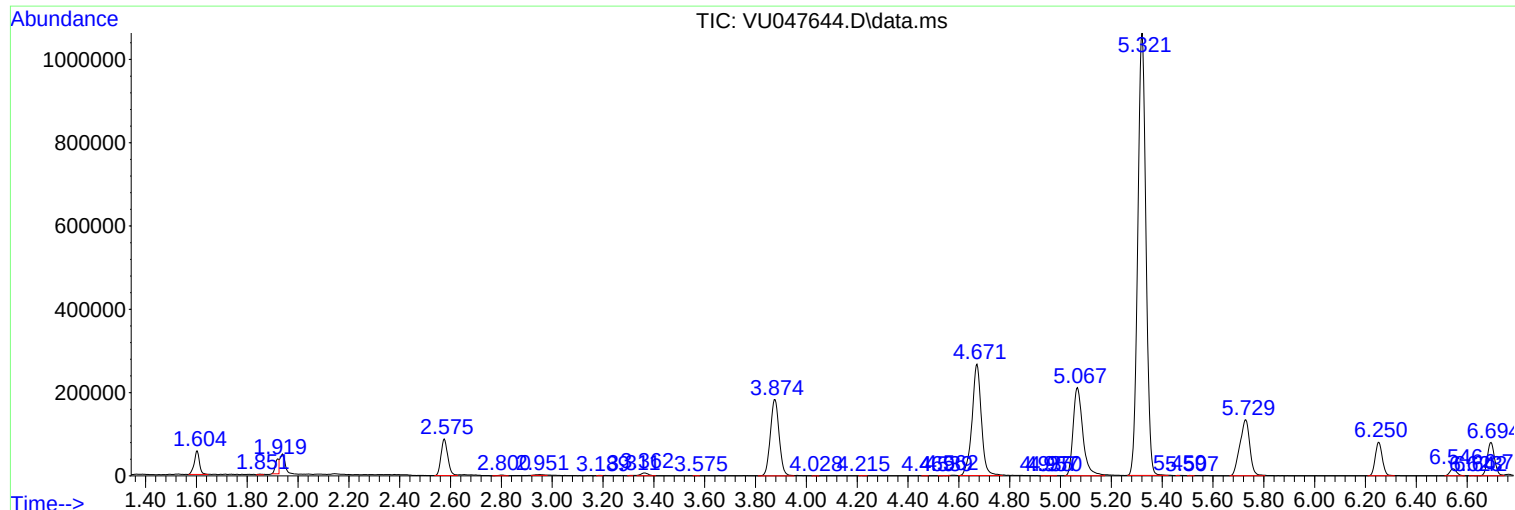

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047644.D
Acq On : 24 Mar 2022 20:00
Operator : SY/MD
Sample : N2081-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047644.D
Acq On : 24 Mar 2022 20:00
Operator : SY/MD
Sample : N2081-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------