

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047646.D
 Acq On : 24 Mar 2022 20:46
 Operator : SY/MD
 Sample : N2081-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	94	rBV	62707	72238	6.76%	1.351%
2	1.919	172	180	191	rBV	48346	64819	6.07%	1.212%
3	2.575	371	384	406	rBV3	120870	222710	20.85%	4.164%
4	2.790	449	451	453	rBV	360	223	0.02%	0.004%
5	2.928	488	494	500	rBV2	315	520	0.05%	0.010%
6	3.144	557	561	562	rBV2	332	259	0.02%	0.005%
7	3.182	567	573	574	rVV3	558	562	0.05%	0.011%
8	3.195	574	577	584	rVB3	685	736	0.07%	0.014%
9	3.295	605	608	611	rBV2	301	242	0.02%	0.005%
10	3.363	619	629	641	rVB4	3357	6152	0.58%	0.115%
11	3.575	687	695	698	rBV2	304	350	0.03%	0.007%
12	3.617	702	708	709	rBV	268	265	0.02%	0.005%
13	3.755	746	751	755	rBV2	382	439	0.04%	0.008%
14	3.874	770	788	808	rBV2	79971	191048	17.88%	3.572%
15	4.028	834	836	840	rVB3	380	211	0.02%	0.004%
16	4.054	840	844	848	rVB2	346	308	0.03%	0.006%
17	4.083	848	853	857	rBV3	314	400	0.04%	0.007%
18	4.218	891	895	897	rBV2	197	191	0.02%	0.004%
19	4.253	903	906	910	rVB	300	265	0.02%	0.005%
20	4.372	938	943	946	rBV	299	297	0.03%	0.006%
21	4.395	946	950	954	rVV2	408	426	0.04%	0.008%
22	4.420	956	958	962	rVV2	313	230	0.02%	0.004%
23	4.575	1002	1006	1009	rBV2	198	212	0.02%	0.004%
24	4.662	1014	1033	1074	rVV3	50977	199586	18.68%	3.731%
25	4.854	1091	1093	1100	rVB3	515	381	0.04%	0.007%
26	4.919	1110	1113	1121	rVB3	408	456	0.04%	0.009%
27	5.067	1142	1159	1186	rBV2	99525	236805	22.17%	4.427%
28	5.195	1196	1199	1204	rVV4	379	313	0.03%	0.006%
29	5.321	1219	1238	1264	rBV	474301	1068331	100.00%	19.973%
30	5.481	1286	1288	1292	rVB3	278	226	0.02%	0.004%
31	5.565	1311	1314	1317	rVB	352	218	0.02%	0.004%
32	5.729	1344	1365	1394	rVV2	183220	497830	46.60%	9.307%
33	6.250	1514	1527	1545	rBV	114560	218294	20.43%	4.081%
34	6.542	1606	1618	1632	rBV3	17688	34090	3.19%	0.637%
35	6.694	1651	1665	1683	rBV	108893	216669	20.28%	4.051%
36	6.809	1698	1701	1705	rVB2	319	205	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047646.D
 Acq On : 24 Mar 2022 20:46
 Operator : SY/MD
 Sample : N2081-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.208	1822	1825	1827	rVB2	304	202	0.02%	0.004%
38	7.295	1846	1852	1855	rBV2	330	299	0.03%	0.006%
39	7.568	1924	1937	1956	rBV	61904	109208	10.22%	2.042%
40	7.661	1963	1966	1974	rVB3	330	455	0.04%	0.009%
41	7.845	2019	2023	2026	rBV2	330	306	0.03%	0.006%
42	7.899	2027	2040	2056	rBV	217886	383207	35.87%	7.164%
43	8.182	2117	2128	2141	rBV	43579	75948	7.11%	1.420%
44	8.404	2190	2197	2206	rVB5	1167	1479	0.14%	0.028%
45	8.475	2210	2219	2231	rVB2	5625	9955	0.93%	0.186%
46	8.555	2232	2244	2258	rBV	51106	86824	8.13%	1.623%
47	8.639	2258	2270	2304	rBV	148559	293406	27.46%	5.485%
48	8.845	2331	2334	2341	rVB2	300	322	0.03%	0.006%
49	8.964	2368	2371	2376	rVB3	328	236	0.02%	0.004%
50	9.124	2419	2421	2428	rVB3	432	405	0.04%	0.008%
51	9.169	2428	2435	2438	rBV2	424	409	0.04%	0.008%
52	9.192	2438	2442	2446	rVV2	254	268	0.03%	0.005%
53	9.266	2462	2465	2469	rVB2	342	202	0.02%	0.004%
54	9.417	2499	2512	2534	rBV	176594	302772	28.34%	5.661%
55	9.571	2553	2560	2567	rBV	890	1137	0.11%	0.021%
56	9.648	2580	2584	2590	rBV2	284	335	0.03%	0.006%
57	9.693	2593	2598	2604	rBV3	871	1018	0.10%	0.019%
58	9.922	2665	2669	2673	rVV2	293	296	0.03%	0.006%
59	10.079	2714	2718	2720	rBV	345	268	0.03%	0.005%
60	10.108	2720	2727	2732	rVB4	596	763	0.07%	0.014%
61	10.285	2778	2782	2785	rVB2	278	220	0.02%	0.004%
62	10.314	2787	2791	2795	rVV2	318	299	0.03%	0.006%
63	10.398	2814	2817	2821	rBV2	283	211	0.02%	0.004%
64	10.449	2829	2833	2838	rVB3	431	494	0.05%	0.009%
65	10.475	2838	2841	2843	rBV3	333	214	0.02%	0.004%
66	10.491	2843	2846	2850	rVB	448	344	0.03%	0.006%
67	10.520	2850	2855	2858	rBV2	376	340	0.03%	0.006%
68	10.581	2871	2874	2878	rBV2	309	273	0.03%	0.005%
69	10.671	2896	2902	2908	rBV3	1131	1172	0.11%	0.022%
70	10.693	2908	2909	2915	rVB	336	194	0.02%	0.004%
71	10.758	2915	2929	2943	rBV	176084	281520	26.35%	5.263%
72	10.896	2958	2972	2983	rBV2	8196	13712	1.28%	0.256%
73	11.089	3024	3032	3035	rBV3	805	1071	0.10%	0.020%
74	11.134	3043	3046	3048	rBV2	334	225	0.02%	0.004%
75	11.208	3066	3069	3072	rBV	329	283	0.03%	0.005%
76	11.250	3078	3082	3086	rVB2	348	355	0.03%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047646.D
 Acq On : 24 Mar 2022 20:46
 Operator : SY/MD
 Sample : N2081-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.282	3087	3092	3093	rBV2	394	264	0.02%	0.005%
78	11.365	3115	3118	3125	rBV2	190	238	0.02%	0.004%
79	11.468	3141	3150	3160	rVV5	2810	4680	0.44%	0.087%
80	11.510	3160	3163	3167	rVV2	357	234	0.02%	0.004%
81	11.700	3219	3222	3226	rVB	398	257	0.02%	0.005%
82	11.742	3232	3235	3238	rBV2	532	404	0.04%	0.008%
83	11.812	3245	3257	3277	rBV	207752	328026	30.70%	6.133%
84	11.893	3277	3282	3286	rBV	1322	1390	0.13%	0.026%
85	11.967	3301	3305	3308	rBV4	347	323	0.03%	0.006%
86	12.073	3336	3338	3341	rBV3	428	260	0.02%	0.005%
87	12.195	3363	3376	3393	rBV	238492	391803	36.67%	7.325%
88	12.333	3416	3419	3422	rBV3	321	193	0.02%	0.004%
89	12.407	3437	3442	3446	rBV3	226	255	0.02%	0.005%
90	12.558	3486	3489	3493	rBV3	202	214	0.02%	0.004%
91	12.742	3538	3546	3549	rBV3	306	465	0.04%	0.009%
92	12.777	3549	3557	3564	rVV3	1457	2349	0.22%	0.044%
93	12.931	3601	3605	3608	rBV3	272	310	0.03%	0.006%
94	13.092	3652	3655	3662	rBV3	308	282	0.03%	0.005%
95	13.230	3693	3698	3704	rVB5	989	1330	0.12%	0.025%
96	13.291	3714	3717	3722	rVB3	349	303	0.03%	0.006%
97	13.320	3723	3726	3729	rBV2	327	289	0.03%	0.005%
98	13.844	3884	3889	3898	rVB5	1157	1598	0.15%	0.030%
99	14.098	3957	3968	3974	rBV	3306	5060	0.47%	0.095%
100	14.333	4036	4041	4048	rBV3	1058	1159	0.11%	0.022%




Sum of corrected areas: 5348840

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047646.D
Acq On : 24 Mar 2022 20:46
Operator : SY/MD
Sample : N2081-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

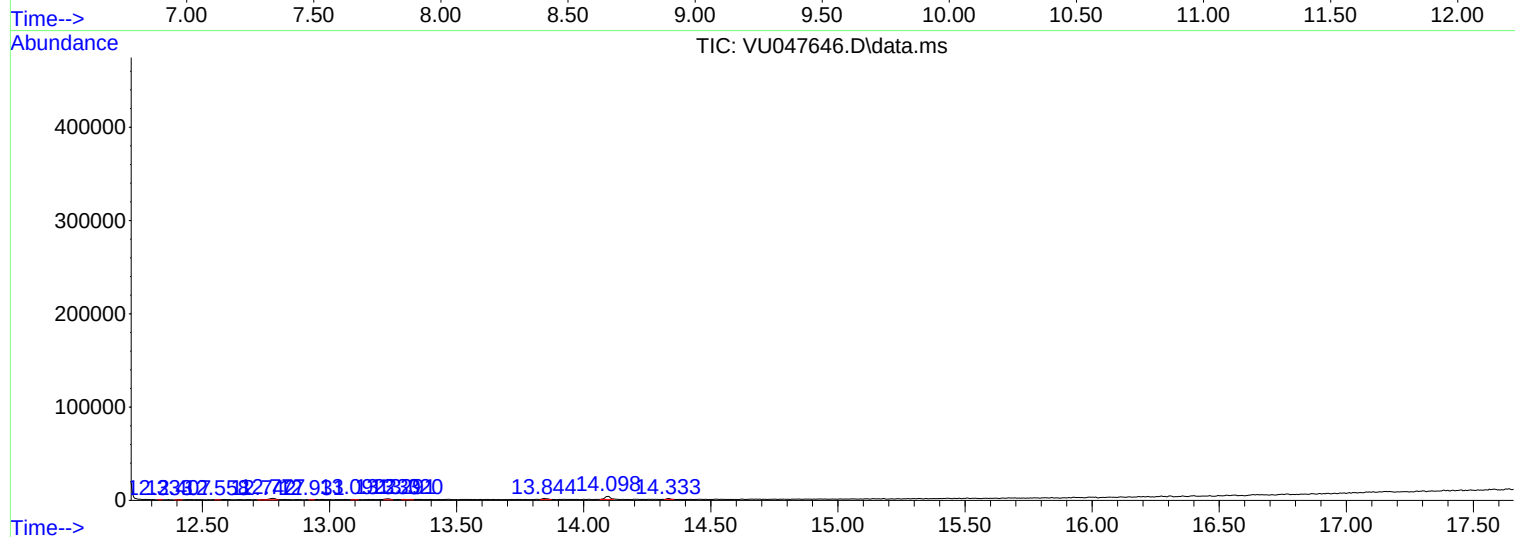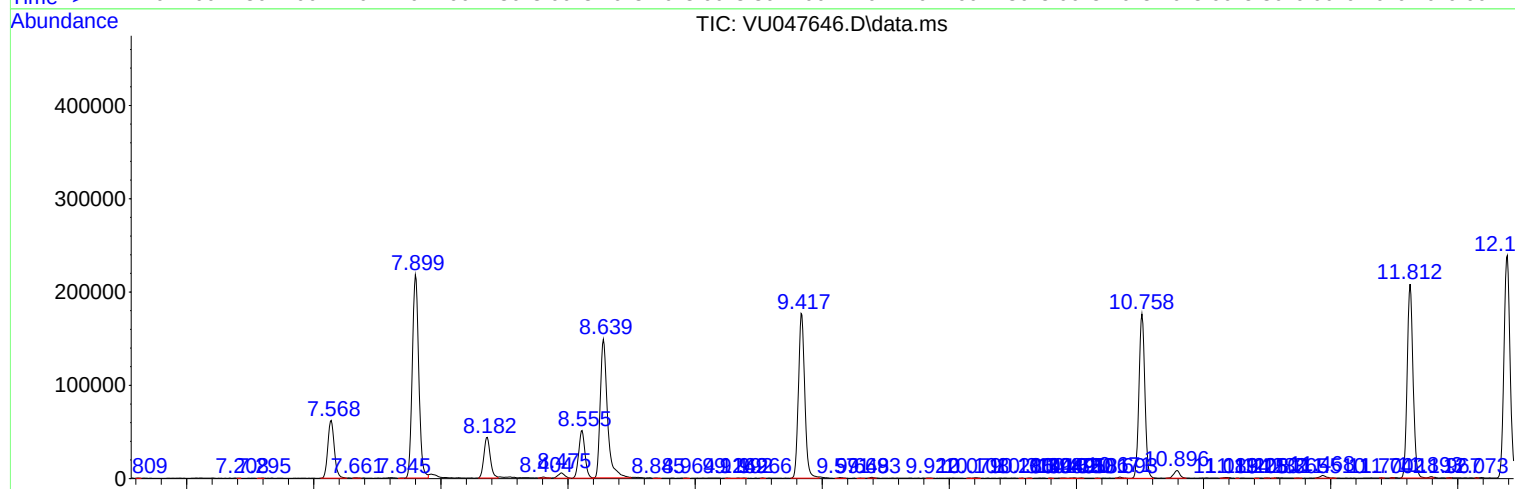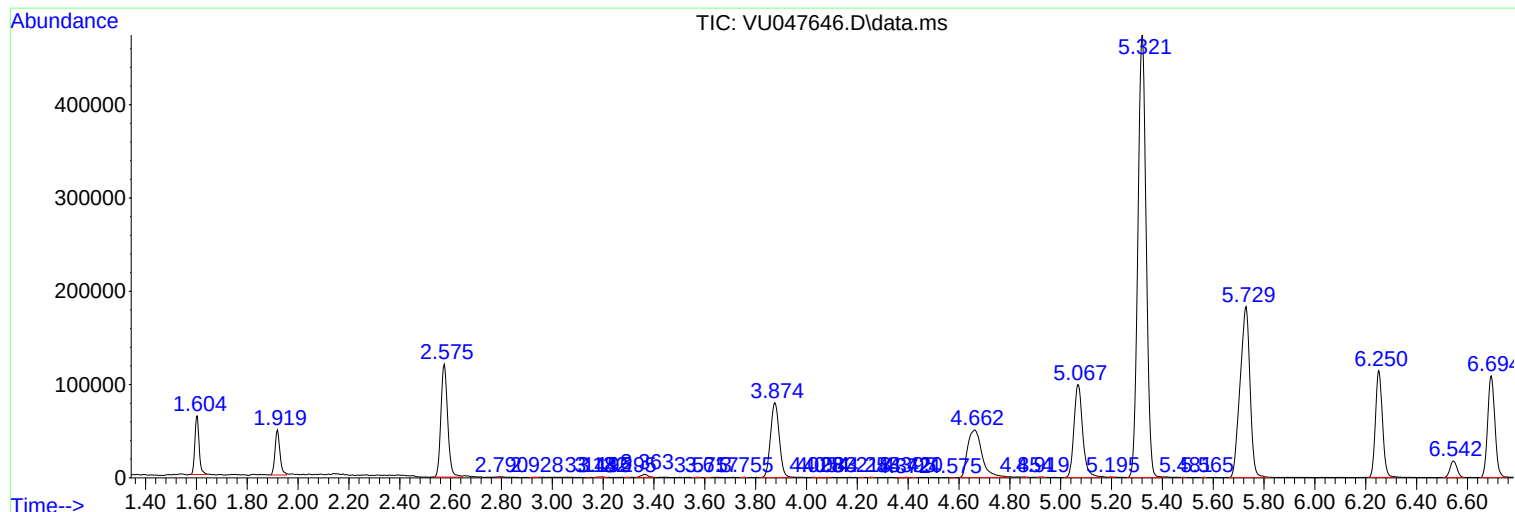

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047646.D
Acq On : 24 Mar 2022 20:46
Operator : SY/MD
Sample : N2081-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047646.D
Acq On : 24 Mar 2022 20:46
Operator : SY/MD
Sample : N2081-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------