

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047648.D
 Acq On : 24 Mar 2022 21:31
 Operator : SY/MD
 Sample : N2081-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rVB	122234	146525	14.27%	1.547%
2	1.694	105	110	120	rVB2	6088	8537	0.83%	0.090%
3	1.919	172	180	197	rVB	101054	134175	13.07%	1.416%
4	2.572	370	383	400	rBV2	229167	405901	39.53%	4.284%
5	2.719	427	429	433	rVB3	586	313	0.03%	0.003%
6	2.803	446	455	460	rBV3	1038	1863	0.18%	0.020%
7	3.051	529	532	538	rBV3	419	411	0.04%	0.004%
8	3.099	542	547	553	rBV3	314	388	0.04%	0.004%
9	3.195	567	577	585	rBV3	796	1494	0.15%	0.016%
10	3.305	609	611	615	rVB2	498	299	0.03%	0.003%
11	3.362	619	629	642	rVV5	3488	6294	0.61%	0.066%
12	3.465	654	661	665	rVB2	255	356	0.03%	0.004%
13	3.578	692	696	697	rBV2	508	349	0.03%	0.004%
14	3.633	709	713	717	rBV2	275	293	0.03%	0.003%
15	3.768	753	755	764	rVB	312	339	0.03%	0.004%
16	3.874	770	788	811	rBV	89187	214894	20.93%	2.268%
17	4.076	846	851	854	rBV2	304	258	0.03%	0.003%
18	4.301	914	921	925	rBV2	242	303	0.03%	0.003%
19	4.472	966	974	982	rVB6	730	967	0.09%	0.010%
20	4.639	1006	1026	1030	rBV	119369	254430	24.78%	2.686%
21	5.067	1143	1159	1181	rVV	188554	419474	40.86%	4.428%
22	5.321	1219	1238	1261	rBV	446192	1005583	97.94%	10.614%
23	5.546	1305	1308	1311	rVV2	381	309	0.03%	0.003%
24	5.729	1344	1365	1394	rBV2	379480	1026717	100.00%	10.837%
25	5.967	1435	1439	1440	rBV2	417	291	0.03%	0.003%
26	6.057	1462	1467	1470	rVV3	352	311	0.03%	0.003%
27	6.108	1480	1483	1489	rBV3	286	307	0.03%	0.003%
28	6.160	1495	1499	1503	rVB5	439	483	0.05%	0.005%
29	6.250	1512	1527	1547	rBV	227766	437560	42.62%	4.619%
30	6.546	1607	1619	1638	rVV2	30716	57759	5.63%	0.610%
31	6.694	1648	1665	1685	rBV	234996	458040	44.61%	4.835%
32	7.115	1793	1796	1798	rBV	511	371	0.04%	0.004%
33	7.185	1816	1818	1824	rBV	524	604	0.06%	0.006%
34	7.259	1838	1841	1846	rBV2	285	307	0.03%	0.003%
35	7.295	1846	1852	1853	rBV2	335	317	0.03%	0.003%
36	7.568	1924	1937	1958	rBV	131130	233150	22.71%	2.461%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047648.D
 Acq On : 24 Mar 2022 21:31
 Operator : SY/MD
 Sample : N2081-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.693	1970	1976	1983	rVB5	737	1011	0.10%	0.011%
38	7.796	1999	2008	2013	rBV5	1217	1616	0.16%	0.017%
39	7.899	2027	2040	2057	rBV	490217	844917	82.29%	8.918%
40	8.182	2113	2128	2149	rBV	91513	167067	16.27%	1.763%
41	8.362	2180	2184	2186	rBV2	287	251	0.02%	0.003%
42	8.404	2193	2197	2205	rVB4	949	889	0.09%	0.009%
43	8.472	2210	2218	2229	rVB3	4299	7361	0.72%	0.078%
44	8.555	2233	2244	2257	rBV2	90786	155259	15.12%	1.639%
45	8.636	2257	2269	2312	rVV	375354	710348	69.19%	7.498%
46	8.783	2313	2315	2322	rVB5	961	880	0.09%	0.009%
47	8.883	2343	2346	2349	rBV4	440	351	0.03%	0.004%
48	8.980	2372	2376	2379	rBV2	314	259	0.03%	0.003%
49	9.298	2469	2475	2479	rVB5	539	650	0.06%	0.007%
50	9.417	2494	2512	2531	rBV	344022	581954	56.68%	6.143%
51	9.552	2552	2554	2555	rBV2	508	246	0.02%	0.003%
52	9.571	2556	2560	2568	rVB3	1273	1588	0.15%	0.017%
53	9.693	2591	2598	2600	rBV4	1518	1715	0.17%	0.018%
54	9.851	2642	2647	2650	rBV	316	302	0.03%	0.003%
55	10.102	2719	2725	2732	rBV6	1071	1565	0.15%	0.017%
56	10.189	2749	2752	2760	rVB3	294	405	0.04%	0.004%
57	10.439	2825	2830	2835	rBV2	357	368	0.04%	0.004%
58	10.488	2838	2845	2851	rVB3	504	839	0.08%	0.009%
59	10.542	2859	2862	2866	rVB2	362	266	0.03%	0.003%
60	10.597	2876	2879	2883	rVB2	330	275	0.03%	0.003%
61	10.642	2888	2893	2894	rBV3	788	549	0.05%	0.006%
62	10.671	2894	2902	2909	rVB6	3702	5548	0.54%	0.059%
63	10.758	2915	2929	2948	rBV	360897	584978	56.98%	6.175%
64	10.896	2961	2972	2985	rVB4	7746	14813	1.44%	0.156%
65	10.976	2994	2997	2999	rBV2	381	264	0.03%	0.003%
66	10.999	2999	3004	3009	rBV3	1332	1676	0.16%	0.018%
67	11.089	3024	3032	3043	rBV3	3960	6337	0.62%	0.067%
68	11.205	3063	3068	3071	rBV4	621	620	0.06%	0.007%
69	11.243	3076	3080	3084	rVV3	458	448	0.04%	0.005%
70	11.291	3088	3095	3107	rVB3	3182	4797	0.47%	0.051%
71	11.385	3119	3124	3127	rVB	397	337	0.03%	0.004%
72	11.468	3139	3150	3165	rVB2	21490	34120	3.32%	0.360%
73	11.645	3201	3205	3208	rBV2	447	394	0.04%	0.004%
74	11.684	3213	3217	3218	rBV2	939	626	0.06%	0.007%
75	11.697	3218	3221	3227	rVB4	1718	1746	0.17%	0.018%
76	11.738	3229	3234	3235	rBV2	785	572	0.06%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047648.D
 Acq On : 24 Mar 2022 21:31
 Operator : SY/MD
 Sample : N2081-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.812	3244	3257	3274	rBV	392524	623811	60.76%	6.584%
78	11.896	3276	3283	3290	rVB3	6437	8415	0.82%	0.089%
79	11.973	3302	3307	3317	rVB5	2882	4360	0.42%	0.046%
80	12.095	3338	3345	3351	rBV4	2735	4371	0.43%	0.046%
81	12.192	3362	3375	3395	rVB	508183	826847	80.53%	8.727%
82	12.279	3400	3402	3411	rVB4	1647	1490	0.15%	0.016%
83	12.333	3413	3419	3421	rBV3	1098	1171	0.11%	0.012%
84	12.475	3456	3463	3465	rBV4	2014	2210	0.22%	0.023%
85	12.571	3488	3493	3504	rVB3	2244	2997	0.29%	0.032%
86	12.623	3504	3509	3512	rBV4	578	620	0.06%	0.007%
87	12.671	3520	3524	3526	rBV2	418	328	0.03%	0.003%
88	12.774	3547	3556	3569	rBV4	1763	3137	0.31%	0.033%
89	12.877	3581	3588	3596	rBV3	649	1087	0.11%	0.011%
90	12.970	3614	3617	3627	rVB2	1007	1140	0.11%	0.012%
91	13.028	3628	3635	3646	rVB4	1714	2627	0.26%	0.028%
92	13.156	3669	3675	3679	rBB3	445	485	0.05%	0.005%
93	13.298	3715	3719	3724	rBV3	573	439	0.04%	0.005%
94	13.449	3760	3766	3774	rBV5	2275	3403	0.33%	0.036%
95	13.529	3789	3791	3795	rVB2	497	299	0.03%	0.003%
96	13.841	3883	3888	3899	rVB5	934	1607	0.16%	0.017%
97	14.089	3957	3965	3986	rVB	12346	20712	2.02%	0.219%
98	14.944	4228	4231	4233	rBV3	487	341	0.03%	0.004%
99	15.076	4269	4272	4274	rBV2	412	277	0.03%	0.003%
100	15.230	4312	4320	4330	rBV4	2096	3702	0.36%	0.039%




Sum of corrected areas: 9474055

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047648.D
Acq On : 24 Mar 2022 21:31
Operator : SY/MD
Sample : N2081-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

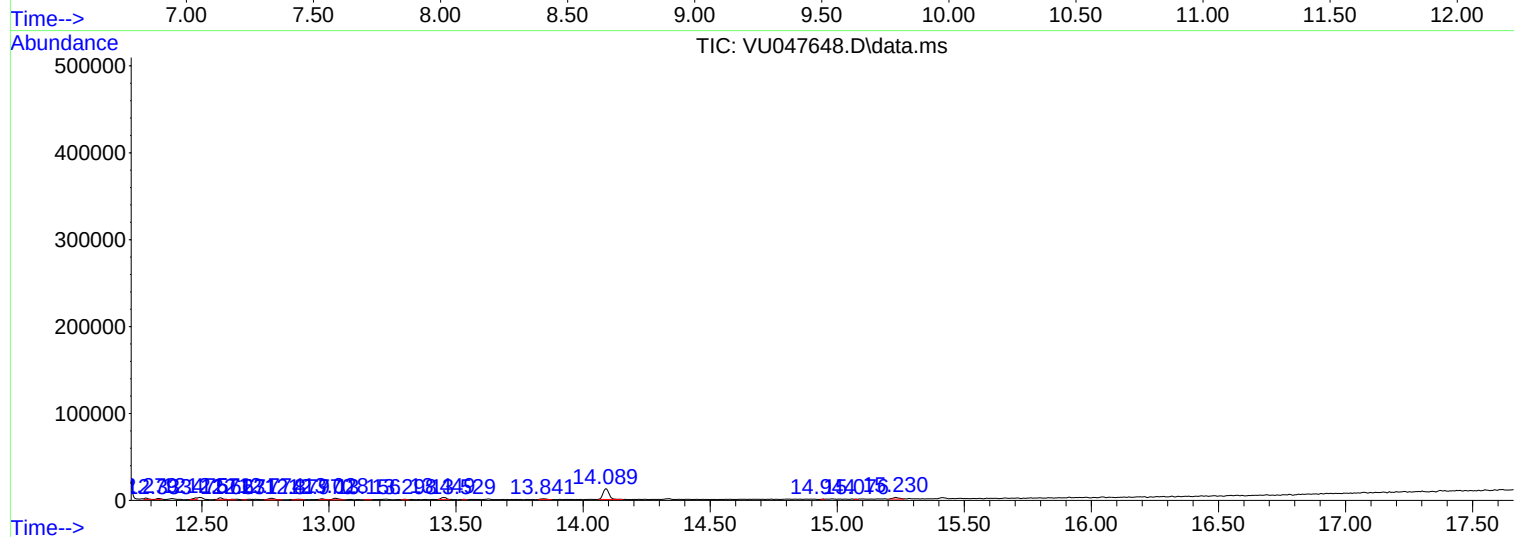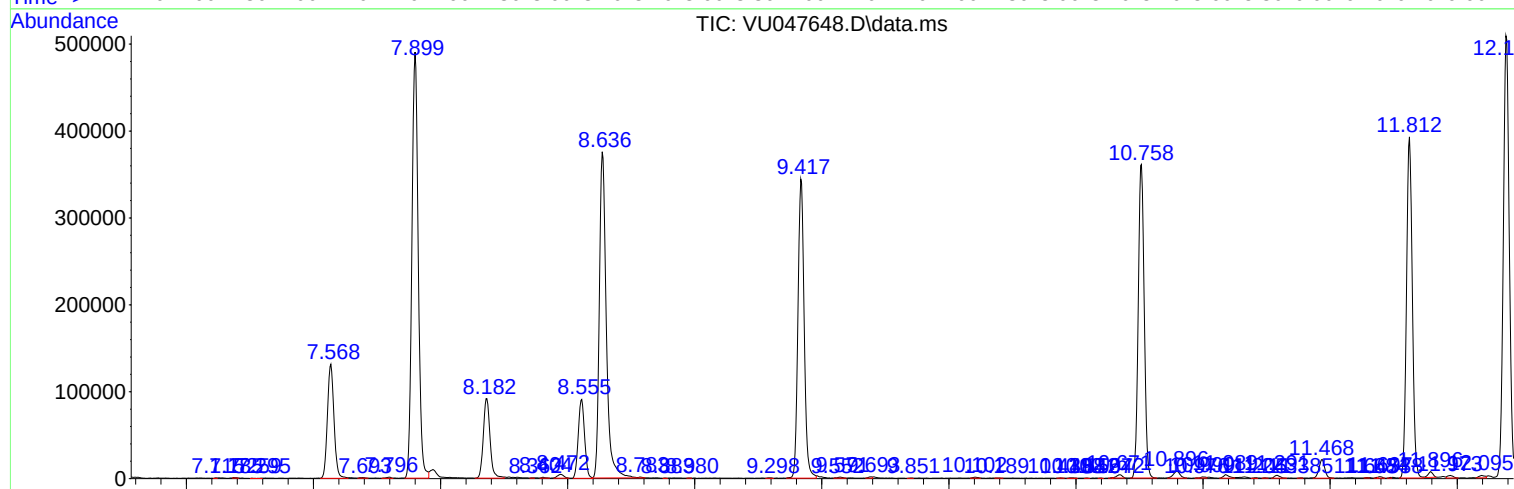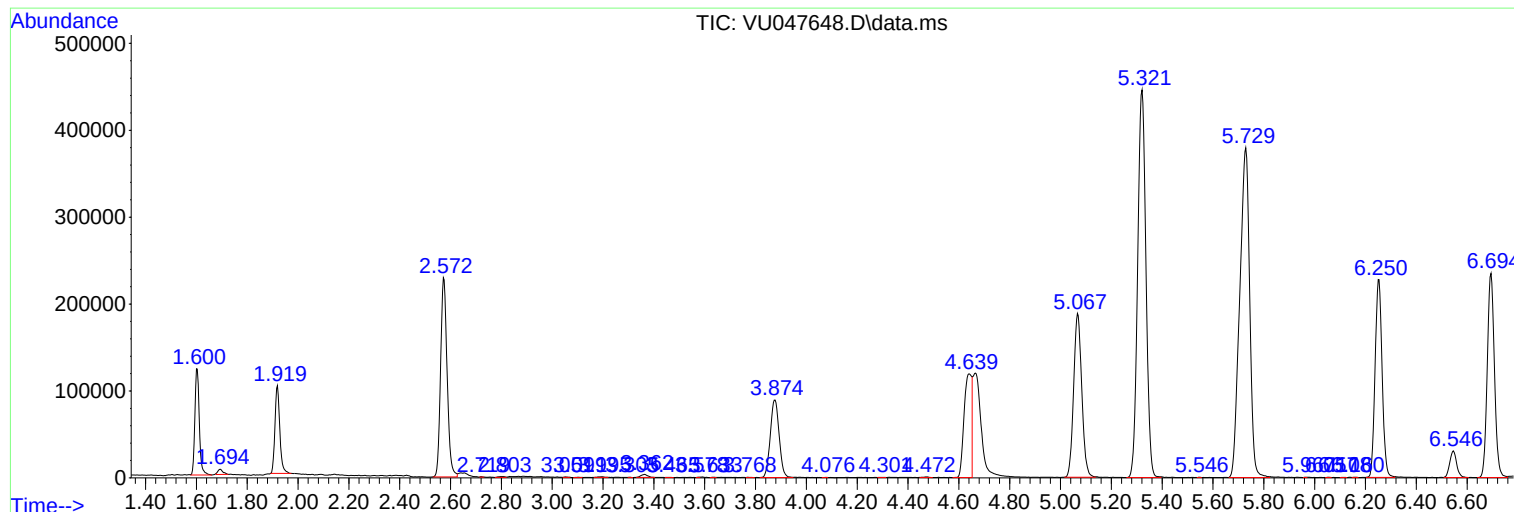

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047648.D
Acq On : 24 Mar 2022 21:31
Operator : SY/MD
Sample : N2081-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047648.D
Acq On : 24 Mar 2022 21:31
Operator : SY/MD
Sample : N2081-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------