

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047654.D
 Acq On : 24 Mar 2022 23:47
 Operator : SY/MD
 Sample : N2081-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047654.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	103	rVB	131800	158169	11.33%	1.349%
2	1.919	171	180	203	rBV	103108	142044	10.18%	1.211%
3	2.571	371	383	418	rBV2	249508	445067	31.89%	3.796%
4	2.787	445	450	451	rBV3	718	580	0.04%	0.005%
5	2.960	501	504	507	rBV4	265	227	0.02%	0.002%
6	3.009	515	519	522	rBV2	329	344	0.02%	0.003%
7	3.047	526	531	532	rBV2	451	393	0.03%	0.003%
8	3.192	572	576	578	rVV4	411	229	0.02%	0.002%
9	3.359	618	628	639	rVB2	3391	5937	0.43%	0.051%
10	3.533	676	682	685	rBV2	364	313	0.02%	0.003%
11	3.636	710	714	719	rBV3	227	251	0.02%	0.002%
12	3.665	719	723	731	rBV3	278	400	0.03%	0.003%
13	3.874	772	788	806	rBV	47675	110701	7.93%	0.944%
14	4.044	838	841	842	rBV	375	208	0.01%	0.002%
15	4.224	893	897	901	rBV	194	214	0.02%	0.002%
16	4.436	955	963	968	rBV3	278	532	0.04%	0.005%
17	4.517	985	988	994	rVB3	406	329	0.02%	0.003%
18	4.658	1013	1032	1074	rBV2	113950	463429	33.21%	3.953%
19	5.067	1143	1159	1188	rVB	202452	445022	31.89%	3.796%
20	5.321	1217	1238	1259	rBV	624218	1395615	100.00%	11.903%
21	5.504	1291	1295	1298	rVB3	271	208	0.01%	0.002%
22	5.526	1298	1302	1307	rVB3	349	302	0.02%	0.003%
23	5.552	1307	1310	1312	rBV	316	231	0.02%	0.002%
24	5.632	1332	1335	1338	rBV3	327	228	0.02%	0.002%
25	5.729	1343	1365	1394	rBV2	414301	1116184	79.98%	9.520%
26	5.886	1409	1414	1417	rBV2	474	336	0.02%	0.003%
27	6.054	1462	1466	1468	rBV2	334	252	0.02%	0.002%
28	6.121	1482	1487	1491	rVB4	598	679	0.05%	0.006%
29	6.166	1499	1501	1507	rVB2	347	257	0.02%	0.002%
30	6.250	1512	1527	1552	rBV	385543	734801	52.65%	6.267%
31	6.375	1563	1566	1568	rVB3	345	208	0.01%	0.002%
32	6.472	1594	1596	1600	rVB3	324	243	0.02%	0.002%
33	6.546	1605	1619	1637	rBV	85206	161725	11.59%	1.379%
34	6.693	1650	1665	1687	rBV	253920	495786	35.52%	4.228%
35	6.812	1700	1702	1705	rVB3	394	185	0.01%	0.002%
36	6.951	1739	1745	1748	rVB3	231	255	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047654.D
 Acq On : 24 Mar 2022 23:47
 Operator : SY/MD
 Sample : N2081-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.047	1772	1775	1776	rBV2	412	256	0.02%	0.002%
38	7.121	1793	1798	1803	rBV3	334	389	0.03%	0.003%
39	7.192	1812	1820	1822	rBV3	657	889	0.06%	0.008%
40	7.275	1841	1846	1850	rVB2	312	279	0.02%	0.002%
41	7.298	1850	1853	1857	rVB	224	191	0.01%	0.002%
42	7.333	1857	1864	1867	rBV2	326	447	0.03%	0.004%
43	7.404	1883	1886	1891	rVB3	230	245	0.02%	0.002%
44	7.500	1909	1916	1917	rBV3	271	279	0.02%	0.002%
45	7.568	1924	1937	1954	rBV	144587	253892	18.19%	2.165%
46	7.697	1973	1977	1982	rVB5	762	897	0.06%	0.008%
47	7.800	2005	2009	2017	rVB4	845	825	0.06%	0.007%
48	7.899	2023	2040	2056	rBV	536145	931569	66.75%	7.945%
49	8.179	2114	2127	2147	rBV2	104994	190204	13.63%	1.622%
50	8.404	2189	2197	2205	rVB5	1379	2172	0.16%	0.019%
51	8.475	2210	2219	2231	rVB2	2764	5196	0.37%	0.044%
52	8.555	2231	2244	2257	rBV	203066	345302	24.74%	2.945%
53	8.639	2257	2270	2304	rVV	387290	737078	52.81%	6.286%
54	8.809	2320	2323	2325	rBV2	376	281	0.02%	0.002%
55	9.015	2385	2387	2396	rVB4	323	502	0.04%	0.004%
56	9.057	2396	2400	2403	rBV2	230	208	0.01%	0.002%
57	9.195	2437	2443	2446	rBV3	291	244	0.02%	0.002%
58	9.417	2499	2512	2552	rVV	558743	960054	68.79%	8.188%
59	9.574	2553	2561	2572	rVB3	1033	1755	0.13%	0.015%
60	9.693	2589	2598	2608	rBV	2639	4241	0.30%	0.036%
61	9.754	2612	2617	2624	rVB2	265	372	0.03%	0.003%
62	10.008	2692	2696	2699	rBV2	356	342	0.02%	0.003%
63	10.092	2718	2722	2723	rBV2	769	477	0.03%	0.004%
64	10.147	2736	2739	2742	rVB2	386	207	0.01%	0.002%
65	10.317	2788	2792	2796	rBV	232	199	0.01%	0.002%
66	10.369	2802	2808	2811	rBV2	311	388	0.03%	0.003%
67	10.491	2840	2846	2851	rVB2	682	785	0.06%	0.007%
68	10.561	2865	2868	2872	rVB3	387	344	0.02%	0.003%
69	10.590	2872	2877	2878	rBV	316	220	0.02%	0.002%
70	10.671	2894	2902	2912	rVB4	3478	4577	0.33%	0.039%
71	10.758	2915	2929	2947	rVV	396400	638586	45.76%	5.446%
72	10.822	2947	2949	2952	rVV	537	355	0.03%	0.003%
73	10.841	2952	2955	2957	rVV2	477	268	0.02%	0.002%
74	10.896	2959	2972	2983	rVB3	5770	9430	0.68%	0.080%
75	10.999	2997	3004	3011	rBV5	1537	2704	0.19%	0.023%
76	11.095	3026	3034	3038	rBV4	1104	1568	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047654.D
 Acq On : 24 Mar 2022 23:47
 Operator : SY/MD
 Sample : N2081-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.147	3048	3050	3054	rVB3	520	328	0.02%	0.003%
78	11.205	3065	3068	3071	rVB2	449	270	0.02%	0.002%
79	11.250	3077	3082	3084	rBV2	387	389	0.03%	0.003%
80	11.288	3090	3094	3104	rVB2	1088	1452	0.10%	0.012%
81	11.352	3109	3114	3121	rBV3	252	376	0.03%	0.003%
82	11.468	3140	3150	3160	rVB3	8460	13513	0.97%	0.115%
83	11.577	3182	3184	3187	rVB3	394	213	0.02%	0.002%
84	11.616	3192	3196	3199	rBV2	381	248	0.02%	0.002%
85	11.696	3215	3221	3226	rVB5	1332	1590	0.11%	0.014%
86	11.741	3231	3235	3242	rBV3	734	739	0.05%	0.006%
87	11.812	3244	3257	3274	rBV	618251	987200	70.74%	8.420%
88	11.941	3294	3297	3301	rBV5	836	765	0.05%	0.007%
89	11.970	3302	3306	3317	rVB6	2223	3165	0.23%	0.027%
90	12.073	3326	3338	3340	rBV5	1390	2185	0.16%	0.019%
91	12.192	3362	3375	3392	rBV	550268	902034	64.63%	7.693%
92	12.330	3414	3418	3423	rVB2	1098	1146	0.08%	0.010%
93	12.401	3438	3440	3446	rVB4	500	440	0.03%	0.004%
94	12.484	3456	3466	3485	rBV2	8670	15147	1.09%	0.129%
95	12.565	3488	3491	3492	rBV	534	289	0.02%	0.002%
96	12.770	3548	3555	3565	rVB4	1201	2160	0.15%	0.018%
97	12.925	3598	3603	3606	rBV2	465	540	0.04%	0.005%
98	13.221	3691	3695	3697	rBV3	929	732	0.05%	0.006%
99	13.844	3883	3889	3896	rVB2	1201	1612	0.12%	0.014%
100	14.092	3957	3966	3976	rBV2	5444	8252	0.59%	0.070%




Sum of corrected areas: 11724886

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047654.D
Acq On : 24 Mar 2022 23:47
Operator : SY/MD
Sample : N2081-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

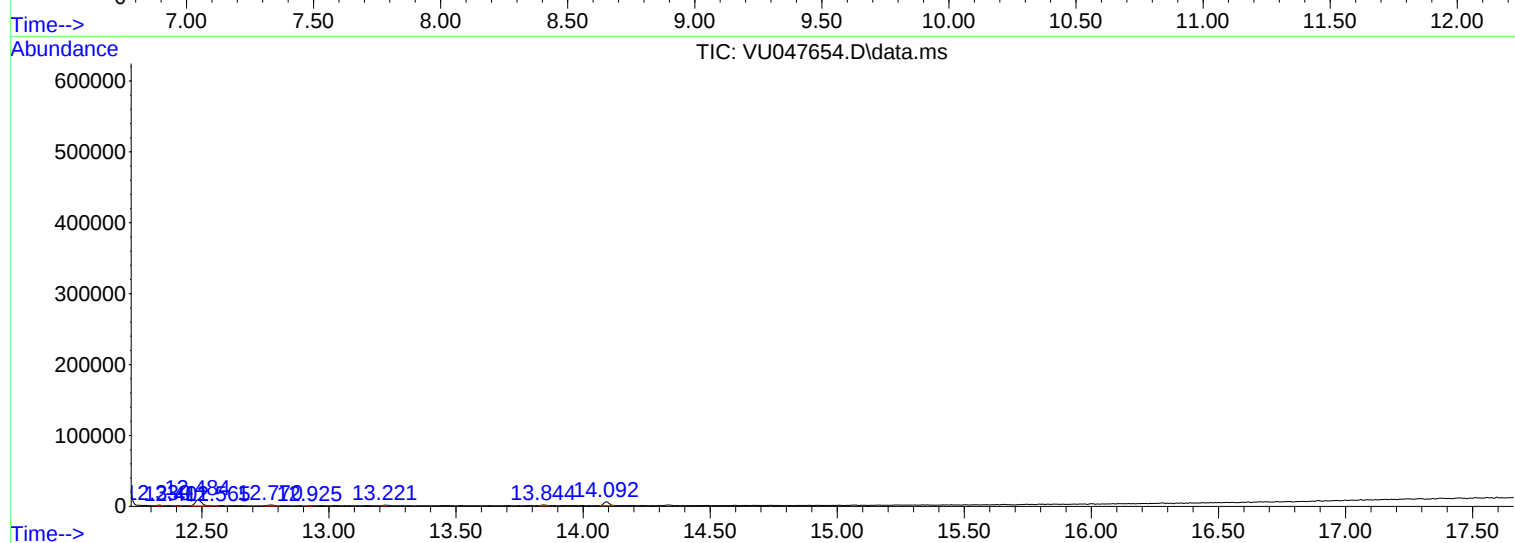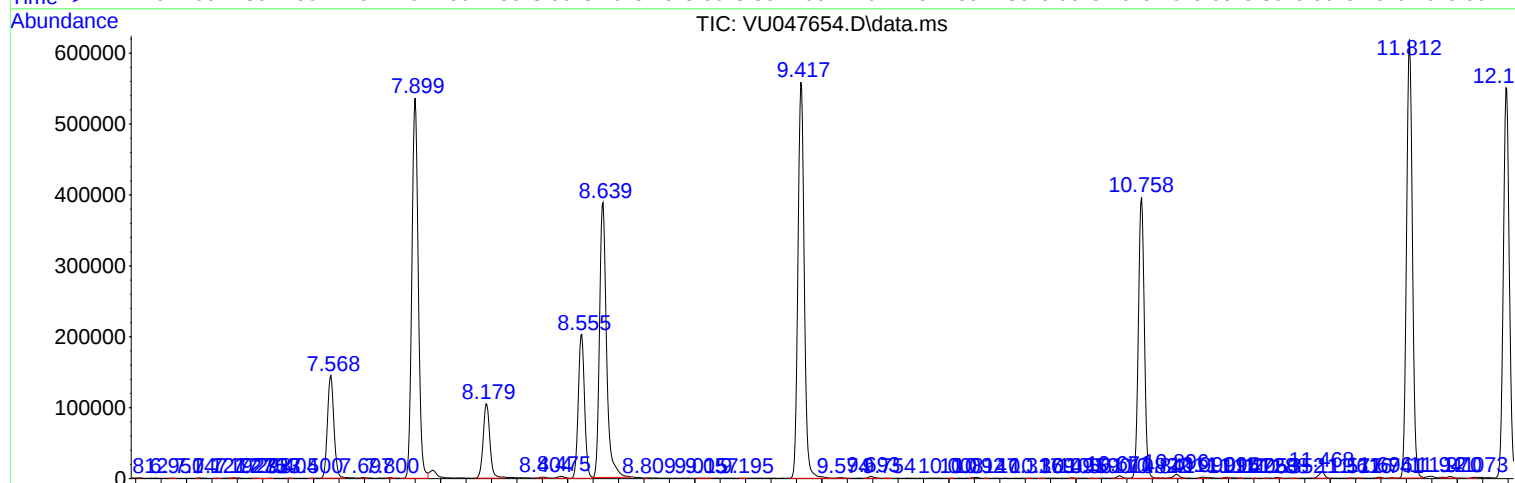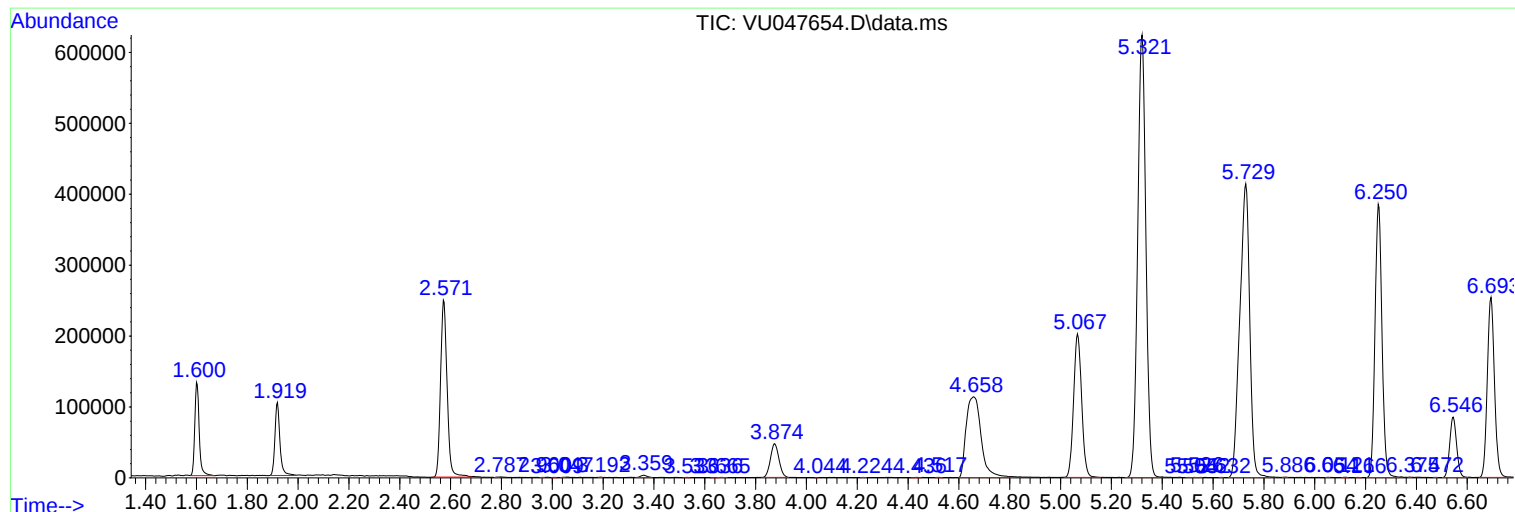

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047654.D
Acq On : 24 Mar 2022 23:47
Operator : SY/MD
Sample : N2081-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047654.D
Acq On : 24 Mar 2022 23:47
Operator : SY/MD
Sample : N2081-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------