

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047661.D
 Acq On : 25 Mar 2022 02:25
 Operator : SY/MD
 Sample : N2081-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	105	rVB	126821	151402	2.52%	0.666%
2	1.919	171	180	199	rBV	99424	135706	2.26%	0.597%
3	2.086	225	232	241	rBV	10432	14132	0.23%	0.062%
4	2.144	242	250	256	rBV2	16523	24329	0.40%	0.107%
5	2.584	369	387	409	rBV4	993509	1816923	30.19%	7.992%
6	2.835	462	465	469	rBV2	469	367	0.01%	0.002%
7	2.941	493	498	499	rBV	452	360	0.01%	0.002%
8	3.050	519	532	544	rBV3	4885	9414	0.16%	0.041%
9	3.186	567	574	580	rVB2	425	663	0.01%	0.003%
10	3.224	580	586	591	rBV3	369	381	0.01%	0.002%
11	3.266	594	599	603	rBV2	291	251	0.00%	0.001%
12	3.359	614	628	645	rBV2	31216	61672	1.02%	0.271%
13	3.449	653	656	659	rVB2	424	281	0.00%	0.001%
14	3.468	659	662	665	rBV2	303	209	0.00%	0.001%
15	3.626	709	711	714	rBV2	289	195	0.00%	0.001%
16	3.649	714	718	722	rVV2	385	380	0.01%	0.002%
17	3.671	722	725	728	rVV2	371	296	0.00%	0.001%
18	3.803	762	766	768	rBV3	241	230	0.00%	0.001%
19	3.874	768	788	815	rBV	709417	1678555	27.89%	7.384%
20	4.231	893	899	905	rBV3	371	437	0.01%	0.002%
21	4.349	931	936	941	rVB2	288	357	0.01%	0.002%
22	4.394	945	950	953	rBV	233	214	0.00%	0.001%
23	4.423	955	959	962	rVB2	309	263	0.00%	0.001%
24	4.481	973	977	981	rBV2	279	278	0.00%	0.001%
25	4.668	1010	1035	1078	rBV2	518209	1404588	23.34%	6.178%
26	4.919	1111	1113	1119	rVB3	544	314	0.01%	0.001%
27	5.066	1142	1159	1184	rVV	201249	472585	7.85%	2.079%
28	5.153	1184	1186	1191	rVB2	444	336	0.01%	0.001%
29	5.321	1215	1238	1276	rBV	2710520	6017424	100.00%	26.469%
30	5.597	1322	1324	1329	rVB2	498	410	0.01%	0.002%
31	5.729	1343	1365	1400	rVV2	411952	1107976	18.41%	4.874%
32	5.928	1425	1427	1430	rVB2	433	257	0.00%	0.001%
33	6.198	1506	1511	1513	rBV2	237	224	0.00%	0.001%
34	6.250	1513	1527	1550	rBV	413226	791589	13.15%	3.482%
35	6.542	1604	1618	1640	rBV	557030	1053910	17.51%	4.636%
36	6.693	1651	1665	1684	rBV	251227	486069	8.08%	2.138%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047661.D
 Acq On : 25 Mar 2022 02:25
 Operator : SY/MD
 Sample : N2081-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.944	1737	1743	1749	rBV3	368	627	0.01%	0.003%
38	7.005	1758	1762	1766	rBV	331	348	0.01%	0.002%
39	7.041	1769	1773	1775	rBV2	425	307	0.01%	0.001%
40	7.099	1788	1791	1792	rBV2	334	194	0.00%	0.001%
41	7.131	1798	1801	1805	rBV3	286	306	0.01%	0.001%
42	7.185	1815	1818	1819	rBV2	407	226	0.00%	0.001%
43	7.259	1837	1841	1844	rVB3	541	376	0.01%	0.002%
44	7.298	1851	1853	1860	rVB2	305	303	0.01%	0.001%
45	7.340	1860	1866	1869	rBV3	267	245	0.00%	0.001%
46	7.362	1869	1873	1879	rVB3	320	309	0.01%	0.001%
47	7.568	1923	1937	1956	rBV	141012	252314	4.19%	1.110%
48	7.681	1966	1972	1974	rBV4	626	641	0.01%	0.003%
49	7.796	1999	2008	2011	rBV5	667	858	0.01%	0.004%
50	7.899	2024	2040	2056	rBV	530738	915292	15.21%	4.026%
51	8.127	2106	2111	2116	rBV3	320	341	0.01%	0.001%
52	8.179	2116	2127	2151	rBV	99080	172020	2.86%	0.757%
53	8.401	2186	2196	2208	rBV2	22693	38247	0.64%	0.168%
54	8.475	2211	2219	2226	rBV3	2941	4379	0.07%	0.019%
55	8.555	2230	2244	2259	rBV	981068	1659756	27.58%	7.301%
56	8.639	2259	2270	2304	rVB	381977	732931	12.18%	3.224%
57	8.886	2344	2347	2350	rBV4	487	299	0.00%	0.001%
58	9.269	2462	2466	2468	rBV2	298	215	0.00%	0.001%
59	9.311	2475	2479	2482	rBV2	261	201	0.00%	0.001%
60	9.327	2482	2484	2491	rVB2	288	287	0.00%	0.001%
61	9.417	2496	2512	2547	rBV	616691	1042790	17.33%	4.587%
62	9.558	2552	2556	2563	rVV3	581	715	0.01%	0.003%
63	9.693	2591	2598	2606	rVB4	1400	2059	0.03%	0.009%
64	9.812	2632	2635	2642	rVB2	184	199	0.00%	0.001%
65	9.925	2667	2670	2674	rBV2	254	225	0.00%	0.001%
66	10.008	2690	2696	2702	rVB2	491	580	0.01%	0.003%
67	10.102	2723	2725	2732	rVB4	669	709	0.01%	0.003%
68	10.333	2793	2797	2800	rVV2	423	391	0.01%	0.002%
69	10.446	2827	2832	2834	rBV2	348	283	0.00%	0.001%
70	10.529	2853	2858	2860	rBV	322	287	0.00%	0.001%
71	10.671	2893	2902	2910	rBV2	2392	3371	0.06%	0.015%
72	10.758	2914	2929	2952	rVB	393600	633001	10.52%	2.784%
73	10.893	2961	2971	2982	rVB	5380	8452	0.14%	0.037%
74	10.970	2991	2995	2997	rBV2	356	274	0.00%	0.001%
75	10.999	2997	3004	3009	rVV3	532	642	0.01%	0.003%
76	11.079	3024	3029	3030	rBV2	695	472	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047661.D
 Acq On : 25 Mar 2022 02:25
 Operator : SY/MD
 Sample : N2081-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.205	3065	3068	3072	rBV2	272	288	0.00%	0.001%
78	11.266	3081	3087	3088	rBV2	373	382	0.01%	0.002%
79	11.468	3138	3150	3158	rBV5	4413	7329	0.12%	0.032%
80	11.520	3162	3166	3172	rBV3	268	334	0.01%	0.001%
81	11.680	3213	3216	3217	rBV2	347	212	0.00%	0.001%
82	11.693	3217	3220	3228	rVB3	1082	1358	0.02%	0.006%
83	11.745	3233	3236	3237	rBV2	466	240	0.00%	0.001%
84	11.812	3244	3257	3277	rBV	699787	1106933	18.40%	4.869%
85	11.896	3279	3283	3290	rVB5	1888	2268	0.04%	0.010%
86	11.970	3302	3306	3315	rVB7	1832	2610	0.04%	0.011%
87	12.066	3333	3336	3338	rBV	447	317	0.01%	0.001%
88	12.192	3362	3375	3392	rBV	542881	890485	14.80%	3.917%
89	12.330	3413	3418	3423	rVB4	711	884	0.01%	0.004%
90	12.372	3427	3431	3436	rVV4	473	406	0.01%	0.002%
91	12.487	3459	3467	3480	rVB4	1986	3298	0.05%	0.015%
92	12.770	3552	3555	3564	rVB2	1426	1901	0.03%	0.008%
93	12.931	3602	3605	3609	rBV2	263	215	0.00%	0.001%
94	12.970	3615	3617	3621	rVB2	377	209	0.00%	0.001%
95	13.153	3669	3674	3677	rBV2	277	264	0.00%	0.001%
96	13.175	3678	3681	3688	rVV2	287	277	0.00%	0.001%
97	13.227	3691	3697	3701	rVV3	549	646	0.01%	0.003%
98	13.844	3883	3889	3893	rBV3	823	944	0.02%	0.004%
99	14.092	3962	3966	3975	rVB4	2388	3164	0.05%	0.014%
100	14.208	3997	4002	4003	rBV2	490	410	0.01%	0.002%




Sum of corrected areas: 22733823

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047661.D
Acq On : 25 Mar 2022 02:25
Operator : SY/MD
Sample : N2081-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

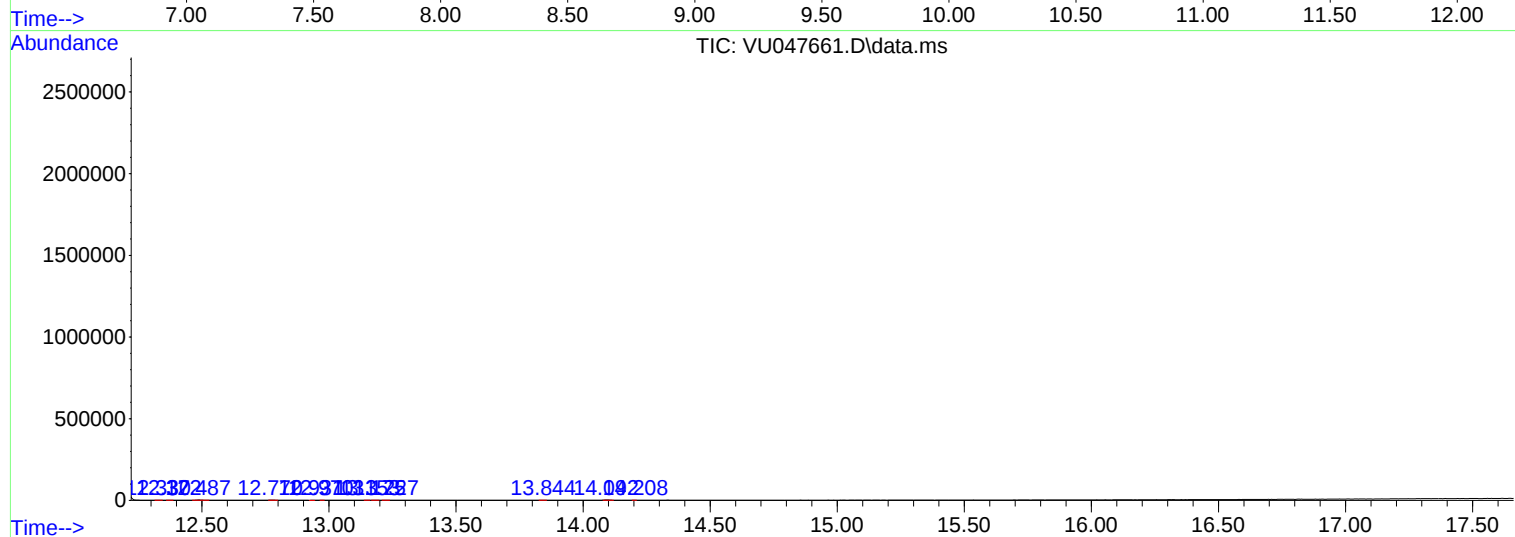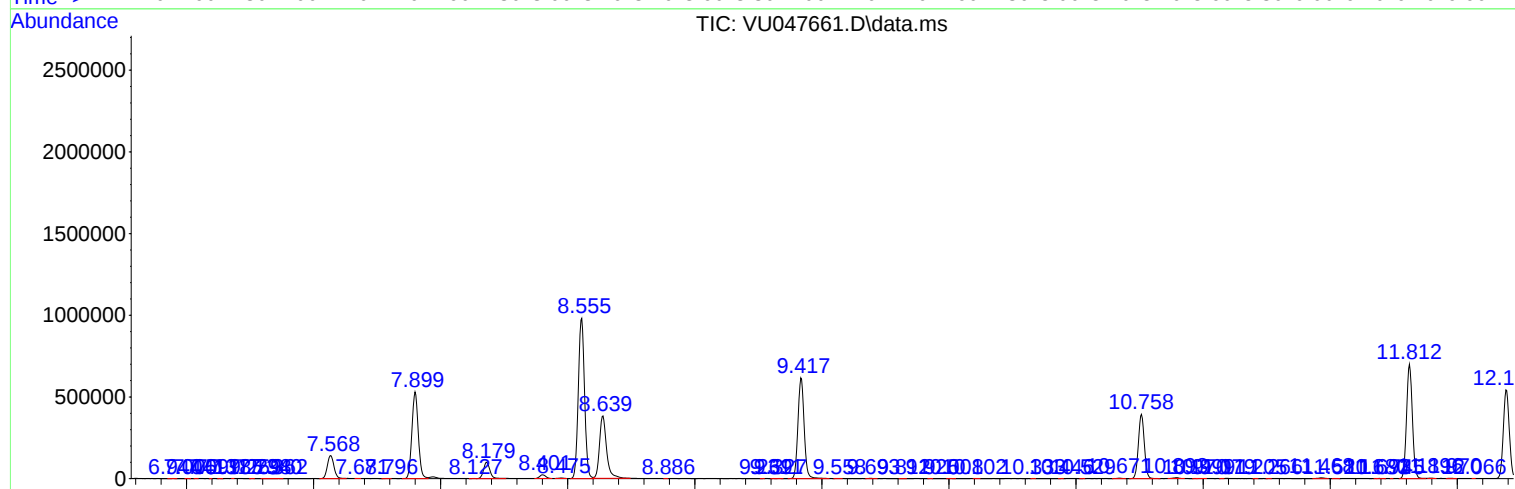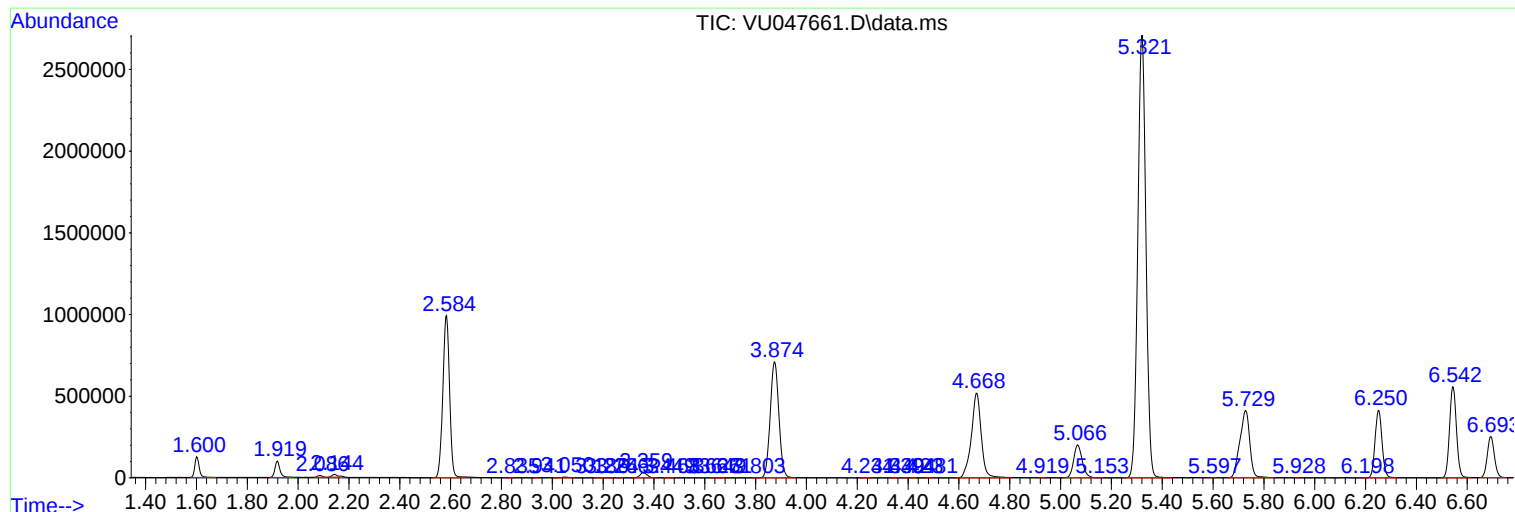

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047661.D
Acq On : 25 Mar 2022 02:25
Operator : SY/MD
Sample : N2081-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
Data File : VU047661.D
Acq On : 25 Mar 2022 02:25
Operator : SY/MD
Sample : N2081-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------