


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032422\
 Data File : VU047631.D
 Acq On : 24 Mar 2022 11:36
 Operator : SY/MD
 Sample : BFB053
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB053

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 30 01:20:49 2022

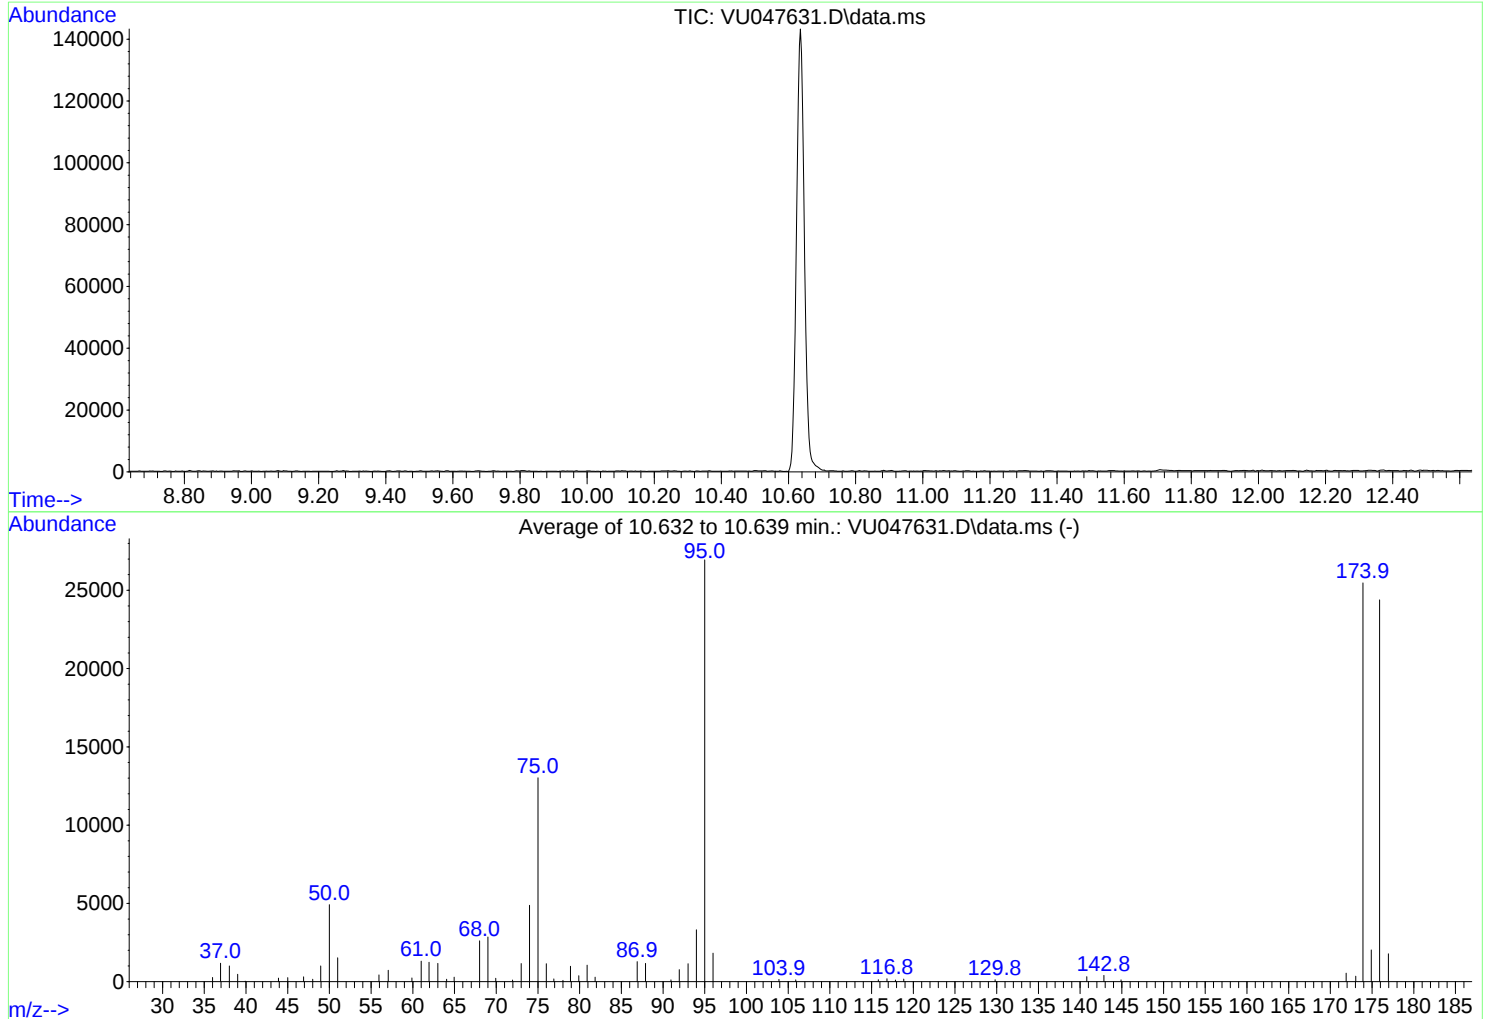

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	4922	PASS
75	95	30	80	48.3	13021	PASS
95	95	100	100	100.0	26947	PASS
96	95	5	9	6.7	1818	PASS
173	174	0.00	2	1.4	351	PASS
174	95	50	120	94.5	25469	PASS
175	174	5	9	8.0	2028	PASS
176	174	95	101	95.8	24389	PASS
177	176	5	9	7.3	1774	PASS

m/z	Abundance
43.80	179.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
36.00	294.0
37.00	1257.0
38.00	1115.0
39.00	452.0
44.00	396.0
45.00	261.0
46.90	319.0
48.00	137.0
48.90	1017.0
50.00	5005.0
51.00	1565.0
56.00	450.0
57.00	797.0
59.90	234.0
61.00	1350.0
61.90	1286.0
63.00	1198.0
64.00	152.0
65.00	278.0
68.00	2566.0
69.00	2836.0
70.00	190.0
72.00	105.0
73.00	1131.0
74.00	5092.0
75.00	13078.0
76.00	1130.0
76.90	182.0
78.00	126.0
78.90	1017.0
79.90	401.0
80.90	1071.0
81.90	272.0
86.90	1252.0
87.90	1144.0
91.00	110.0
92.00	786.0
93.00	1100.0
94.00	3362.0
95.00	26920.0
96.00	1808.0
103.90	133.0
105.90	116.0
115.80	122.0
116.80	190.0
117.80	163.0
118.80	162.0
129.80	128.0
140.80	337.0
142.80	365.0
145.00	116.0
171.90	557.0
173.10	364.0
173.90	24752.0
174.90	1968.0
175.90	23456.0
177.00	1752.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
36.00	286.0
36.90	1211.0
38.00	990.0
39.00	485.0
39.90	101.0
43.90	406.0
45.00	276.0
46.90	308.0
48.00	165.0
49.00	1037.0
50.00	5130.0
51.00	1580.0
55.90	441.0
57.00	750.0
59.90	239.0
61.00	1372.0
61.90	1277.0
63.00	1203.0
64.00	148.0
65.00	288.0
68.00	2707.0
69.00	2931.0
69.90	230.0
72.00	107.0
73.00	1193.0
74.00	5054.0
75.00	13406.0
76.00	1203.0
76.90	182.0
78.00	111.0
78.90	1012.0
79.90	407.0
80.90	1086.0
81.90	288.0
86.90	1338.0
87.90	1204.0
91.00	111.0
91.90	784.0
93.00	1173.0
94.00	3416.0
95.00	27704.0
96.00	1890.0
103.90	144.0
105.90	114.0
115.80	125.0
116.80	175.0
117.90	136.0
118.90	161.0
129.80	123.0
140.80	328.0
142.80	405.0
144.90	115.0
171.90	562.0
173.10	354.0
173.90	26208.0
174.90	2121.0
175.90	25104.0
176.90	1843.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
36.00	225.0
36.90	1072.0
38.00	888.0
39.00	485.0
43.90	402.0
45.00	230.0
46.90	288.0
48.00	157.0
49.00	946.0
50.00	4630.0
51.00	1433.0
55.90	388.0
57.10	627.0
59.90	221.0
61.00	1216.0
62.00	1147.0
63.00	1103.0
64.10	165.0
64.90	283.0
68.00	2536.0
69.00	2781.0
69.90	241.0
71.90	103.0
73.00	1131.0
74.00	4497.0
75.00	12578.0
76.00	1110.0
76.90	156.0
78.90	928.0
79.90	331.0
80.90	1001.0
81.80	288.0
86.90	1240.0
87.90	1150.0
90.90	105.0
91.90	740.0
93.00	1162.0
94.00	3168.0
95.00	26216.0
96.00	1757.0
103.90	144.0
105.90	109.0
115.80	121.0
116.90	178.0
118.90	163.0
129.80	109.0
140.80	284.0
142.90	423.0
144.80	118.0
171.90	497.0
173.00	334.0
173.90	25448.0
174.90	1994.0
175.90	24608.0
176.90	1726.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053