




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
 Data File : VU053403.D
 Acq On : 24 Mar 2023 20:25
 Operator : JC/MD
 Sample : 02053-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYF70

Manual IntegrationsAPPROVED

Quant Time: Mar 25 00:42:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 25 00:39:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/27/2023
 Supervised By :Mahesh Dadoda 03/27/2023

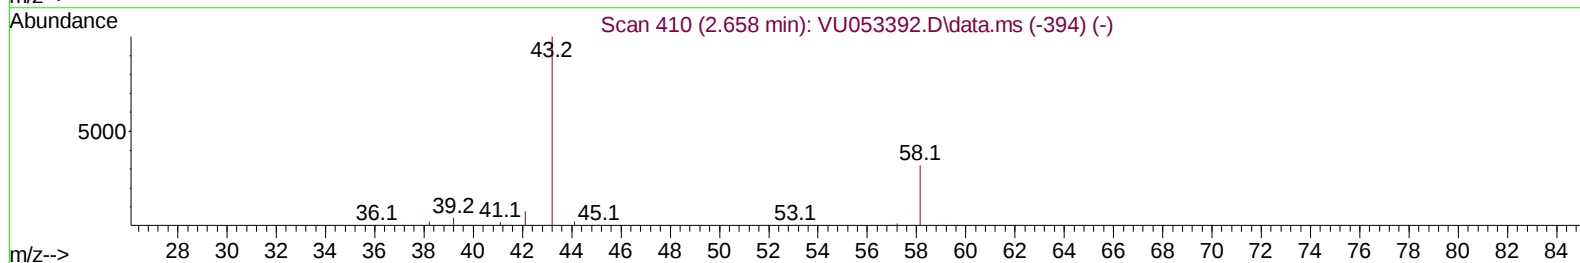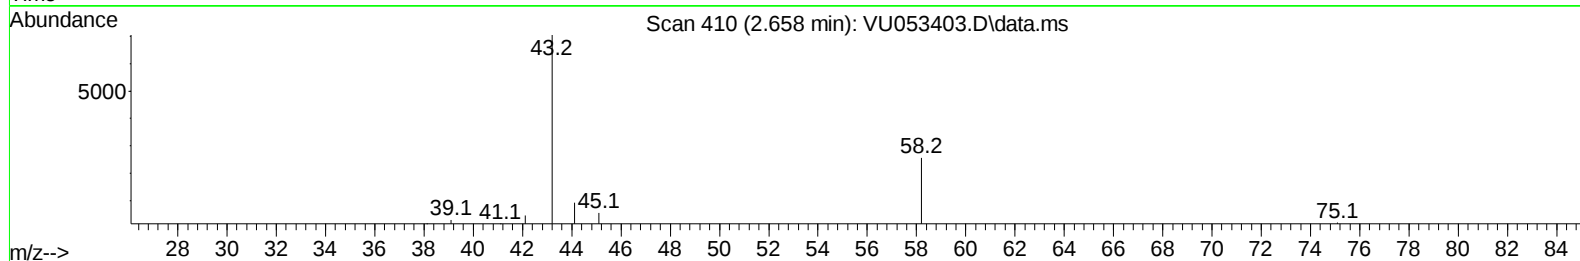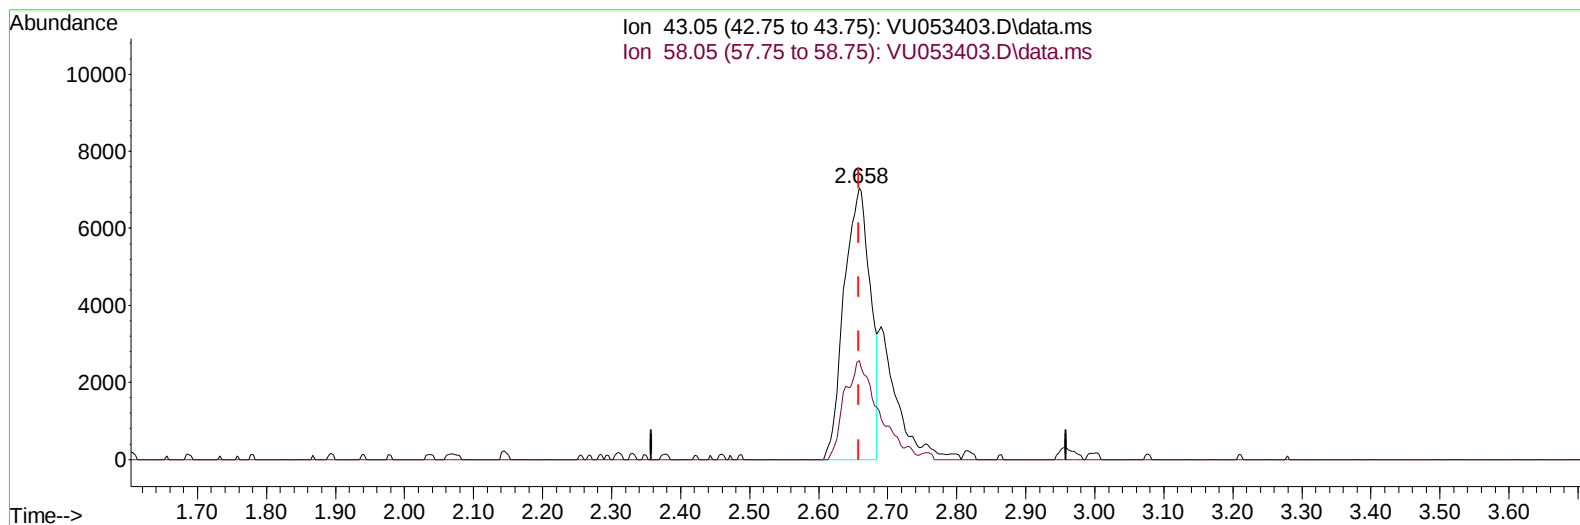

TIC: VU053403.D\data.ms

(13) Acetone (T)

2.658min (+ 0.000) 13.95 ug/L

response 18606

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	16.10	45.77#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
 Data File : VU053403.D
 Acq On : 24 Mar 2023 20:25
 Operator : JC/MD
 Sample : 02053-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYF70

Manual IntegrationsAPPROVED

Quant Time: Mar 25 00:42:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 25 00:39:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/27/2023
 Supervised By :Mahesh Dadoda 03/27/2023

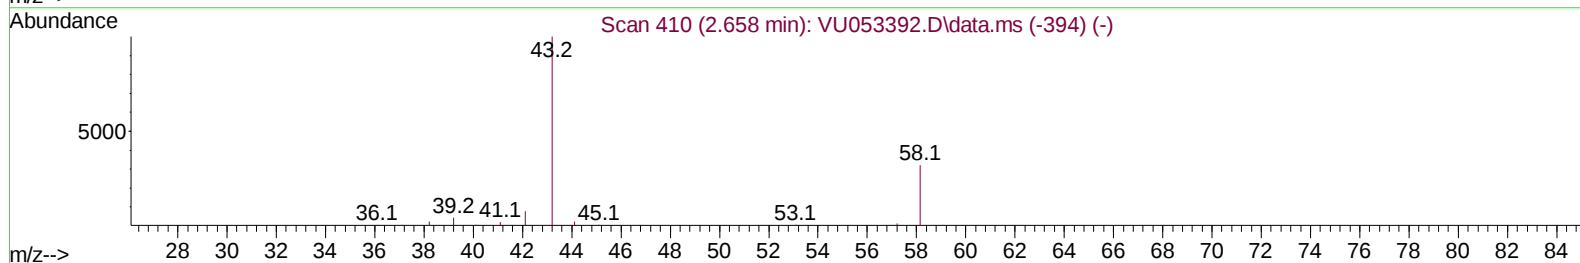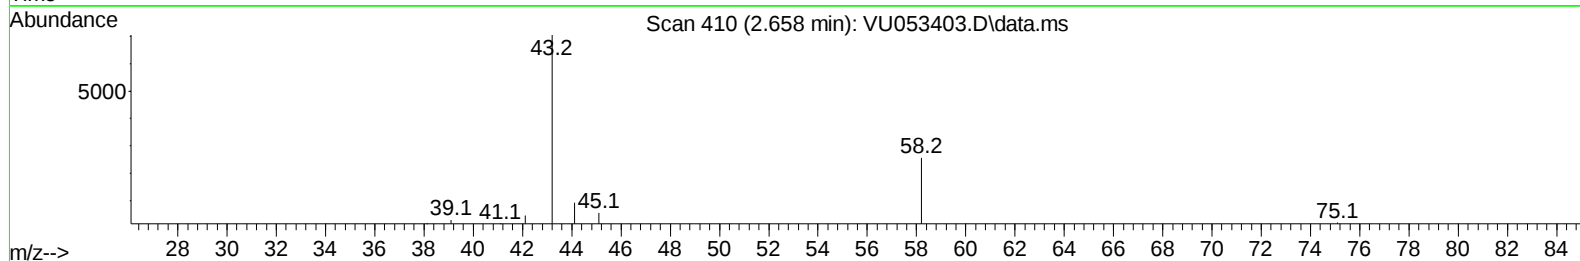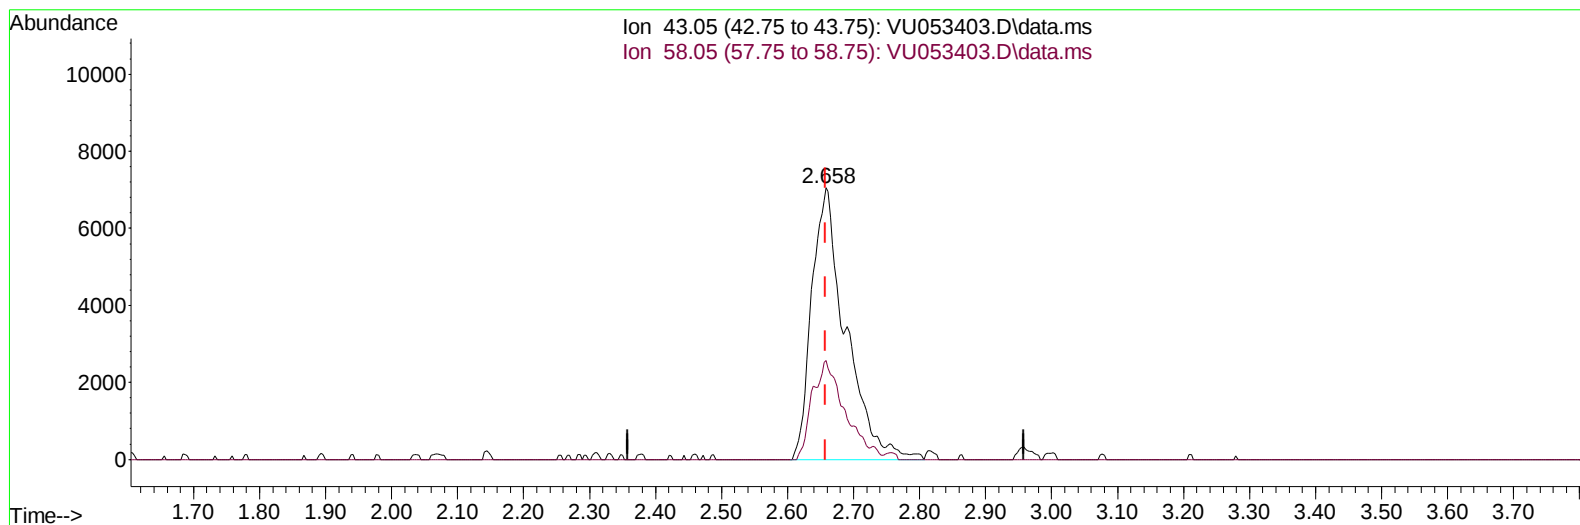

TIC: VU053403.D\data.ms

(13) Acetone (T)

2.658min (+ 0.000) 18.87 ug/L m

response 25180

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	16.10	33.82#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
 Data File : VU053403.D
 Acq On : 24 Mar 2023 20:25
 Operator : JC/MD
 Sample : 02053-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYF70

Manual IntegrationsAPPROVED

Quant Time: Mar 25 00:42:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 25 00:39:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/27/2023
 Supervised By :Mahesh Dadoda 03/27/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.243	114		142650	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117		133704	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152		64639	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.597	65		47773	4.868	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.400%	
7) Chloroethane-d5	1.912	69		44211	4.964	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.200%	
11) 1,1-Dichloroethene-d2	2.565	65		20610	4.930	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.600%	
20) 2-Butanone-d5	4.633	46		121018	53.831	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.660%	
24) Chloroform-d	5.057	84		91346	5.021	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%	
26) 1,2-Dichloroethane-d4	5.697	65		48164	5.166	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.400%	
32) Benzene-d6	5.723	84		193907	5.117	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.400%	
36) 1,2-Dichloropropane-d6	6.687	67		60425	5.233	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.600%	
41) Toluene-d8	7.893	98		176838	4.947	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%	
43) trans-1,3-Dichloroprop...	8.176	79		20546	4.637	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.800%	
46) 2-Hexanone-d5	8.629	63		91528	50.857	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.720%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84		47079	4.899	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.000%	
66) 1,2-Dichlorobenzene-d4	12.189	152		60770	5.226	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.600%	
Target Compounds							
13) Acetone	2.658	43		25180m	18.873	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
Data File : VU053403.D
Acq On : 24 Mar 2023 20:25
Operator : JC/MD
Sample : 02053-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF70

Manual IntegrationsAPPROVED

Quant Time: Mar 25 00:42:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Mar 25 00:39:08 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/27/2023
Supervised By :Mahesh Dadoda 03/27/2023

