

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
 Data File : VU053395.D
 Acq On : 24 Mar 2023 17:12
 Operator : JC/MD
 Sample : 02053-03DL 4X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYF69DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053395.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	96	rVB	63640	75021	15.69%	1.658%
2	1.912	169	178	196	rBV	55902	76409	15.98%	1.689%
3	2.565	368	381	397	rVB	103428	165133	34.54%	3.649%
4	3.047	520	531	544	rBV3	8309	15530	3.25%	0.343%
5	4.633	1008	1024	1057	rBV2	58487	196710	41.15%	4.347%
6	4.813	1072	1080	1088	rBV4	4045	7774	1.63%	0.172%
7	5.057	1140	1156	1177	rVB	94897	207064	43.31%	4.576%
8	5.723	1343	1363	1383	rBV2	181978	474066	99.16%	10.476%
9	6.243	1510	1525	1545	rBV	179321	338876	70.88%	7.489%
10	6.536	1602	1616	1635	rBV	202675	389530	81.48%	8.608%
11	6.684	1648	1662	1688	rBV	114545	221366	46.30%	4.892%
12	7.562	1923	1935	1955	rBV2	53569	98233	20.55%	2.171%
13	7.893	2025	2038	2056	rBV	232908	405317	84.78%	8.957%
14	8.176	2115	2126	2142	rBV2	33796	56965	11.92%	1.259%
15	8.629	2253	2267	2303	rBV2	231866	478065	100.00%	10.565%
16	9.414	2498	2511	2530	rBV	245407	415206	86.85%	9.176%
17	10.751	2916	2927	2946	rVB	91742	144570	30.24%	3.195%
18	11.806	3241	3255	3276	rBV	249272	407579	85.26%	9.007%
19	12.189	3362	3374	3396	rVB	212972	346317	72.44%	7.653%
20	12.973	3607	3618	3624	rBV2	4002	5417	1.13%	0.120%




Sum of corrected areas: 4525148

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
Data File : VU053395.D
Acq On : 24 Mar 2023 17:12
Operator : JC/MD
Sample : 02053-03DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

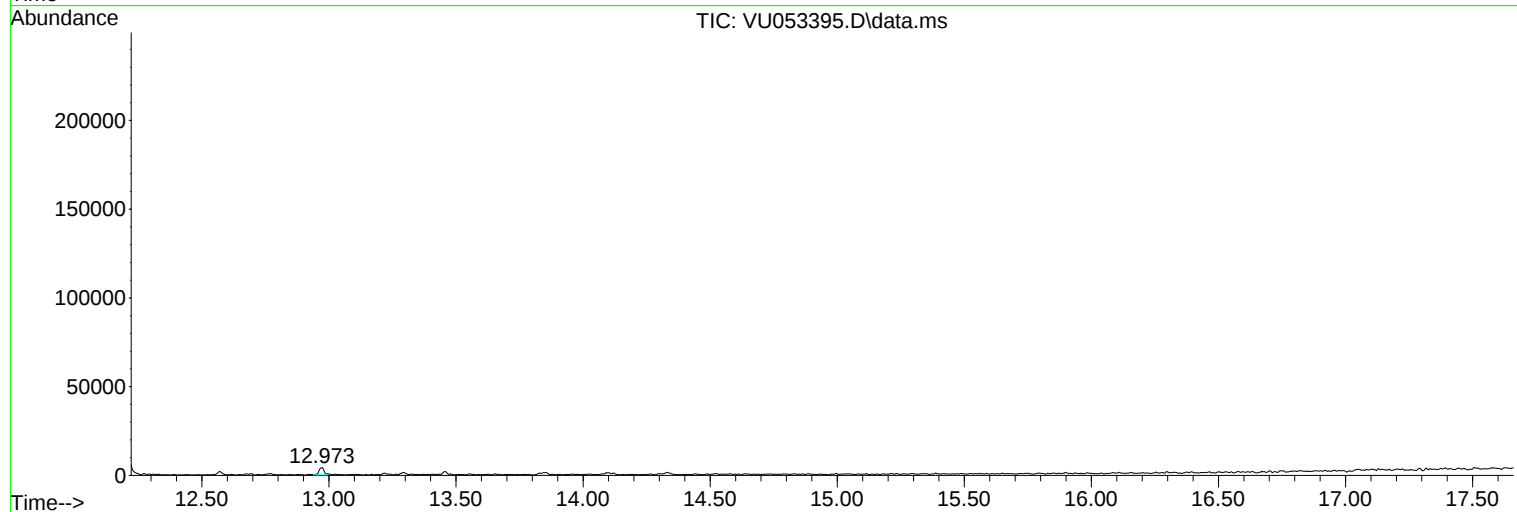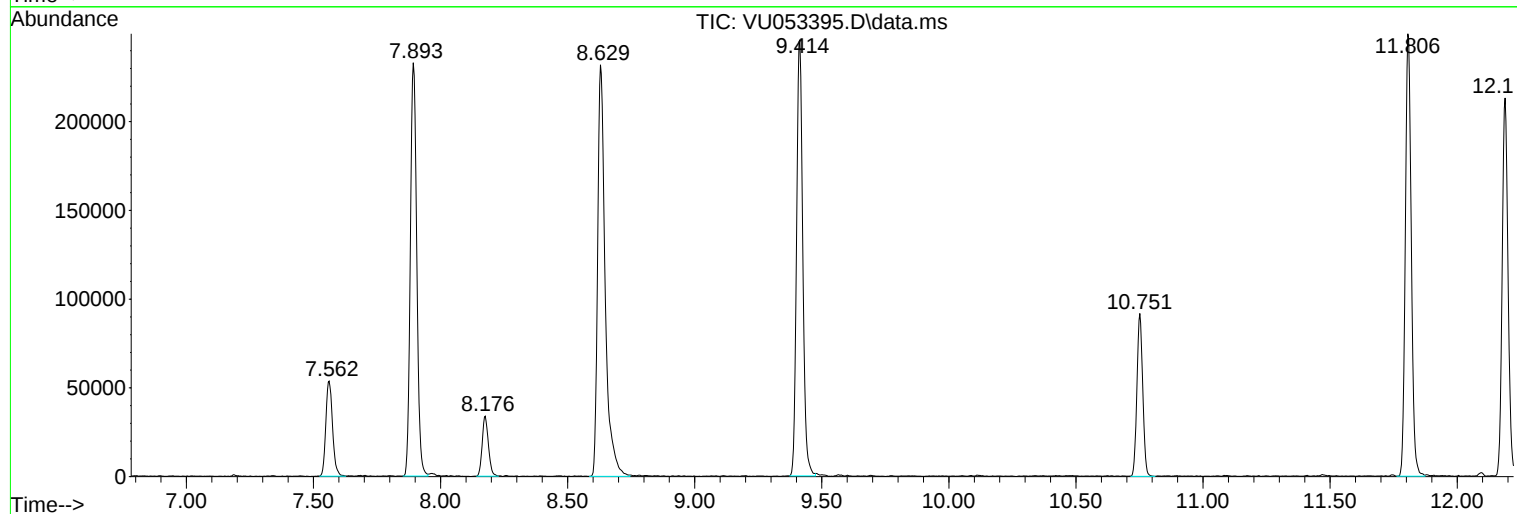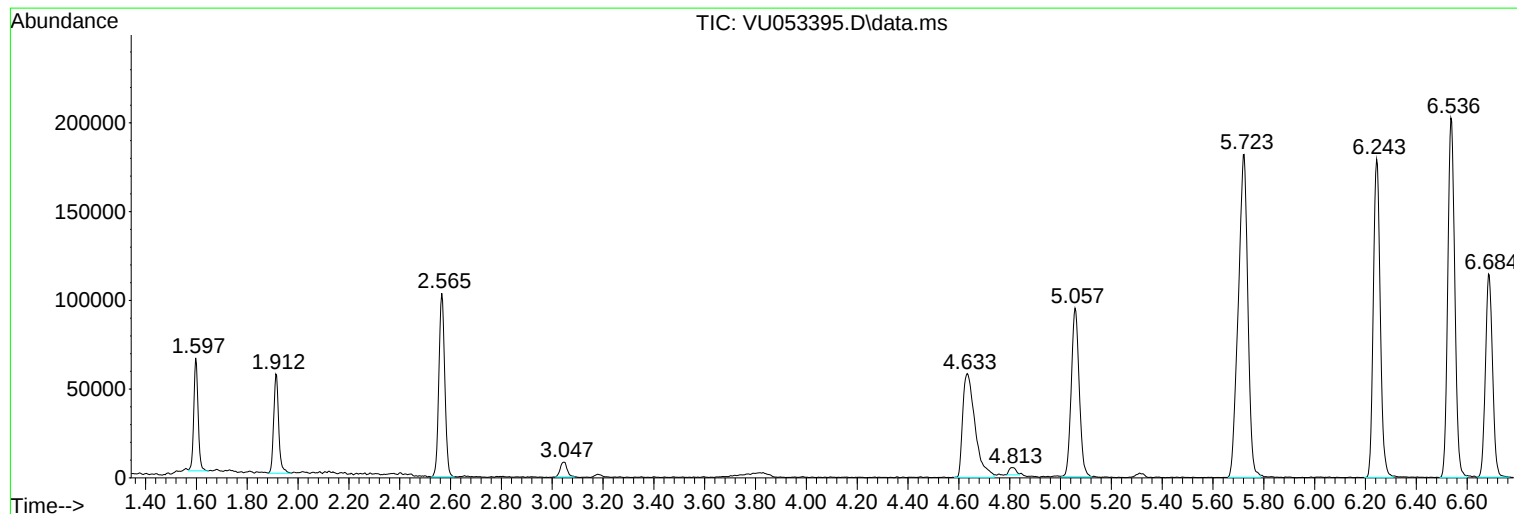

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
Data File : VU053395.D
Acq On : 24 Mar 2023 17:12
Operator : JC/MD
Sample : 02053-03DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
Data File : VU053395.D
Acq On : 24 Mar 2023 17:12
Operator : JC/MD
Sample : 02053-03DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc