

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
 Data File : VU053403.D
 Acq On : 24 Mar 2023 20:25
 Operator : JC/MD
 Sample : 02053-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYF70

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053403.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	68	80	94	rBV	69791	82920	15.98%	1.859%
2	1.912	170	178	192	rVB	59267	80429	15.50%	1.803%
3	2.565	369	381	394	rBV	117258	182930	35.26%	4.101%
4	2.658	394	410	432	rBV	11142	36462	7.03%	0.817%
5	4.636	1011	1025	1066	rBV	59767	212124	40.89%	4.755%
6	4.806	1066	1078	1105	rVB2	30485	75291	14.51%	1.688%
7	5.057	1141	1156	1175	rVB2	100850	223654	43.11%	5.014%
8	5.723	1342	1363	1390	rBV3	198946	515580	99.38%	11.558%
9	6.243	1512	1525	1546	rBV	171401	324125	62.48%	7.266%
10	6.539	1609	1617	1626	rVB7	4340	6892	1.33%	0.155%
11	6.687	1647	1663	1682	rBV	124273	241758	46.60%	5.420%
12	7.562	1923	1935	1950	rBV2	59799	105132	20.27%	2.357%
13	7.893	2024	2038	2054	rBV	257401	443576	85.50%	9.944%
14	8.176	2115	2126	2140	rBV2	35820	60008	11.57%	1.345%
15	8.629	2256	2267	2302	rBV3	253924	518785	100.00%	11.630%
16	9.414	2497	2511	2530	rBV	237685	400807	77.26%	8.985%
17	10.751	2916	2927	2942	rBV2	98242	154834	29.85%	3.471%
18	11.809	3243	3256	3276	rBV	241003	392472	75.65%	8.798%
19	12.189	3361	3374	3392	rBV	236829	380656	73.37%	8.533%
20	12.883	3582	3590	3602	rBV5	13781	22362	4.31%	0.501%




Sum of corrected areas: 4460797

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
Data File : VU053403.D
Acq On : 24 Mar 2023 20:25
Operator : JC/MD
Sample : 02053-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

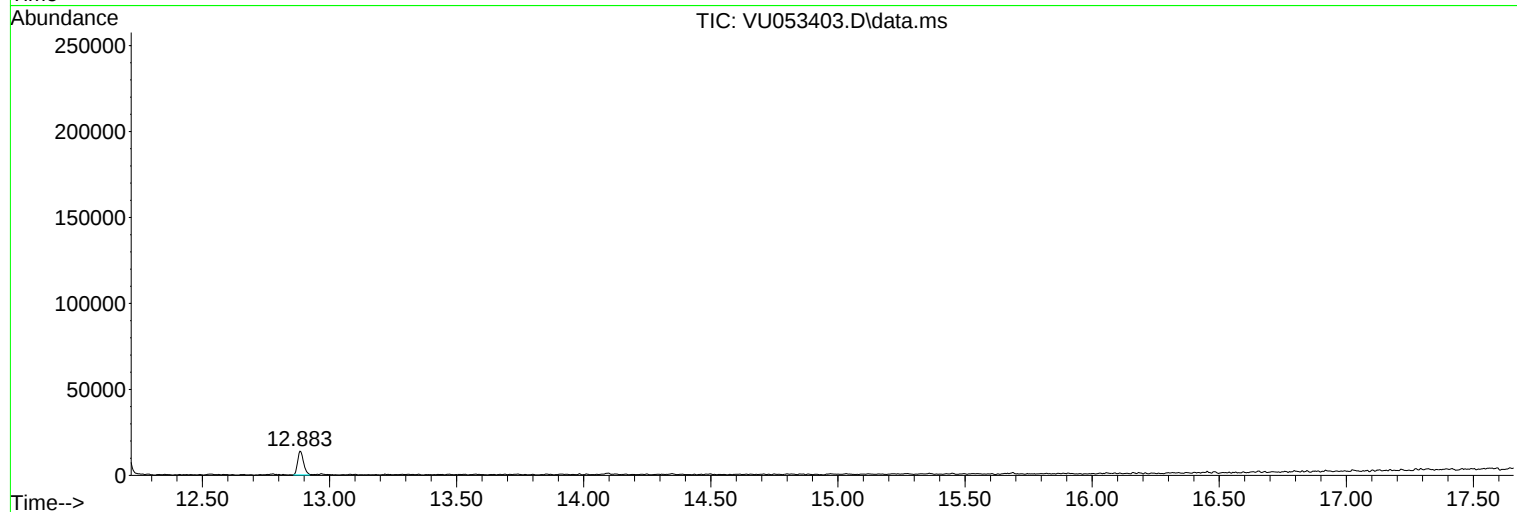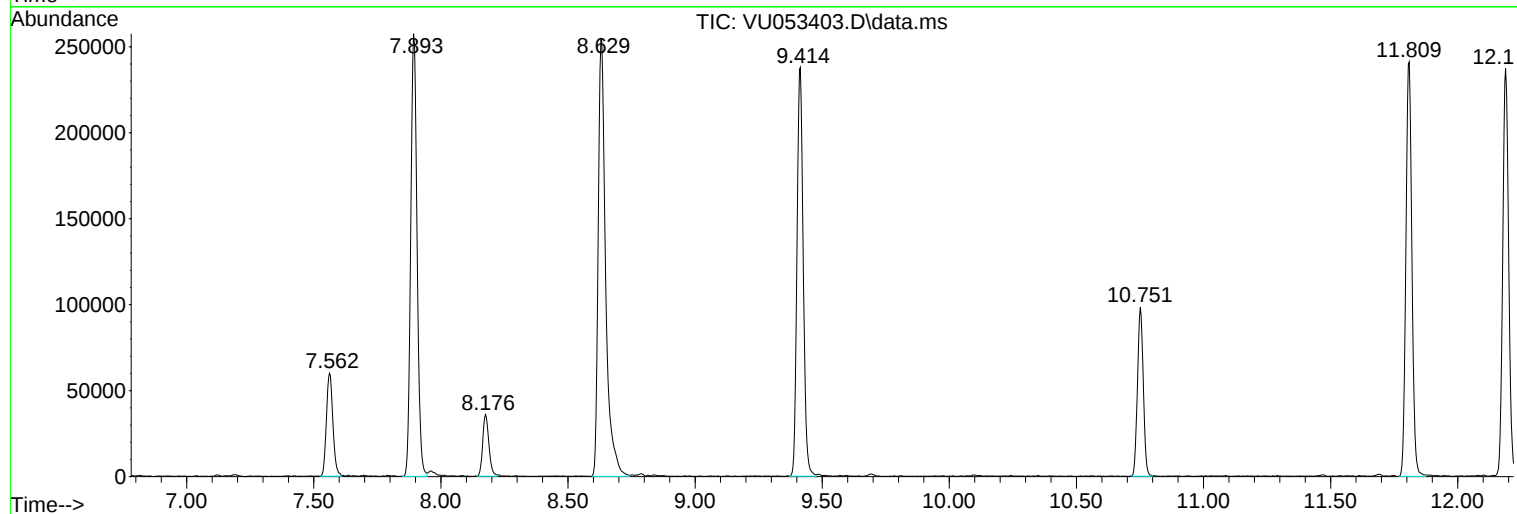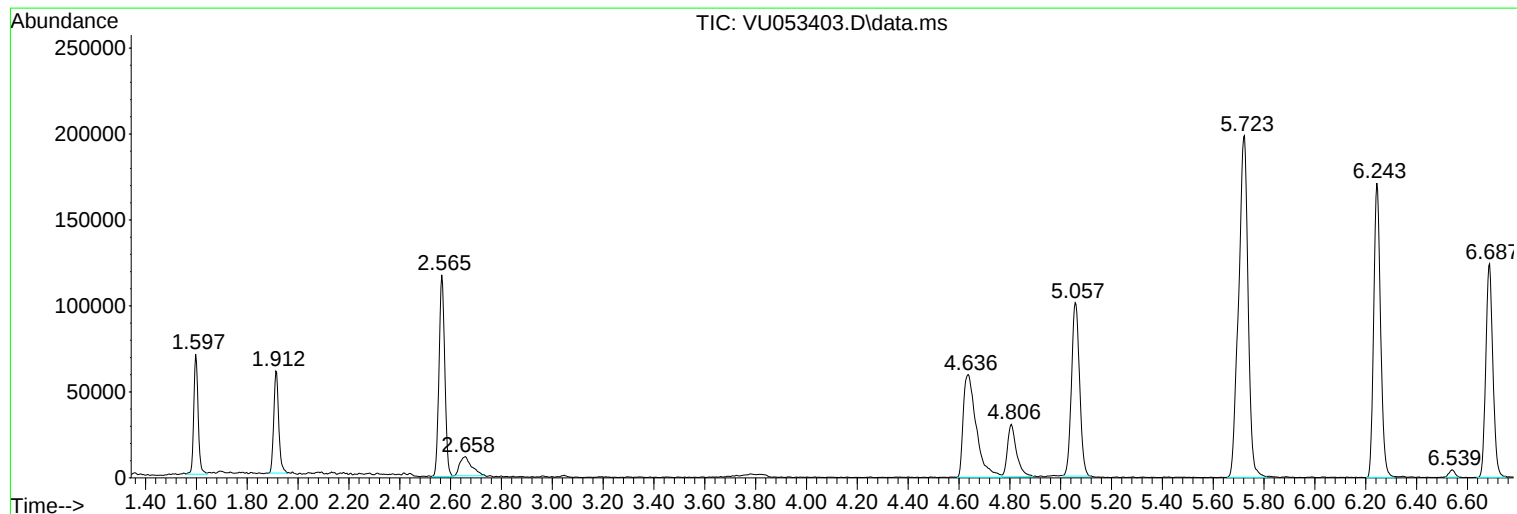

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
Data File : VU053403.D
Acq On : 24 Mar 2023 20:25
Operator : JC/MD
Sample : 02053-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF70









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethyl Acetate Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.806	1.16 ug/L	75291	1,4-Difluorobenzene	6.243

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethyl Acetate	88	C4H8O2	000141-78-6	83
2			Ethyl Acetate	88	C4H8O2	000141-78-6	83
3			Ethyl Acetate	88	C4H8O2	000141-78-6	83
4			Ethyl Acetate	88	C4H8O2	000141-78-6	50
5			CH3C(O)CH2CH2OH	88	C4H8O2	000590-90-9	9

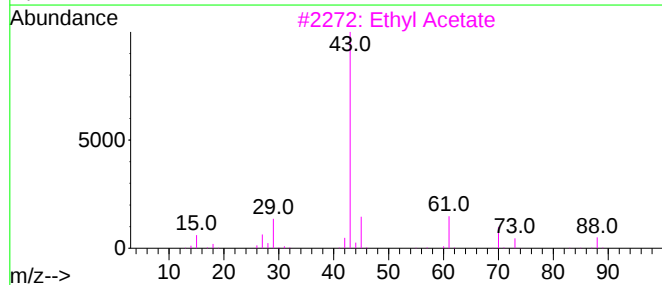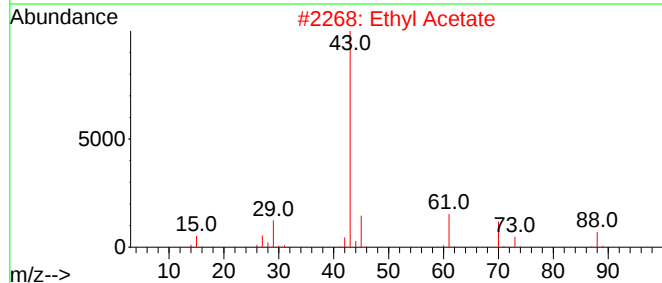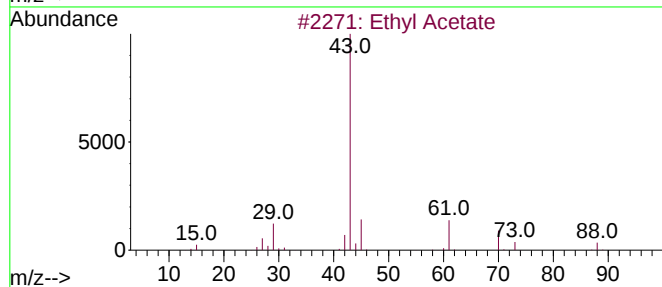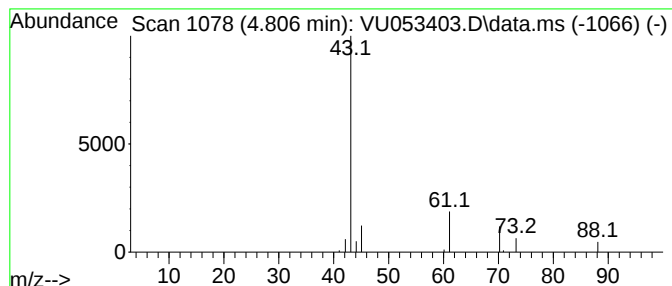

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
Data File : VU053403.D
Acq On : 24 Mar 2023 20:25
Operator : JC/MD
Sample : 02053-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethyl Acetate	4.806	1.2	ug/L	75291	1	6.243	324125	5.0