

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
 Data File : VU053407.D
 Acq On : 24 Mar 2023 22:00
 Operator : JC/MD
 Sample : 02092-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CB964

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.388	10	15	28	rVB	11068	11936	2.34%	0.264%
2	1.597	71	80	90	rBV	70920	82636	16.21%	1.825%
3	1.913	168	178	193	rBV	59808	80502	15.79%	1.778%
4	2.565	369	381	395	rVB	112827	183010	35.89%	4.042%
5	3.359	614	628	644	rBV4	8005	20138	3.95%	0.445%
6	4.652	1014	1030	1082	rBV2	39638	195765	38.40%	4.323%
7	5.057	1142	1156	1185	rVB2	99904	230388	45.19%	5.088%
8	5.719	1339	1362	1384	rBV2	196139	506618	99.37%	11.188%
9	6.244	1511	1525	1545	rBV2	158534	308357	60.48%	6.810%
10	6.687	1646	1663	1681	rBV2	118069	236117	46.31%	5.214%
11	7.562	1924	1935	1956	rBV2	57072	99958	19.61%	2.207%
12	7.893	2024	2038	2056	rBV	246999	428682	84.08%	9.467%
13	8.176	2116	2126	2149	rBV2	34693	59375	11.65%	1.311%
14	8.633	2256	2268	2300	rBV2	221339	492743	96.64%	10.882%
15	9.414	2494	2511	2539	rBV2	229945	509855	100.00%	11.259%
16	9.681	2586	2594	2608	rVB10	3916	7068	1.39%	0.156%
17	10.751	2916	2927	2943	rVB	97599	156819	30.76%	3.463%
18	11.411	3124	3132	3142	rVB3	6665	10863	2.13%	0.240%
19	11.603	3178	3192	3202	rBV4	8871	15528	3.05%	0.343%
20	11.806	3244	3255	3279	rBV	238607	403997	79.24%	8.922%
21	12.189	3357	3374	3391	rBV	232268	387353	75.97%	8.554%
22	12.626	3496	3510	3519	rVB	3405	6887	1.35%	0.152%
23	12.758	3543	3551	3561	rVB4	6848	10267	2.01%	0.227%
24	13.227	3688	3697	3711	rBV8	13163	24080	4.72%	0.532%
25	13.877	3892	3899	3915	rVB3	12333	21566	4.23%	0.476%
26	14.111	3962	3972	3980	rVB8	4761	7177	1.41%	0.158%
27	14.877	4200	4210	4218	rVB8	4477	7055	1.38%	0.156%
28	15.420	4368	4379	4389	rVB4	9614	17725	3.48%	0.391%
29	15.912	4525	4532	4542	rVB7	3506	5778	1.13%	0.128%




Sum of corrected areas: 4528243

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
Data File : VU053407.D
Acq On : 24 Mar 2023 22:00
Operator : JC/MD
Sample : 02092-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB964

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

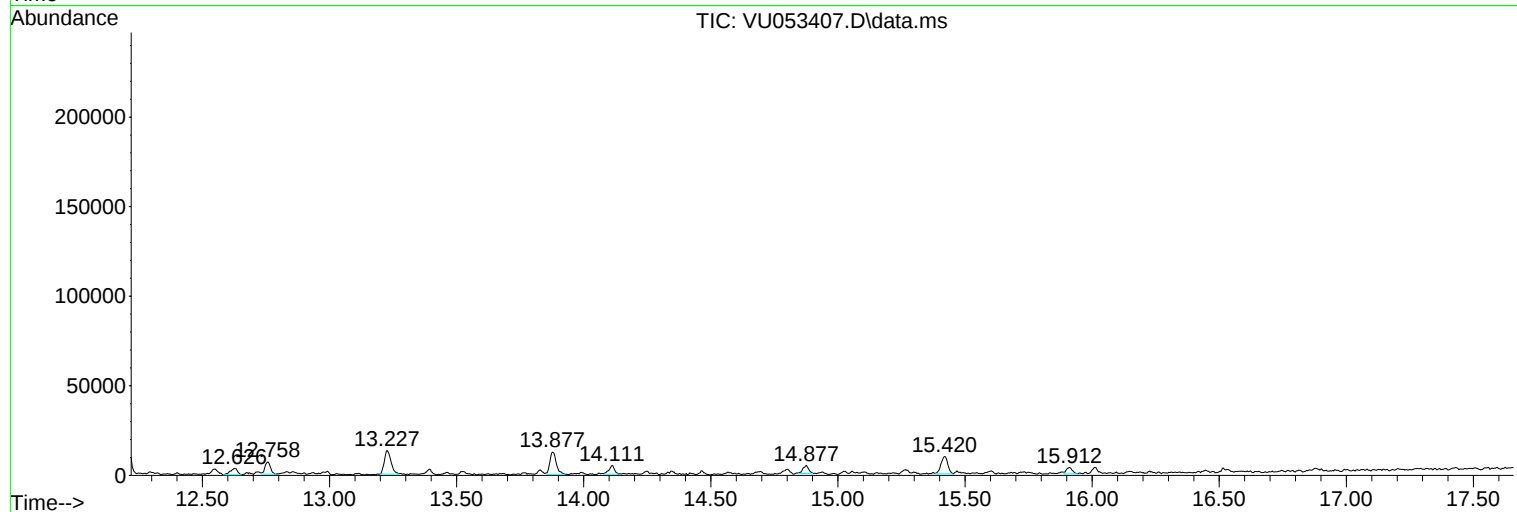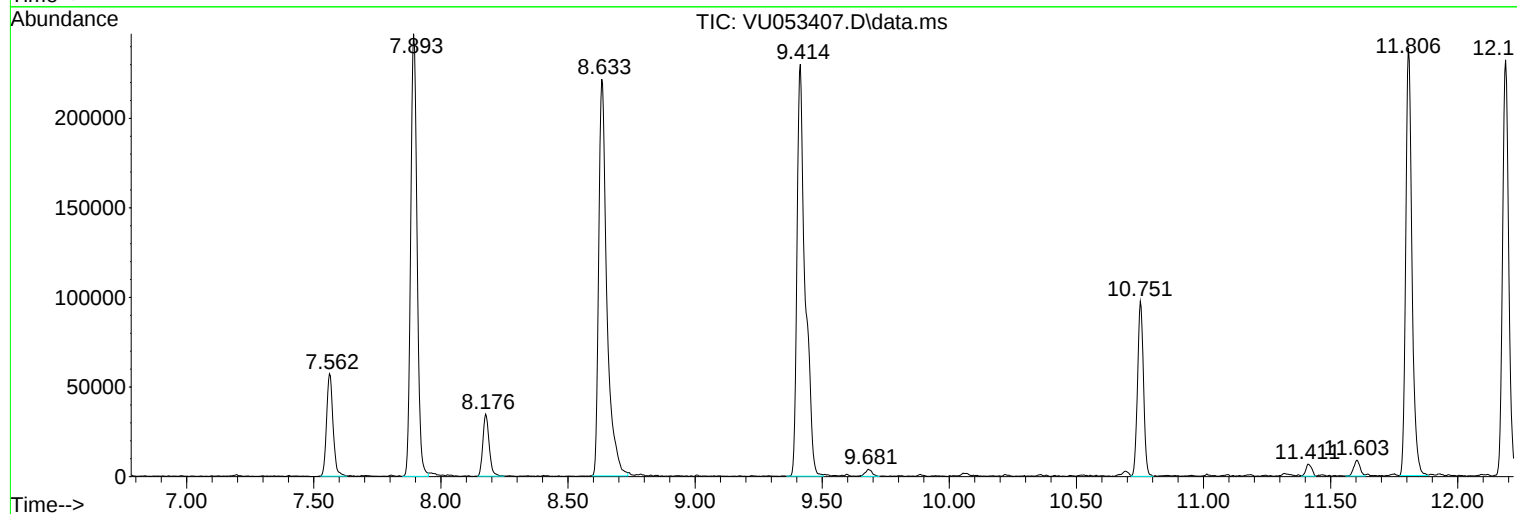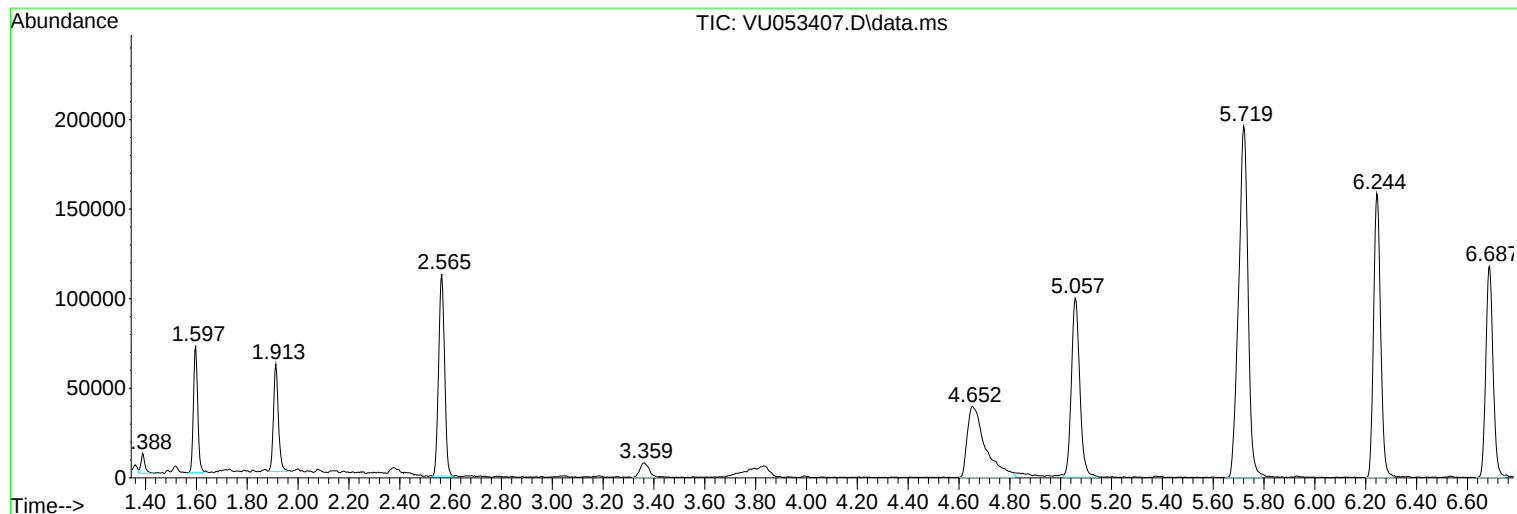

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
Data File : VU053407.D
Acq On : 24 Mar 2023 22:00
Operator : JC/MD
Sample : 02092-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB964

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
Data File : VU053407.D
Acq On : 24 Mar 2023 22:00
Operator : JC/MD
Sample : 02092-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB964

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------