
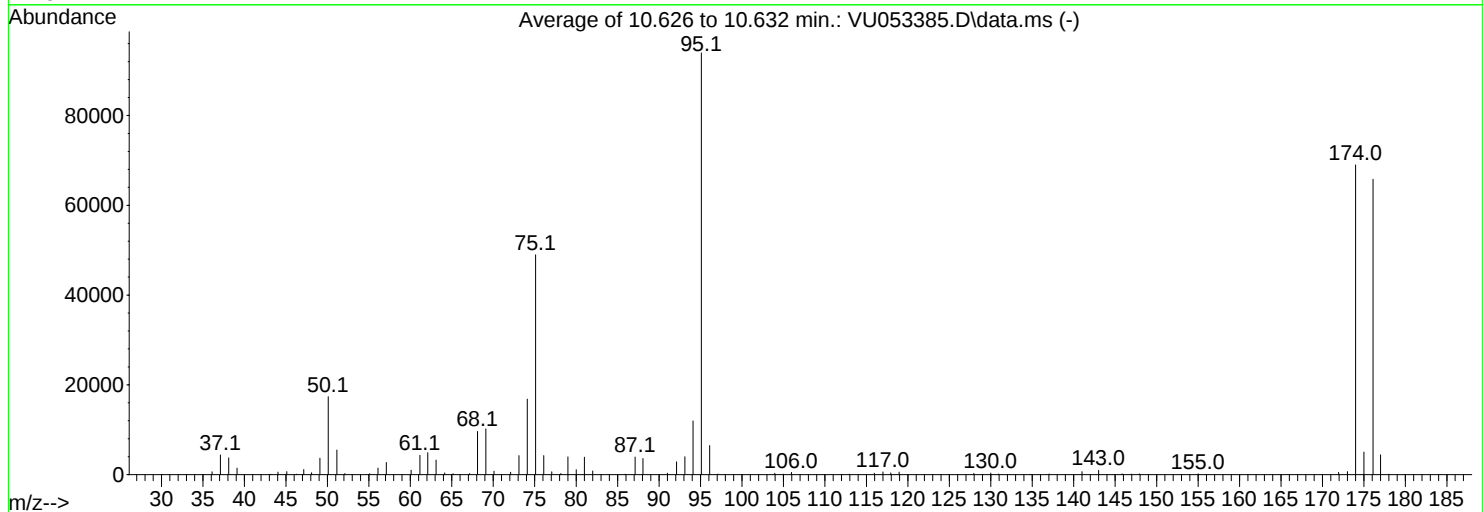


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032423\
Data File : VU053385.D
Acq On : 24 Mar 2023 11:43
Operator : JC/MD
Sample : BFB001
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB001

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Mar 25 00:39:08 2023

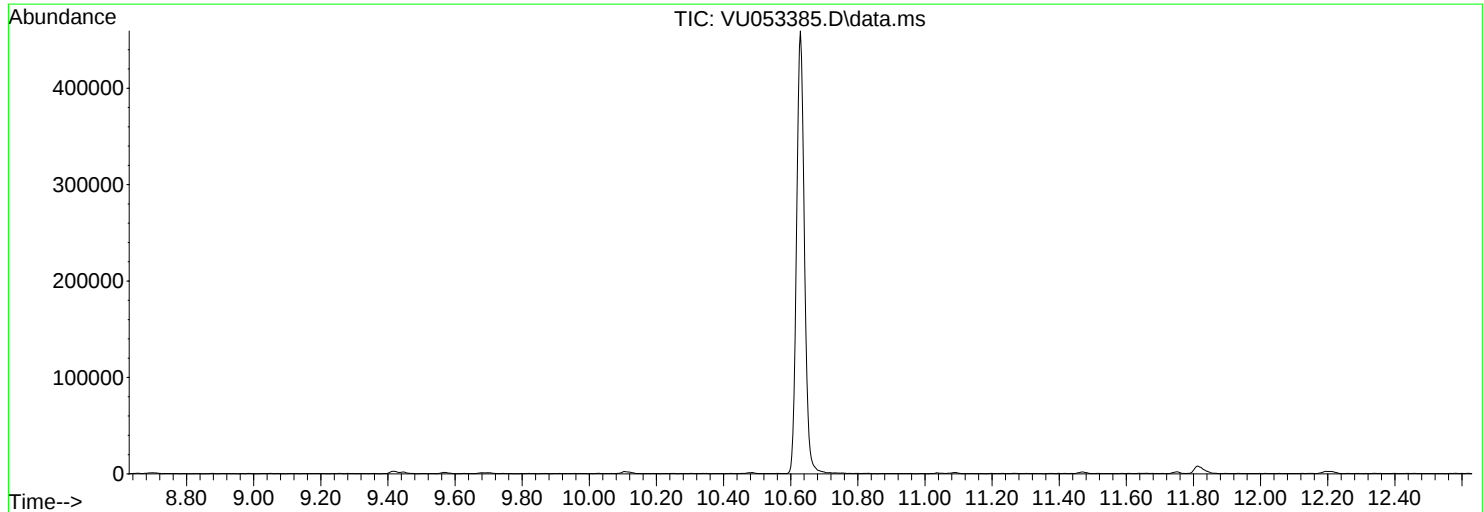

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	17363	PASS
75	95	30	80	52.1	48984	PASS
95	95	100	100	100.0	93957	PASS
96	95	5	9	6.9	6486	PASS
173	174	0.00	2	1.0	676	PASS
174	95	50	120	73.4	68995	PASS
175	174	5	9	7.3	5036	PASS
176	174	95	101	95.4	65795	PASS
177	176	5	9	6.7	4420	PASS

m/z	Abundance
40.20	102.0
44.10	270.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
36.10	673.0
37.10	4379.0
38.10	3706.0
39.10	1540.0
43.20	105.0
44.10	862.0
45.10	713.0
46.30	174.0
47.20	1300.0
48.10	500.0
49.10	3814.0
50.10	18000.0
51.10	5600.0
52.10	303.0
55.10	220.0
56.10	1475.0
57.10	2711.0
60.10	995.0
61.20	4159.0
62.10	5082.0
63.10	3280.0
64.10	424.0
65.20	199.0
67.20	286.0
68.10	9655.0
69.10	10455.0
70.10	752.0
72.10	548.0
73.10	4188.0
74.10	16285.0
75.10	49280.0
76.10	4427.0
77.10	678.0
78.10	260.0
79.00	4111.0
80.00	1071.0
81.00	3880.0
82.00	759.0
85.90	103.0
87.10	4358.0
88.10	3526.0
91.00	397.0
92.10	3096.0
93.10	4098.0
94.10	11743.0
95.10	93136.0
96.10	6343.0
97.10	131.0
103.90	358.0
105.00	153.0
106.00	512.0
112.90	198.0
115.90	305.0
117.00	639.0
117.90	293.0
119.00	590.0
128.00	249.0
129.10	106.0
130.00	374.0
130.90	120.0
137.10	174.0
141.00	674.0
143.00	938.0
144.90	129.0
145.90	203.0
147.00	112.0
147.90	137.0
155.00	209.0
171.90	492.0
173.00	677.0
174.00	67440.0
175.00	4946.0
176.10	64192.0
177.00	4489.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
36.10	659.0
37.10	4549.0
38.10	4006.0
39.10	1466.0
43.20	117.0
44.00	886.0
45.10	702.0
46.30	122.0
47.20	1216.0
48.10	452.0
49.10	3779.0
50.10	17952.0
51.10	5697.0
52.10	278.0
55.10	235.0
56.10	1529.0
57.10	2834.0
58.00	112.0
60.10	1011.0
61.10	4387.0
62.10	5024.0
63.10	3306.0
64.20	388.0
65.10	232.0
67.10	281.0
68.10	9909.0
69.10	10559.0
70.10	791.0
72.10	583.0
73.10	4457.0
74.10	17576.0
75.10	50552.0
76.10	4381.0
77.10	662.0
78.20	224.0
79.00	4117.0
80.00	1178.0
81.00	3958.0
82.00	835.0
85.90	118.0
87.10	4096.0
88.00	3776.0
91.00	339.0
92.10	2915.0
93.10	4138.0
94.10	12402.0
95.10	97352.0
96.10	6639.0
97.10	141.0
104.00	316.0
105.00	144.0
105.90	508.0
113.00	143.0
116.00	329.0
117.00	612.0
118.00	391.0
118.90	590.0
128.00	286.0
130.00	391.0
130.90	155.0
134.70	130.0
137.10	120.0
141.00	690.0
143.00	1035.0
145.80	192.0
147.00	131.0
147.90	212.0
155.00	167.0
161.00	107.0
172.00	519.0
173.00	709.0
174.00	70872.0
175.00	5161.0
176.10	67840.0
177.00	4533.0
178.00	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
36.10	592.0
37.10	4255.0
38.10	3540.0
39.10	1373.0
44.10	831.0
45.10	612.0
47.10	876.0
48.10	379.0
49.10	3432.0
50.10	16137.0
51.20	5203.0
52.10	196.0
55.10	247.0
56.10	1432.0
57.10	2612.0
60.10	983.0
61.10	4348.0
62.10	4561.0
63.10	3192.0
64.20	367.0
65.10	232.0
67.10	234.0
68.10	9316.0
69.10	9586.0
70.10	791.0
72.10	515.0
73.10	4117.0
74.10	16632.0
75.10	47120.0
76.10	3939.0
77.00	624.0
78.10	236.0
79.00	3686.0
80.00	1110.0
81.00	3794.0
82.00	833.0
83.10	103.0
85.90	106.0
87.10	3263.0
88.00	3499.0
91.00	251.0
92.10	2552.0
93.10	3718.0
94.10	11752.0
95.10	91384.0
96.10	6475.0
97.10	116.0
104.00	273.0
105.90	456.0
116.00	360.0
117.00	563.0
118.00	444.0
118.90	497.0
127.90	292.0
129.00	110.0
130.00	309.0
131.00	152.0
134.80	111.0
137.00	111.0
141.00	728.0
143.00	975.0
145.90	150.0
146.90	140.0
147.90	238.0
155.00	151.0
161.00	141.0
172.00	457.0
173.00	642.0
174.00	68672.0
175.00	5002.0
176.10	65352.0
177.00	4239.0
178.00	202.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001