

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030406.D
 Acq On : 25 Mar 2019 16:44
 Operator : JC/SP
 Sample : K2065-23
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	37	rVB	17348	17763	1.04%	0.135%
2	1.399	88	96	107	rBV	244786	257449	15.05%	1.958%
3	1.672	174	181	193	rBV	185525	231863	13.56%	1.763%
4	2.270	356	367	380	rVB	388729	586488	34.29%	4.460%
5	2.331	381	386	389	rBV5	3812	3777	0.22%	0.029%
6	2.434	415	418	422	rBV3	1659	1372	0.08%	0.010%
7	2.463	422	427	430	rVV	2640	2730	0.16%	0.021%
8	2.482	430	433	438	rVB2	1750	1486	0.09%	0.011%
9	2.553	450	455	462	rVB	2443	3238	0.19%	0.025%
10	2.595	462	468	474	rBV	2120	3100	0.18%	0.024%
11	2.630	474	479	482	rVB	1555	1167	0.07%	0.009%
12	2.669	488	491	494	rBV	1720	1156	0.07%	0.009%
13	2.698	494	500	503	rBV3	1908	1758	0.10%	0.013%
14	2.733	508	511	516	rVB	2404	1913	0.11%	0.015%
15	2.788	522	528	531	rBV	1472	1270	0.07%	0.010%
16	2.823	535	539	542	rBV	1883	1639	0.10%	0.012%
17	2.932	569	573	576	rVV	1548	1464	0.09%	0.011%
18	2.958	578	581	584	rVV	1984	1347	0.08%	0.010%
19	2.997	588	593	594	rBV	1468	1207	0.07%	0.009%
20	3.048	606	609	617	rVB	1769	2232	0.13%	0.017%
21	3.100	621	625	629	rBV	2310	2182	0.13%	0.017%
22	3.145	635	639	642	rVV	2211	1775	0.10%	0.013%
23	3.167	642	646	650	rVV	2127	1867	0.11%	0.014%
24	3.190	650	653	661	rVB	1516	1760	0.10%	0.013%
25	3.382	708	713	715	rBV	1579	1128	0.07%	0.009%
26	3.408	715	721	725	rVB	1345	1557	0.09%	0.012%
27	3.550	761	765	772	rVB	1650	1897	0.11%	0.014%
28	3.588	772	777	781	rBV	2056	2150	0.13%	0.016%
29	3.614	781	785	790	rBV	2427	2456	0.14%	0.019%
30	3.691	803	809	811	rBV	2053	2017	0.12%	0.015%
31	3.768	829	833	840	rBV	1424	1583	0.09%	0.012%
32	3.817	845	848	853	rVB2	1529	1266	0.07%	0.010%
33	3.858	853	861	869	rVB	1941	3416	0.20%	0.026%
34	3.907	869	876	877	rBV	1960	1625	0.10%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030406.D
 Acq On : 25 Mar 2019 16:44
 Operator : JC/SP
 Sample : K2065-23
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	3.971	892	896	902	rBV	2989	3145	0.18%	0.024%
36	4.016	906	910	913	rVB	1258	1187	0.07%	0.009%
37	4.103	934	937	941	rVB	1801	1212	0.07%	0.009%
38	4.177	947	960	991	rBV	184789	497069	29.06%	3.780%
39	4.643	1087	1105	1123	rBV	269406	642500	37.56%	4.886%
40	5.074	1235	1239	1241	rBV	1532	1147	0.07%	0.009%
41	5.109	1246	1250	1256	rVB	1946	1994	0.12%	0.015%
42	5.148	1256	1262	1266	rBV	1089	1614	0.09%	0.012%
43	5.334	1296	1320	1344	rBV2	578032	1710381	100.00%	13.006%
44	5.710	1431	1437	1444	rVB2	984	1645	0.10%	0.013%
45	5.881	1478	1490	1523	rBV	504853	1017007	59.46%	7.733%
46	6.328	1613	1629	1647	rBV	388578	793552	46.40%	6.034%
47	6.460	1665	1670	1672	rBV3	2300	2557	0.15%	0.019%
48	6.511	1681	1686	1690	rBV	2181	2356	0.14%	0.018%
49	6.572	1702	1705	1708	rVB	1624	1184	0.07%	0.009%
50	6.595	1708	1712	1714	rBV	1851	1358	0.08%	0.010%
51	6.640	1723	1726	1731	rVB	1610	1383	0.08%	0.011%
52	6.739	1752	1757	1760	rBV2	1763	1607	0.09%	0.012%
53	7.090	1863	1866	1872	rVB	1343	1332	0.08%	0.010%
54	7.135	1873	1880	1882	rBV	1215	1463	0.09%	0.011%
55	7.225	1896	1908	1929	rBV	212975	400318	23.41%	3.044%
56	7.418	1965	1968	1972	rBV2	1596	1299	0.08%	0.010%
57	7.562	2000	2013	2035	rBV	706293	1263140	73.85%	9.605%
58	7.845	2088	2101	2129	rBV	144757	272758	15.95%	2.074%
59	8.308	2234	2245	2280	rBV	621106	1129347	66.03%	8.588%
60	8.778	2387	2391	2396	rBV	2495	2929	0.17%	0.022%
61	8.855	2409	2415	2417	rBV	2201	2009	0.12%	0.015%
62	8.974	2447	2452	2455	rBV	1466	1584	0.09%	0.012%
63	9.016	2460	2465	2469	rVV	2194	1897	0.11%	0.014%
64	9.086	2475	2487	2509	rBV	719266	1235289	72.22%	9.393%
65	9.318	2556	2559	2564	rVB2	2184	2055	0.12%	0.016%
66	9.469	2603	2606	2611	rVB	1661	1302	0.08%	0.010%
67	9.533	2621	2626	2629	rVB	1186	1223	0.07%	0.009%
68	9.620	2650	2653	2657	rBV	1770	1265	0.07%	0.010%
69	9.890	2734	2737	2742	rBV2	1812	1992	0.12%	0.015%
70	9.942	2750	2753	2758	rBV2	1430	1626	0.10%	0.012%
71	10.086	2791	2798	2805	rBV	2479	3507	0.21%	0.027%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030406.D
 Acq On : 25 Mar 2019 16:44
 Operator : JC/SP
 Sample : K2065-23
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.170	2819	2824	2832	rBV	2932	3810	0.22%	0.029%
73	10.209	2832	2836	2840	rVB	1494	1295	0.08%	0.010%
74	10.427	2891	2904	2936	rBV	528241	852178	49.82%	6.480%
75	10.604	2955	2959	2963	rBV2	1818	1659	0.10%	0.013%
76	10.688	2983	2985	2991	rBV	1303	1304	0.08%	0.010%
77	10.765	3006	3009	3017	rBV2	1316	1436	0.08%	0.011%
78	10.845	3030	3034	3038	rVB	2000	1452	0.08%	0.011%
79	10.900	3048	3051	3054	rBV	1818	1470	0.09%	0.011%
80	10.964	3067	3071	3075	rBV	2035	1895	0.11%	0.014%
81	11.421	3207	3213	3220	rBV2	3671	5165	0.30%	0.039%
82	11.482	3220	3232	3255	rVV	618625	1040306	60.82%	7.911%
83	11.858	3335	3349	3372	rBV	607998	1050940	61.44%	7.991%
84	12.160	3438	3443	3446	rBV2	1736	1806	0.11%	0.014%
85	12.575	3569	3572	3576	rVB	1983	1441	0.08%	0.011%
86	12.717	3610	3616	3620	rBV2	1490	1814	0.11%	0.014%
87	12.742	3620	3624	3627	rBV2	1848	1505	0.09%	0.011%
88	13.369	3816	3819	3824	rVB	1653	1348	0.08%	0.010%
89	13.832	3959	3963	3965	rBV2	1925	1388	0.08%	0.011%
90	13.970	4003	4006	4010	rBV	1690	1596	0.09%	0.012%
91	14.151	4059	4062	4066	rBV2	1249	1209	0.07%	0.009%
92	14.270	4096	4099	4103	rBV3	1894	1408	0.08%	0.011%
93	14.315	4109	4113	4116	rBV	1578	1247	0.07%	0.009%
94	14.356	4122	4126	4129	rBV2	1617	1832	0.11%	0.014%
95	14.395	4134	4138	4143	rBV	2133	2553	0.15%	0.019%
96	14.665	4219	4222	4228	rBV	1630	1909	0.11%	0.015%
97	14.797	4260	4263	4268	rBV2	1523	1227	0.07%	0.009%
98	15.183	4380	4383	4386	rBV2	1836	1446	0.08%	0.011%
99	15.466	4466	4471	4475	rBV2	1999	2272	0.13%	0.017%
100	16.347	4742	4745	4747	rBV2	2429	1668	0.10%	0.013%


Sum of corrected areas: 13150910

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032519\
Data File : VU030406.D
Acq On : 25 Mar 2019 16:44
Operator : JC/SP
Sample : K2065-23
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

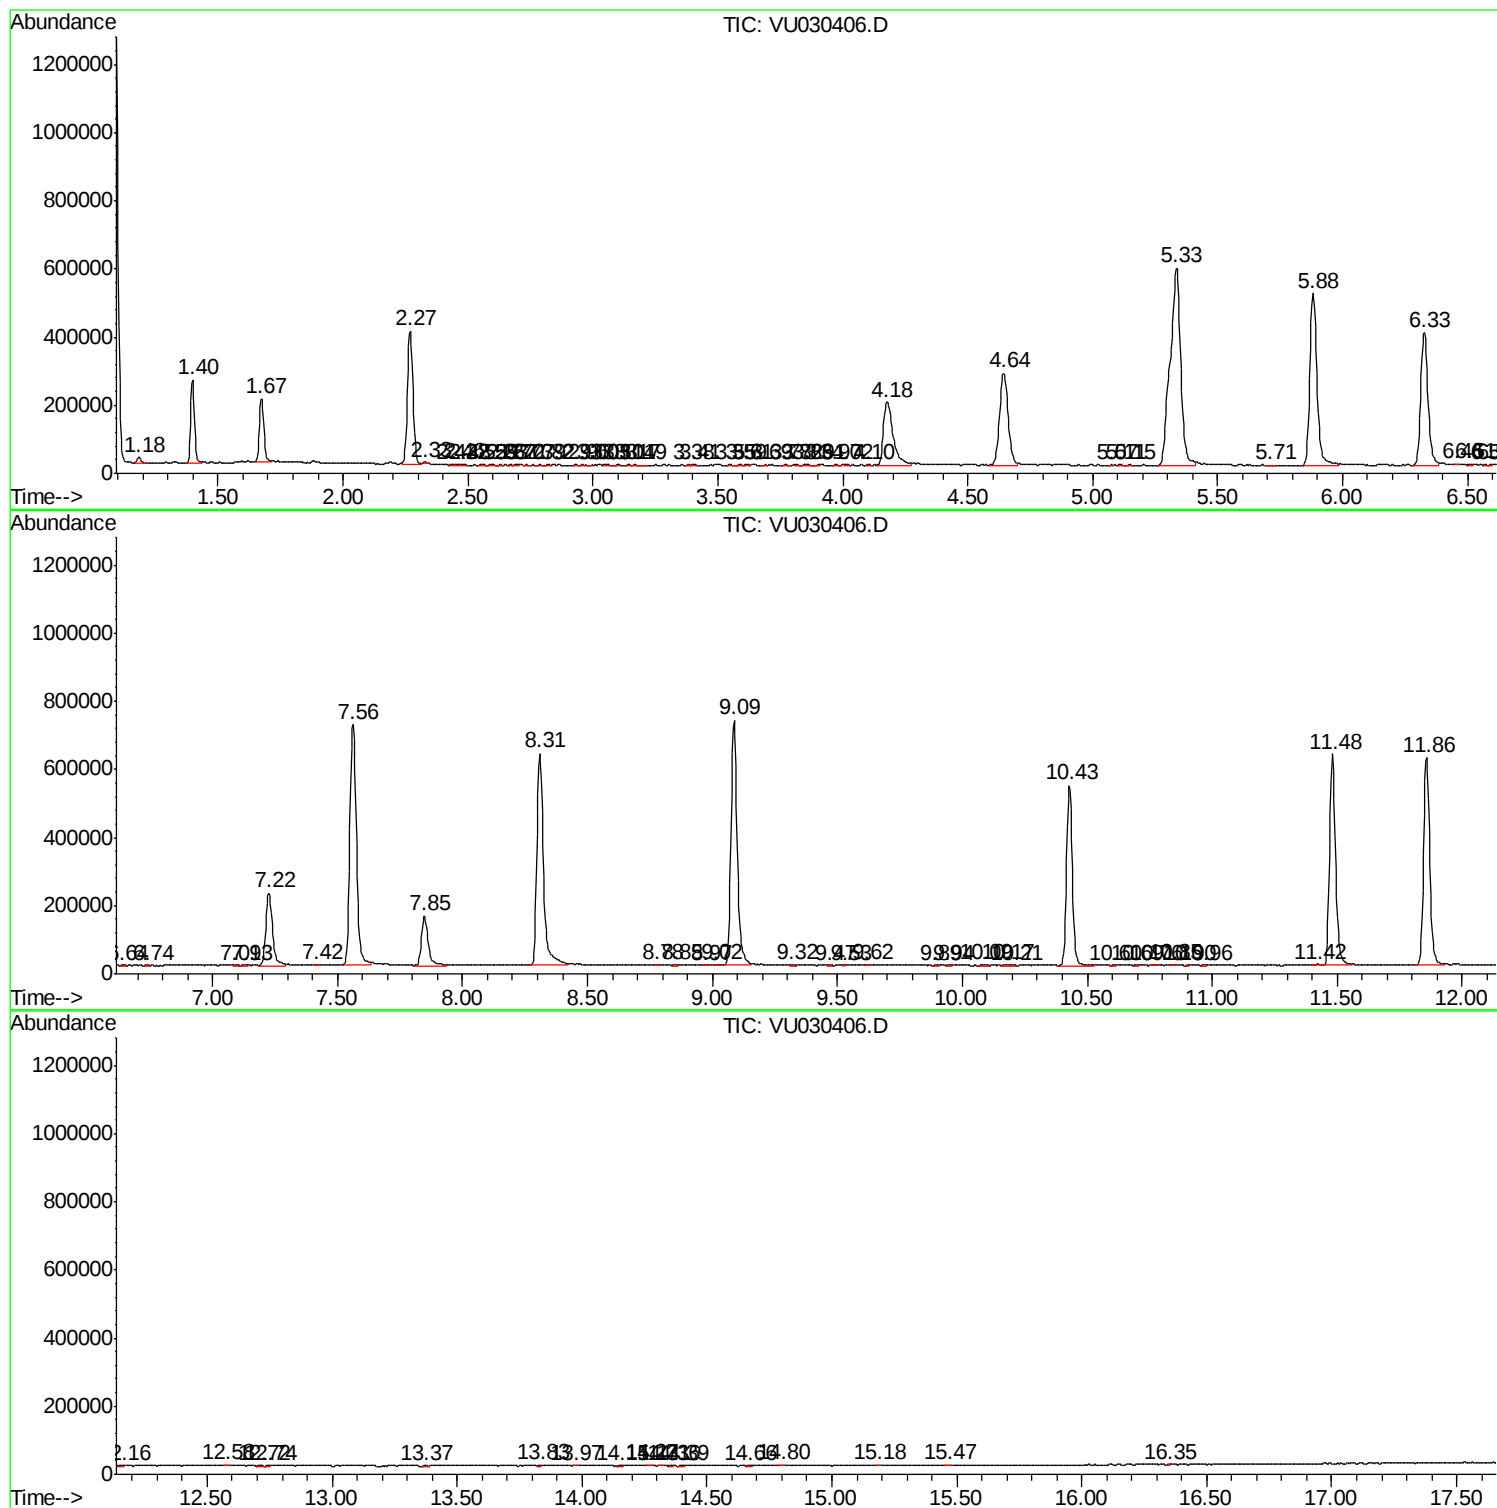

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032519\
Data File : VU030406.D
Acq On : 25 Mar 2019 16:44
Operator : JC/SP
Sample : K2065-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032519\
Data File : VU030406.D
Acq On : 25 Mar 2019 16:44
Operator : JC/SP
Sample : K2065-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc