

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030411.D
 Acq On : 25 Mar 2019 18:42
 Operator : JC/SP
 Sample : K2062-08DL 4X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1D7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.184	24	29	39	rVB3	19961	21545	1.11%	0.140%
2	1.399	89	96	111	rBV	315166	320738	16.57%	2.078%
3	1.676	174	182	201	rVB	219624	288203	14.89%	1.867%
4	2.270	356	367	381	rBV	456480	693141	35.80%	4.491%
5	2.447	415	422	434	rVB2	13187	21905	1.13%	0.142%
6	2.939	572	575	577	rBV	1459	994	0.05%	0.006%
7	3.319	690	693	696	rBV	1784	1286	0.07%	0.008%
8	3.540	760	762	768	rVB	1294	1251	0.06%	0.008%
9	3.746	819	826	829	rBV	2504	3063	0.16%	0.020%
10	3.939	883	886	894	rBV	1879	2258	0.12%	0.015%
11	3.974	894	897	900	rBV	1792	1169	0.06%	0.008%
12	4.174	947	959	988	rBV	194094	503330	26.00%	3.261%
13	4.576	1080	1084	1087	rBV	1876	1420	0.07%	0.009%
14	4.643	1089	1105	1127	rVV	305063	728018	37.61%	4.717%
15	4.987	1207	1212	1216	rBV	1863	2186	0.11%	0.014%
16	5.048	1225	1231	1236	rVB	2389	2773	0.14%	0.018%
17	5.081	1236	1241	1245	rBV	2225	2292	0.12%	0.015%
18	5.338	1296	1321	1347	rBV2	650085	1935951	100.00%	12.543%
19	5.598	1400	1402	1404	rBV	1655	877	0.05%	0.006%
20	5.630	1409	1412	1415	rBV	1226	1006	0.05%	0.007%
21	5.881	1475	1490	1525	rBV	563992	1154327	59.63%	7.479%
22	6.190	1579	1586	1597	rVB5	9190	19018	0.98%	0.123%
23	6.238	1597	1601	1605	rVB	1281	1395	0.07%	0.009%
24	6.267	1606	1610	1614	rVB	1720	1411	0.07%	0.009%
25	6.328	1614	1629	1653	rBV2	424498	883362	45.63%	5.723%
26	6.508	1682	1685	1689	rVB	2453	1790	0.09%	0.012%
27	6.572	1701	1705	1708	rVB	1543	1219	0.06%	0.008%
28	6.656	1727	1731	1734	rVB	1529	1208	0.06%	0.008%
29	6.672	1734	1736	1739	rBV	1814	1105	0.06%	0.007%
30	6.733	1751	1755	1758	rBV	1445	1244	0.06%	0.008%
31	6.797	1772	1775	1781	rVB2	1483	1420	0.07%	0.009%
32	6.884	1797	1802	1807	rVB	1582	1603	0.08%	0.010%
33	7.051	1850	1854	1862	rVB	1825	2362	0.12%	0.015%
34	7.100	1862	1869	1874	rVB	2309	3163	0.16%	0.020%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030411.D
 Acq On : 25 Mar 2019 18:42
 Operator : JC/SP
 Sample : K2062-08DL 4X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1D7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	7.158	1880	1887	1892	rBV	2646	4221	0.22%	0.027%
36	7.225	1896	1908	1933	rBV	237793	432320	22.33%	2.801%
37	7.563	1999	2013	2034	rBV	821223	1476009	76.24%	9.563%
38	7.846	2091	2101	2118	rBV	164897	290995	15.03%	1.885%
39	8.064	2167	2169	2172	rVB	1703	995	0.05%	0.006%
40	8.129	2185	2189	2191	rBV2	1446	1396	0.07%	0.009%
41	8.222	2206	2218	2234	rBV	491267	856637	44.25%	5.550%
42	8.309	2235	2245	2276	rVB	596888	1089975	56.30%	7.062%
43	8.736	2376	2378	2382	rBV2	1410	995	0.05%	0.006%
44	8.855	2412	2415	2418	rBV2	1451	1013	0.05%	0.007%
45	8.971	2448	2451	2455	rBV	1517	1095	0.06%	0.007%
46	9.016	2462	2465	2471	rBV	1657	1647	0.09%	0.011%
47	9.087	2475	2487	2509	rBV	820907	1414123	73.05%	9.162%
48	9.257	2533	2540	2543	rBV3	1316	1813	0.09%	0.012%
49	9.280	2544	2547	2550	rVV3	1259	1235	0.06%	0.008%
50	9.315	2554	2558	2561	rBV	1355	1056	0.05%	0.007%
51	9.444	2596	2598	2602	rVB	1733	1037	0.05%	0.007%
52	9.505	2614	2617	2622	rVB	1311	1072	0.06%	0.007%
53	9.531	2622	2625	2631	rVB	2448	2108	0.11%	0.014%
54	9.566	2632	2636	2641	rBV	1631	1722	0.09%	0.011%
55	9.601	2641	2647	2651	rBV	2086	2158	0.11%	0.014%
56	9.630	2651	2656	2663	rVB	1693	1857	0.10%	0.012%
57	9.666	2663	2667	2669	rBV2	1477	1286	0.07%	0.008%
58	9.711	2678	2681	2685	rBV	1455	1530	0.08%	0.010%
59	9.836	2716	2720	2725	rVB	2406	2007	0.10%	0.013%
60	9.958	2755	2758	2762	rVB	1741	1288	0.07%	0.008%
61	9.981	2762	2765	2772	rBV	1417	1720	0.09%	0.011%
62	10.022	2772	2778	2780	rBV3	1116	1174	0.06%	0.008%
63	10.042	2780	2784	2788	rVB	1789	1502	0.08%	0.010%
64	10.093	2797	2800	2804	rBV2	1167	972	0.05%	0.006%
65	10.248	2840	2848	2851	rBV	1988	2411	0.12%	0.016%
66	10.315	2863	2869	2870	rBV2	1661	1364	0.07%	0.009%
67	10.366	2880	2885	2888	rBV	1200	1369	0.07%	0.009%
68	10.428	2892	2904	2924	rBV	555540	896342	46.30%	5.807%
69	10.530	2933	2936	2937	rBV2	1538	906	0.05%	0.006%
70	10.543	2938	2940	2946	rVB	2331	2015	0.10%	0.013%
71	10.569	2946	2948	2951	rVB2	1847	1138	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030411.D
 Acq On : 25 Mar 2019 18:42
 Operator : JC/SP
 Sample : K2062-08DL 4X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1D7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.691	2981	2986	2987	rBV	1636	1365	0.07%	0.009%
73	10.736	2995	3000	3003	rVB	1944	1788	0.09%	0.012%
74	10.765	3003	3009	3012	rBV	1082	982	0.05%	0.006%
75	10.881	3041	3045	3049	rBV	1992	1927	0.10%	0.012%
76	10.907	3050	3053	3058	rVV	1200	1168	0.06%	0.008%
77	11.032	3088	3092	3096	rBV	2658	2300	0.12%	0.015%
78	11.154	3125	3130	3131	rBV2	1337	962	0.05%	0.006%
79	11.215	3146	3149	3156	rBV2	1214	1771	0.09%	0.011%
80	11.347	3187	3190	3193	rBV2	1298	1054	0.05%	0.007%
81	11.431	3210	3216	3220	rBV3	1912	2504	0.13%	0.016%
82	11.479	3220	3231	3255	rBV	670935	1133694	58.56%	7.345%
83	11.855	3334	3348	3371	rBV	667630	1147870	59.29%	7.437%
84	12.161	3435	3443	3447	rBV	2398	3186	0.16%	0.021%
85	12.186	3448	3451	3455	rVB2	1897	1560	0.08%	0.010%
86	12.604	3577	3581	3582	rBV	1577	959	0.05%	0.006%
87	12.727	3616	3619	3621	rBV	1369	932	0.05%	0.006%
88	12.868	3659	3663	3666	rBV	1604	1332	0.07%	0.009%
89	12.932	3680	3683	3686	rVB	1819	1165	0.06%	0.008%
90	12.958	3686	3691	3697	rBV2	1771	2102	0.11%	0.014%
91	13.009	3704	3707	3710	rBV	1426	973	0.05%	0.006%
92	13.173	3755	3758	3760	rBV2	1324	1008	0.05%	0.007%
93	13.325	3802	3805	3808	rBV	1353	1144	0.06%	0.007%
94	13.466	3843	3849	3852	rBV	1846	2440	0.13%	0.016%
95	13.540	3868	3872	3874	rVV2	1600	1214	0.06%	0.008%
96	13.672	3909	3913	3922	rVB	2679	3275	0.17%	0.021%
97	13.865	3970	3973	3979	rVB3	1265	951	0.05%	0.006%
98	13.945	3995	3998	4000	rBV	1606	1191	0.06%	0.008%
99	14.077	4035	4039	4041	rBV	1617	1301	0.07%	0.008%
100	15.717	4546	4549	4554	rBV	2320	2070	0.11%	0.013%


Sum of corrected areas: 15434724

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032519\
Data File : VU030411.D
Acq On : 25 Mar 2019 18:42
Operator : JC/SP
Sample : K2062-08DL 4X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1D7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

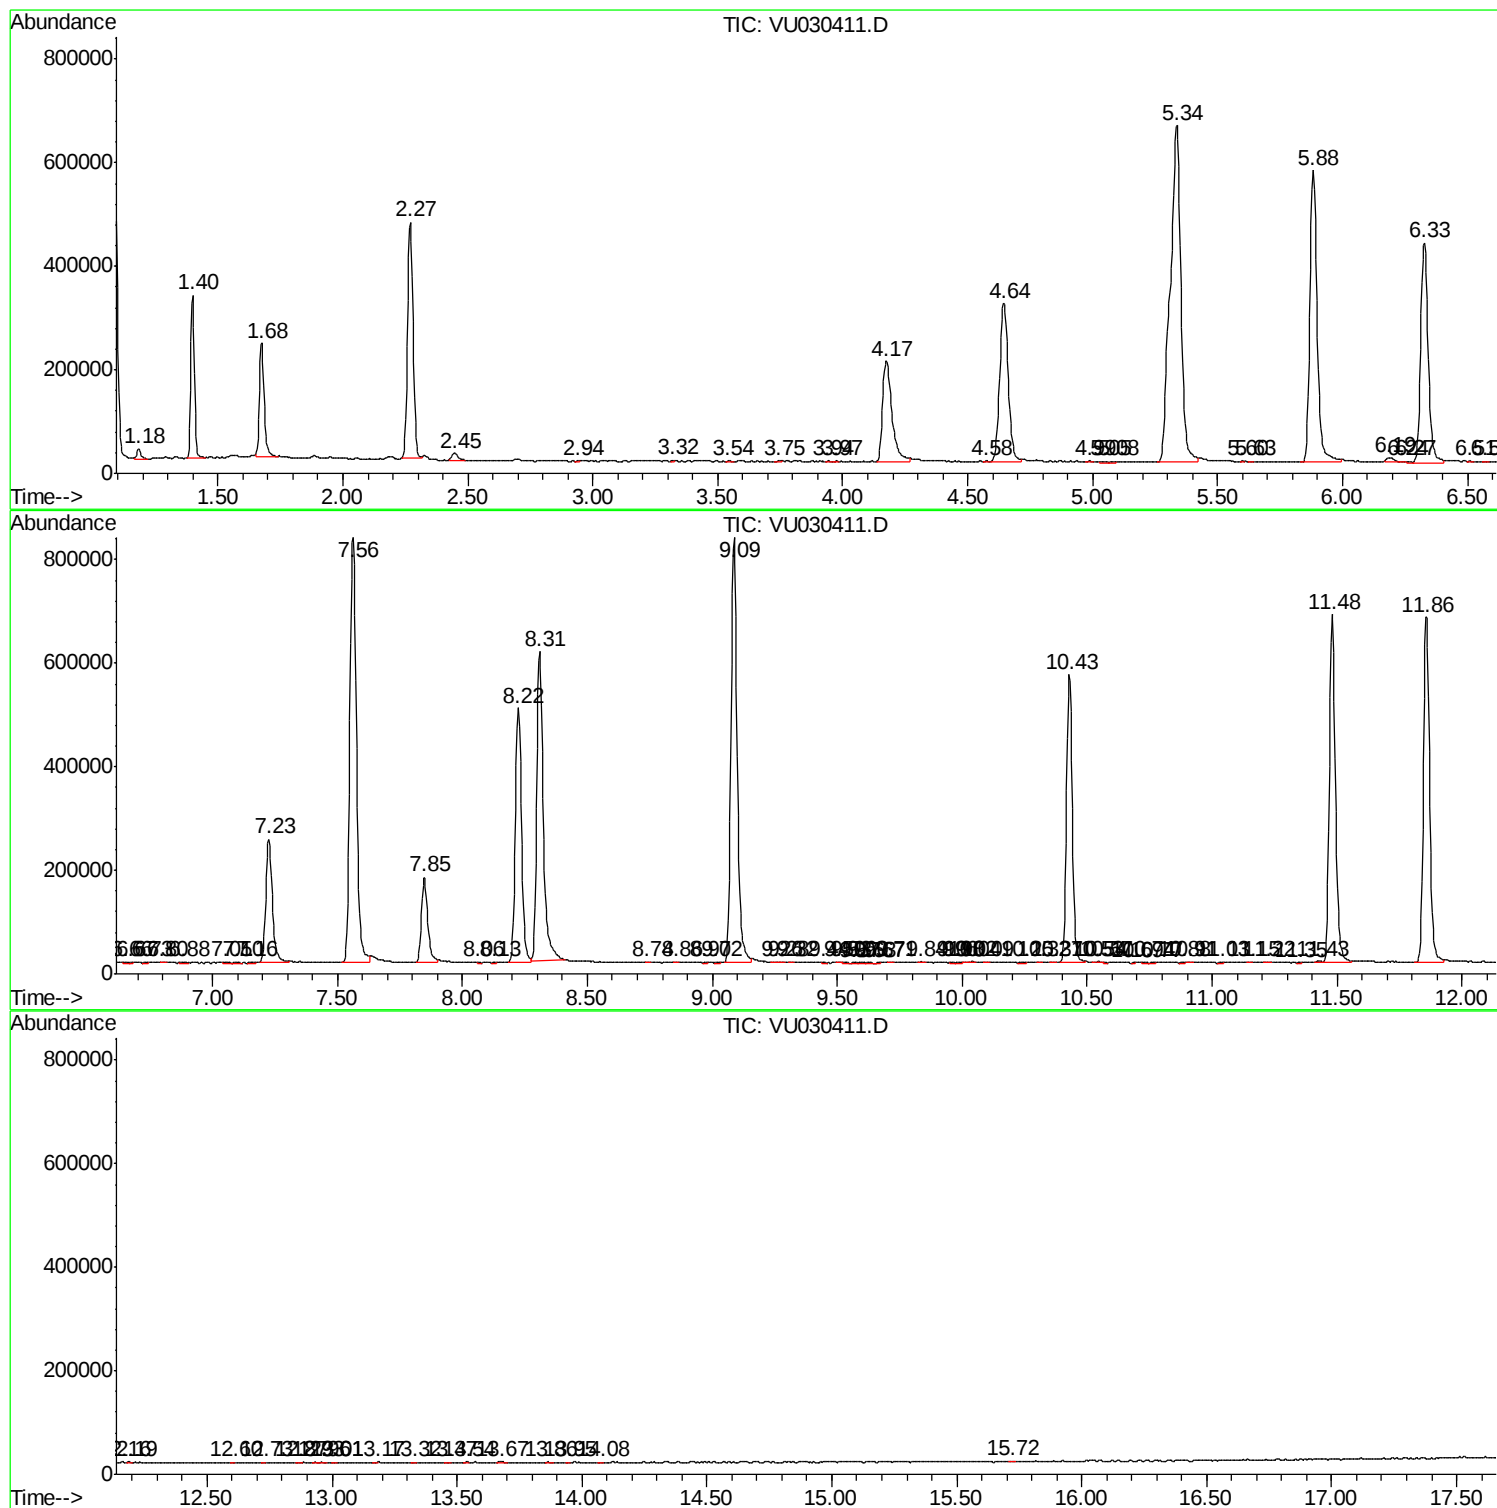

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032519\
Data File : VU030411.D
Acq On : 25 Mar 2019 18:42
Operator : JC/SP
Sample : K2062-08DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1D7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032519\
Data File : VU030411.D
Acq On : 25 Mar 2019 18:42
Operator : JC/SP
Sample : K2062-08DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1D7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc