

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030423.D
 Acq On : 25 Mar 2019 23:26
 Operator : JC/SP
 Sample : K2070-05 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	36	rVB	16635	15539	0.78%	0.100%
2	1.399	89	96	112	rBV	300424	312575	15.60%	2.017%
3	1.672	175	181	208	rVB	224955	322458	16.09%	2.081%
4	2.270	356	367	380	rBV	440619	681826	34.03%	4.400%
5	2.447	410	422	437	rBV	20720	38209	1.91%	0.247%
6	2.656	484	487	492	rBV2	1556	1283	0.06%	0.008%
7	2.698	492	500	502	rVV3	1983	2626	0.13%	0.017%
8	2.778	518	525	526	rBV2	1600	1217	0.06%	0.008%
9	2.849	545	547	553	rVB2	1736	1558	0.08%	0.010%
10	2.900	559	563	567	rBV	1550	1335	0.07%	0.009%
11	2.981	584	588	592	rVB	2041	1831	0.09%	0.012%
12	3.003	592	595	597	rBV	1330	961	0.05%	0.006%
13	3.077	613	618	621	rVB	1297	1228	0.06%	0.008%
14	3.112	626	629	636	rVB	1748	1463	0.07%	0.009%
15	3.148	636	640	644	rVB	1661	1254	0.06%	0.008%
16	3.199	652	656	660	rVB	1782	1360	0.07%	0.009%
17	3.302	683	688	689	rBV	1008	905	0.05%	0.006%
18	3.540	760	762	770	rVB2	1122	1362	0.07%	0.009%
19	3.653	793	797	801	rBV	1983	1935	0.10%	0.012%
20	3.878	864	867	872	rVB	1159	912	0.05%	0.006%
21	3.971	887	896	900	rBV3	1355	2363	0.12%	0.015%
22	4.174	947	959	988	rBV	190995	501465	25.03%	3.236%
23	4.643	1088	1105	1125	rVV	305975	724102	36.14%	4.673%
24	4.739	1131	1135	1138	rBV3	1540	1240	0.06%	0.008%
25	4.952	1197	1201	1206	rVV4	1435	1470	0.07%	0.009%
26	5.000	1213	1216	1224	rVB	2243	2530	0.13%	0.016%
27	5.061	1233	1235	1242	rVB2	1928	1581	0.08%	0.010%
28	5.116	1248	1252	1253	rBV2	1402	939	0.05%	0.006%
29	5.196	1274	1277	1280	rVB	1377	901	0.04%	0.006%
30	5.225	1283	1286	1290	rVB	1583	1021	0.05%	0.007%
31	5.337	1295	1321	1328	rBV2	661279	1899382	94.80%	12.257%
32	5.720	1435	1440	1442	rBV3	1416	1146	0.06%	0.007%
33	5.752	1446	1450	1453	rBV	1419	1254	0.06%	0.008%
34	5.884	1476	1491	1521	rBV	572094	1167281	58.26%	7.533%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030423.D
 Acq On : 25 Mar 2019 23:26
 Operator : JC/SP
 Sample : K2070-05 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.193	1578	1587	1595	rVB8	3385	6219	0.31%	0.040%
36	6.328	1612	1629	1650	rBV	435225	886644	44.25%	5.722%
37	6.791	1770	1773	1782	rVB2	1112	1039	0.05%	0.007%
38	6.919	1810	1813	1816	rBV	1404	1079	0.05%	0.007%
39	7.022	1841	1845	1848	rBV	1682	1259	0.06%	0.008%
40	7.170	1888	1891	1896	rVB	1162	891	0.04%	0.006%
41	7.225	1896	1908	1931	rBV	227382	424265	21.17%	2.738%
42	7.562	1999	2013	2043	rBV	821084	1498129	74.77%	9.667%
43	7.784	2079	2082	2089	rBV2	1130	1107	0.06%	0.007%
44	7.849	2090	2102	2126	rBV	157880	281642	14.06%	1.817%
45	8.103	2176	2181	2184	rBV2	1309	1276	0.06%	0.008%
46	8.199	2208	2211	2217	rVB	2074	1820	0.09%	0.012%
47	8.308	2234	2245	2283	rBV	581657	1080980	53.95%	6.976%
48	8.717	2368	2372	2374	rBV2	1387	1111	0.06%	0.007%
49	8.784	2386	2393	2397	rVB2	1284	1749	0.09%	0.011%
50	8.810	2397	2401	2406	rVB	1315	1192	0.06%	0.008%
51	8.842	2406	2411	2413	rBV	1403	1150	0.06%	0.007%
52	8.968	2447	2450	2457	rBV	1128	1269	0.06%	0.008%
53	9.009	2457	2463	2466	rBV3	1297	1145	0.06%	0.007%
54	9.090	2473	2488	2490	rBV	897805	1288447	64.30%	8.314%
55	9.331	2560	2563	2565	rBV	1266	981	0.05%	0.006%
56	9.347	2565	2568	2573	rVV4	917	989	0.05%	0.006%
57	9.460	2600	2603	2606	rBV2	1493	1128	0.06%	0.007%
58	9.524	2614	2623	2624	rBV3	1739	2448	0.12%	0.016%
59	9.662	2661	2666	2669	rBV2	1174	1190	0.06%	0.008%
60	9.688	2669	2674	2677	rVB	838	915	0.05%	0.006%
61	9.726	2683	2686	2692	rBV2	1258	1260	0.06%	0.008%
62	9.984	2764	2766	2771	rVB2	1004	894	0.04%	0.006%
63	10.022	2771	2778	2782	rBV	1348	1297	0.06%	0.008%
64	10.106	2800	2804	2806	rBV2	1102	975	0.05%	0.006%
65	10.186	2825	2829	2832	rVB	1316	1173	0.06%	0.008%
66	10.308	2864	2867	2876	rBV	1016	1312	0.07%	0.008%
67	10.350	2877	2880	2885	rVB	1502	1059	0.05%	0.007%
68	10.427	2891	2904	2922	rBV	556109	897385	44.79%	5.791%
69	10.723	2992	2996	3000	rVB	1356	1181	0.06%	0.008%
70	10.755	3000	3006	3009	rBV2	1326	1503	0.08%	0.010%
71	10.887	3044	3047	3053	rVB	1831	1845	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030423.D
 Acq On : 25 Mar 2019 23:26
 Operator : JC/SP
 Sample : K2070-05 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09A8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.939	3053	3063	3066	rBV3	1582	2417	0.12%	0.016%
73	11.038	3088	3094	3097	rBV	1296	1337	0.07%	0.009%
74	11.238	3152	3156	3160	rVB	1224	1205	0.06%	0.008%
75	11.267	3160	3165	3167	rBV2	1530	1262	0.06%	0.008%
76	11.418	3203	3212	3220	rBV3	33382	53972	2.69%	0.348%
77	11.482	3220	3232	3236	rBV	775653	1261054	62.94%	8.138%
78	11.861	3335	3350	3380	rBV3	840770	2003653	100.00%	12.930%
79	12.131	3431	3434	3436	rBV2	1420	1035	0.05%	0.007%
80	12.180	3446	3449	3454	rVB2	1299	981	0.05%	0.006%
81	12.324	3489	3494	3498	rVB	1815	1869	0.09%	0.012%
82	12.347	3498	3501	3503	rBV	1443	1100	0.05%	0.007%
83	12.633	3584	3590	3598	rVB2	1575	2474	0.12%	0.016%
84	12.704	3609	3612	3616	rVB2	1576	1240	0.06%	0.008%
85	12.733	3617	3621	3626	rBV3	968	1053	0.05%	0.007%
86	13.035	3711	3715	3718	rVV2	1266	964	0.05%	0.006%
87	13.070	3718	3726	3729	rVV3	1117	1664	0.08%	0.011%
88	13.205	3763	3768	3774	rBV2	1011	1567	0.08%	0.010%
89	13.508	3854	3862	3876	rBV2	19649	43989	2.20%	0.284%
90	13.797	3948	3952	3955	rBV	1496	1110	0.06%	0.007%
91	13.842	3960	3966	3969	rBV	1531	1817	0.09%	0.012%
92	13.897	3980	3983	3988	rBV	1325	1422	0.07%	0.009%
93	13.983	4006	4010	4012	rBV2	1761	1311	0.07%	0.008%
94	14.000	4012	4015	4018	rBV	1542	1277	0.06%	0.008%
95	14.067	4033	4036	4040	rVB	1611	1063	0.05%	0.007%
96	14.090	4040	4043	4047	rBV	1163	946	0.05%	0.006%
97	14.257	4090	4095	4098	rBV3	2213	1944	0.10%	0.013%
98	14.385	4132	4135	4139	rVB	1403	1019	0.05%	0.007%
99	14.807	4259	4266	4272	rBV3	1806	2354	0.12%	0.015%
100	15.459	4466	4469	4471	rBV	1458	1000	0.05%	0.006%


Sum of corrected areas: 15496559

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032519\
Data File : VU030423.D
Acq On : 25 Mar 2019 23:26
Operator : JC/SP
Sample : K2070-05 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

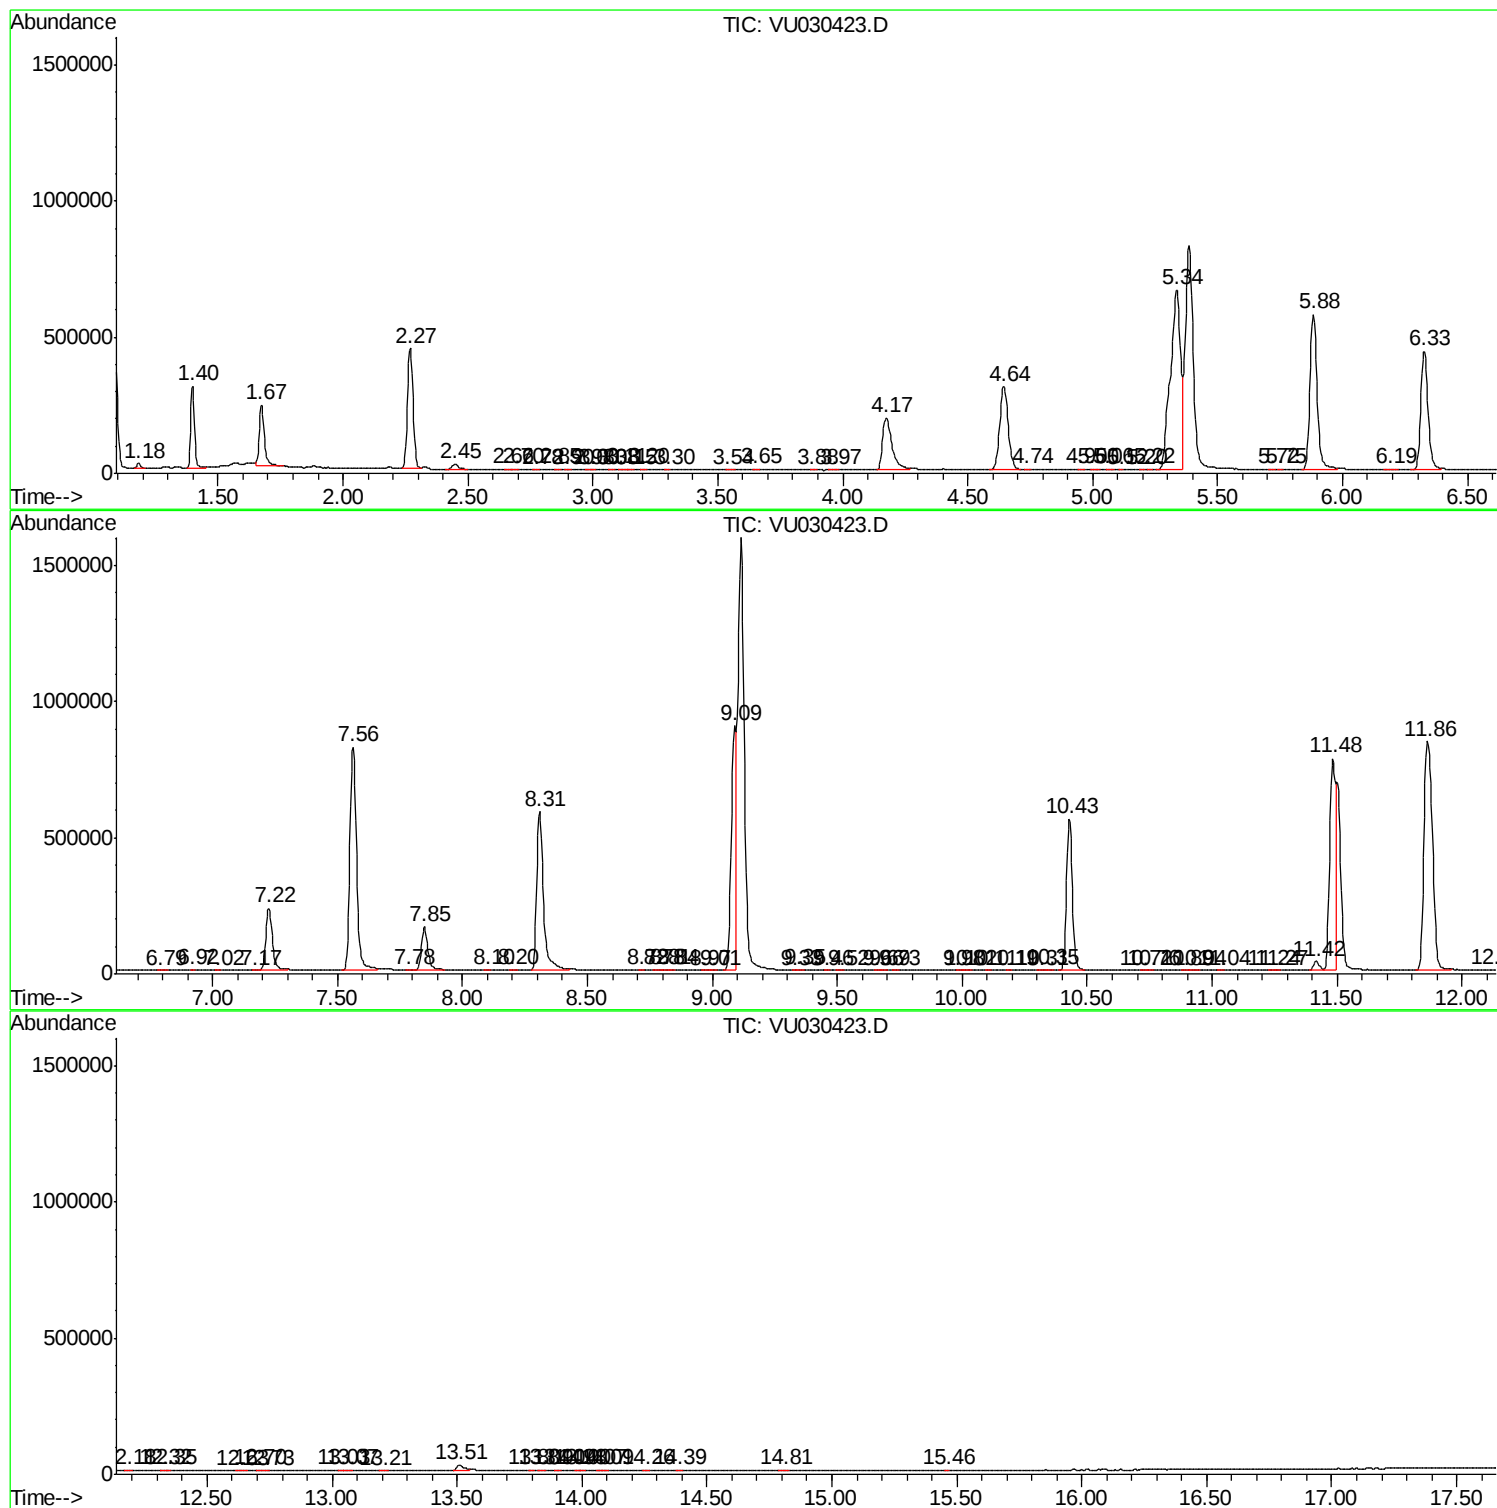

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032519\
Data File : VU030423.D
Acq On : 25 Mar 2019 23:26
Operator : JC/SP
Sample : K2070-05 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032519\
Data File : VU030423.D
Acq On : 25 Mar 2019 23:26
Operator : JC/SP
Sample : K2070-05 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09A8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc