

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030424.D
 Acq On : 25 Mar 2019 23:50
 Operator : JC/SP
 Sample : K2070-07DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09C6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	35	rBV2	15352	13775	0.68%	0.086%
2	1.399	89	96	109	rBV	310676	311330	15.41%	1.951%
3	1.675	175	182	203	rVB	224326	305087	15.10%	1.912%
4	2.270	356	367	380	rBV	446582	675049	33.41%	4.230%
5	2.447	415	422	436	rVB	13262	22185	1.10%	0.139%
6	2.569	457	460	467	rVB	1350	1040	0.05%	0.007%
7	2.662	482	489	493	rBV5	1280	1815	0.09%	0.011%
8	2.746	510	515	520	rBV2	989	1169	0.06%	0.007%
9	2.801	527	532	533	rBV2	1059	883	0.04%	0.006%
10	2.929	565	572	576	rBV2	1334	1800	0.09%	0.011%
11	2.981	584	588	591	rBV2	1527	1700	0.08%	0.011%
12	3.119	624	631	632	rBV	1322	1371	0.07%	0.009%
13	3.167	643	646	649	rBV2	1080	852	0.04%	0.005%
14	3.244	667	670	676	rBV2	1130	1210	0.06%	0.008%
15	3.309	687	690	695	rBV2	1361	1072	0.05%	0.007%
16	3.386	710	714	722	rVB2	1162	1569	0.08%	0.010%
17	3.614	778	785	787	rBV3	736	911	0.05%	0.006%
18	3.694	805	810	817	rVB2	925	1050	0.05%	0.007%
19	3.762	826	831	834	rVB	1213	1147	0.06%	0.007%
20	3.900	870	874	876	rVV	1208	850	0.04%	0.005%
21	3.916	876	879	884	rVV2	1110	1019	0.05%	0.006%
22	4.032	910	915	920	rVB2	1237	1174	0.06%	0.007%
23	4.174	947	959	987	rBV	189907	499091	24.70%	3.127%
24	4.527	1064	1069	1075	rBV3	1252	1599	0.08%	0.010%
25	4.643	1085	1105	1130	rBV	305465	725380	35.90%	4.545%
26	4.842	1164	1167	1170	rVB2	1453	927	0.05%	0.006%
27	4.868	1170	1175	1176	rBV3	1621	1261	0.06%	0.008%
28	4.984	1209	1211	1220	rVB3	1951	2064	0.10%	0.013%
29	5.038	1223	1228	1230	rBV2	1675	1540	0.08%	0.010%
30	5.337	1297	1321	1350	rBV2	653234	2007171	99.33%	12.577%
31	5.752	1444	1450	1452	rBV2	845	1001	0.05%	0.006%
32	5.884	1477	1491	1512	rBV	564872	1136726	56.26%	7.123%
33	6.135	1567	1569	1571	rBV2	1596	869	0.04%	0.005%
34	6.328	1615	1629	1663	rBV	428679	885636	43.83%	5.549%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030424.D
 Acq On : 25 Mar 2019 23:50
 Operator : JC/SP
 Sample : K2070-07DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09C6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.588	1705	1710	1713	rBV2	2541	2227	0.11%	0.014%
36	6.624	1717	1721	1725	rVV	1317	988	0.05%	0.006%
37	6.839	1785	1788	1794	rVB2	897	1082	0.05%	0.007%
38	6.900	1800	1807	1810	rBV	1221	1276	0.06%	0.008%
39	6.919	1810	1813	1817	rVB	1269	1118	0.06%	0.007%
40	7.016	1839	1843	1847	rBV2	1340	1454	0.07%	0.009%
41	7.225	1893	1908	1925	rBV	227487	413822	20.48%	2.593%
42	7.427	1968	1971	1976	rVB	1415	1112	0.06%	0.007%
43	7.489	1983	1990	1991	rBV3	1298	1143	0.06%	0.007%
44	7.562	1998	2013	2047	rBV	807242	1479239	73.21%	9.269%
45	7.849	2091	2102	2122	rBV	154946	272436	13.48%	1.707%
46	7.984	2141	2144	2148	rVV	1205	854	0.04%	0.005%
47	8.042	2158	2162	2167	rBV2	1556	1571	0.08%	0.010%
48	8.077	2168	2173	2176	rBV2	1302	1142	0.06%	0.007%
49	8.157	2193	2198	2201	rBV3	1071	1131	0.06%	0.007%
50	8.308	2234	2245	2280	rBV	581182	1078081	53.35%	6.755%
51	8.533	2313	2315	2318	rVB2	1956	1139	0.06%	0.007%
52	8.553	2318	2321	2324	rBV2	1385	950	0.05%	0.006%
53	8.948	2437	2444	2446	rBV2	978	999	0.05%	0.006%
54	8.968	2446	2450	2454	rVB3	1452	1267	0.06%	0.008%
55	9.016	2462	2465	2469	rBV	1355	1160	0.06%	0.007%
56	9.087	2474	2487	2492	rBV	844515	1448772	71.70%	9.078%
57	9.276	2543	2546	2550	rVB	2046	1277	0.06%	0.008%
58	9.411	2581	2588	2592	rBV2	1561	1840	0.09%	0.012%
59	9.495	2610	2614	2616	rBV	1364	1142	0.06%	0.007%
60	9.575	2632	2639	2640	rBV	1183	1336	0.07%	0.008%
61	9.611	2646	2650	2653	rBV2	887	865	0.04%	0.005%
62	9.813	2710	2713	2718	rBV	1189	1265	0.06%	0.008%
63	9.945	2749	2754	2756	rBV	830	777	0.04%	0.005%
64	10.173	2821	2825	2830	rBV2	1250	1547	0.08%	0.010%
65	10.234	2838	2844	2848	rBV2	1365	1815	0.09%	0.011%
66	10.328	2869	2873	2879	rVB2	862	827	0.04%	0.005%
67	10.427	2889	2904	2923	rBV	542946	896972	44.39%	5.620%
68	10.601	2954	2958	2960	rBV	1313	1032	0.05%	0.006%
69	10.922	3053	3058	3060	rBV2	839	852	0.04%	0.005%
70	10.967	3069	3072	3077	rVV	1025	795	0.04%	0.005%
71	11.003	3081	3083	3087	rVB	1451	850	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030424.D
 Acq On : 25 Mar 2019 23:50
 Operator : JC/SP
 Sample : K2070-07DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09C6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.067	3099	3103	3106	rBV2	1459	1061	0.05%	0.007%
73	11.083	3106	3108	3116	rVV3	1462	1676	0.08%	0.011%
74	11.157	3127	3131	3140	rBV3	1391	2024	0.10%	0.013%
75	11.279	3164	3169	3173	rBV2	924	900	0.04%	0.006%
76	11.414	3194	3211	3221	rBV	132026	218848	10.83%	1.371%
77	11.482	3221	3232	3261	rVB2	782504	2020634	100.00%	12.661%
78	11.791	3325	3328	3334	rVB4	1493	1664	0.08%	0.010%
79	11.858	3334	3349	3376	rBV2	713712	1362598	67.43%	8.538%
80	12.157	3438	3442	3444	rBV3	973	816	0.04%	0.005%
81	12.591	3569	3577	3580	rBV2	1466	1907	0.09%	0.012%
82	12.697	3607	3610	3622	rVB2	1473	2063	0.10%	0.013%
83	12.768	3625	3632	3635	rVV2	1188	1439	0.07%	0.009%
84	12.836	3649	3653	3656	rBV4	1967	1953	0.10%	0.012%
85	12.893	3668	3671	3678	rVB4	1635	1879	0.09%	0.012%
86	12.964	3690	3693	3700	rVB2	1533	1727	0.09%	0.011%
87	13.000	3700	3704	3709	rBV	1700	1717	0.08%	0.011%
88	13.083	3726	3730	3732	rBV3	1439	1153	0.06%	0.007%
89	13.311	3798	3801	3806	rVB2	1489	1090	0.05%	0.007%
90	13.508	3852	3862	3885	rBV4	33486	82495	4.08%	0.517%
91	13.778	3942	3946	3948	rBV	1441	1110	0.05%	0.007%
92	13.961	4000	4003	4006	rBV2	1299	939	0.05%	0.006%
93	14.118	4047	4052	4054	rBV2	1020	1041	0.05%	0.007%
94	14.276	4098	4101	4106	rBV	2108	1733	0.09%	0.011%
95	14.302	4106	4109	4115	rVB	1392	1375	0.07%	0.009%
96	14.771	4251	4255	4257	rBV2	1841	1653	0.08%	0.010%
97	14.803	4262	4265	4271	rVB	2093	1993	0.10%	0.012%
98	15.131	4363	4367	4369	rBV2	1207	982	0.05%	0.006%
99	15.231	4393	4398	4400	rBV2	1511	1424	0.07%	0.009%
100	15.813	4575	4579	4582	rBV3	1806	1902	0.09%	0.012%


Sum of corrected areas: 15959274

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032519\
Data File : VU030424.D
Acq On : 25 Mar 2019 23:50
Operator : JC/SP
Sample : K2070-07DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09C6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

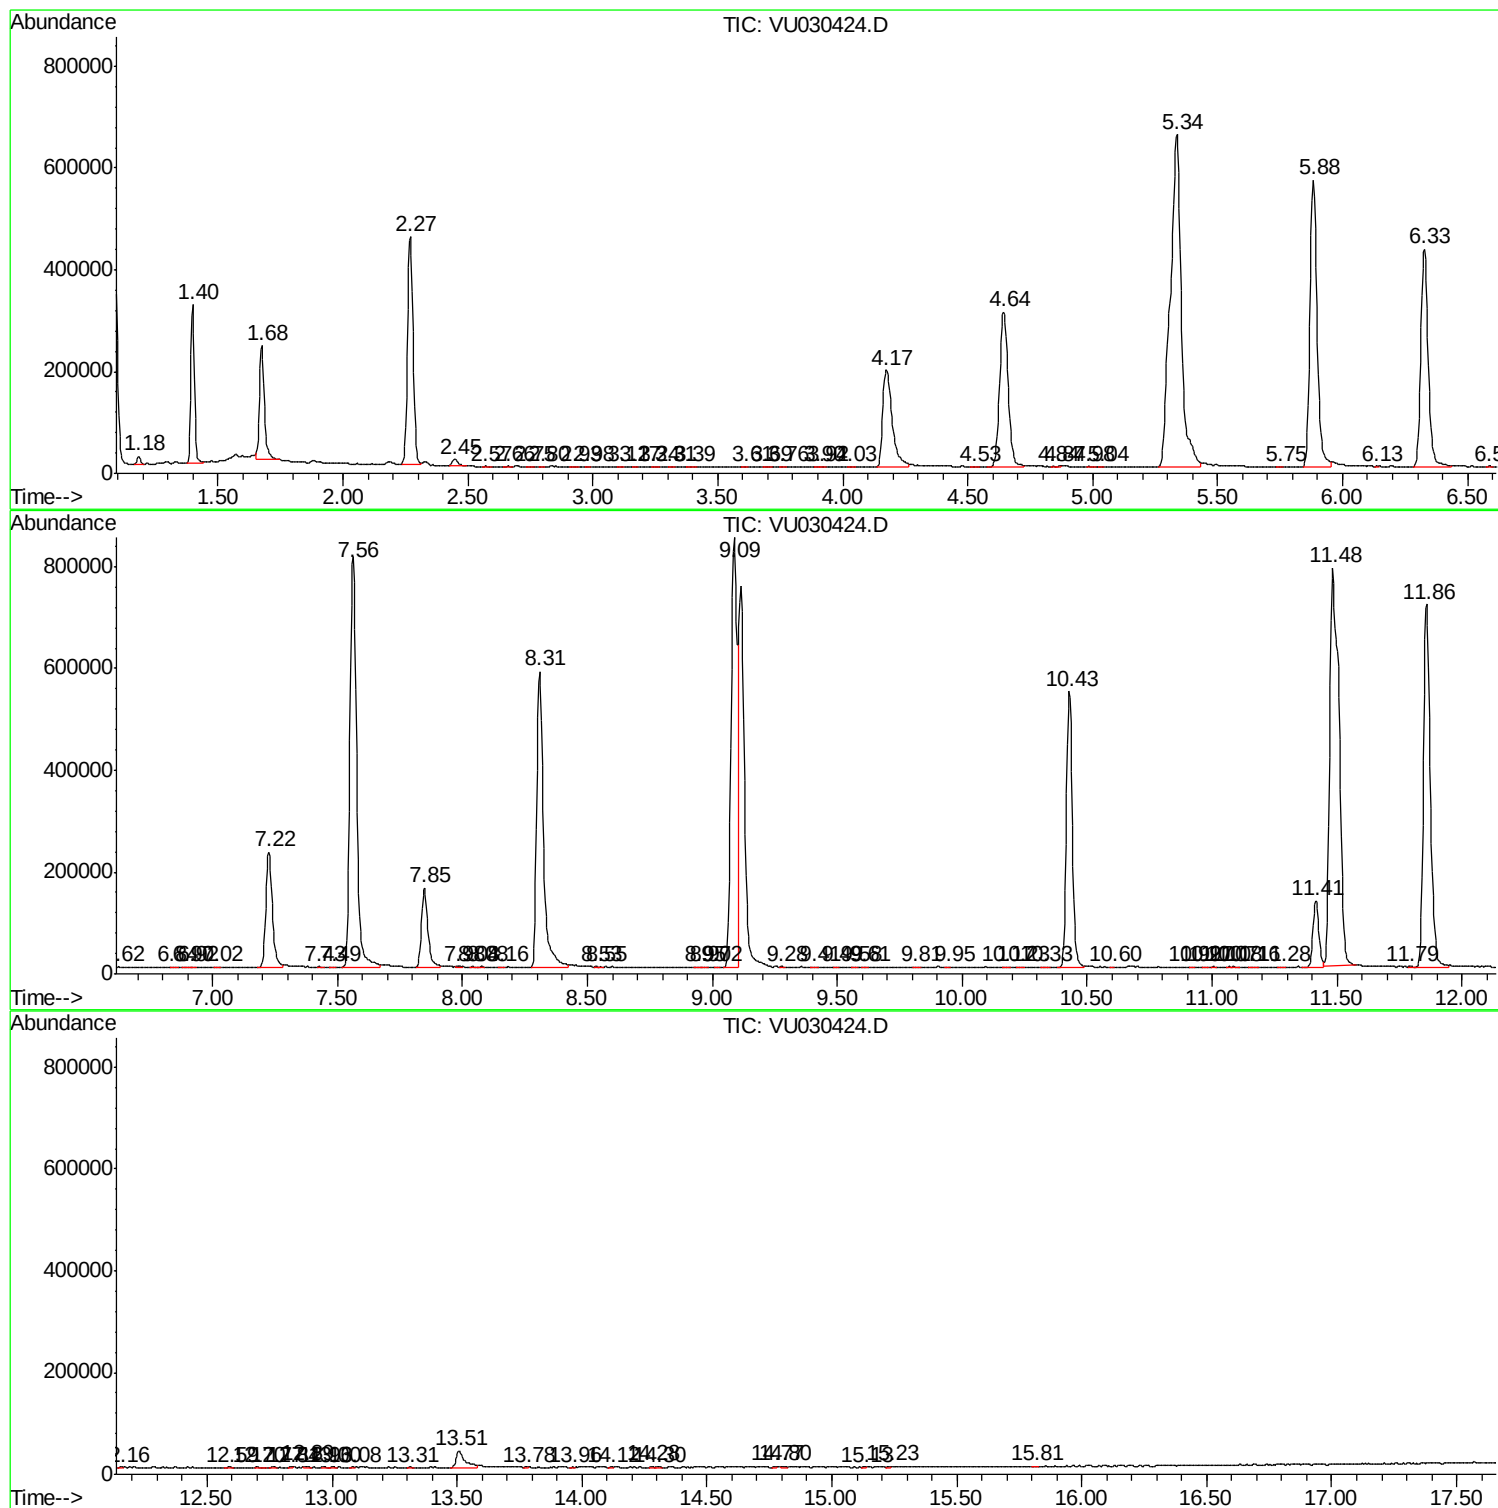

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032519\
Data File : VU030424.D
Acq On : 25 Mar 2019 23:50
Operator : JC/SP
Sample : K2070-07DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09C6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU032519\
Data File : VU030424.D
Acq On : 25 Mar 2019 23:50
Operator : JC/SP
Sample : K2070-07DL 5X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C09C6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc