

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030425.D
 Acq On : 26 Mar 2019 00:13
 Operator : JC/SP
 Sample : K2070-11DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09D6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.184	24	29	38	rVB2	16553	16619	0.84%	0.095%
2	1.399	88	96	108	rBV	295075	302887	15.30%	1.734%
3	1.672	174	181	215	rVB	221119	318468	16.09%	1.824%
4	2.267	356	366	379	rBV	438135	672347	33.96%	3.850%
5	2.451	412	423	434	rBV3	8288	17177	0.87%	0.098%
6	2.611	467	473	475	rBV2	1398	1320	0.07%	0.008%
7	2.698	495	500	509	rVB5	2305	3507	0.18%	0.020%
8	2.778	520	525	532	rBV4	966	1379	0.07%	0.008%
9	2.827	532	540	542	rBV2	2142	2711	0.14%	0.016%
10	3.010	595	597	603	rVB3	1421	1122	0.06%	0.006%
11	3.065	611	614	617	rBV2	1042	853	0.04%	0.005%
12	3.094	620	623	630	rVB2	1267	1574	0.08%	0.009%
13	3.193	651	654	657	rVB	1328	904	0.05%	0.005%
14	3.306	687	689	694	rVB	1139	823	0.04%	0.005%
15	3.364	704	707	710	rBV2	999	890	0.04%	0.005%
16	4.000	900	905	910	rBV2	1240	1280	0.06%	0.007%
17	4.068	922	926	929	rBV	1173	968	0.05%	0.006%
18	4.174	944	959	989	rBV2	190234	505158	25.52%	2.893%
19	4.643	1089	1105	1135	rBV	302409	711267	35.93%	4.073%
20	4.962	1201	1204	1208	rBV3	1942	1297	0.07%	0.007%
21	5.065	1232	1236	1239	rBV2	1838	1764	0.09%	0.010%
22	5.148	1259	1262	1265	rVB	1723	1073	0.05%	0.006%
23	5.193	1271	1276	1280	rBV	1410	1626	0.08%	0.009%
24	5.335	1297	1320	1356	rBV2	642257	1957169	98.87%	11.208%
25	5.814	1465	1469	1472	rBV	1211	1185	0.06%	0.007%
26	5.881	1477	1490	1520	rBV	551814	1127517	56.96%	6.457%
27	6.071	1547	1549	1553	rVB4	1698	993	0.05%	0.006%
28	6.177	1578	1582	1584	rBV4	1508	1090	0.06%	0.006%
29	6.328	1614	1629	1653	rBV	424144	873432	44.12%	5.002%
30	6.470	1669	1673	1678	rVB5	1659	1654	0.08%	0.009%
31	6.556	1697	1700	1706	rVB3	1660	1892	0.10%	0.011%
32	6.611	1713	1717	1721	rVB	1506	1104	0.06%	0.006%
33	6.846	1785	1790	1794	rVV3	1035	1094	0.06%	0.006%
34	6.875	1796	1799	1802	rVV	1495	1007	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030425.D
 Acq On : 26 Mar 2019 00:13
 Operator : JC/SP
 Sample : K2070-11DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09D6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.894	1802	1805	1810	rVV3	981	1112	0.06%	0.006%
36	6.955	1820	1824	1827	rVB2	1035	827	0.04%	0.005%
37	7.010	1838	1841	1846	rBV2	882	999	0.05%	0.006%
38	7.036	1846	1849	1856	rVB	1223	1243	0.06%	0.007%
39	7.138	1874	1881	1885	rBV2	1079	1158	0.06%	0.007%
40	7.225	1892	1908	1937	rBV	228169	423083	21.37%	2.423%
41	7.476	1980	1986	1996	rVB3	1716	3260	0.16%	0.019%
42	7.563	1996	2013	2044	rBV	799436	1459161	73.71%	8.356%
43	7.846	2088	2101	2128	rBV	154072	278256	14.06%	1.593%
44	8.119	2181	2186	2189	rBV5	1147	1199	0.06%	0.007%
45	8.171	2194	2202	2207	rBV3	1620	2347	0.12%	0.013%
46	8.309	2232	2245	2281	rBV	580757	1085033	54.81%	6.213%
47	8.646	2347	2350	2355	rVB	1549	1346	0.07%	0.008%
48	8.679	2355	2360	2362	rBV2	1500	1182	0.06%	0.007%
49	8.724	2370	2374	2378	rVB2	1449	1256	0.06%	0.007%
50	8.753	2378	2383	2388	rBV2	1509	1838	0.09%	0.011%
51	8.900	2425	2429	2433	rBV2	1251	1174	0.06%	0.007%
52	8.974	2448	2452	2456	rBV3	1095	867	0.04%	0.005%
53	9.000	2456	2460	2463	rVB2	1133	815	0.04%	0.005%
54	9.023	2463	2467	2474	rBV2	895	1187	0.06%	0.007%
55	9.087	2474	2487	2527	rBV2	813784	1979547	100.00%	11.336%
56	9.244	2532	2536	2539	rVB3	1490	1053	0.05%	0.006%
57	9.495	2608	2614	2617	rBV2	1135	1167	0.06%	0.007%
58	9.537	2623	2627	2630	rBV	982	957	0.05%	0.005%
59	9.576	2636	2639	2641	rBV	1258	851	0.04%	0.005%
60	9.711	2677	2681	2684	rBV2	984	866	0.04%	0.005%
61	9.785	2701	2704	2708	rVB2	1340	1006	0.05%	0.006%
62	10.055	2784	2788	2794	rVV3	768	850	0.04%	0.005%
63	10.097	2798	2801	2806	rBV	1372	1420	0.07%	0.008%
64	10.177	2822	2826	2829	rBV2	1502	1251	0.06%	0.007%
65	10.289	2857	2861	2864	rVB	1115	897	0.05%	0.005%
66	10.351	2878	2880	2885	rBV2	1115	968	0.05%	0.006%
67	10.428	2892	2904	2927	rVV	553315	889513	44.94%	5.094%
68	10.515	2929	2931	2936	rVB	2229	1446	0.07%	0.008%
69	10.653	2971	2974	2978	rBV	1676	1116	0.06%	0.006%
70	10.704	2985	2990	2993	rVB	1239	1204	0.06%	0.007%
71	10.724	2993	2996	3000	rVB	1337	877	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032519\
 Data File : VU030425.D
 Acq On : 26 Mar 2019 00:13
 Operator : JC/SP
 Sample : K2070-11DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09D6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.756	3000	3006	3011	rBV2	1417	1558	0.08%	0.009%
73	10.820	3020	3026	3032	rVB	1331	1684	0.09%	0.010%
74	10.859	3032	3038	3041	rBV2	1086	1213	0.06%	0.007%
75	10.929	3056	3060	3065	rVB	1392	1117	0.06%	0.006%
76	10.958	3065	3069	3073	rBV2	1149	877	0.04%	0.005%
77	11.010	3079	3085	3087	rBV2	1079	1019	0.05%	0.006%
78	11.061	3097	3101	3105	rBV2	1032	905	0.05%	0.005%
79	11.084	3105	3108	3112	rVB2	1230	1081	0.05%	0.006%
80	11.135	3116	3124	3130	rBV	1660	2910	0.15%	0.017%
81	11.170	3130	3135	3137	rBV	923	863	0.04%	0.005%
82	11.212	3143	3148	3154	rBV3	1416	1787	0.09%	0.010%
83	11.415	3202	3211	3221	rVV	57999	95794	4.84%	0.549%
84	11.482	3221	3232	3263	rVB3	751812	1821239	92.00%	10.429%
85	11.858	3336	3349	3373	rBV3	809609	1752010	88.51%	10.033%
86	12.646	3590	3594	3602	rVB5	3403	4485	0.23%	0.026%
87	12.833	3643	3652	3659	rBV5	3058	4699	0.24%	0.027%
88	12.993	3696	3702	3712	rVB7	3279	5866	0.30%	0.034%
89	13.103	3732	3736	3743	rBV2	1331	1189	0.06%	0.007%
90	13.228	3770	3775	3778	rBV3	1817	1947	0.10%	0.011%
91	13.286	3789	3793	3797	rVV	1092	1087	0.05%	0.006%
92	13.344	3808	3811	3813	rBV	1222	900	0.05%	0.005%
93	13.502	3848	3860	3886	rBV	426096	757281	38.26%	4.337%
94	13.923	3985	3991	3997	rBV	2923	3482	0.18%	0.020%
95	13.987	3999	4011	4037	rVV	159772	304411	15.38%	1.743%
96	14.247	4089	4092	4095	rBV2	1084	838	0.04%	0.005%
97	14.447	4150	4154	4157	rBV	1386	1270	0.06%	0.007%
98	14.624	4205	4209	4211	rBV2	1269	1082	0.05%	0.006%
99	14.723	4238	4240	4246	rVB	1632	1170	0.06%	0.007%
100	16.125	4673	4676	4679	rBV	2083	1505	0.08%	0.009%


Sum of corrected areas: 17462752

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032519\
Data File : VU030425.D
Acq On : 26 Mar 2019 00:13
Operator : JC/SP
Sample : K2070-11DL 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C09D6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

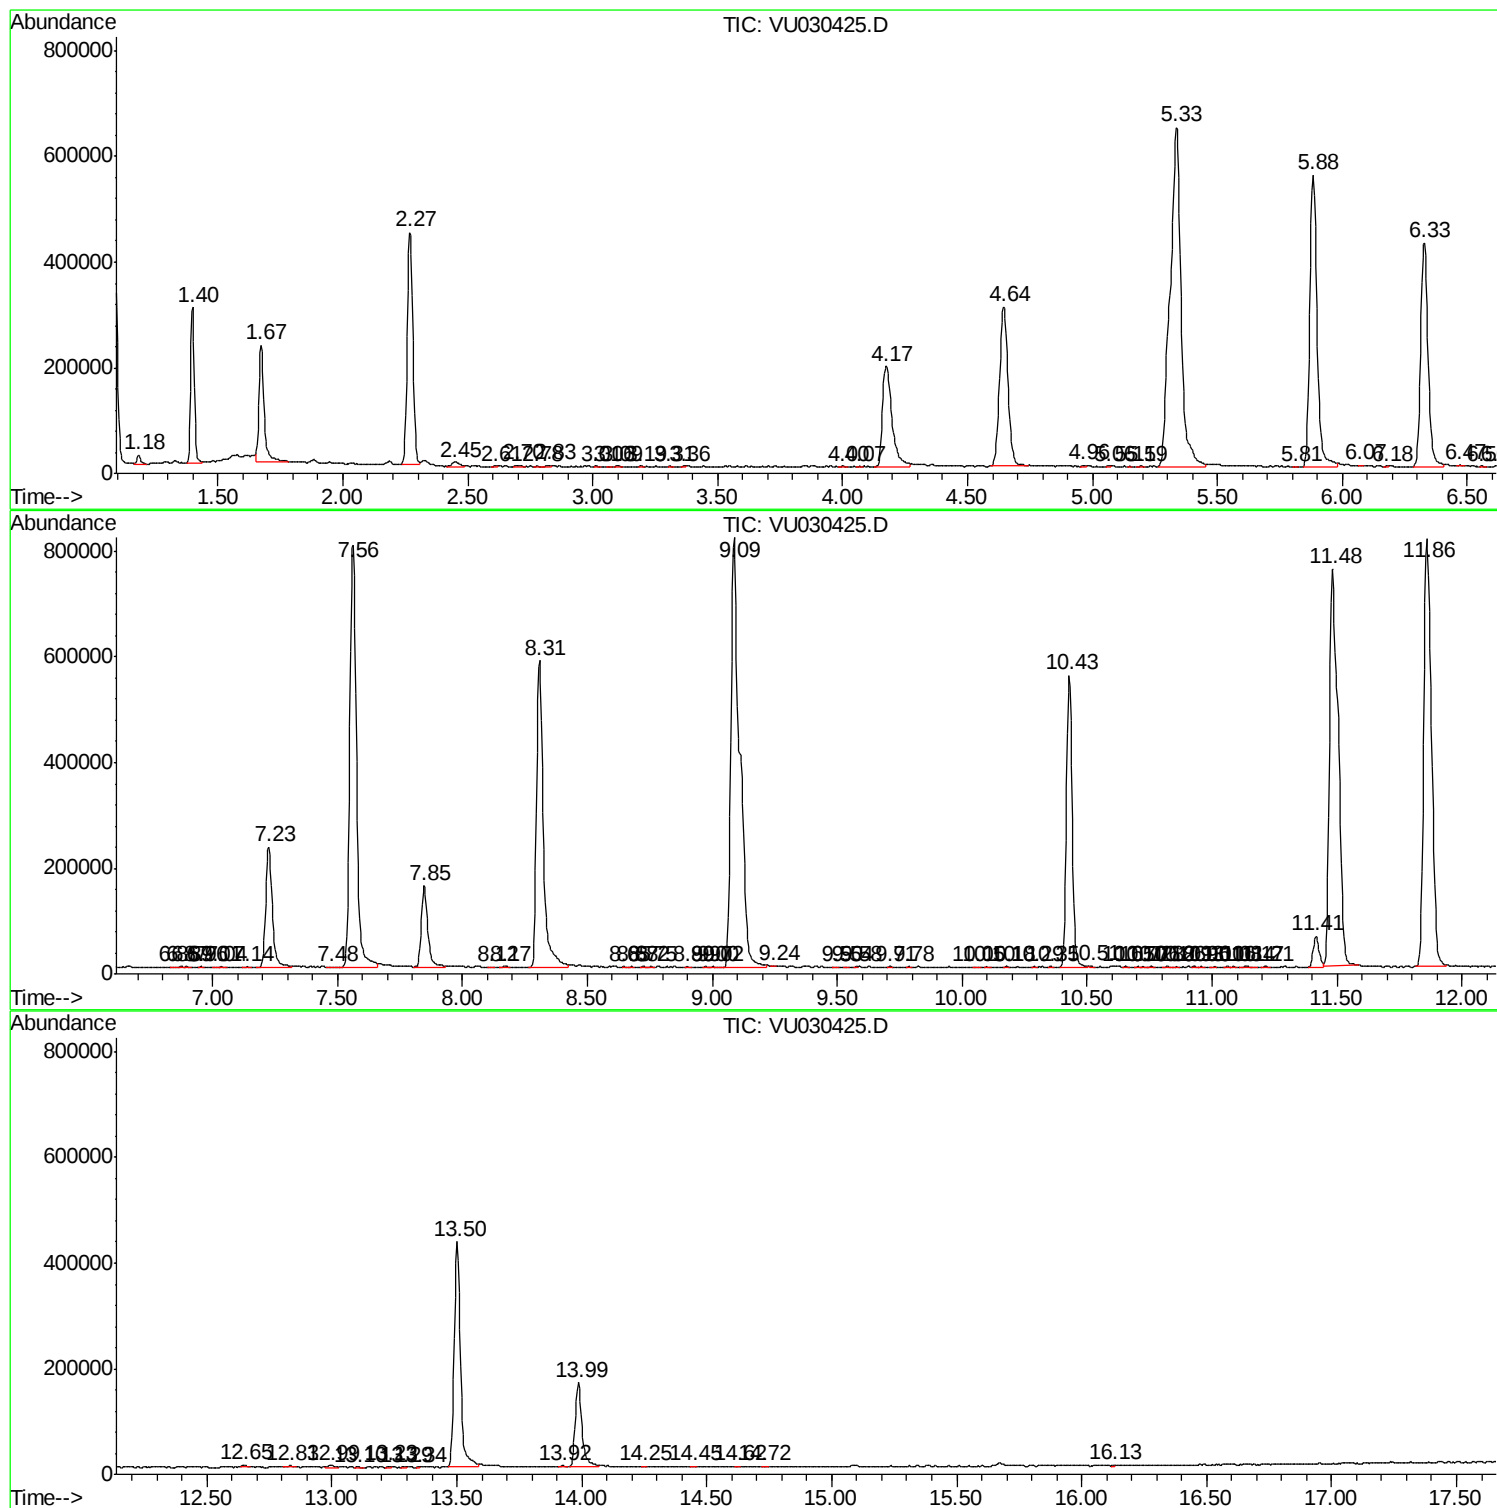

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032519\
Data File : VU030425.D
Acq On : 26 Mar 2019 00:13
Operator : JC/SP
Sample : K2070-11DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09D6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032519\
Data File : VU030425.D
Acq On : 26 Mar 2019 00:13
Operator : JC/SP
Sample : K2070-11DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09D6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc