

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032521\
 Data File : VU042778.D
 Acq On : 25 Mar 2021 12:31
 Operator : SY/MD
 Sample : PB1355334TB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PB1355334TB

Quant Time: Mar 26 02:04:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U032421W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 25 05:42:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.385	168	115060	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.256	114	182852	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.427	117	182679	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.822	152	85742	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.710	65	90756	49.48	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.96%	
35) Dibromofluoromethane	5.298	113	63434	46.48	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.96%	
50) Toluene-d8	7.906	98	229243	47.75	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.50%	
62) 4-Bromofluorobenzene	10.639	95	85511	45.83	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.66%	
Target Compounds						
					Qvalue	
5) Bromomethane	1.858	94	431	Below Cal	#	69
6) Chloroethane	1.932	64	44	Below Cal	#	43
10) Methyl Iodide	2.735	142	557	0.37	ug/l #	58
11) Tert butyl alcohol	3.198	59	1224	3.12	ug/l #	74
16) Acetone	2.636	43	20182	8.71	ug/l	99
17) Carbon Disulfide	2.800	76	709	0.24	ug/l #	75
18) Methyl Acetate	2.957	43	730	0.35	ug/l #	56
20) Methylene Chloride	3.057	84	6727	5.09	ug/l	95
25) 2-Butanone	4.719	43	5517	3.70	ug/l	95
29) Tetrahydrofuran	5.083	42	538	0.58	ug/l #	41
31) Cyclohexane	5.382	56	3105	1.36	ug/l #	29
36) 1,1-Dichloropropene	5.382	75	9218	5.10	ug/l #	50
38) Carbon Tetrachloride	5.382	117	11572	5.61	ug/l #	16
43) Isopropyl Acetate	5.919	43	14424	3.41	ug/l	99
45) 1,2-Dichloropropane	7.047	63	896	0.62	ug/l #	45
48) Methyl methacrylate	6.902	41	4783	2.34	ug/l #	17
49) 1,4-Dioxane	7.047	88	19	Below Cal	#	1
51) 4-Methyl-2-Pentanone	7.800	43	5337	1.80	ug/l	99
54) cis-1,3-Dichloropropene	7.745	75	17949	7.78	ug/l #	62
56) Ethyl methacrylate	8.095	69	2210	1.02	ug/l #	63
57) 1,3-Dichloropropane	8.735	76	11871	4.86	ug/l #	42
59) 2-Hexanone	8.735	43	214284	91.10	ug/l #	53
74) N-amyl acetate	10.330	43	964	0.31	ug/l #	69
76) 1,2,3-Trichloropropane	10.639	75	47801	21.92	ug/l #	37
81) trans-1,4-Dichloro-2-b...	10.639	75	47801	64.95	ug/l #	6
89) n-Butylbenzene	12.217	91	922	0.20	ug/l #	89
91) 1,2-Dichlorobenzene	12.221	146	628	0.23	ug/l	76
93) 1,2,4-Trichlorobenzene	13.848	180	1109	0.64	ug/l	88
94) Hexachlorobutadiene	14.028	225	241	0.24	ug/l #	42
95) Naphthalene	14.095	128	5010	3.39	ug/l	97
96) 1,2,3-Trichlorobenzene	14.339	180	1365	0.77	ug/l	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032521\
Data File : VU042778.D
Acq On : 25 Mar 2021 12:31
Operator : SY/MD
Sample : PB1355334TB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB

Quant Time: Mar 26 02:04:48 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U032421W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 25 05:42:00 2021
Response via : Initial Calibration




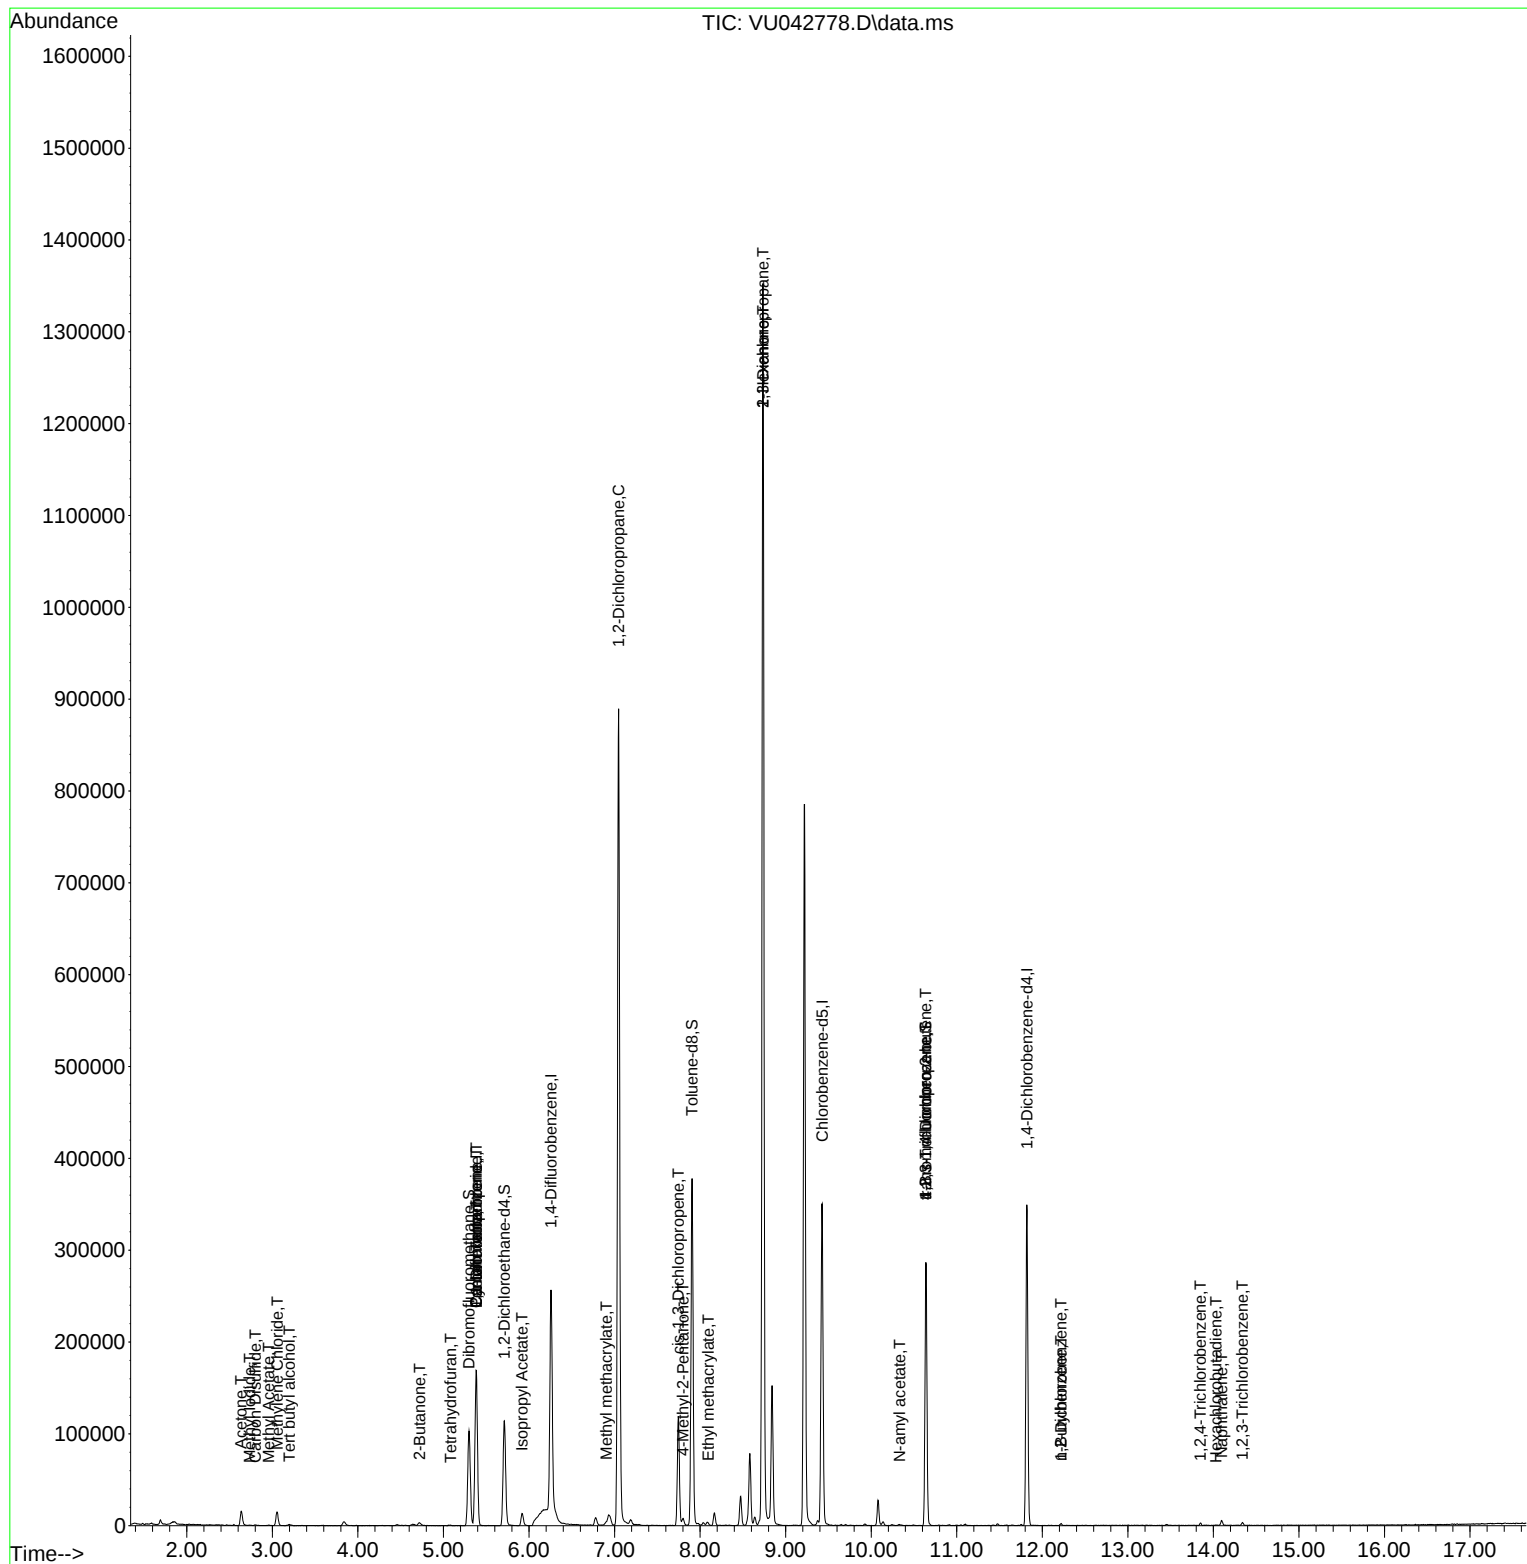




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.385 min Scan# 1258
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31




Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB


Tgt Ion:168 Resp: 115060
Ion Ratio Lower Upper
168 100
99 58.2 46.4 69.6

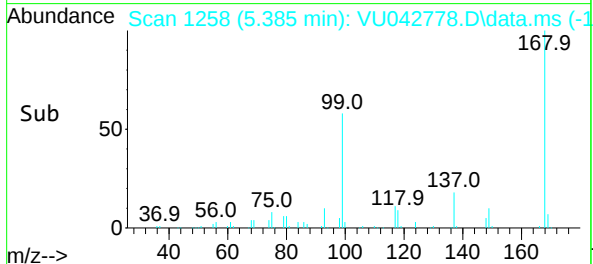

#5
Bromomethane
Concen: Below Cal
RT: 1.858 min Scan# 161
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Tgt Ion: 94 Resp: 431
Ion Ratio Lower Upper
94 100
96 66.2 77.1 115.7#


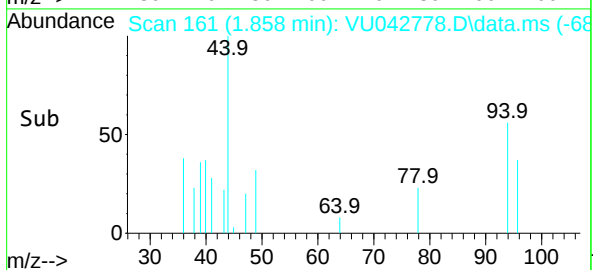

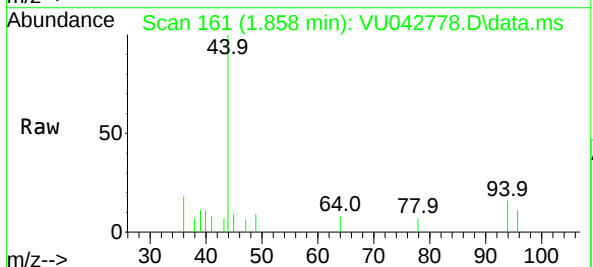




#6
Chloroethane
Concen: Below Cal
RT: 1.932 min Scan# 184
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31




Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB


Tgt Ion: 64 Resp: 44
Ion Ratio Lower Upper
64 100
66 0.0 25.0 37.6#



#10
Methyl Iodide
Concen: 0.37 ug/l
RT: 2.735 min Scan# 434
Delta R.T. 0.006 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Tgt Ion: 142 Resp: 557
Ion Ratio Lower Upper
142 100
127 18.9 38.7 58.1#
141 0.0 12.0 18.0#

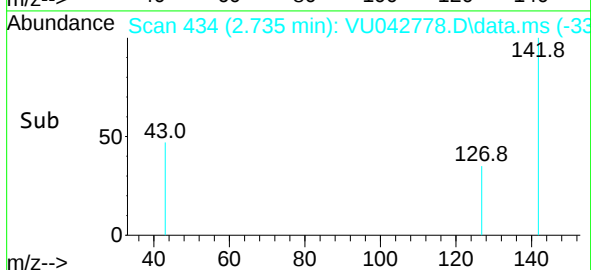







#11

Tert butyl alcohol
Concen: 3.12 ug/l
RT: 3.198 min Scan# 578
Delta R.T. -0.023 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB




Tgt Ion: 59 Resp: 1224
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#




#16

Acetone
Concen: 8.71 ug/l
RT: 2.636 min Scan# 403
Delta R.T. -0.003 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31


Tgt Ion: 43 Resp: 20182
Ion Ratio Lower Upper
43 100
58 26.6 21.6 32.4

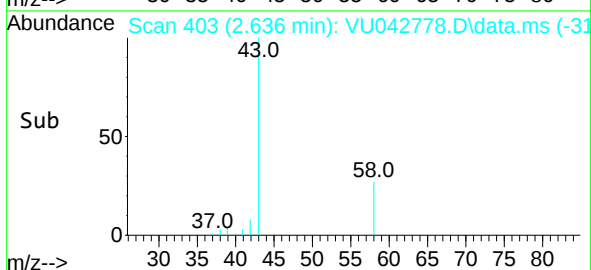






#17
Carbon Disulfide
Concen: 0.24 ug/l
RT: 2.800 min Scan# 454
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31


Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB

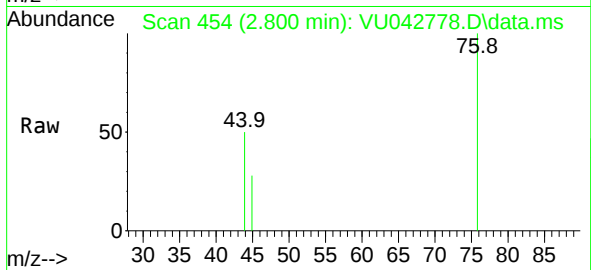



Tgt Ion: 76 Resp: 709
Ion Ratio Lower Upper
76 100
78 0.0 7.3 10.9#

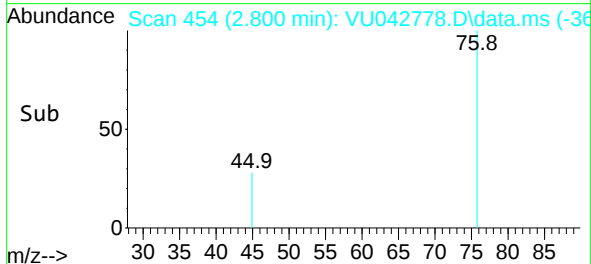


#18
Methyl Acetate
Concen: 0.35 ug/l
RT: 2.957 min Scan# 503
Delta R.T. 0.003 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

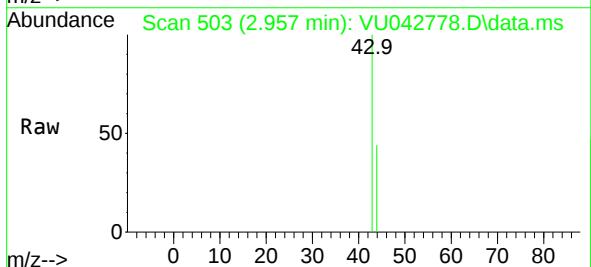

Tgt Ion: 43 Resp: 730
Ion Ratio Lower Upper
43 100
74 0.0 16.2 24.4#

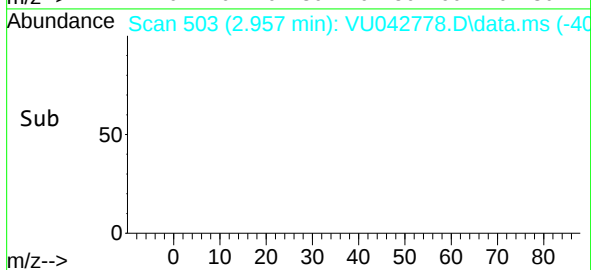



#20

Methylene Chloride

Concen: 5.09 ug/l

RT: 3.057 min Scan# 534

Delta R.T. 0.003 min





Lab File: VU042778.D

Acq: 25 Mar 2021 12:31

Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB

Tgt Ion: 84 Resp: 6727

Ion	Ratio	Lower	Upper
84	100		
49	147.9	113.0	169.4
51	43.2	32.9	49.3
86	67.6	50.5	75.7

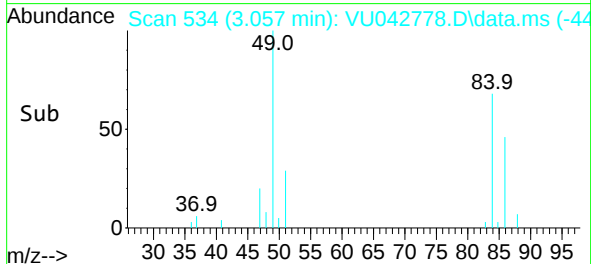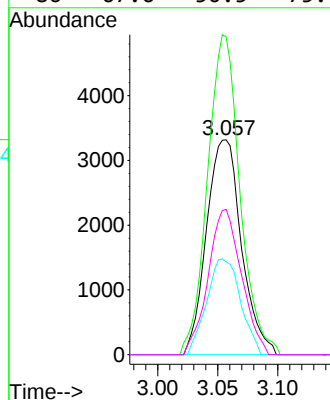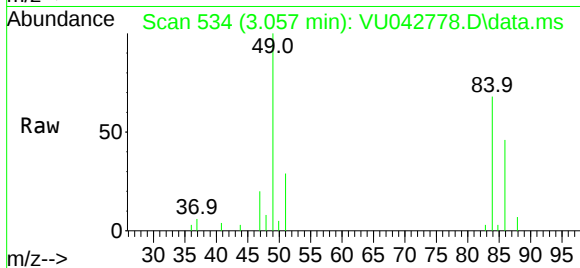

#25

2-Butanone

Concen: 3.70 ug/l

RT: 4.719 min Scan# 1051




Delta R.T. 0.006 min


Lab File: VU042778.D

Acq: 25 Mar 2021 12:31

Tgt Ion: 43 Resp: 5517

Ion	Ratio	Lower	Upper
43	100		
72	19.6	17.7	26.5

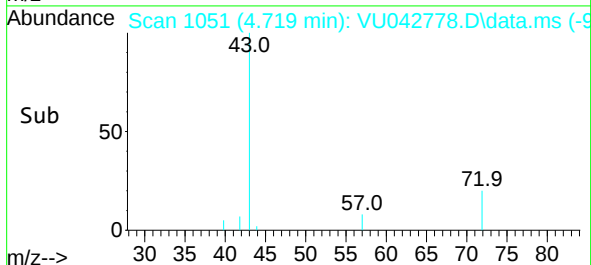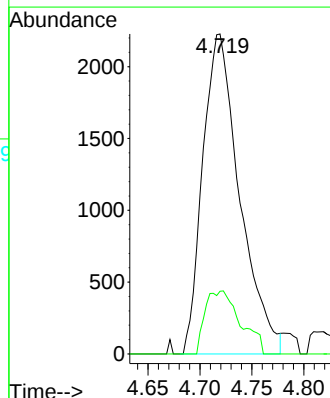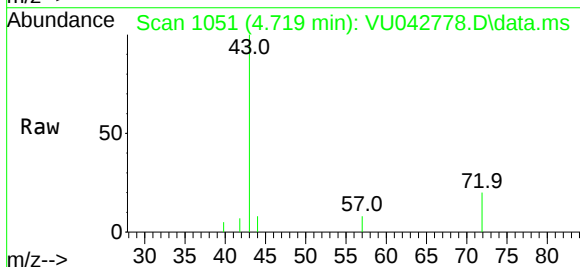



#29

Tetrahydrofuran

Concen: 0.58 ug/l

RT: 5.083 min Scan# 1164





Delta R.T. 0.022 min

Lab File: VU042778.D

Acq: 25 Mar 2021 12:31

Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB

Tgt Ion: 42	Resp: 538
Ion Ratio	Lower Upper
42 100	
72 3.5	30.2 45.4#
71 0.0	28.6 42.8#

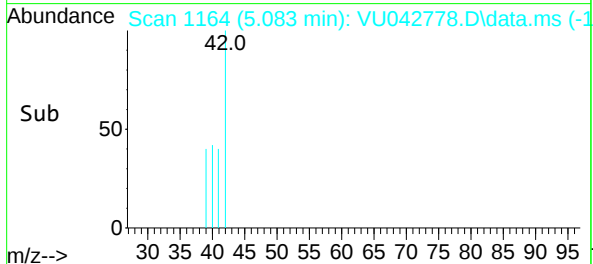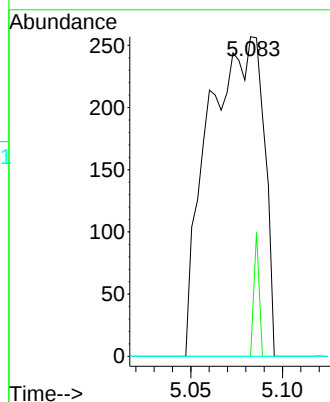

#31

Cyclohexane

Concen: 1.36 ug/l




RT: 5.382 min Scan# 1257


Delta R.T. -0.016 min

Lab File: VU042778.D

Acq: 25 Mar 2021 12:31

Tgt Ion: 56	Resp: 3105		
Ion Ratio	Lower	Upper	
56 100			
69 142.2	23.3	34.9#	
84 94.1	62.2	93.4#	

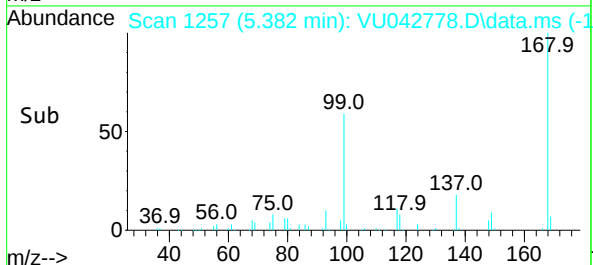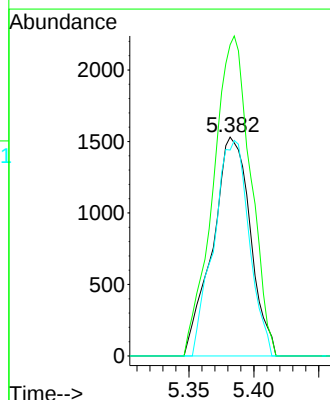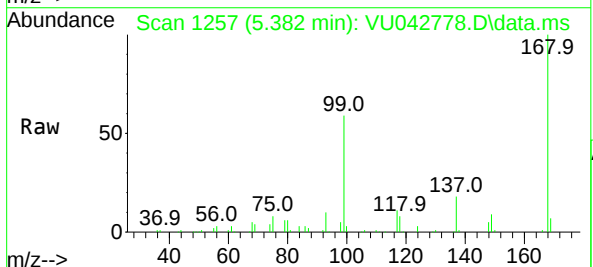



#33

1,2-Dichloroethane-d4

Concen: 49.48 ug/l

RT: 5.710 min Scan# 1359

Delta R.T. -0.000 min

Lab File: VU042778.D

Acq: 25 Mar 2021 12:31

Tgt Ion: 65 Resp: 90756

Ion Ratio Lower Upper

65 100





67 49.7 0.0 98.8

Instrument :

MSVOA_U

ClientSampleId :

PB1355334TB

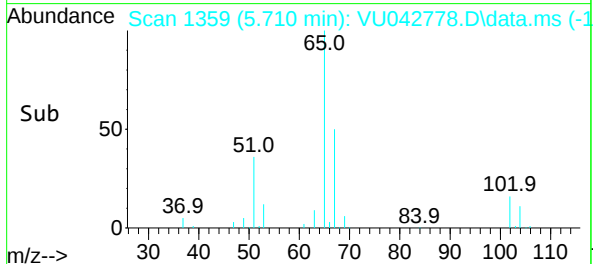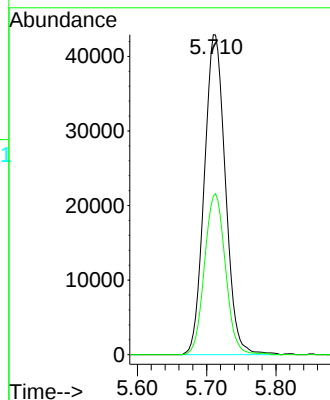

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.256 min Scan# 1529

Delta R.T. -0.004 min

Lab File: VU042778.D

Acq: 25 Mar 2021 12:31




Tgt Ion: 114 Resp: 182852


Ion Ratio Lower Upper

114 100

63 22.9 0.0 46.8


88 15.3 0.0 32.2

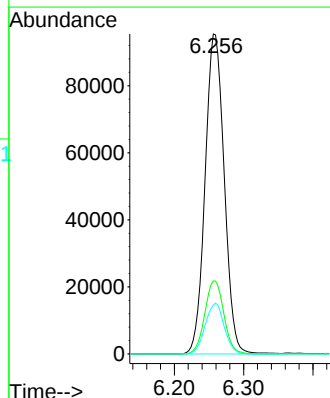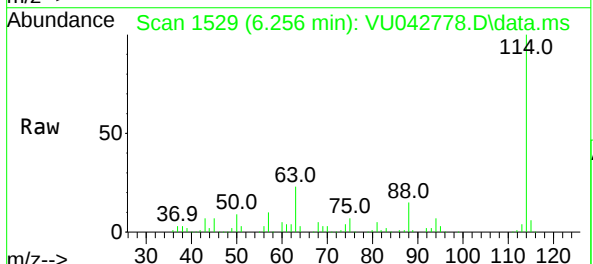






#35
Dibromofluoromethane
Concen: 46.48 ug/l
RT: 5.298 min Scan# 1231
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31


Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB





Tgt Ion:113 Resp: 63434
Ion Ratio Lower Upper
113 100
111 102.5 82.1 123.1
192 21.5 17.6 26.4




#36
1,1-Dichloropropene
Concen: 5.10 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.155 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

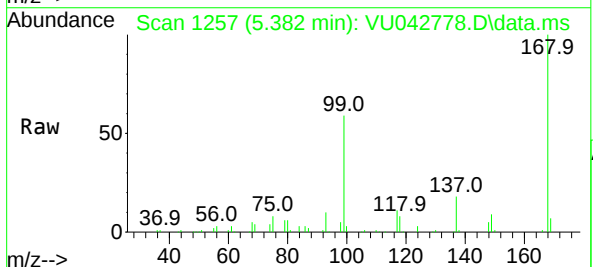


Tgt Ion: 75 Resp: 9218
Ion Ratio Lower Upper
75 100
110 8.0 16.6 49.7#
77 0.0 24.7 37.1#








#38
Carbon Tetrachloride
Concen: 5.61 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.151 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB







Tgt Ion:117 Resp: 11572
Ion Ratio Lower Upper
117 100
119 4.4 75.2 112.8#
121 0.0 24.2 36.4#

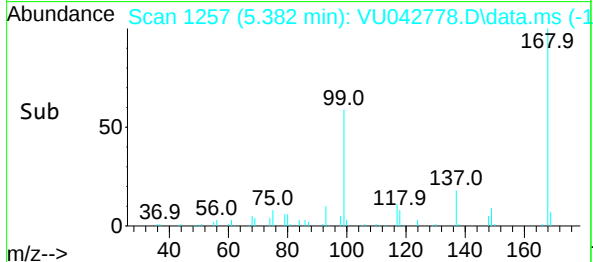

#43
Isopropyl Acetate
Concen: 3.41 ug/l
RT: 5.919 min Scan# 1424
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Tgt Ion: 43 Resp: 14424
Ion Ratio Lower Upper
43 100
61 16.5 13.4 20.0
87 10.0 8.7 13.1


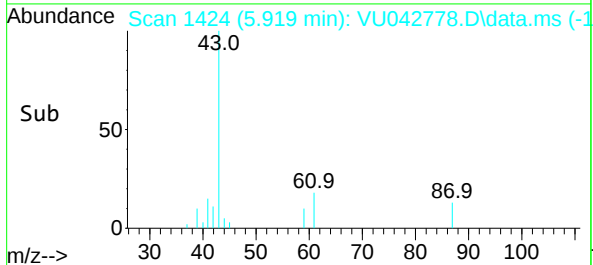

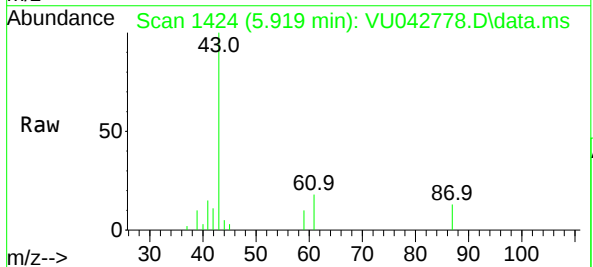




#45
1,2-Dichloropropane
Concen: 0.62 ug/l
RT: 7.047 min Scan# 1775
Delta R.T. 0.247 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31




Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB


Tgt Ion: 63 Resp: 896
Ion Ratio Lower Upper
63 100
65 0.0 23.5 35.3#

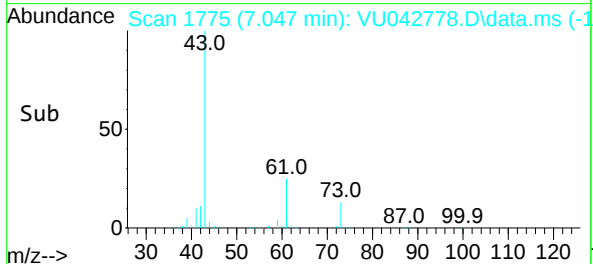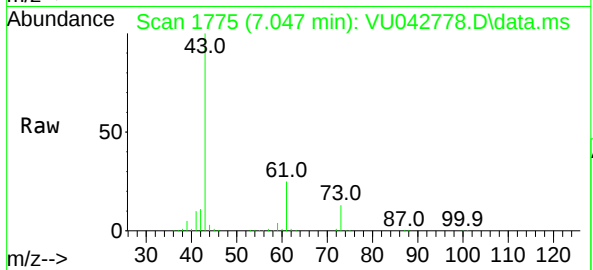

#48
Methyl methacrylate
Concen: 2.34 ug/l
RT: 6.902 min Scan# 1730
Delta R.T. -0.065 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Tgt Ion: 41 Resp: 4783
Ion Ratio Lower Upper
41 100
69 0.0 55.9 83.9#
39 0.0 49.7 74.5#


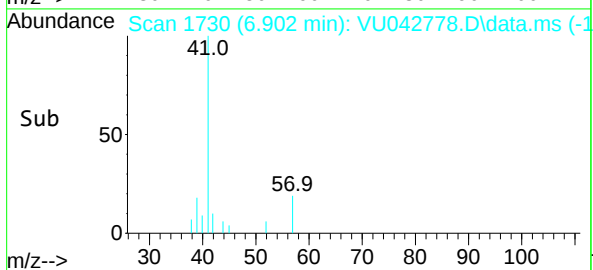

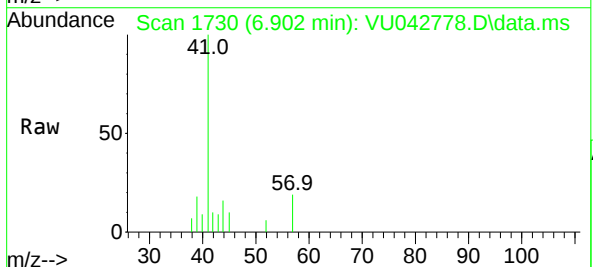




#49
1,4-Dioxane
Concen: Below Cal
RT: 7.047 min Scan# 1775
Delta R.T. 0.048 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31




Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB


Tgt Ion: 88 Resp: 19
Ion Ratio Lower Upper
88 100
43 4505157.9 25.4 38.0#
58 18236.8 62.5 93.7#

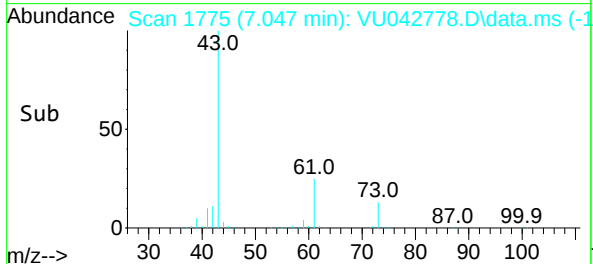

#50
Toluene-d8
Concen: 47.75 ug/l
RT: 7.906 min Scan# 2042
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Tgt Ion: 98 Resp: 229243
Ion Ratio Lower Upper
98 100
100 64.0 50.4 75.6


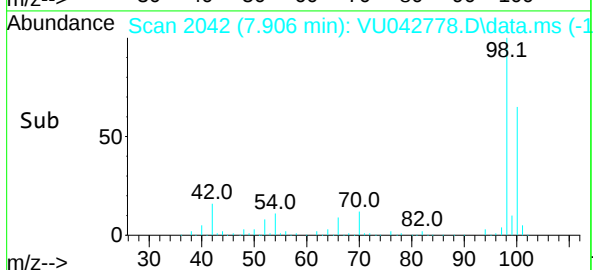






#51
4-Methyl-2-Pentanone
Concen: 1.80 ug/l
RT: 7.800 min Scan# 2009
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31




Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB


Tgt Ion: 43 Resp: 5337
Ion Ratio Lower Upper
43 100
58 33.6 27.4 41.2

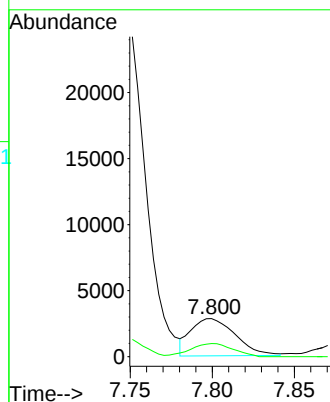

#54
cis-1,3-Dichloropropene
Concen: 7.78 ug/l
RT: 7.745 min Scan# 1992
Delta R.T. 0.128 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Tgt Ion: 75 Resp: 17949
Ion Ratio Lower Upper
75 100
77 0.0 24.8 37.2#
39 39.1 49.2 73.8#


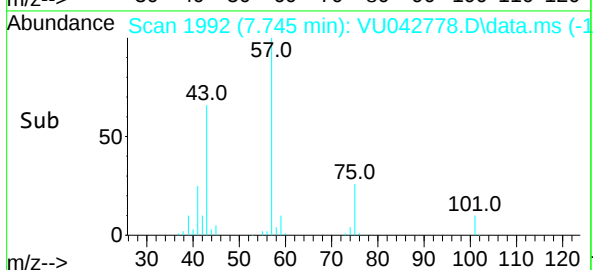
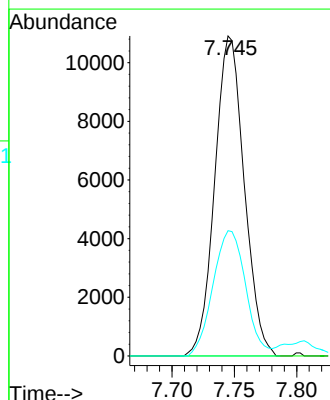





#56
Ethyl methacrylate
Concen: 1.02 ug/l
RT: 8.095 min Scan# 2101
Delta R.T. -0.245 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31




Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB


Tgt Ion: 69 Resp: 2210
Ion Ratio Lower Upper
69 100
41 29.6 64.6 97.0#
39 45.7 38.2 57.2

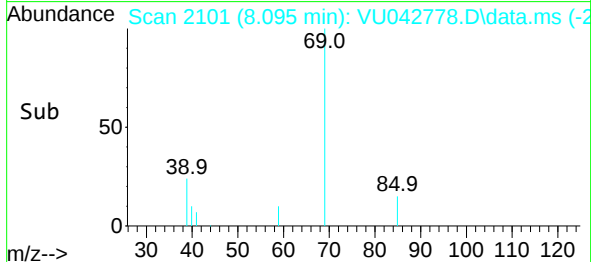

#57
1,3-Dichloropropane
Concen: 4.86 ug/l
RT: 8.735 min Scan# 2300
Delta R.T. 0.151 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Tgt Ion: 76 Resp: 11871
Ion Ratio Lower Upper
76 100
78 0.0 25.9 38.9#


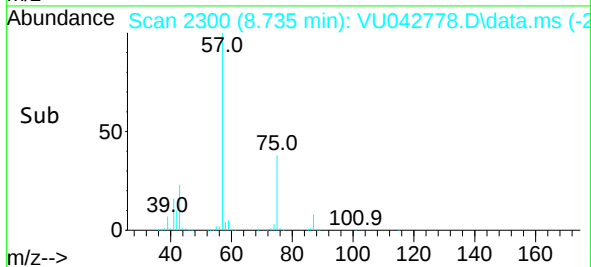

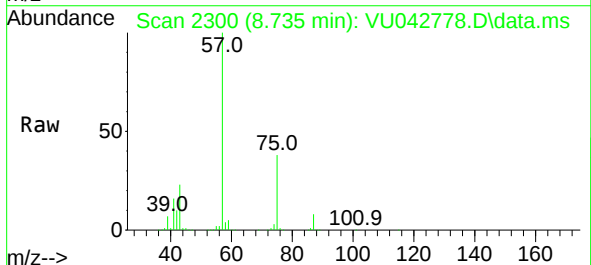




#59
2-Hexanone
Concen: 91.10 ug/l
RT: 8.735 min Scan# 2300
Delta R.T. 0.042 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31




Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB


Tgt Ion: 43 Resp: 214284
Ion Ratio Lower Upper
43 100
58 16.0 23.8 71.2#

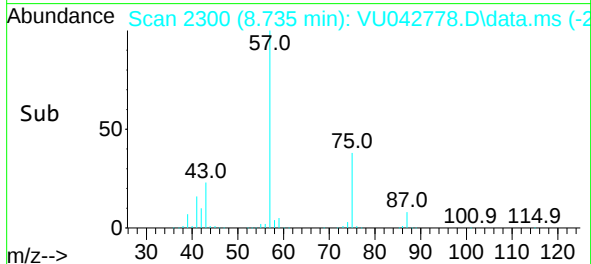

#62
4-Bromofluorobenzene
Concen: 45.83 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Tgt Ion: 95 Resp: 85511
Ion Ratio Lower Upper
95 100
174 87.9 0.0 175.2
176 83.6 0.0 167.4


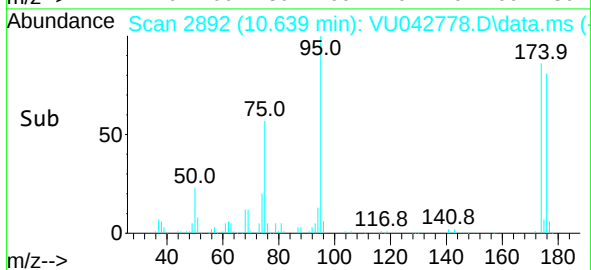

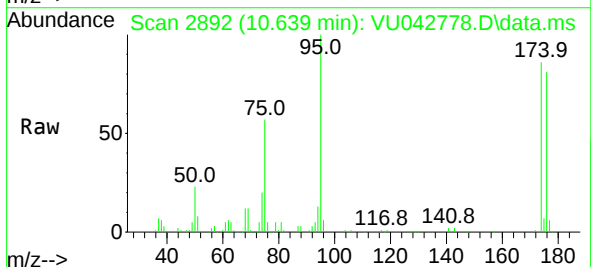




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 9.427 min Scan# 2515
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31




Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB


Tgt Ion:117 Resp: 182679
Ion Ratio Lower Upper
117 100
82 58.2 45.5 68.3
119 31.6 26.2 39.4

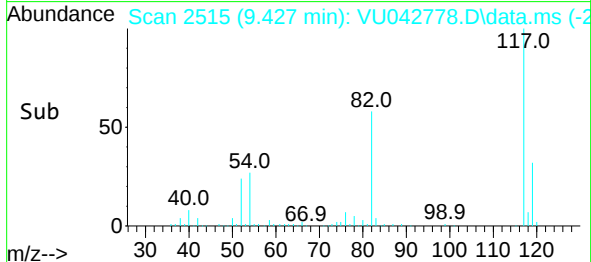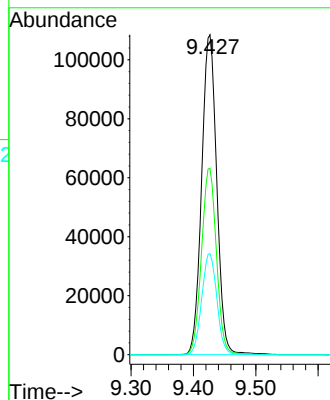

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 11.822 min Scan# 3260
Delta R.T. 0.003 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Tgt Ion:152 Resp: 85742
Ion Ratio Lower Upper
152 100
115 57.6 41.0 123.0
150 155.6 0.0 341.0


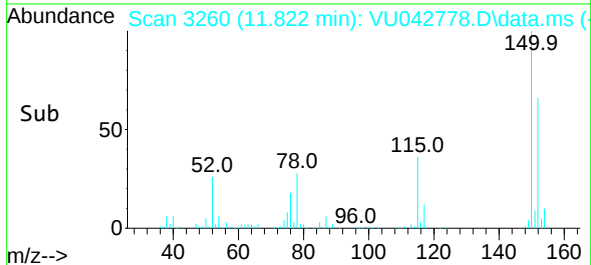
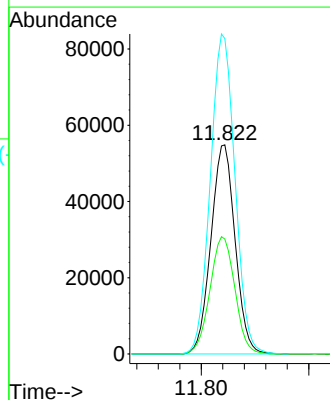
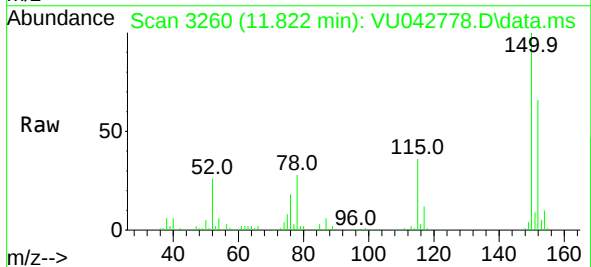




#74
N-amy1 acetate
Concen: 0.31 ug/l
RT: 10.330 min Scan# 2796
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31




Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB


Tgt Ion: 43	Resp: 964
Ion Ratio	Lower Upper
43 100	
70 17.7	27.8 41.6#
55 12.1	18.4 27.6#
61 0.0	16.4 24.6#

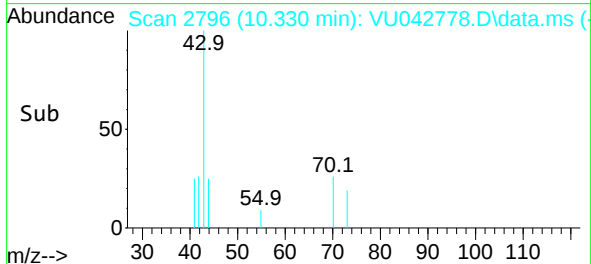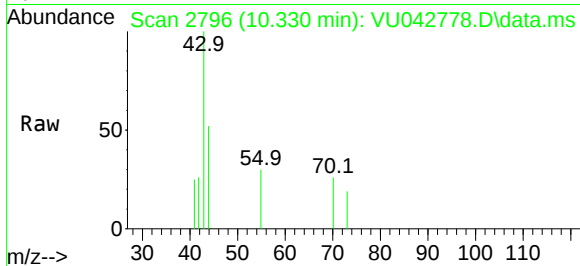

#76
1,2,3-Trichloropropane
Concen: 21.92 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.193 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31


Tgt Ion: 75	Resp: 47801
Ion Ratio	Lower Upper
75 100	
77 0.9	19.6 58.8#

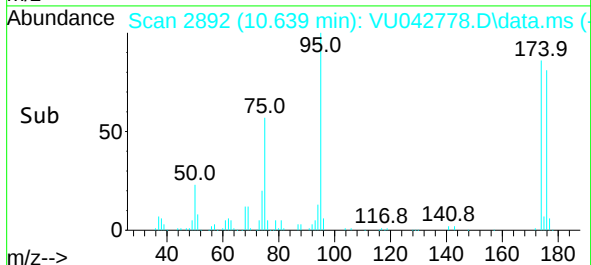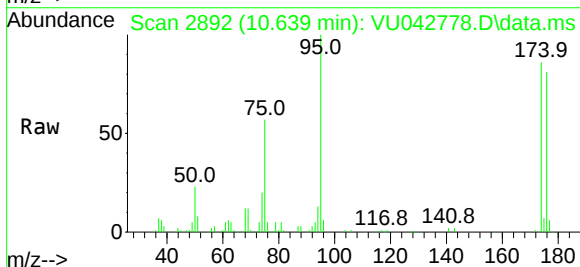






#81
trans-1,4-Dichloro-2-butene
Concen: 64.95 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.083 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB



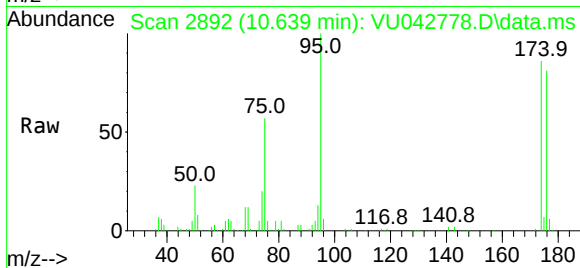



Tgt Ion: 75 Resp: 47801
Ion Ratio Lower Upper
75 100
53 0.0 88.3 132.5#
89 0.0 35.7 53.5#



#89
n-Butylbenzene
Concen: 0.20 ug/l
RT: 12.217 min Scan# 3383
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

Tgt Ion: 91 Resp: 922
Ion Ratio Lower Upper
91 100
92 50.7 25.7 77.1
134 8.9 12.1 36.3#


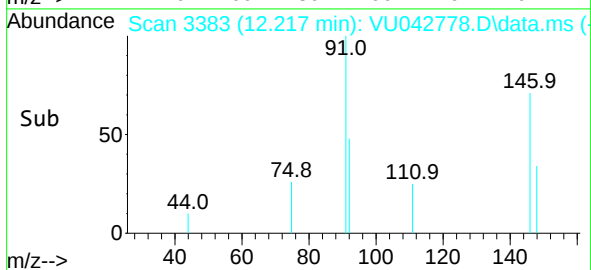

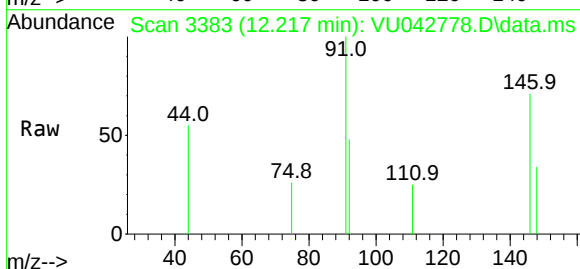




#91
1,2-Dichlorobenzene
Concen: 0.23 ug/l
RT: 12.221 min Scan# 3384
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31




Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB


Tgt Ion:146 Resp: 628
Ion Ratio Lower Upper
146 100
111 29.9 20.0 60.0
148 42.4 32.5 97.4

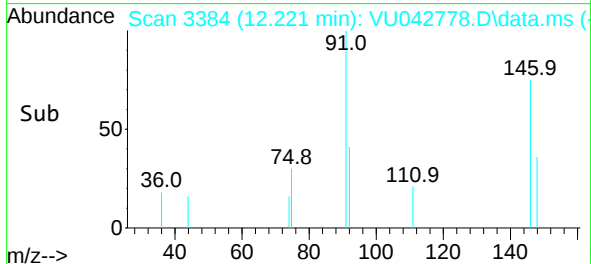

#93
1,2,4-Trichlorobenzene
Concen: 0.64 ug/l
RT: 13.848 min Scan# 3890
Delta R.T. -0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31


Tgt Ion:180 Resp: 1109
Ion Ratio Lower Upper
180 100
182 87.0 48.0 144.0
145 18.5 14.5 43.5

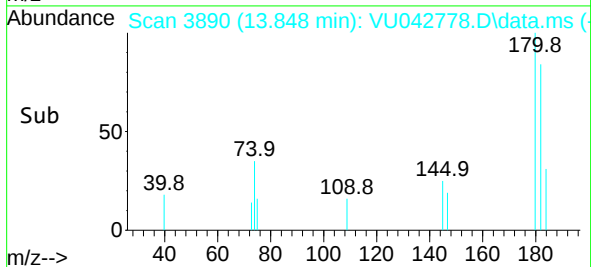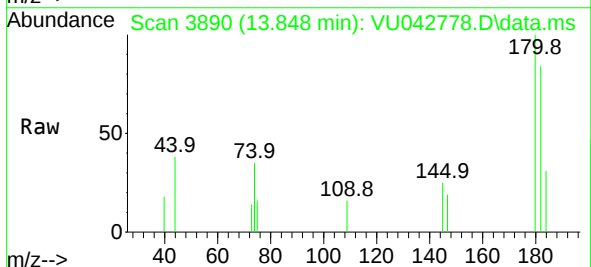






#94
Hexachlorobutadiene
Concen: 0.24 ug/l
RT: 14.028 min Scan# 3946
Delta R.T. -0.003 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31


Instrument :
MSVOA_U
ClientSampleId :
PB1355334TB

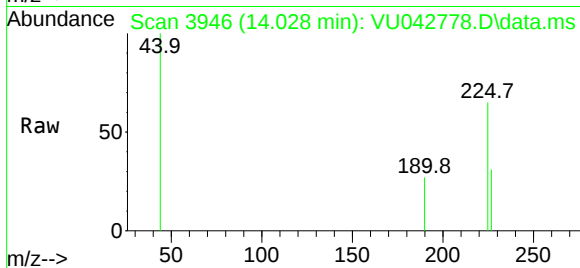



Tgt Ion	Ratio	Lower	Upper
225	100		
223	17.8	31.4	94.3#
227	18.7	31.9	95.5#

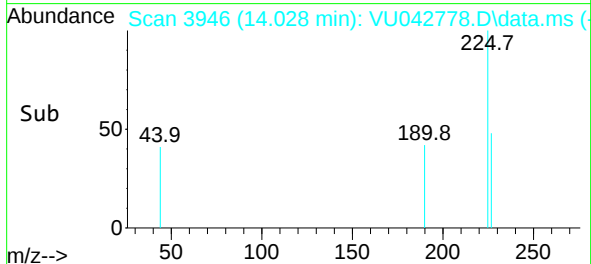


#95
Naphthalene
Concen: 3.39 ug/l
RT: 14.095 min Scan# 3967
Delta R.T. 0.000 min
Lab File: VU042778.D
Acq: 25 Mar 2021 12:31

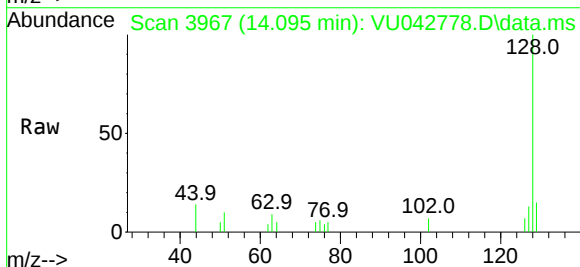

Tgt Ion	Ratio	Lower	Upper
128	100		
127	11.4	10.9	16.3
129	11.1	8.7	13.1

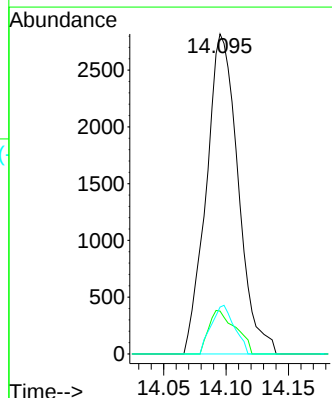

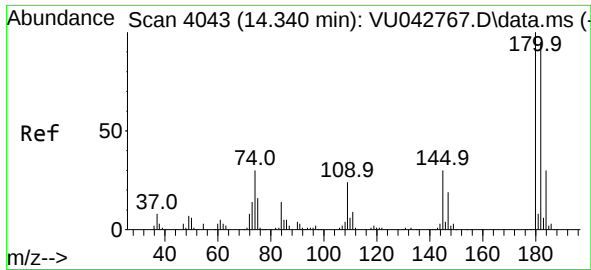

#96
 1,2,3-Trichlorobenzene
 Concen: 0.77 ug/l
 RT: 14.339 min Scan# 4043
 Delta R.T. -0.000 min
 Lab File: VU042778.D
 Acq: 25 Mar 2021 12:31

Instrument :
 MSVOA_U
 ClientSampleId :
 PB1355334TB

Tgt Ion:180 Resp: 1365
 Ion Ratio Lower Upper
 180 100
 182 86.1 47.5 142.6
 145 21.9 15.0 45.0

