
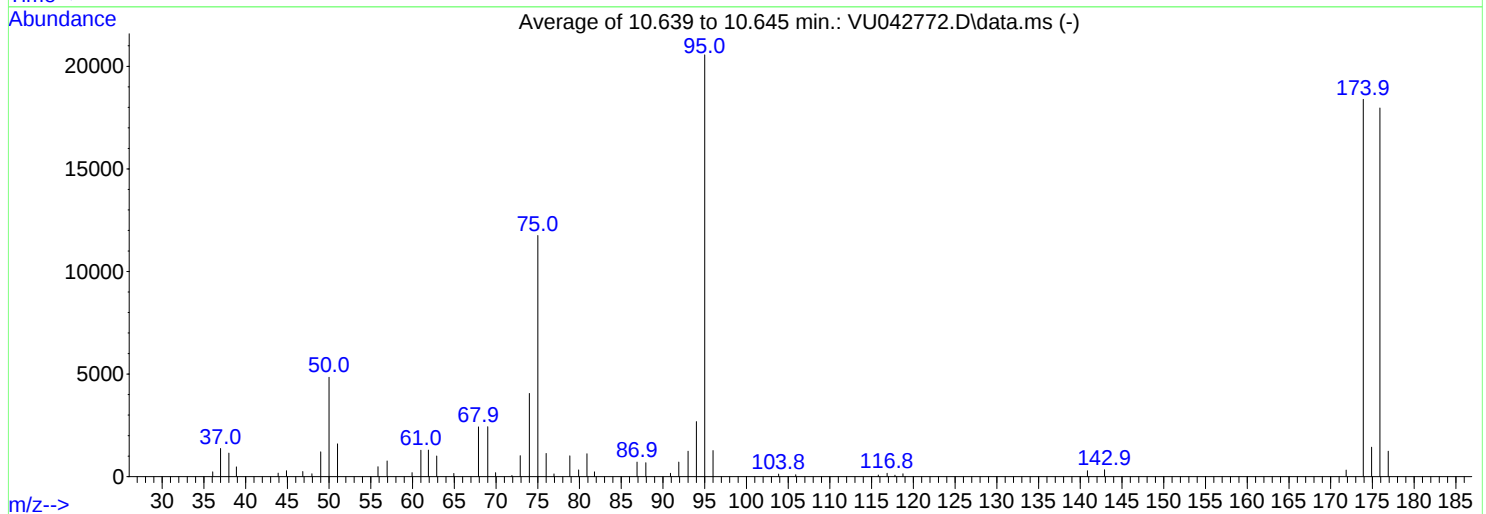


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032521\
Data File : VU042772.D
Acq On : 25 Mar 2021 08:54
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U032421W.M
Title : SW846 8260
Last Update : Thu Mar 25 05:42:00 2021

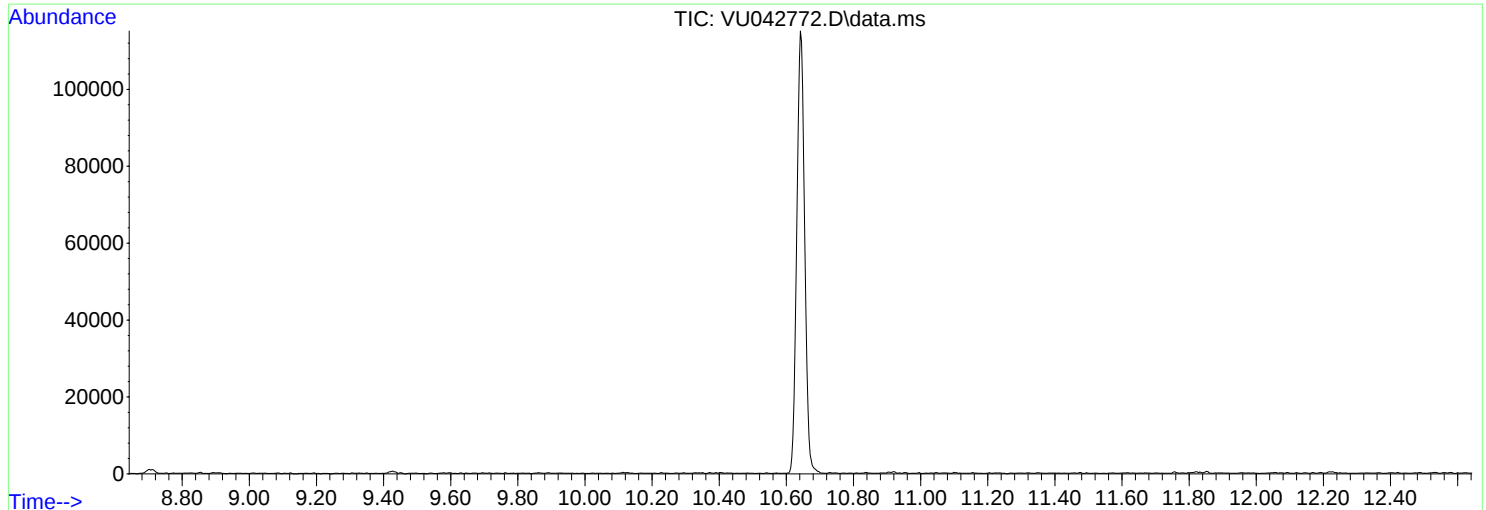

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2880

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.6	4842	PASS
75	95	30	60	57.2	11753	PASS
95	95	100	100	100.0	20560	PASS
96	95	5	9	6.2	1272	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.4	18389	PASS
175	174	5	9	7.8	1433	PASS
176	174	95	101	97.7	17971	PASS
177	176	5	9	6.9	1241	PASS