

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047668.D
 Acq On : 25 Mar 2022 12:34
 Operator : SY/MD
 Sample : N2081-02DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X1DL

Quant Time: Mar 26 02:08:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 26 02:04:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	92985	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	98498	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	56117	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	60027	89.022	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	= 178.040%#	
7) Chloroethane-d5	1.919	69	48944	92.055	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	= 184.120%#	
11) 1,1-Dichloroethene-d2	2.571	63	80482	65.237	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 130.480%#	
21) 2-Butanone-d5	4.639	46	111315	192.333	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	= 192.330%#	
24) Chloroform-d	5.067	84	108797	88.182	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 176.360%#	
26) 1,2-Dichloroethane-d4	5.703	65	70753	93.502	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 187.000%#	
32) Benzene-d6	5.729	84	220967	89.154	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 178.300%#	
36) 1,2-Dichloropropane-d6	6.694	67	68008	89.347	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	= 178.700%#	
41) Toluene-d8	7.899	98	200951	83.217	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 166.440%#	
43) trans-1,3-Dichloroprop...	8.182	79	32734	84.886	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 169.780%#	
47) 2-Hexanone-d5	8.639	63	78843	176.942	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	= 176.940%#	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	111117	85.063	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	= 170.120%#	
66) 1,2-Dichlorobenzene-d4	12.195	152	86645	86.786	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 173.580%#	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.607	62	1041	1.238	ug/L #	1
8) Chloroethane	1.938	64	7079	13.412	ug/L	97
19) 1,1-Dichloroethane	3.874	63	13271	11.185	ug/L	98
20) cis-1,2-Dichloroethene	4.671	96	11995	15.904	ug/L	97
30) 1,1,1-Trichloroethane	5.321	97	28918	25.892	ug/L	98
42) Toluene	7.970	91	5008	1.601	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047668.D
Acq On : 25 Mar 2022 12:34
Operator : SY/MD
Sample : N2081-02DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X1DL

Quant Time: Mar 26 02:08:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 26 02:04:39 2022
Response via : Initial Calibration




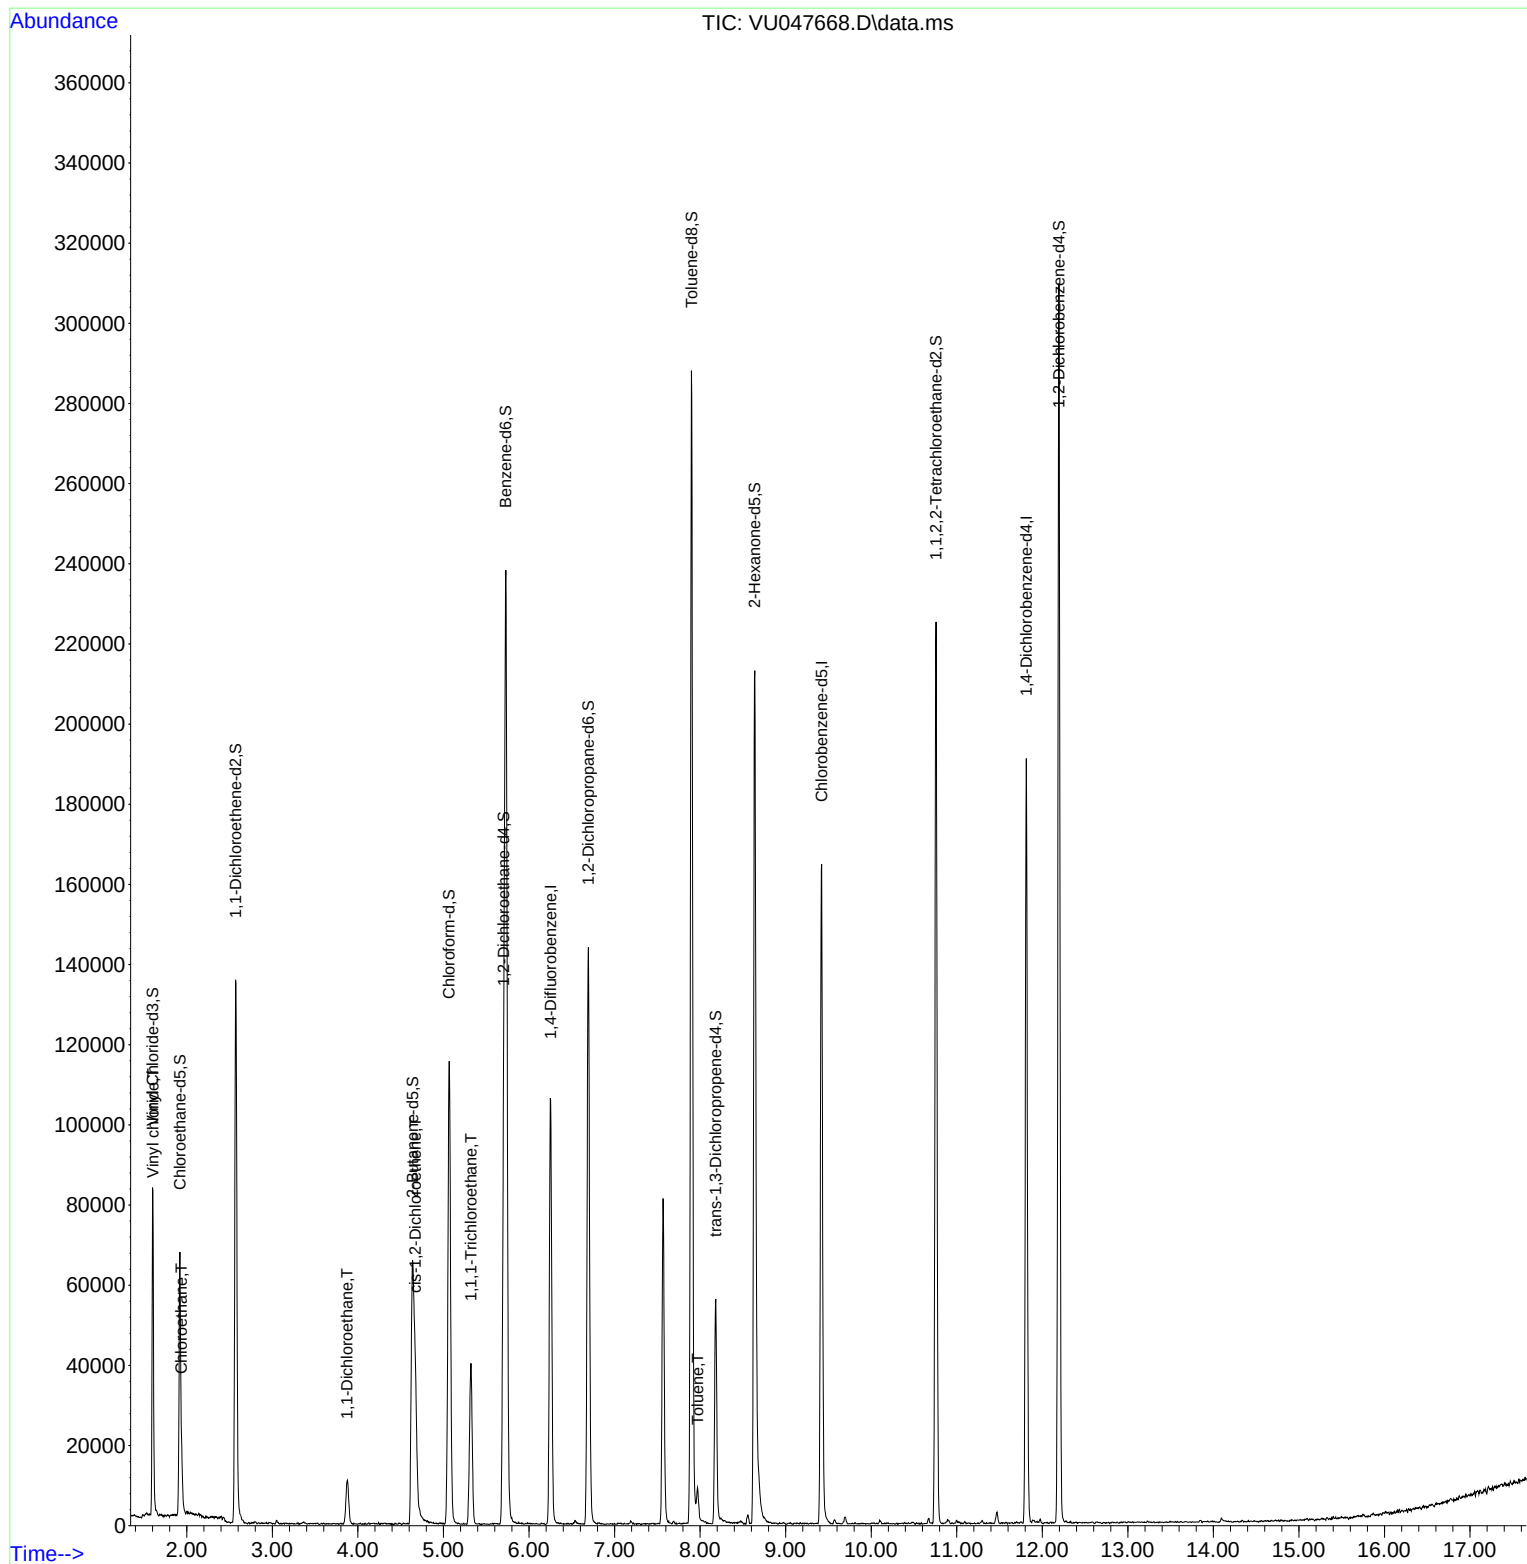


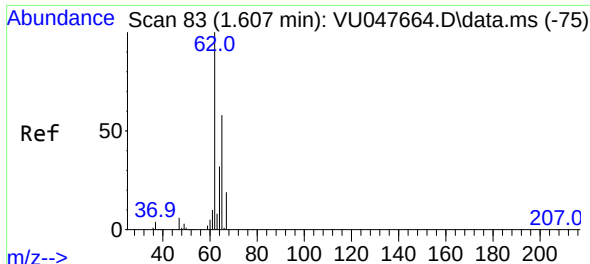

#5
 Vinyl chloride
 Concen: 1.238 ug/L
 RT: 1.607 min Scan# 83
 Delta R.T. 0.000 min
 Lab File: VU047668.D
 Acq: 25 Mar 2022 12:34




Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X1DL


Tgt Ion: 62 Resp: 1041
 Ion Ratio Lower Upper
 62 100
 64 97.7 23.7 43.9#

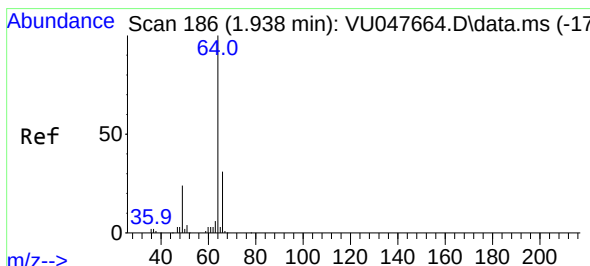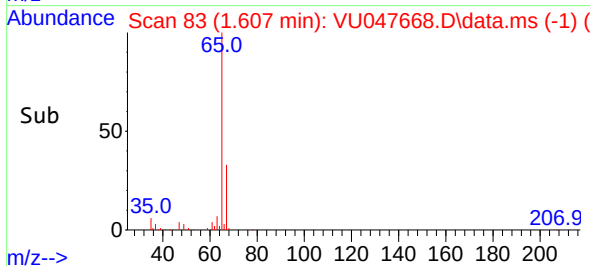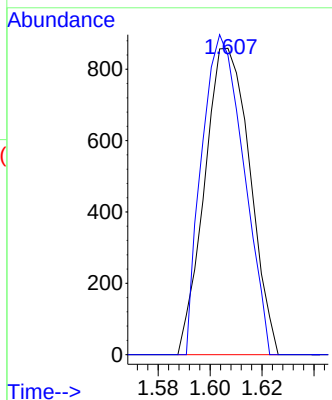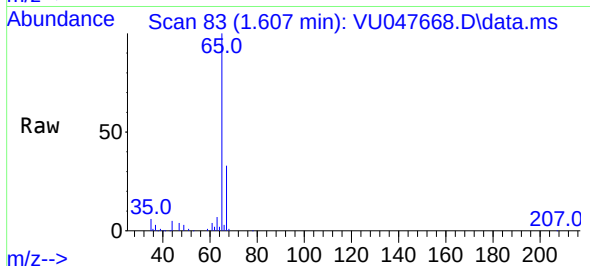

#8
 Chloroethane
 Concen: 13.412 ug/L
 RT: 1.938 min Scan# 186
 Delta R.T. 0.000 min
 Lab File: VU047668.D
 Acq: 25 Mar 2022 12:34

Tgt Ion: 64 Resp: 7079
 Ion Ratio Lower Upper
 64 100
 66 34.8 23.3 43.3

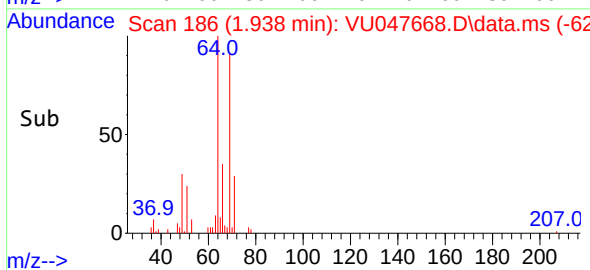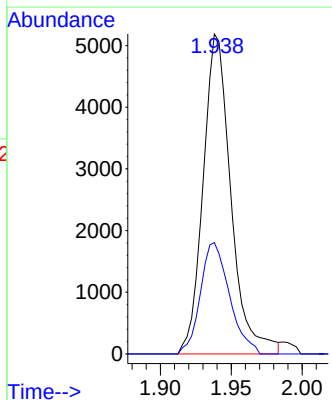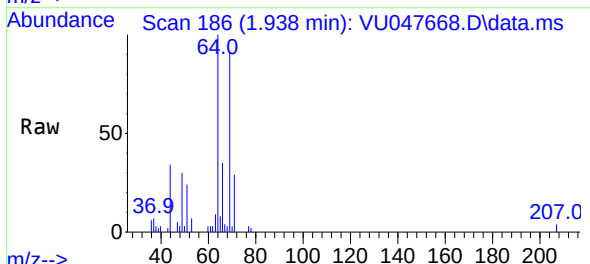

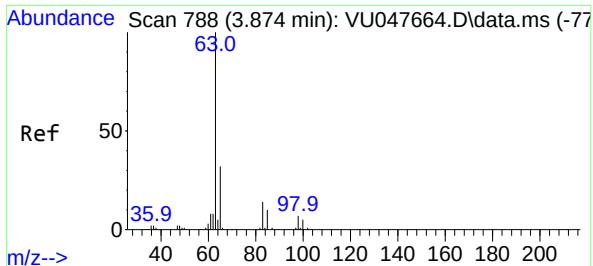

#19

1,1-Dichloroethane

Concen: 11.185 ug/L

RT: 3.874 min Scan# 788

Delta R.T. 0.000 min

Lab File: VU047668.D

Acq: 25 Mar 2022 12:34

Instrument :

MSVOA_U

ClientSampleId :

EW5X1DL





Tgt Ion: 63 Resp: 13271

Ion Ratio Lower Upper

63 100

65 30.8 22.0 41.0

83 12.0 9.7 18.1

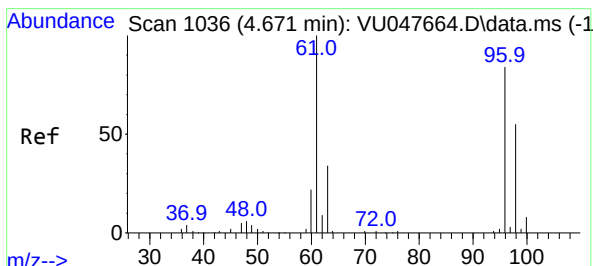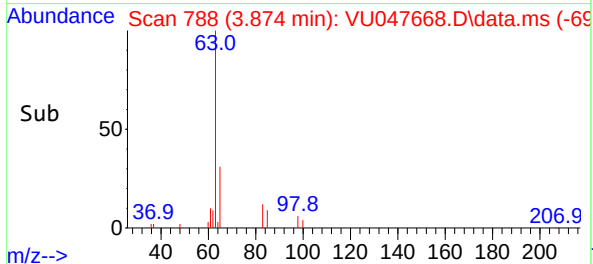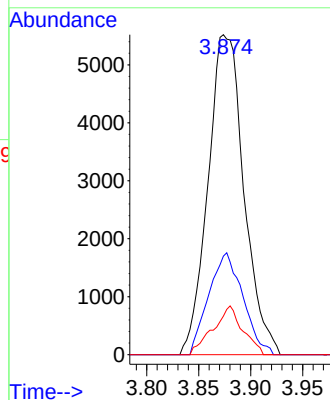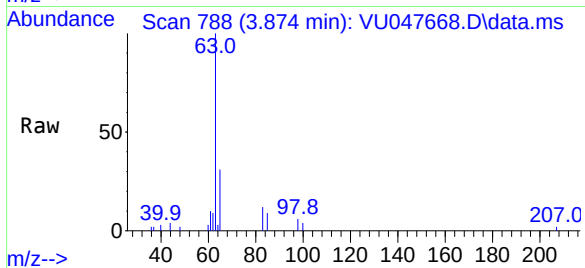

#20

cis-1,2-Dichloroethene

Concen: 15.904 ug/L

RT: 4.671 min Scan# 1036

Delta R.T. 0.000 min

Lab File: VU047668.D

Acq: 25 Mar 2022 12:34




Tgt Ion: 96 Resp: 11995


Ion Ratio Lower Upper

96 100

61 112.4 80.7 149.9

68 0.0 0.0 0.0


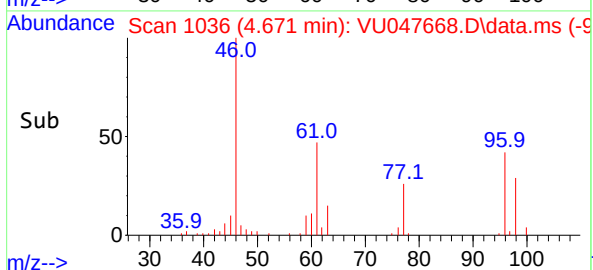
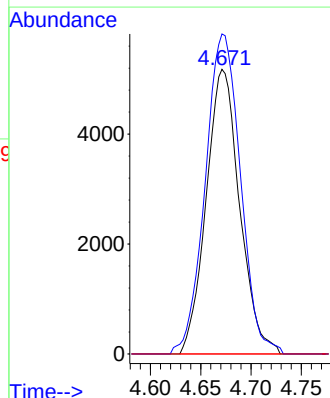
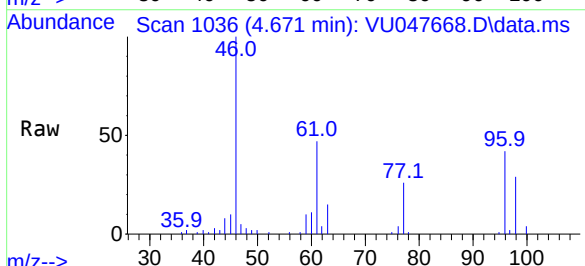


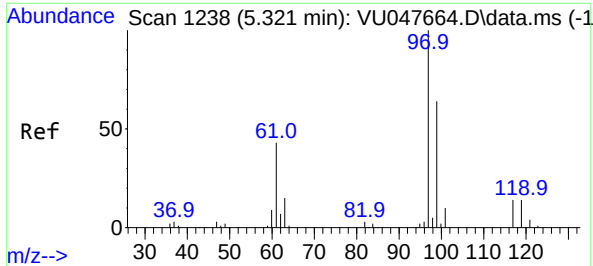

#30
1,1,1-Trichloroethane
Concen: 25.892 ug/L
RT: 5.321 min Scan# 11
Delta R.T. 0.000 min
Lab File: VU047668.D
Acq: 25 Mar 2022 12:34

Instrument :
MSVOA_U
ClientSampleId :
EW5X1DL

Tgt Ion: 97 Resp: 28918
Ion Ratio Lower Upper
97 100
99 66.4 51.6 77.4
61 43.3 34.2 51.4

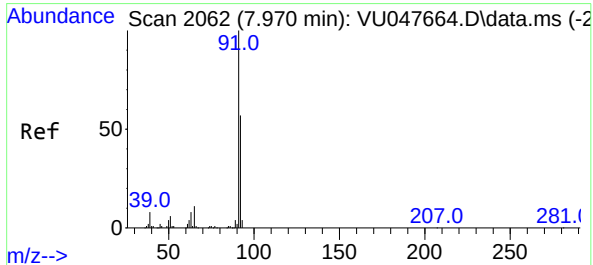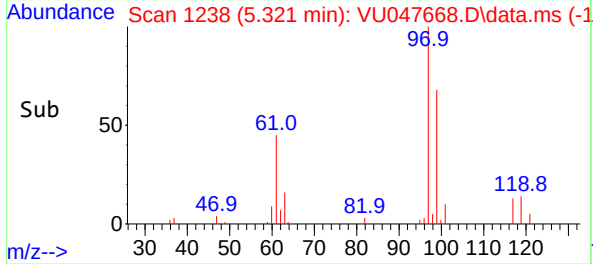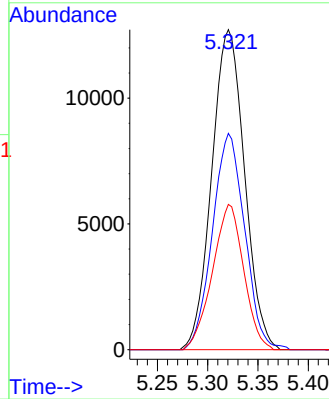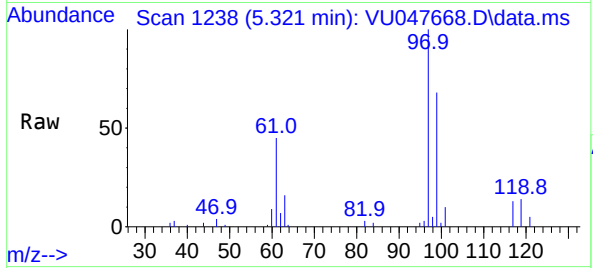

#42
Toluene
Concen: 1.601 ug/L
RT: 7.970 min Scan# 2062
Delta R.T. 0.000 min
Lab File: VU047668.D
Acq: 25 Mar 2022 12:34

Tgt Ion: 91 Resp: 5008
Ion Ratio Lower Upper
91 100
92 64.2 40.4 75.0

