

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047670.D
 Acq On : 25 Mar 2022 13:52
 Operator : SY/MD
 Sample : N2081-03DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X2DL

Quant Time: Mar 26 02:08:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 26 02:04:39 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	244650	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	250759	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	136433	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	107142	60.392	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	= 120.780%		
7) Chloroethane-d5	1.916	69	95125	68.000	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	= 136.000%#		
11) 1,1-Dichloroethene-d2	2.572	63	147784	45.530	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	= 91.060%		
21) 2-Butanone-d5	4.636	46	201452	132.294	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	= 132.290%#		
24) Chloroform-d	5.067	84	197838	60.945	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	= 121.900%		
26) 1,2-Dichloroethane-d4	5.707	65	129288	64.938	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	= 129.880%#		
32) Benzene-d6	5.732	84	411737	65.254	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	= 130.500%#		
36) 1,2-Dichloropropane-d6	6.694	67	129332	66.742	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	= 133.480%#		
41) Toluene-d8	7.899	98	376772	61.288	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	= 122.580%#		
43) trans-1,3-Dichloroprop...	8.182	79	61256	62.396	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	= 124.800%		
47) 2-Hexanone-d5	8.639	63	148331	130.759	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	= 130.760%#		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	201018	60.446	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	= 120.900%#		
66) 1,2-Dichlorobenzene-d4	12.195	152	162801	67.072	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	= 134.140%#		
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.607	62	1341	0.606	ug/L #	1
8) Chloroethane	1.941	64	3222	2.320	ug/L	100
12) 1,1-Dichloroethene	2.572	96	1795	1.070	ug/L #	1
19) 1,1-Dichloroethane	3.874	63	17490	5.603	ug/L	97
20) cis-1,2-Dichloroethene	4.671	96	11742	5.917	ug/L	96
30) 1,1,1-Trichloroethane	5.321	97	60027	21.111	ug/L	98
46) Tetrachloroethene	8.552	164	2512	1.469	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047670.D
Acq On : 25 Mar 2022 13:52
Operator : SY/MD
Sample : N2081-03DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X2DL

Quant Time: Mar 26 02:08:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 26 02:04:39 2022
Response via : Initial Calibration




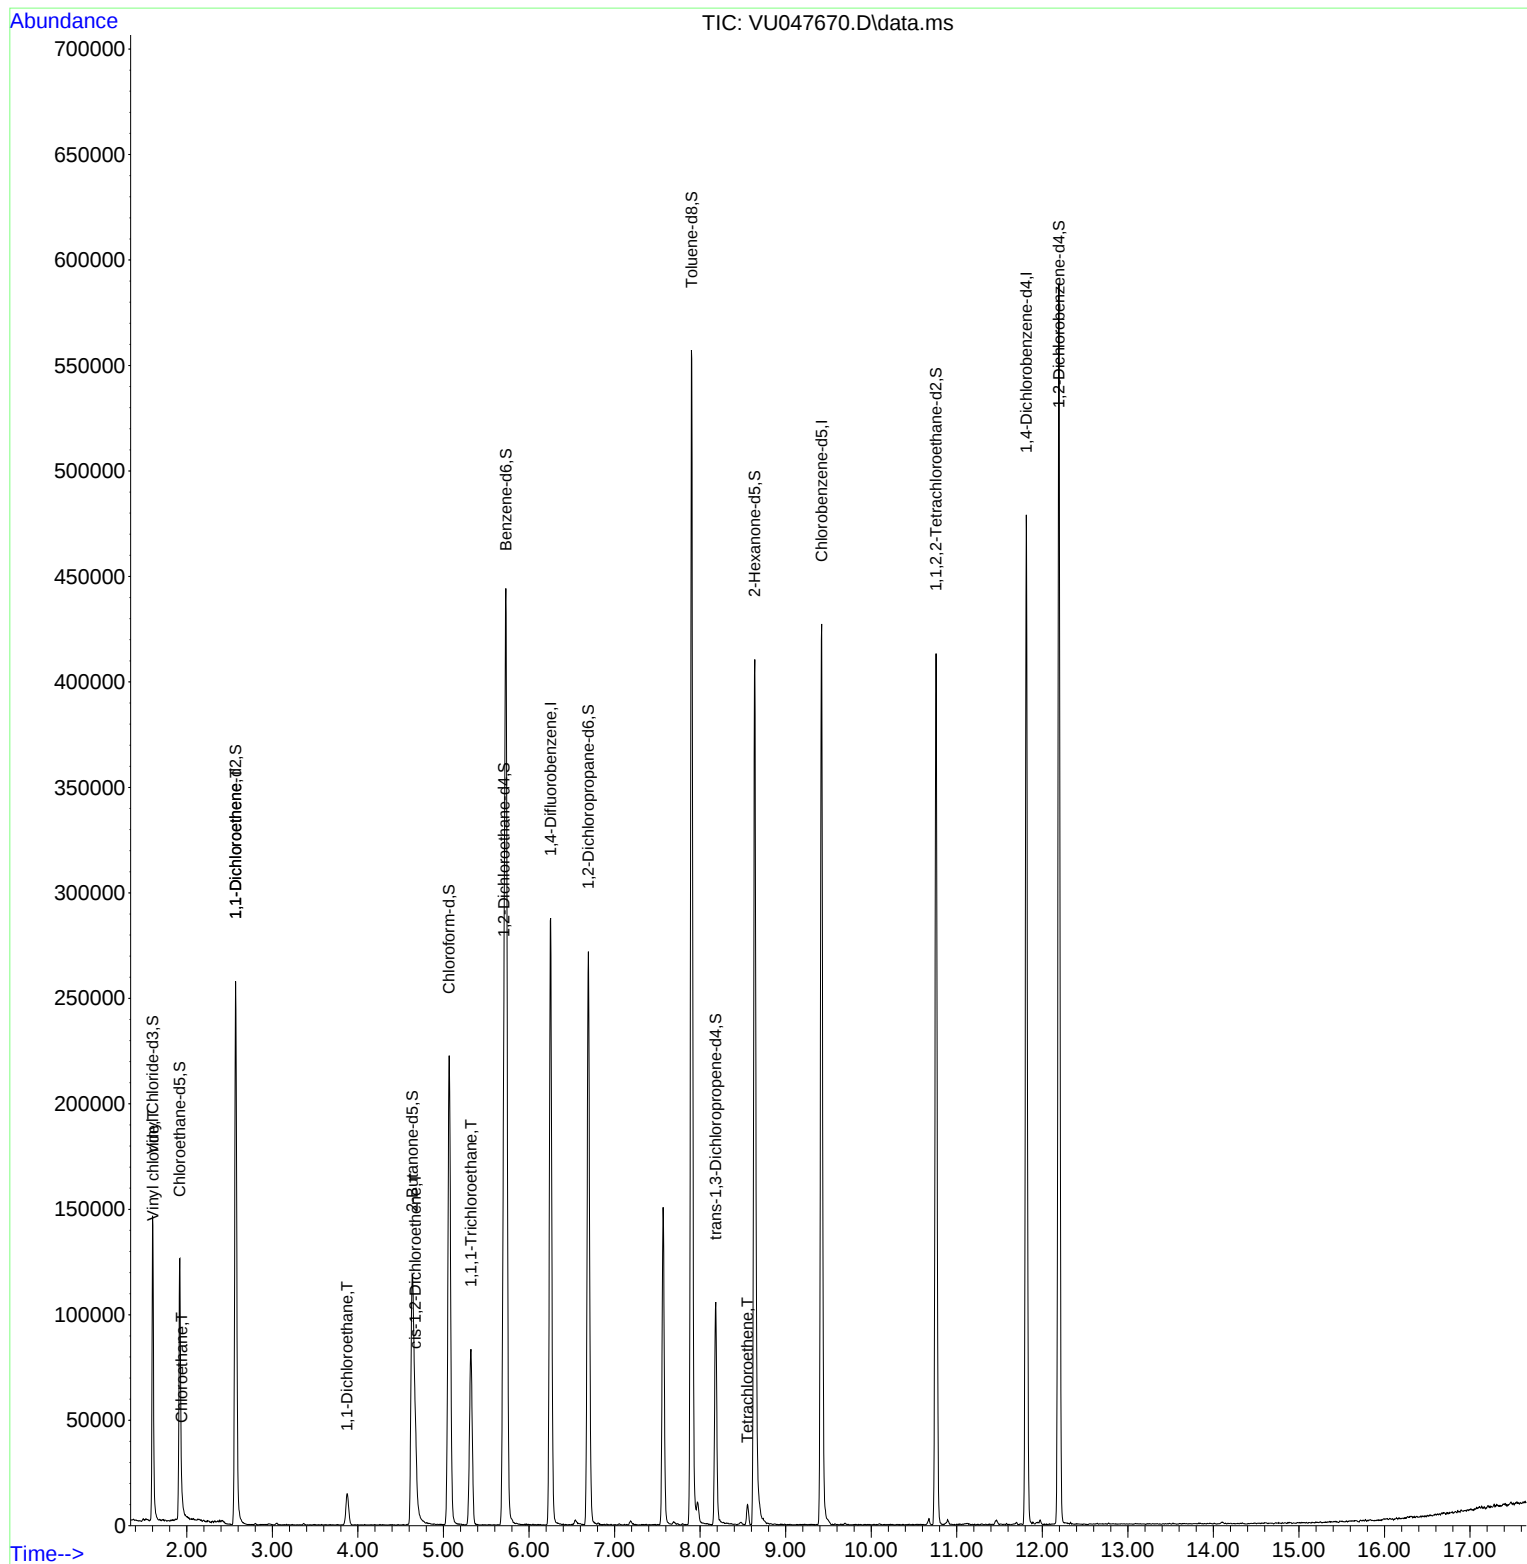


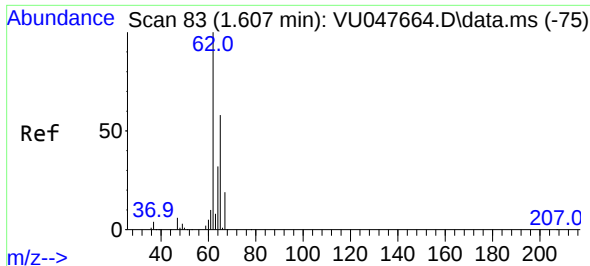

#5
 Vinyl chloride
 Concen: 0.606 ug/L
 RT: 1.607 min Scan# 81
 Delta R.T. 0.000 min
 Lab File: VU047670.D
 Acq: 25 Mar 2022 13:52




Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X2DL


Tgt Ion: 62 Resp: 1341
 Ion Ratio Lower Upper
 62 100
 64 93.5 23.7 43.9#

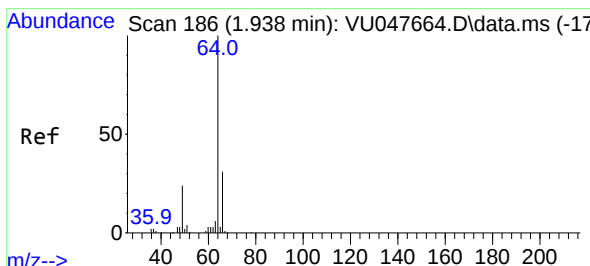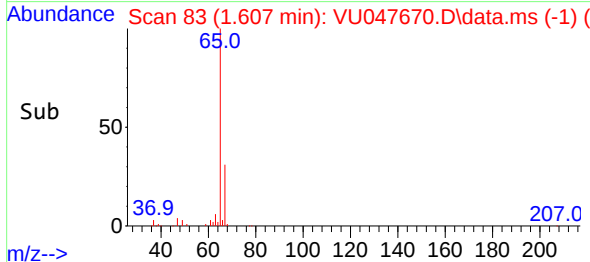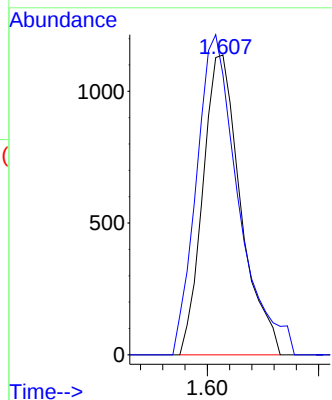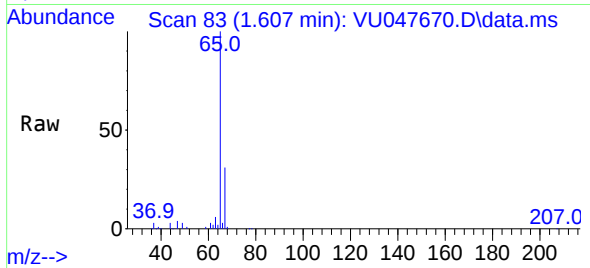

#8
 Chloroethane
 Concen: 2.320 ug/L
 RT: 1.941 min Scan# 187
 Delta R.T. 0.003 min
 Lab File: VU047670.D
 Acq: 25 Mar 2022 13:52

Tgt Ion: 64 Resp: 3222
 Ion Ratio Lower Upper
 64 100
 66 33.3 23.3 43.3

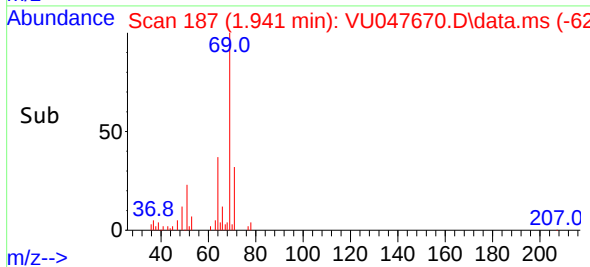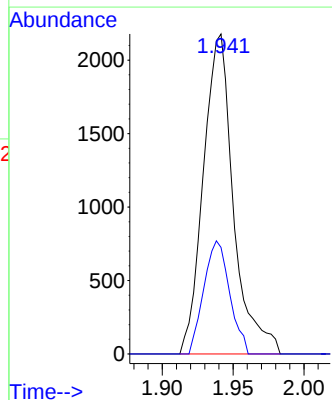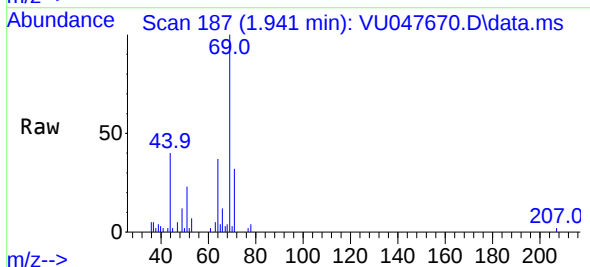

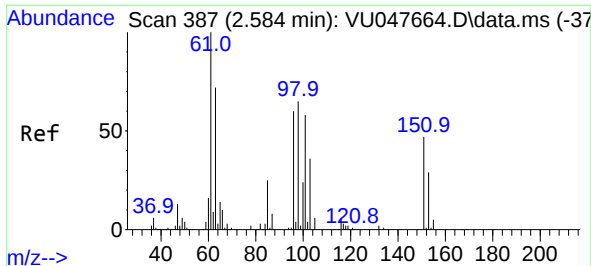

#12

1,1-Dichloroethene

Concen: 1.070 ug/L

RT: 2.572 min Scan# 383

Delta R.T. -0.013 min

Lab File: VU047670.D

Acq: 25 Mar 2022 13:52

Instrument :

MSVOA_U

ClientSampleId :

EW5X2DL





Tgt Ion: 96 Resp: 1795

Ion Ratio Lower Upper

96 100

61 1207.6 113.1 210.1#

63 9899.2 94.8 176.0#

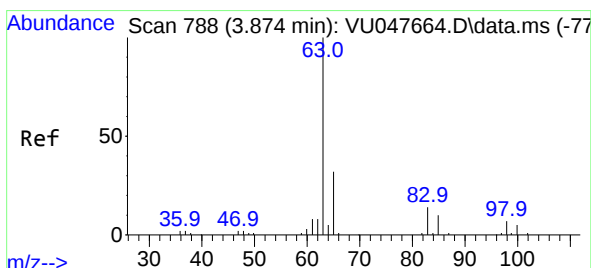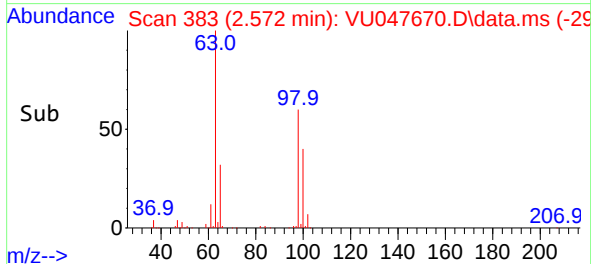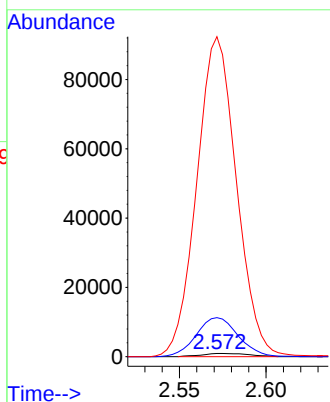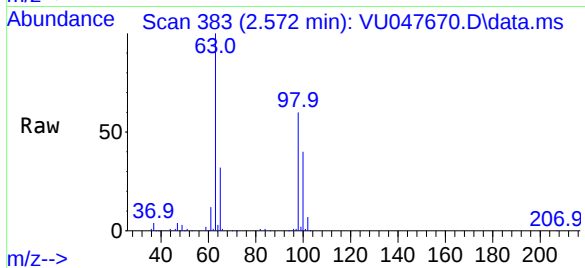

#19

1,1-Dichloroethane

Concen: 5.603 ug/L

RT: 3.874 min Scan# 788

Delta R.T. 0.000 min

Lab File: VU047670.D

Acq: 25 Mar 2022 13:52




Tgt Ion: 63 Resp: 17490


Ion Ratio Lower Upper

63 100

65 32.2 22.0 41.0

83 16.2 9.7 18.1


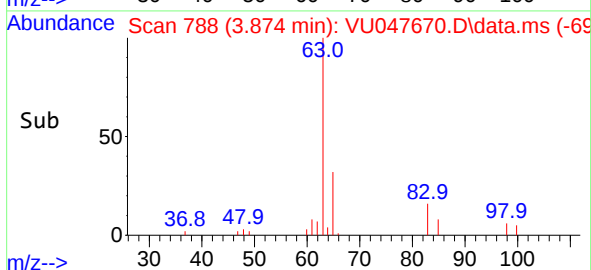
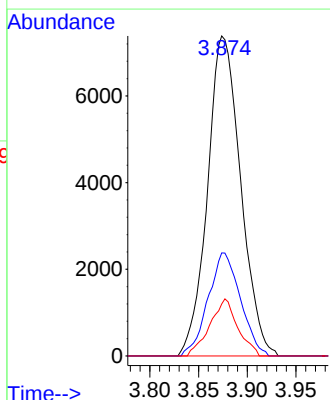
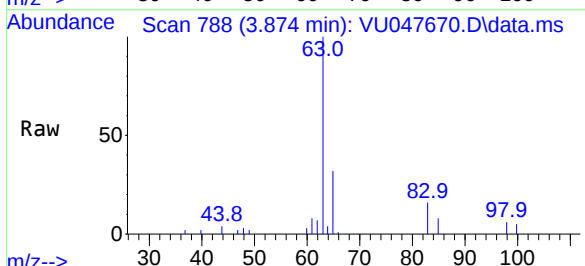


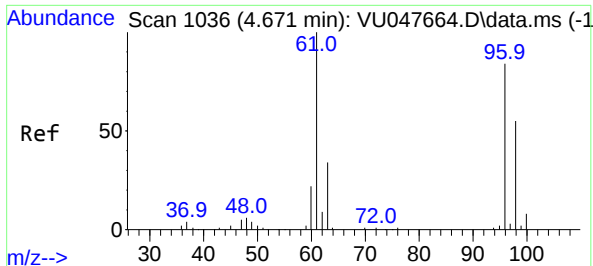

#20
 cis-1,2-Dichloroethene
 Concen: 5.917 ug/L
 RT: 4.671 min Scan# 1036
 Delta R.T. 0.000 min
 Lab File: VU047670.D
 Acq: 25 Mar 2022 13:52




Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X2DL


Tgt Ion: 96 Resp: 11742
 Ion Ratio Lower Upper
 96 100
 61 119.3 80.7 149.9
 68 0.0 0.0 0.0

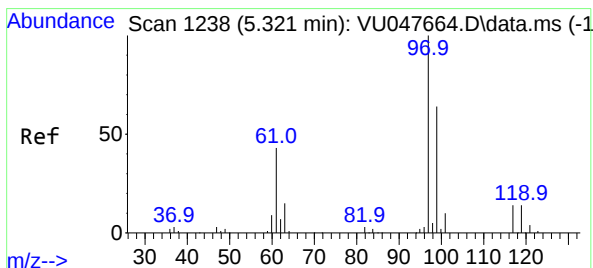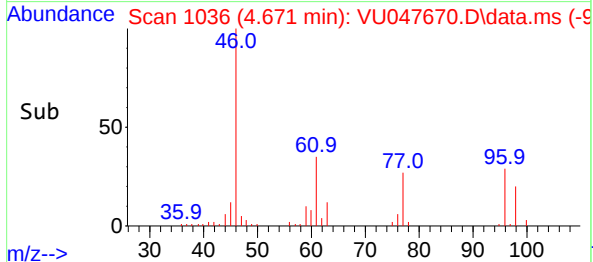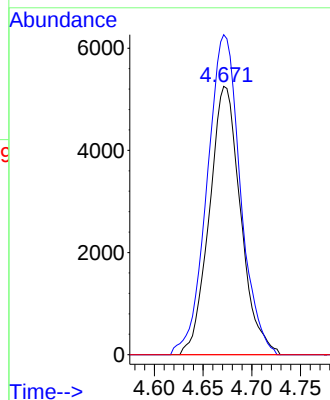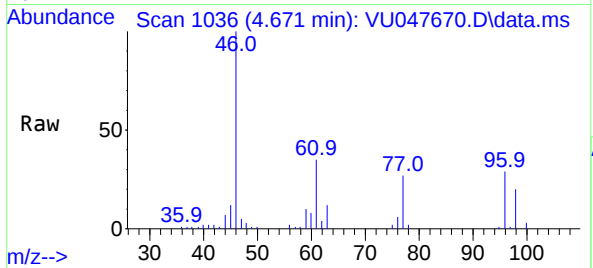

#30
 1,1,1-Trichloroethane
 Concen: 21.111 ug/L
 RT: 5.321 min Scan# 1238
 Delta R.T. 0.000 min
 Lab File: VU047670.D
 Acq: 25 Mar 2022 13:52


Tgt Ion: 97 Resp: 60027
 Ion Ratio Lower Upper
 97 100
 99 64.3 51.6 77.4
 61 45.1 34.2 51.4

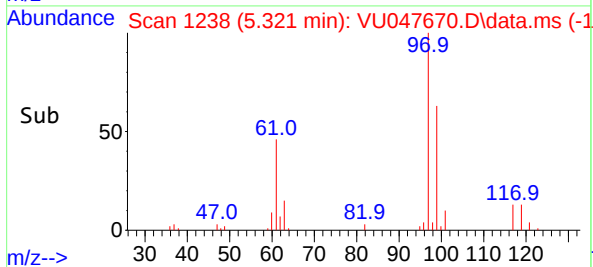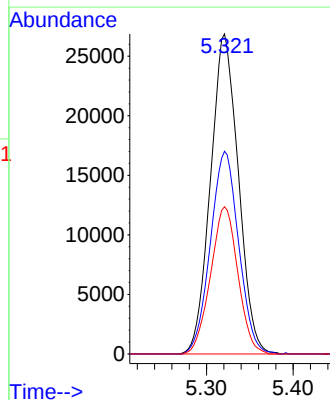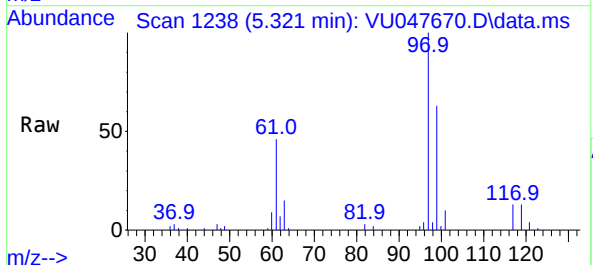

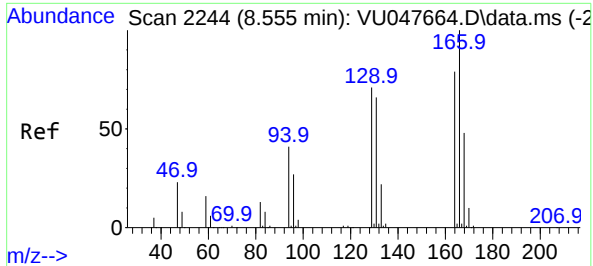

#46
Tetrachloroethene
Concen: 1.469 ug/L
RT: 8.552 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU047670.D
Acq: 25 Mar 2022 13:52

Instrument :
MSVOA_U
ClientSampleId :
EW5X2DL

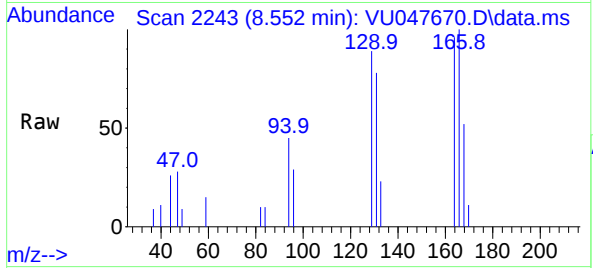

Tgt Ion:164 Resp: 2512

Ion	Ratio	Lower	Upper
164	100		
129	92.5	62.4	116.0
131	81.4	60.7	112.7
166	104.5	89.0	165.4

