

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047665.D
 Acq On : 25 Mar 2022 11:01
 Operator : SY/MD
 Sample : VU0325WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK071

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rBV	119880	142476	15.07%	1.876%
2	1.919	171	180	204	rBV	92350	128807	13.62%	1.696%
3	2.346	310	313	315	rBV3	780	496	0.05%	0.007%
4	2.571	371	383	424	rBV	200413	343870	36.36%	4.528%
5	2.761	439	442	447	rBV2	325	278	0.03%	0.004%
6	2.790	449	451	455	rBV2	428	420	0.04%	0.006%
7	2.838	461	466	471	rVB2	329	389	0.04%	0.005%
8	2.867	471	475	477	rBV	218	195	0.02%	0.003%
9	3.047	526	531	541	rVB3	887	1588	0.17%	0.021%
10	3.112	546	551	554	rBV2	293	264	0.03%	0.003%
11	3.247	590	593	598	rVB2	353	265	0.03%	0.003%
12	3.285	602	605	608	rVV	208	196	0.02%	0.003%
13	3.317	612	615	622	rVB3	244	302	0.03%	0.004%
14	3.633	710	713	717	rBV2	266	256	0.03%	0.003%
15	3.825	771	773	779	rBV2	242	198	0.02%	0.003%
16	4.131	865	868	871	rBV	253	202	0.02%	0.003%
17	4.231	896	899	905	rVB2	263	165	0.02%	0.002%
18	4.417	955	957	961	rVB	298	193	0.02%	0.003%
19	4.446	961	966	968	rBV2	275	312	0.03%	0.004%
20	4.497	978	982	986	rBV2	305	303	0.03%	0.004%
21	4.645	1013	1028	1078	rBV2	75110	271116	28.67%	3.570%
22	4.957	1120	1125	1128	rBV3	355	310	0.03%	0.004%
23	4.980	1129	1132	1136	rVB3	404	338	0.04%	0.004%
24	4.999	1136	1138	1141	rBV	282	209	0.02%	0.003%
25	5.067	1142	1159	1180	rBV	166290	368451	38.96%	4.852%
26	5.282	1223	1226	1227	rBV2	393	175	0.02%	0.002%
27	5.362	1247	1251	1253	rBV	175	165	0.02%	0.002%
28	5.600	1321	1325	1329	rBV2	235	247	0.03%	0.003%
29	5.636	1329	1336	1339	rBV2	256	346	0.04%	0.005%
30	5.729	1344	1365	1395	rBV2	354415	945636	100.00%	12.451%
31	5.886	1411	1414	1416	rBV3	241	163	0.02%	0.002%
32	6.025	1453	1457	1459	rBV2	204	186	0.02%	0.002%
33	6.076	1471	1473	1476	rBV2	264	170	0.02%	0.002%
34	6.179	1502	1505	1509	rVB2	313	200	0.02%	0.003%
35	6.253	1513	1528	1549	rBV	274361	517824	54.76%	6.818%
36	6.475	1593	1597	1604	rBV2	260	343	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047665.D
 Acq On : 25 Mar 2022 11:01
 Operator : SY/MD
 Sample : VU0325WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK071

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.520	1608	1611	1612	rBV	385	172	0.02%	0.002%
38	6.536	1612	1616	1618	rBV2	545	442	0.05%	0.006%
39	6.616	1638	1641	1644	rVB3	403	209	0.02%	0.003%
40	6.693	1651	1665	1687	rBV	213729	416530	44.05%	5.485%
41	7.002	1755	1761	1764	rBV3	424	481	0.05%	0.006%
42	7.038	1768	1772	1775	rBV2	309	311	0.03%	0.004%
43	7.182	1812	1817	1822	rBV5	1272	1634	0.17%	0.022%
44	7.327	1858	1862	1867	rVB3	215	300	0.03%	0.004%
45	7.568	1924	1937	1953	rBV	120636	212565	22.48%	2.799%
46	7.697	1969	1977	1985	rVB5	987	1638	0.17%	0.022%
47	7.783	2000	2004	2005	rBV	276	170	0.02%	0.002%
48	7.806	2005	2011	2015	rBV5	768	848	0.09%	0.011%
49	7.828	2015	2018	2021	rVB2	336	202	0.02%	0.003%
50	7.902	2027	2041	2056	rBV	433316	761781	80.56%	10.031%
51	8.182	2116	2128	2144	rBV	86022	146184	15.46%	1.925%
52	8.414	2197	2200	2204	rBV2	340	314	0.03%	0.004%
53	8.465	2213	2216	2218	rBV2	297	216	0.02%	0.003%
54	8.555	2242	2244	2248	rVB	351	193	0.02%	0.003%
55	8.639	2256	2270	2312	rBV	303854	599255	63.37%	7.891%
56	9.153	2424	2430	2437	rBV3	419	643	0.07%	0.008%
57	9.195	2440	2443	2449	rBB2	206	209	0.02%	0.003%
58	9.240	2454	2457	2460	rBV2	195	167	0.02%	0.002%
59	9.291	2471	2473	2478	rBV2	237	201	0.02%	0.003%
60	9.420	2500	2513	2536	rBV	405167	689002	72.86%	9.072%
61	9.571	2558	2560	2566	rVB2	564	411	0.04%	0.005%
62	9.693	2593	2598	2606	rVB2	1071	1433	0.15%	0.019%
63	9.799	2628	2631	2634	rBV2	357	242	0.03%	0.003%
64	10.047	2705	2708	2710	rBV	227	161	0.02%	0.002%
65	10.098	2719	2724	2726	rBV	484	437	0.05%	0.006%
66	10.153	2739	2741	2748	rVB3	254	288	0.03%	0.004%
67	10.333	2794	2797	2800	rBV2	285	194	0.02%	0.003%
68	10.398	2814	2817	2819	rBV	356	195	0.02%	0.003%
69	10.488	2840	2845	2851	rVB3	428	615	0.07%	0.008%
70	10.590	2875	2877	2881	rVV2	248	173	0.02%	0.002%
71	10.674	2896	2903	2911	rVB2	2143	3327	0.35%	0.044%
72	10.758	2917	2929	2948	rBV	326067	532003	56.26%	7.005%
73	10.873	2962	2965	2968	rBV2	288	176	0.02%	0.002%
74	10.893	2968	2971	2973	rBV3	551	415	0.04%	0.005%
75	11.037	3014	3016	3019	rVB2	287	186	0.02%	0.002%
76	11.092	3029	3033	3039	rBV3	391	519	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047665.D
 Acq On : 25 Mar 2022 11:01
 Operator : SY/MD
 Sample : VU0325WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK071

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.160	3052	3054	3059	rVB2	354	232	0.02%	0.003%
78	11.295	3094	3096	3105	rVB3	476	502	0.05%	0.007%
79	11.336	3105	3109	3113	rBV2	232	257	0.03%	0.003%
80	11.459	3140	3147	3150	rBV2	1881	2147	0.23%	0.028%
81	11.526	3164	3168	3173	rBV2	287	322	0.03%	0.004%
82	11.587	3182	3187	3190	rBV3	386	360	0.04%	0.005%
83	11.693	3216	3220	3226	rVB3	752	966	0.10%	0.013%
84	11.748	3231	3237	3244	rBV3	778	1136	0.12%	0.015%
85	11.812	3245	3257	3278	rBV	461999	730706	77.27%	9.621%
86	11.934	3293	3295	3296	rBV	605	331	0.04%	0.004%
87	11.976	3304	3308	3313	rVB3	1563	1382	0.15%	0.018%
88	12.195	3363	3376	3394	rBV	459231	741308	78.39%	9.761%
89	12.285	3402	3404	3407	rBV4	311	231	0.02%	0.003%
90	12.340	3417	3421	3428	rBV4	688	702	0.07%	0.009%
91	12.410	3439	3443	3450	rVB3	427	498	0.05%	0.007%
92	12.465	3456	3460	3464	rVB3	369	331	0.04%	0.004%
93	12.552	3485	3487	3490	rBV	262	193	0.02%	0.003%
94	12.606	3501	3504	3507	rVB	333	206	0.02%	0.003%
95	12.642	3508	3515	3520	rBV3	551	679	0.07%	0.009%
96	13.224	3693	3696	3707	rVB5	1006	1223	0.13%	0.016%
97	13.365	3733	3740	3745	rBV3	420	767	0.08%	0.010%
98	14.092	3958	3966	3979	rBV	3555	6262	0.66%	0.082%
99	14.336	4038	4042	4049	rVB2	1759	1924	0.20%	0.025%
100	15.105	4279	4281	4284	rBV2	632	406	0.04%	0.005%


Sum of corrected areas: 7594567

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047665.D
Acq On : 25 Mar 2022 11:01
Operator : SY/MD
Sample : VU0325WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK071

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

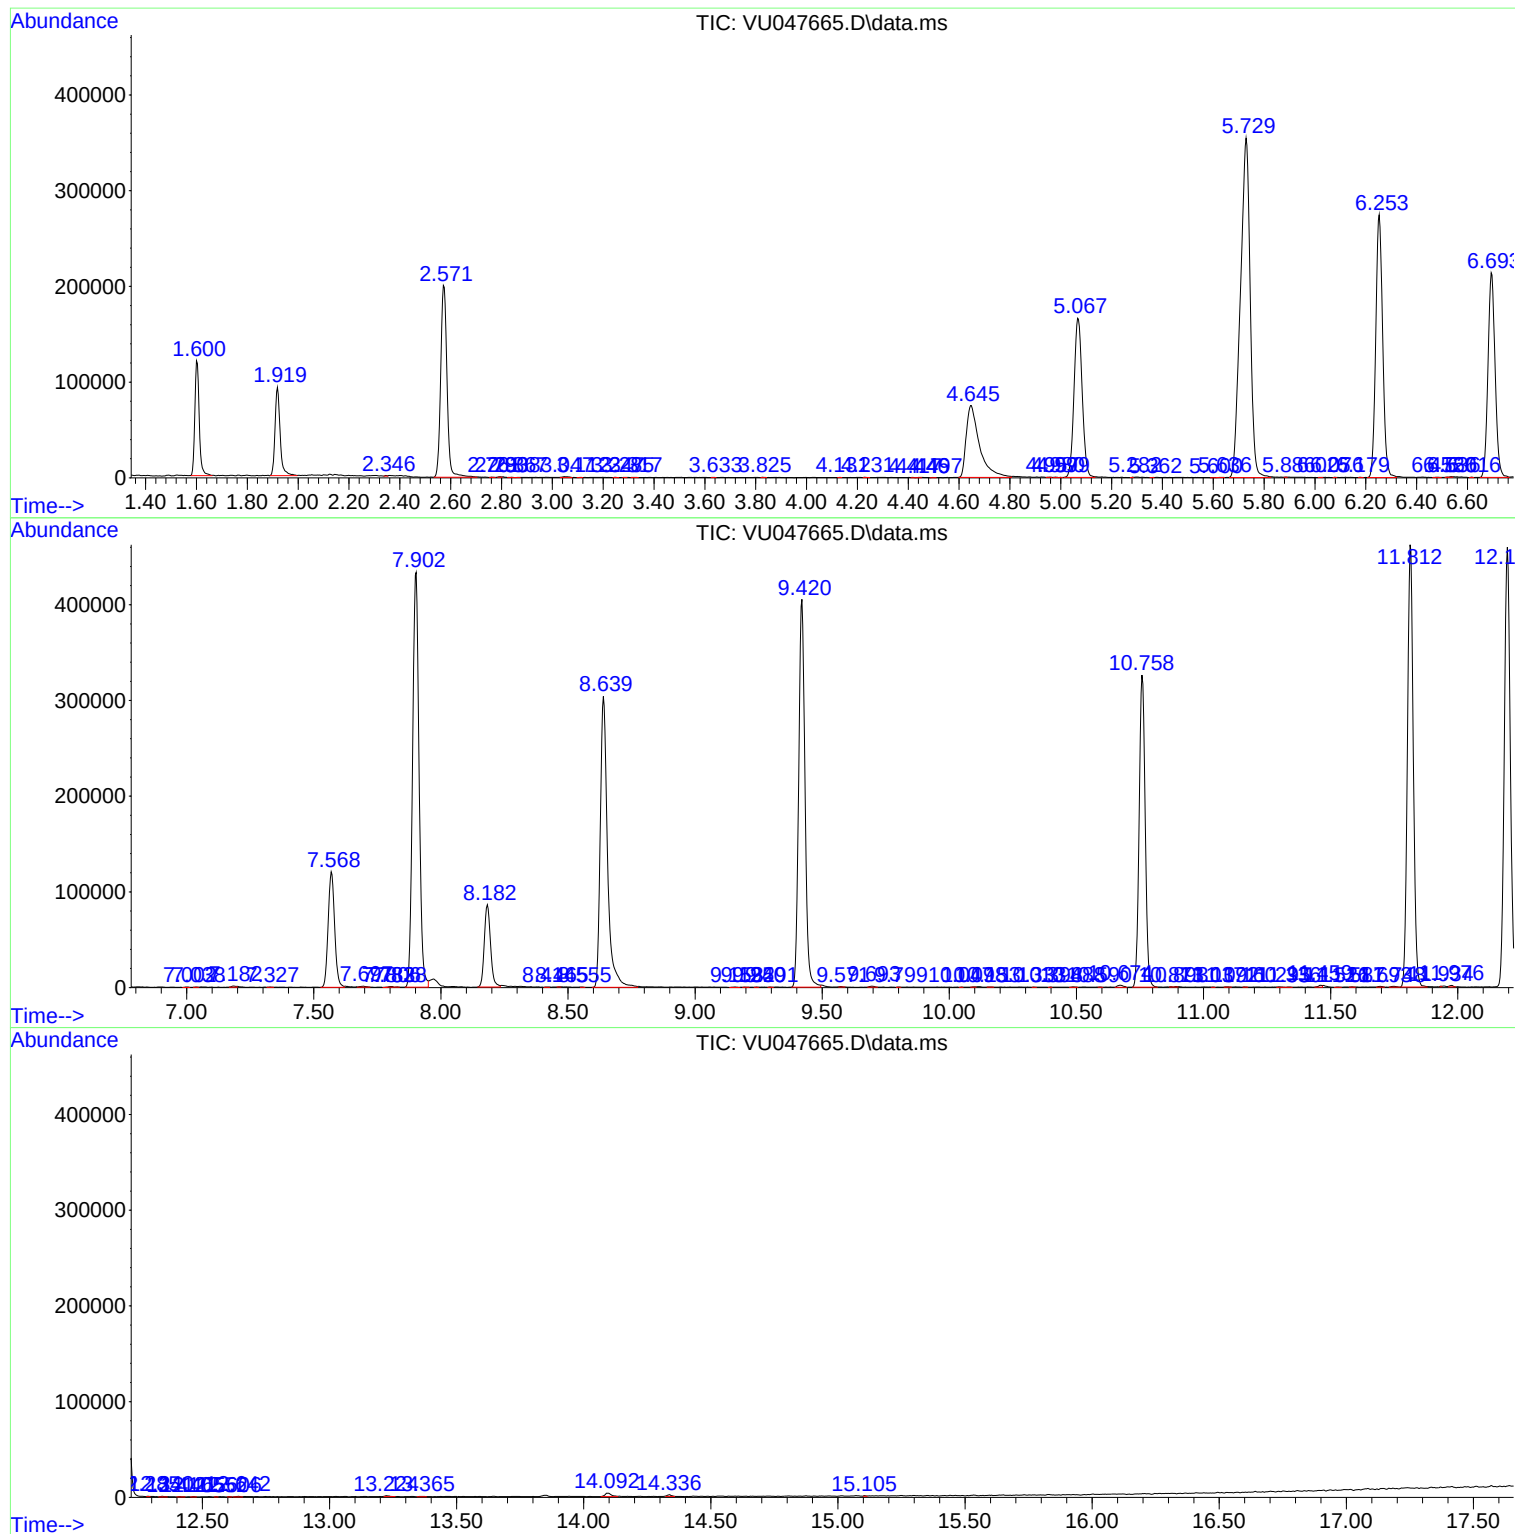

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047665.D
Acq On : 25 Mar 2022 11:01
Operator : SY/MD
Sample : VU0325WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK071

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047665.D
Acq On : 25 Mar 2022 11:01
Operator : SY/MD
Sample : VU0325WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK071

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------