

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047666.D
 Acq On : 25 Mar 2022 11:49
 Operator : SY/MD
 Sample : N2081-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047666.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	101	rBV	156887	186050	14.24%	1.549%
2	1.919	171	180	199	rBV	120265	166333	12.73%	1.385%
3	2.571	370	383	415	rBV2	275170	487128	37.28%	4.055%
4	2.716	426	428	435	rVB	624	320	0.02%	0.003%
5	2.797	447	453	459	rBV2	671	961	0.07%	0.008%
6	2.867	471	475	476	rBV	239	190	0.01%	0.002%
7	2.893	481	483	486	rVB	307	181	0.01%	0.002%
8	2.944	496	499	501	rBV2	339	204	0.02%	0.002%
9	3.047	527	531	535	rBV4	624	552	0.04%	0.005%
10	3.121	549	554	557	rBV2	327	304	0.02%	0.003%
11	3.179	567	572	573	rBV2	494	364	0.03%	0.003%
12	3.359	620	628	637	rVV2	2376	4203	0.32%	0.035%
13	3.433	648	651	656	rBV2	320	266	0.02%	0.002%
14	3.616	704	708	710	rBV2	209	179	0.01%	0.001%
15	3.877	771	789	808	rBV2	43090	102287	7.83%	0.851%
16	4.022	830	834	839	rBV2	147	182	0.01%	0.002%
17	4.247	898	904	906	rBV	286	297	0.02%	0.002%
18	4.642	1011	1027	1068	rBV	117831	423906	32.45%	3.528%
19	5.070	1143	1160	1188	rBV	221881	485154	37.13%	4.038%
20	5.218	1203	1206	1209	rBV2	357	264	0.02%	0.002%
21	5.321	1220	1238	1268	rBV	581912	1306517	100.00%	10.875%
22	5.652	1336	1341	1343	rBV	279	279	0.02%	0.002%
23	5.729	1343	1365	1387	rBV2	457803	1227899	93.98%	10.221%
24	6.012	1451	1453	1460	rVB3	295	228	0.02%	0.002%
25	6.044	1460	1463	1465	rBV	392	249	0.02%	0.002%
26	6.253	1514	1528	1550	rVV	341096	651817	49.89%	5.426%
27	6.394	1570	1572	1577	rVB2	291	212	0.02%	0.002%
28	6.478	1592	1598	1601	rBV2	369	366	0.03%	0.003%
29	6.504	1602	1606	1607	rBV2	244	181	0.01%	0.002%
30	6.546	1607	1619	1635	rVV2	82223	155654	11.91%	1.296%
31	6.693	1651	1665	1687	rBV	279593	543690	41.61%	4.526%
32	6.935	1736	1740	1744	rBV2	303	215	0.02%	0.002%
33	6.964	1744	1749	1752	rBV3	228	186	0.01%	0.002%
34	7.047	1770	1775	1777	rBV2	313	308	0.02%	0.003%
35	7.083	1783	1786	1790	rBV3	345	227	0.02%	0.002%
36	7.111	1790	1795	1799	rBV2	197	231	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047666.D
 Acq On : 25 Mar 2022 11:49
 Operator : SY/MD
 Sample : N2081-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.134	1799	1802	1806	rVB3	283	199	0.02%	0.002%
38	7.185	1808	1818	1826	rBV3	1770	2823	0.22%	0.023%
39	7.333	1860	1864	1869	rVB2	278	215	0.02%	0.002%
40	7.388	1876	1881	1886	rVB2	309	271	0.02%	0.002%
41	7.484	1908	1911	1916	rVB3	267	230	0.02%	0.002%
42	7.568	1924	1937	1961	rBV	160315	282493	21.62%	2.351%
43	7.793	1999	2007	2010	rBV5	594	755	0.06%	0.006%
44	7.902	2026	2041	2057	rBV	578697	1021589	78.19%	8.503%
45	8.182	2113	2128	2151	rBV	117922	212214	16.24%	1.766%
46	8.401	2191	2196	2202	rVB5	1389	1512	0.12%	0.013%
47	8.478	2209	2220	2231	rVB	7898	13817	1.06%	0.115%
48	8.555	2231	2244	2258	rBV	199585	338411	25.90%	2.817%
49	8.639	2258	2270	2316	rVB	424395	801420	61.34%	6.671%
50	8.877	2340	2344	2347	rBV2	512	376	0.03%	0.003%
51	8.906	2350	2353	2357	rVB2	292	222	0.02%	0.002%
52	8.928	2358	2360	2363	rVB2	334	201	0.02%	0.002%
53	8.947	2363	2366	2367	rBV2	290	188	0.01%	0.002%
54	9.041	2388	2395	2398	rBV2	346	378	0.03%	0.003%
55	9.134	2420	2424	2429	rVB2	363	366	0.03%	0.003%
56	9.253	2456	2461	2463	rBV2	216	220	0.02%	0.002%
57	9.420	2500	2513	2539	rBV	517902	871684	66.72%	7.256%
58	9.552	2549	2554	2556	rVB3	246	213	0.02%	0.002%
59	9.568	2556	2559	2566	rBV5	518	683	0.05%	0.006%
60	9.623	2573	2576	2579	rBV2	215	192	0.01%	0.002%
61	9.812	2630	2635	2637	rBV2	237	234	0.02%	0.002%
62	9.864	2648	2651	2657	rVB2	179	238	0.02%	0.002%
63	9.893	2657	2660	2664	rBV3	286	263	0.02%	0.002%
64	9.941	2671	2675	2678	rBV3	314	307	0.02%	0.003%
65	10.073	2712	2716	2720	rBV3	218	215	0.02%	0.002%
66	10.095	2720	2723	2726	rBV	441	312	0.02%	0.003%
67	10.153	2738	2741	2745	rBV3	318	278	0.02%	0.002%
68	10.475	2837	2841	2843	rBV2	336	238	0.02%	0.002%
69	10.674	2893	2903	2910	rBV3	3100	4484	0.34%	0.037%
70	10.758	2916	2929	2947	rBV	430736	701269	53.67%	5.837%
71	10.896	2958	2972	2987	rBV2	13281	23297	1.78%	0.194%
72	11.024	3010	3012	3019	rVB2	491	502	0.04%	0.004%
73	11.060	3019	3023	3026	rBV2	228	186	0.01%	0.002%
74	11.098	3026	3035	3039	rBV4	801	1149	0.09%	0.010%
75	11.147	3047	3050	3056	rVB4	689	487	0.04%	0.004%
76	11.205	3066	3068	3070	rVV3	328	185	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047666.D
 Acq On : 25 Mar 2022 11:49
 Operator : SY/MD
 Sample : N2081-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.217	3070	3072	3077	rVB3	300	211	0.02%	0.002%
78	11.301	3093	3098	3100	rBV2	326	315	0.02%	0.003%
79	11.330	3104	3107	3110	rVV3	267	210	0.02%	0.002%
80	11.388	3122	3125	3128	rVB	403	242	0.02%	0.002%
81	11.420	3128	3135	3139	rBV2	445	564	0.04%	0.005%
82	11.462	3139	3148	3161	rVB8	3005	5616	0.43%	0.047%
83	11.577	3180	3184	3186	rVV	352	254	0.02%	0.002%
84	11.700	3214	3222	3227	rBV3	1593	2168	0.17%	0.018%
85	11.745	3234	3236	3245	rVB2	649	517	0.04%	0.004%
86	11.815	3245	3258	3274	rBV	605998	951320	72.81%	7.918%
87	12.041	3325	3328	3332	rBV2	223	199	0.02%	0.002%
88	12.092	3342	3344	3348	rVB2	303	208	0.02%	0.002%
89	12.195	3361	3376	3398	rBV	620473	1009433	77.26%	8.402%
90	12.333	3415	3419	3424	rVB4	596	627	0.05%	0.005%
91	12.407	3438	3442	3445	rVB4	431	375	0.03%	0.003%
92	12.497	3463	3470	3472	rBV2	223	305	0.02%	0.003%
93	12.568	3489	3492	3493	rBV2	313	179	0.01%	0.001%
94	12.619	3505	3508	3510	rBV2	312	196	0.02%	0.002%
95	12.722	3538	3540	3542	rBV2	333	193	0.01%	0.002%
96	12.774	3548	3556	3565	rVB3	1988	3203	0.25%	0.027%
97	13.230	3688	3698	3703	rBV3	1048	2019	0.15%	0.017%
98	13.844	3885	3889	3890	rBV2	707	522	0.04%	0.004%
99	14.095	3962	3967	3979	rVB3	1874	2785	0.21%	0.023%
100	14.224	4004	4007	4012	rVB3	375	336	0.03%	0.003%




Sum of corrected areas: 12013897

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047666.D
Acq On : 25 Mar 2022 11:49
Operator : SY/MD
Sample : N2081-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

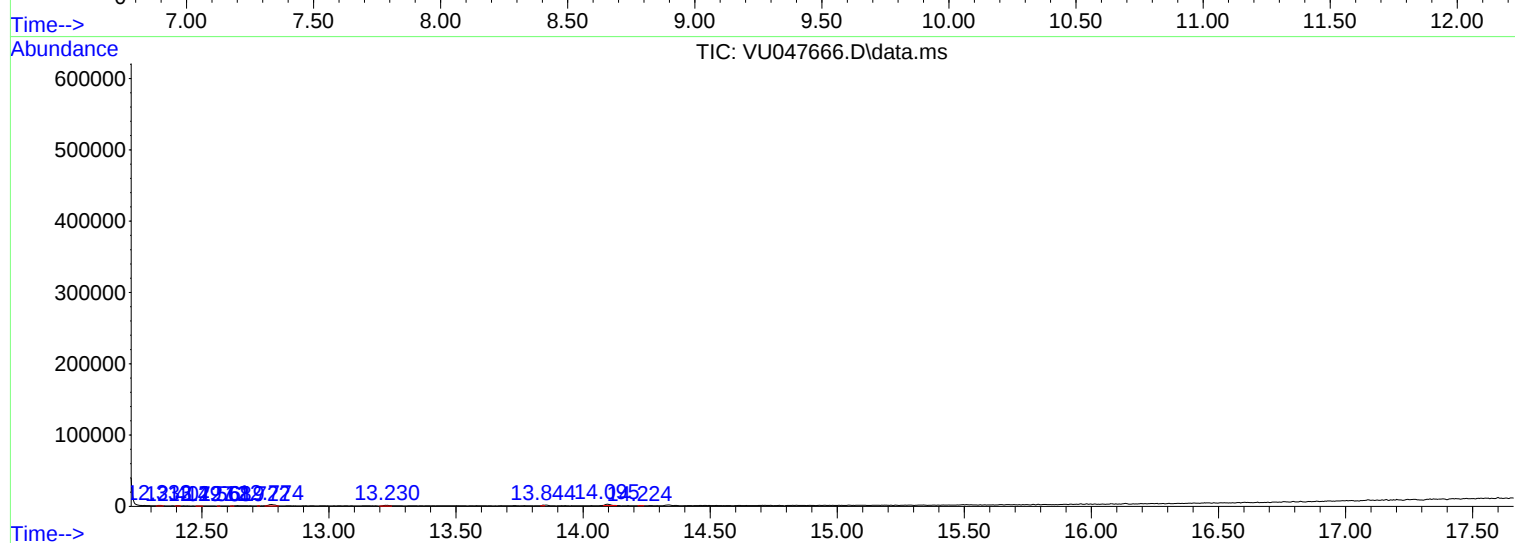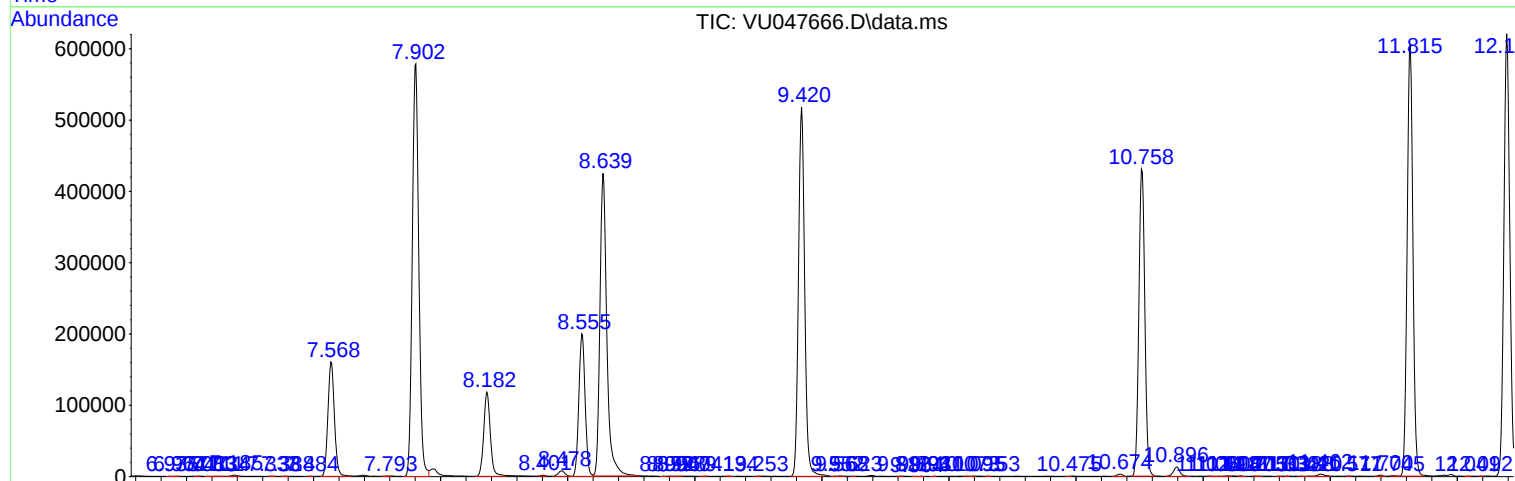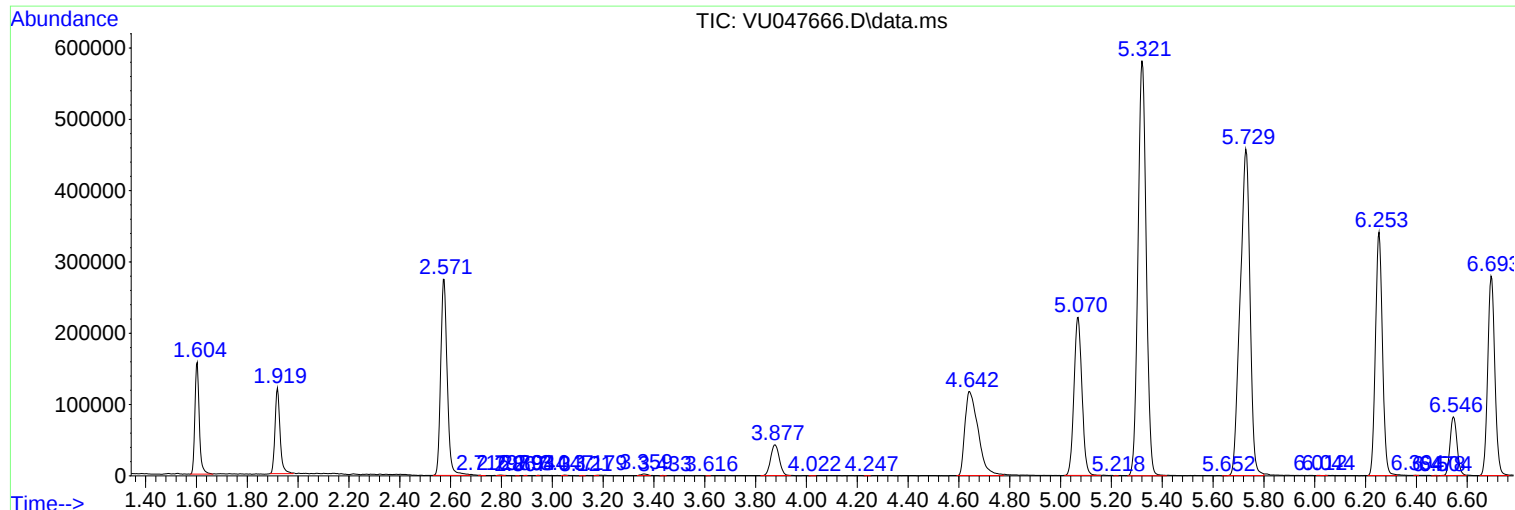

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047666.D
Acq On : 25 Mar 2022 11:49
Operator : SY/MD
Sample : N2081-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047666.D
Acq On : 25 Mar 2022 11:49
Operator : SY/MD
Sample : N2081-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------