

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047667.D
 Acq On : 25 Mar 2022 12:12
 Operator : SY/MD
 Sample : N2081-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	99	rBV	169364	200371	9.30%	1.400%
2	1.919	171	180	199	rBV	132064	180618	8.38%	1.262%
3	2.575	371	384	423	rBV2	312691	571084	26.50%	3.990%
4	2.768	441	444	447	rVV2	630	404	0.02%	0.003%
5	2.803	447	455	461	rVV3	517	784	0.04%	0.005%
6	2.957	496	503	508	rBV2	338	514	0.02%	0.004%
7	2.986	508	512	515	rVB3	380	293	0.01%	0.002%
8	3.054	527	533	534	rBV3	753	672	0.03%	0.005%
9	3.134	555	558	561	rVB2	322	220	0.01%	0.002%
10	3.240	586	591	593	rVV	272	287	0.01%	0.002%
11	3.276	597	602	606	rBV3	358	406	0.02%	0.003%
12	3.359	616	628	643	rBV2	21283	42124	1.95%	0.294%
13	3.684	725	729	733	rVB3	287	237	0.01%	0.002%
14	3.735	741	745	748	rBV3	279	253	0.01%	0.002%
15	3.764	752	754	760	rVB2	287	199	0.01%	0.001%
16	3.806	765	767	771	rVB2	310	276	0.01%	0.002%
17	3.877	771	789	808	rBV	164634	388859	18.05%	2.717%
18	3.957	812	814	822	rVB2	387	312	0.01%	0.002%
19	4.015	830	832	838	rVB2	314	223	0.01%	0.002%
20	4.170	877	880	885	rBV2	214	213	0.01%	0.001%
21	4.420	953	958	961	rVB2	306	350	0.02%	0.002%
22	4.443	961	965	967	rBV2	295	274	0.01%	0.002%
23	4.578	1004	1007	1011	rBV	273	262	0.01%	0.002%
24	4.671	1011	1036	1066	rBV2	822856	2154782	100.00%	15.053%
25	5.067	1143	1159	1183	rVV	242272	534186	24.79%	3.732%
26	5.218	1204	1206	1210	rVB3	467	291	0.01%	0.002%
27	5.321	1218	1238	1261	rBV	503000	1137016	52.77%	7.943%
28	5.449	1276	1278	1283	rVB	527	293	0.01%	0.002%
29	5.523	1297	1301	1305	rVV2	412	334	0.02%	0.002%
30	5.546	1305	1308	1317	rVB3	364	459	0.02%	0.003%
31	5.729	1342	1365	1397	rBV2	498100	1359724	63.10%	9.499%
32	6.018	1452	1455	1458	rVB2	323	209	0.01%	0.001%
33	6.038	1458	1461	1463	rBV3	459	353	0.02%	0.002%
34	6.054	1464	1466	1470	rVB3	584	345	0.02%	0.002%
35	6.108	1479	1483	1486	rBV3	338	280	0.01%	0.002%
36	6.253	1512	1528	1549	rBV	338090	649367	30.14%	4.536%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047667.D
 Acq On : 25 Mar 2022 12:12
 Operator : SY/MD
 Sample : N2081-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.546	1606	1619	1633	rBV3	19134	37611	1.75%	0.263%
38	6.694	1650	1665	1685	rBV	307103	601115	27.90%	4.199%
39	6.809	1696	1701	1703	rBV3	627	562	0.03%	0.004%
40	6.832	1707	1708	1714	rVB2	362	209	0.01%	0.001%
41	7.057	1772	1778	1785	rVB3	527	875	0.04%	0.006%
42	7.095	1787	1790	1794	rVB2	241	211	0.01%	0.001%
43	7.185	1806	1818	1829	rBV3	2325	3922	0.18%	0.027%
44	7.263	1840	1842	1849	rVB2	379	330	0.02%	0.002%
45	7.308	1849	1856	1857	rBV	448	442	0.02%	0.003%
46	7.568	1923	1937	1958	rBV	173432	309720	14.37%	2.164%
47	7.677	1967	1971	1972	rBV3	702	443	0.02%	0.003%
48	7.687	1972	1974	1975	rBV2	582	279	0.01%	0.002%
49	7.899	2025	2040	2056	rBV	627370	1115308	51.76%	7.792%
50	8.179	2115	2127	2144	rBV	123333	215390	10.00%	1.505%
51	8.404	2190	2197	2206	rVB3	2113	3157	0.15%	0.022%
52	8.475	2210	2219	2231	rVB2	4500	8112	0.38%	0.057%
53	8.555	2231	2244	2257	rBV2	121270	204976	9.51%	1.432%
54	8.636	2257	2269	2298	rBV	473919	890550	41.33%	6.221%
55	8.812	2322	2324	2329	rVB4	353	220	0.01%	0.002%
56	8.838	2329	2332	2336	rBV3	293	208	0.01%	0.001%
57	8.880	2341	2345	2350	rBV3	305	392	0.02%	0.003%
58	9.282	2466	2470	2473	rBV2	238	227	0.01%	0.002%
59	9.327	2481	2484	2488	rBV3	339	307	0.01%	0.002%
60	9.417	2499	2512	2550	rBV	513453	866648	40.22%	6.054%
61	9.578	2555	2562	2571	rVB5	704	1335	0.06%	0.009%
62	9.674	2588	2592	2593	rBV2	297	195	0.01%	0.001%
63	9.690	2594	2597	2598	rBV	598	356	0.02%	0.002%
64	9.742	2609	2613	2619	rVB2	284	251	0.01%	0.002%
65	9.819	2634	2637	2641	rVB2	320	297	0.01%	0.002%
66	10.095	2720	2723	2726	rVV2	406	383	0.02%	0.003%
67	10.147	2735	2739	2743	rVB2	288	253	0.01%	0.002%
68	10.198	2753	2755	2759	rVB	375	204	0.01%	0.001%
69	10.230	2762	2765	2767	rVV	334	208	0.01%	0.001%
70	10.246	2767	2770	2777	rVB2	283	252	0.01%	0.002%
71	10.491	2843	2846	2852	rVB2	489	392	0.02%	0.003%
72	10.674	2894	2903	2912	rBV5	3321	5024	0.23%	0.035%
73	10.758	2916	2929	2946	rBV	482586	770605	35.76%	5.383%
74	10.893	2960	2971	2984	rVB2	7339	13084	0.61%	0.091%
75	10.992	2997	3002	3006	rBV3	452	444	0.02%	0.003%
76	11.086	3028	3031	3032	rBV2	405	267	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047667.D
 Acq On : 25 Mar 2022 12:12
 Operator : SY/MD
 Sample : N2081-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.124	3039	3043	3048	rBV5	636	539	0.03%	0.004%
78	11.153	3048	3052	3058	rVB3	738	794	0.04%	0.006%
79	11.208	3064	3069	3073	rBV2	452	496	0.02%	0.003%
80	11.459	3139	3147	3148	rBV3	2618	2651	0.12%	0.019%
81	11.545	3169	3174	3176	rBV	346	333	0.02%	0.002%
82	11.581	3179	3185	3188	rBV3	663	682	0.03%	0.005%
83	11.626	3196	3199	3206	rBV3	364	425	0.02%	0.003%
84	11.697	3214	3221	3228	rBV2	1600	2114	0.10%	0.015%
85	11.812	3245	3257	3278	rBV	584368	925014	42.93%	6.462%
86	11.941	3292	3297	3299	rBV4	1117	1112	0.05%	0.008%
87	11.970	3303	3306	3315	rVB6	2840	3558	0.17%	0.025%
88	12.111	3347	3350	3357	rVB2	335	310	0.01%	0.002%
89	12.195	3360	3376	3397	rBV	668285	1087580	50.47%	7.598%
90	12.307	3409	3411	3414	rBV2	348	220	0.01%	0.002%
91	12.327	3414	3417	3421	rBV5	599	512	0.02%	0.004%
92	12.394	3435	3438	3445	rVB5	563	594	0.03%	0.004%
93	12.632	3509	3512	3515	rBV3	330	275	0.01%	0.002%
94	12.777	3548	3557	3564	rVB2	1569	2690	0.12%	0.019%
95	12.815	3564	3569	3571	rBV3	338	338	0.02%	0.002%
96	13.150	3668	3673	3675	rBV	369	348	0.02%	0.002%
97	13.230	3692	3698	3701	rBV2	552	649	0.03%	0.005%
98	13.848	3886	3890	3892	rBV2	668	575	0.03%	0.004%
99	14.581	4113	4118	4121	rBV3	514	571	0.03%	0.004%
100	15.455	4388	4390	4393	rVB2	590	292	0.01%	0.002%




Sum of corrected areas: 14314310

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047667.D
Acq On : 25 Mar 2022 12:12
Operator : SY/MD
Sample : N2081-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

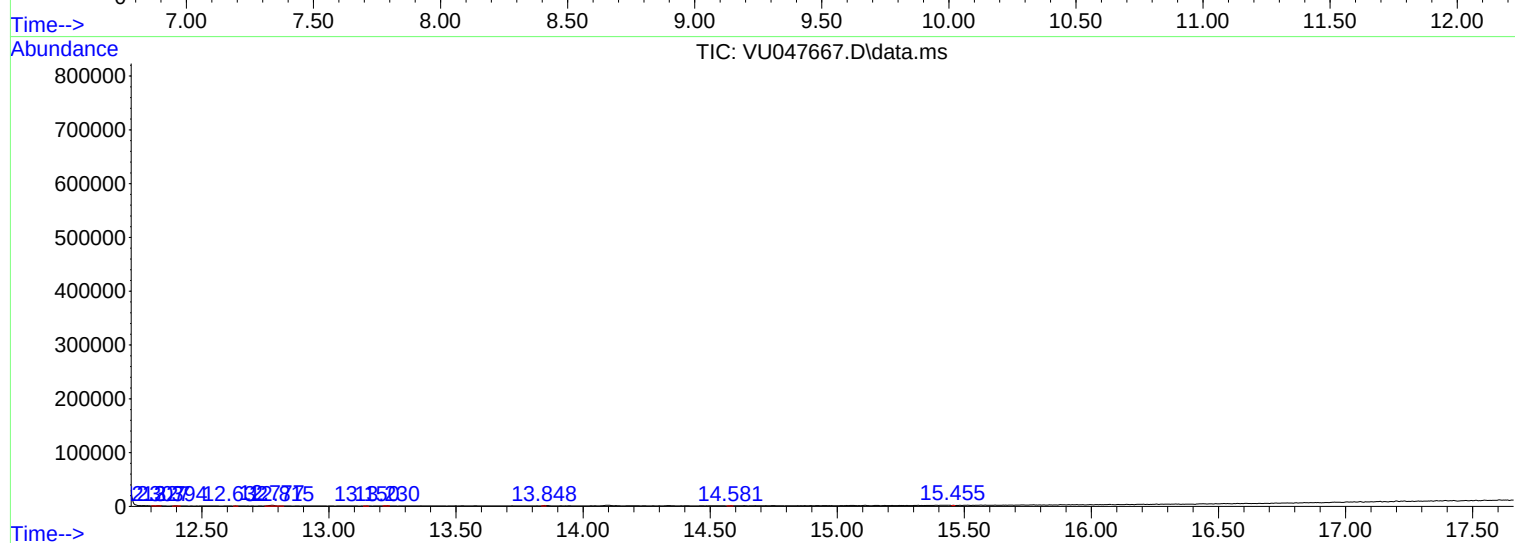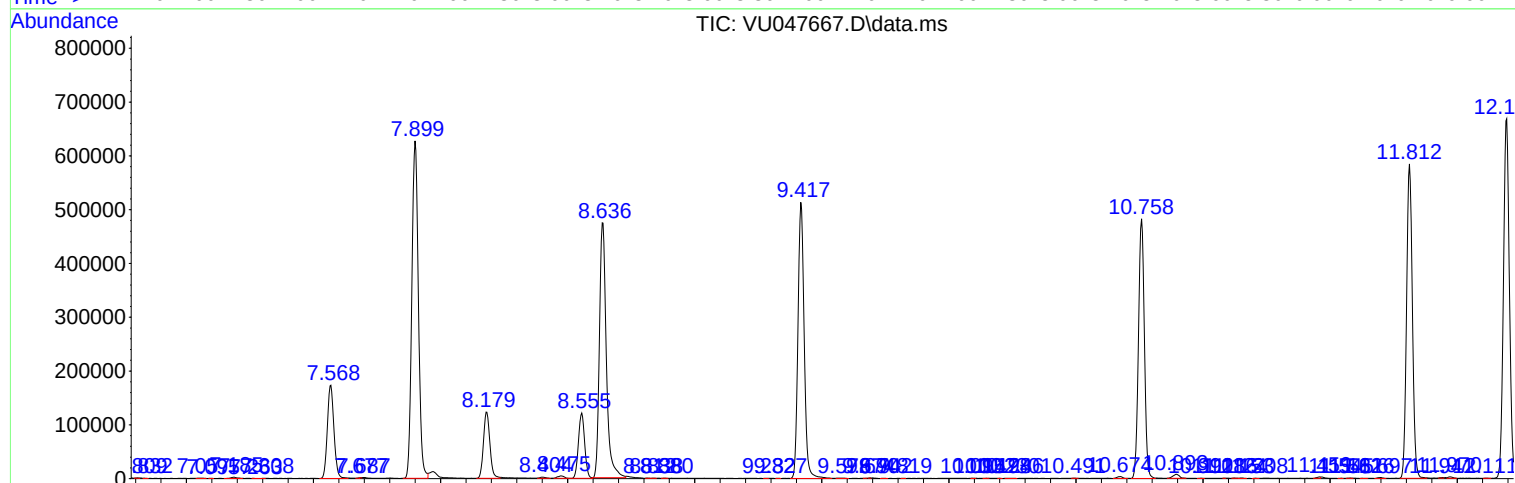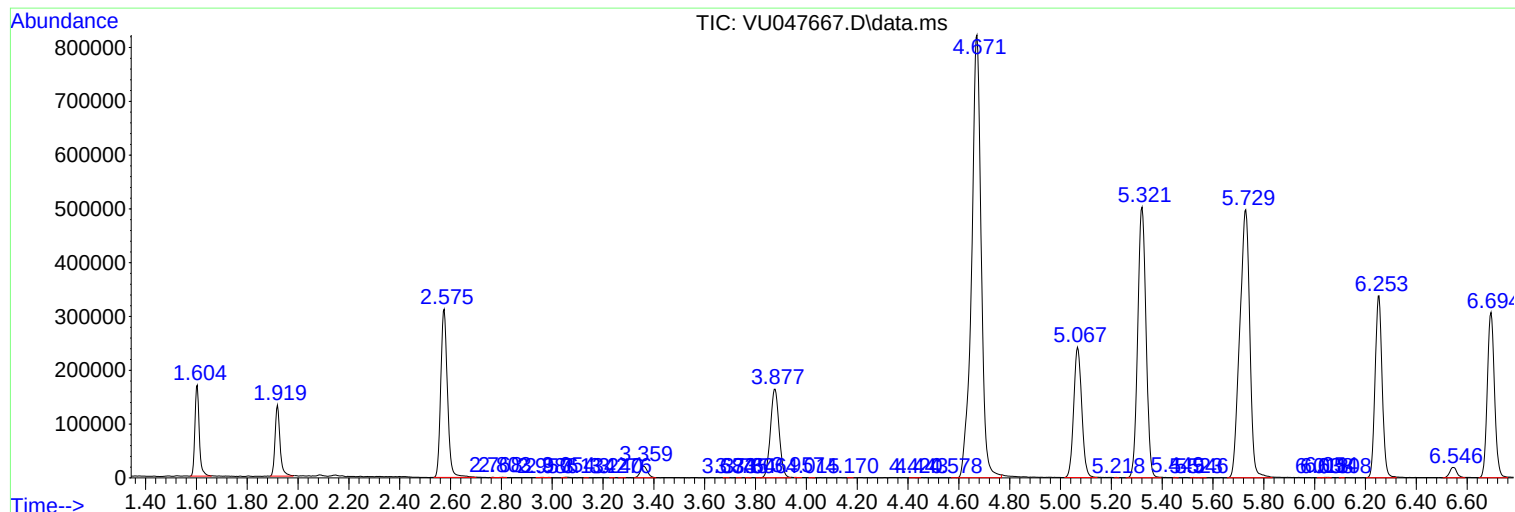

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047667.D
Acq On : 25 Mar 2022 12:12
Operator : SY/MD
Sample : N2081-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047667.D
Acq On : 25 Mar 2022 12:12
Operator : SY/MD
Sample : N2081-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc