

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047668.D
 Acq On : 25 Mar 2022 12:34
 Operator : SY/MD
 Sample : N2081-02DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047668.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	93	rBV	81590	96194	15.07%	1.991%
2	1.919	172	180	202	rVB2	65241	102435	16.05%	2.120%
3	2.571	371	383	407	rBV	135360	231502	36.28%	4.792%
4	2.726	426	431	434	rBV2	359	358	0.06%	0.007%
5	2.793	449	452	454	rBV	356	255	0.04%	0.005%
6	2.838	462	466	472	rVB3	289	325	0.05%	0.007%
7	2.961	500	504	506	rBV3	363	303	0.05%	0.006%
8	3.009	517	519	525	rVB3	208	186	0.03%	0.004%
9	3.051	525	532	537	rBV4	940	1198	0.19%	0.025%
10	3.150	560	563	566	rVV	238	232	0.04%	0.005%
11	3.292	604	607	610	rVB2	298	204	0.03%	0.004%
12	3.337	614	621	622	rBV3	232	217	0.03%	0.004%
13	3.369	623	631	634	rVV3	390	447	0.07%	0.009%
14	3.877	774	789	805	rBV3	10947	25254	3.96%	0.523%
15	4.028	833	836	840	rVB2	324	209	0.03%	0.004%
16	4.128	862	867	871	rVB	362	344	0.05%	0.007%
17	4.243	901	903	906	rVB2	410	186	0.03%	0.004%
18	4.308	919	923	925	rBV3	221	178	0.03%	0.004%
19	4.362	938	940	944	rVB	233	194	0.03%	0.004%
20	4.388	944	948	950	rVB	326	246	0.04%	0.005%
21	4.404	950	953	958	rBV3	258	180	0.03%	0.004%
22	4.433	958	962	966	rBV2	363	351	0.06%	0.007%
23	4.530	990	992	997	rVV2	323	314	0.05%	0.006%
24	4.639	1012	1026	1067	rBV2	65887	235968	36.98%	4.884%
25	4.960	1119	1126	1128	rBV3	332	409	0.06%	0.008%
26	5.067	1143	1159	1185	rVV2	115506	253776	39.77%	5.253%
27	5.321	1223	1238	1257	rBV	40196	89118	13.96%	1.845%
28	5.575	1314	1317	1320	rVB	270	182	0.03%	0.004%
29	5.594	1320	1323	1330	rBV2	237	340	0.05%	0.007%
30	5.729	1343	1365	1385	rBV2	237992	638157	100.00%	13.210%
31	5.964	1434	1438	1441	rBV2	247	231	0.04%	0.005%
32	6.250	1510	1527	1548	rBV2	106399	207300	32.48%	4.291%
33	6.340	1553	1555	1558	rVV	347	213	0.03%	0.004%
34	6.520	1607	1611	1612	rBV	381	205	0.03%	0.004%
35	6.536	1613	1616	1620	rBV3	533	407	0.06%	0.008%
36	6.694	1651	1665	1684	rBV2	143892	281287	44.08%	5.823%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047668.D
 Acq On : 25 Mar 2022 12:34
 Operator : SY/MD
 Sample : N2081-02DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.919	1729	1735	1739	rBV2	178	230	0.04%	0.005%
38	7.041	1770	1773	1777	rBV3	269	217	0.03%	0.004%
39	7.189	1816	1819	1827	rVB4	825	937	0.15%	0.019%
40	7.452	1895	1901	1904	rVB3	298	360	0.06%	0.007%
41	7.568	1924	1937	1955	rBV	81212	141991	22.25%	2.939%
42	7.632	1955	1957	1959	rVB2	502	205	0.03%	0.004%
43	7.681	1969	1972	1973	rBV2	426	237	0.04%	0.005%
44	7.803	2006	2010	2011	rBV2	242	179	0.03%	0.004%
45	7.899	2027	2040	2055	rBV	287592	506675	79.40%	10.488%
46	8.182	2115	2128	2144	rBV	56057	97864	15.34%	2.026%
47	8.388	2189	2192	2196	rBV2	256	188	0.03%	0.004%
48	8.455	2208	2213	2216	rBV3	399	414	0.06%	0.009%
49	8.472	2216	2218	2224	rVB3	428	379	0.06%	0.008%
50	8.558	2238	2245	2251	rBV5	2206	3347	0.52%	0.069%
51	8.639	2257	2270	2302	rBV	212752	418845	65.63%	8.670%
52	8.931	2355	2361	2363	rBV2	341	289	0.05%	0.006%
53	8.976	2369	2375	2377	rBV2	315	371	0.06%	0.008%
54	9.031	2387	2392	2396	rVV3	299	382	0.06%	0.008%
55	9.054	2396	2399	2402	rVV2	358	229	0.04%	0.005%
56	9.070	2402	2404	2409	rVB	268	182	0.03%	0.004%
57	9.099	2409	2413	2415	rBV2	314	255	0.04%	0.005%
58	9.169	2432	2435	2441	rBV2	384	317	0.05%	0.007%
59	9.201	2441	2445	2449	rBB3	244	241	0.04%	0.005%
60	9.311	2476	2479	2484	rVB3	208	225	0.04%	0.005%
61	9.420	2500	2513	2539	rBV	164446	280352	43.93%	5.803%
62	9.571	2554	2560	2567	rBV2	1033	1530	0.24%	0.032%
63	9.697	2593	2599	2609	rVB3	1726	2667	0.42%	0.055%
64	9.812	2631	2635	2638	rVB	329	205	0.03%	0.004%
65	9.954	2673	2679	2682	rBV2	199	219	0.03%	0.005%
66	10.099	2718	2724	2732	rVB3	937	1273	0.20%	0.026%
67	10.295	2780	2785	2789	rBV2	280	248	0.04%	0.005%
68	10.330	2792	2796	2800	rBV	217	252	0.04%	0.005%
69	10.391	2812	2815	2819	rVB2	318	212	0.03%	0.004%
70	10.529	2853	2858	2861	rBV2	415	417	0.07%	0.009%
71	10.584	2871	2875	2878	rVV	342	192	0.03%	0.004%
72	10.674	2895	2903	2908	rBV5	1278	1659	0.26%	0.034%
73	10.758	2917	2929	2950	rBV	224939	366727	57.47%	7.591%
74	10.877	2962	2966	2968	rBV3	299	264	0.04%	0.005%
75	10.893	2968	2971	2972	rBV	593	349	0.05%	0.007%
76	10.944	2984	2987	2993	rVB3	266	259	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047668.D
 Acq On : 25 Mar 2022 12:34
 Operator : SY/MD
 Sample : N2081-02DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.996	3000	3003	3008	rVV3	834	840	0.13%	0.017%
78	11.018	3008	3010	3013	rVV	455	273	0.04%	0.006%
79	11.034	3013	3015	3018	rVB3	473	266	0.04%	0.006%
80	11.095	3027	3034	3038	rVB2	539	572	0.09%	0.012%
81	11.298	3087	3097	3103	rBV4	821	1202	0.19%	0.025%
82	11.471	3140	3151	3162	rVB5	2946	5012	0.79%	0.104%
83	11.520	3162	3166	3170	rBV2	354	305	0.05%	0.006%
84	11.539	3170	3172	3175	rBV	255	188	0.03%	0.004%
85	11.578	3179	3184	3186	rBV3	357	313	0.05%	0.006%
86	11.603	3189	3192	3196	rBV2	308	321	0.05%	0.007%
87	11.745	3231	3236	3237	rBV2	322	238	0.04%	0.005%
88	11.812	3245	3257	3273	rBV	190834	308667	48.37%	6.389%
89	11.886	3277	3280	3282	rBV	661	534	0.08%	0.011%
90	11.976	3303	3308	3315	rVB3	1060	1168	0.18%	0.024%
91	12.098	3340	3346	3349	rBV3	334	387	0.06%	0.008%
92	12.195	3363	3376	3396	rVB	309023	507576	79.54%	10.507%
93	12.385	3430	3435	3436	rBV2	206	189	0.03%	0.004%
94	12.632	3507	3512	3514	rBV2	430	506	0.08%	0.010%
95	12.713	3534	3537	3541	rBV3	286	288	0.05%	0.006%
96	12.751	3547	3549	3553	rBV3	217	192	0.03%	0.004%
97	12.796	3560	3563	3566	rBV2	284	229	0.04%	0.005%
98	13.880	3897	3900	3903	rBV2	305	269	0.04%	0.006%
99	14.095	3963	3967	3976	rBV2	743	855	0.13%	0.018%
100	14.783	4179	4181	4184	rBV3	396	284	0.04%	0.006%




Sum of corrected areas: 4830963

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047668.D
Acq On : 25 Mar 2022 12:34
Operator : SY/MD
Sample : N2081-02DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

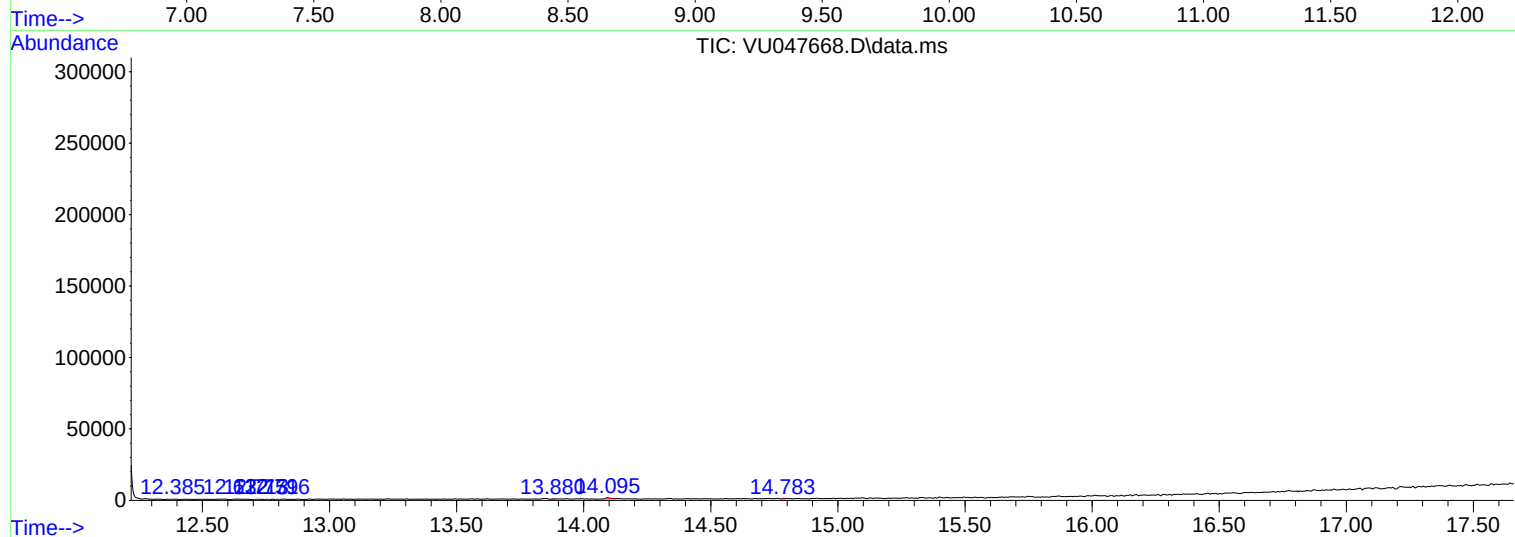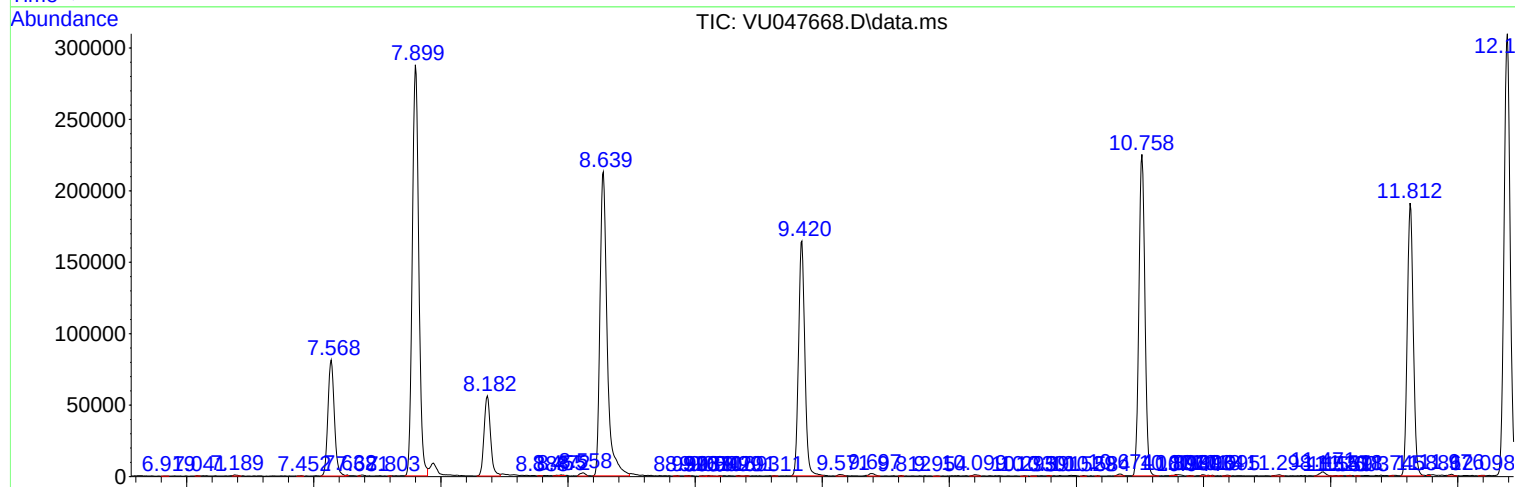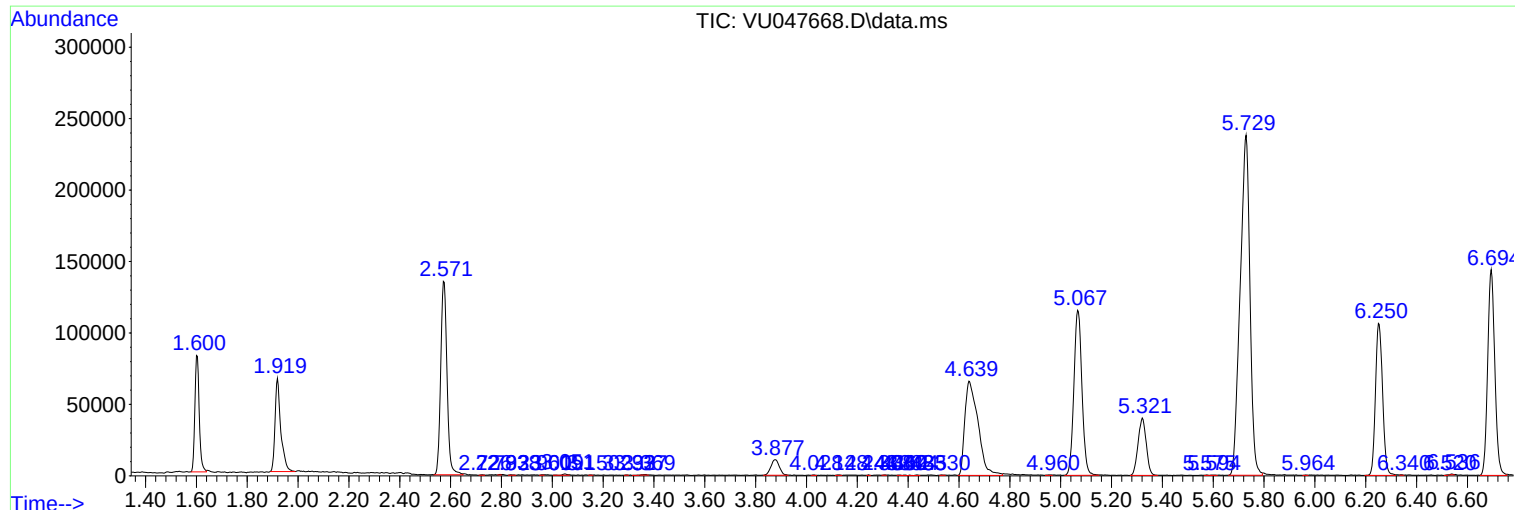

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047668.D
Acq On : 25 Mar 2022 12:34
Operator : SY/MD
Sample : N2081-02DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047668.D
Acq On : 25 Mar 2022 12:34
Operator : SY/MD
Sample : N2081-02DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------