

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047669.D
 Acq On : 25 Mar 2022 12:57
 Operator : SY/MD
 Sample : N2081-05DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	103	rVB	109994	131656	15.24%	2.016%
2	1.919	171	180	201	rBV	88463	123043	14.25%	1.885%
3	2.366	317	319	321	rBV	711	308	0.04%	0.005%
4	2.571	370	383	411	rBV	190138	322347	37.32%	4.937%
5	2.713	424	427	430	rBV	267	198	0.02%	0.003%
6	2.777	444	447	449	rBV2	309	174	0.02%	0.003%
7	3.054	528	533	540	rVB6	968	1274	0.15%	0.020%
8	3.121	551	554	557	rBV2	210	187	0.02%	0.003%
9	3.353	623	626	628	rBV	245	177	0.02%	0.003%
10	3.478	662	665	671	rVV3	218	212	0.02%	0.003%
11	3.549	684	687	690	rVB2	352	231	0.03%	0.004%
12	3.594	699	701	705	rVV2	283	215	0.02%	0.003%
13	3.623	705	710	714	rVB2	261	273	0.03%	0.004%
14	3.751	747	750	754	rBV2	212	223	0.03%	0.003%
15	3.780	756	759	764	rVB2	197	185	0.02%	0.003%
16	3.809	764	768	772	rBV3	191	189	0.02%	0.003%
17	3.874	772	788	805	rBV2	13702	33038	3.83%	0.506%
18	4.012	827	831	833	rBV2	325	181	0.02%	0.003%
19	4.025	833	835	843	rVB3	281	181	0.02%	0.003%
20	4.089	851	855	858	rBV2	276	269	0.03%	0.004%
21	4.295	916	919	922	rBV2	262	208	0.02%	0.003%
22	4.404	950	953	956	rBV3	262	173	0.02%	0.003%
23	4.636	1008	1025	1059	rBV2	88932	263523	30.51%	4.036%
24	4.883	1100	1102	1109	rVB3	361	251	0.03%	0.004%
25	5.066	1143	1159	1184	rVV	155408	343483	39.77%	5.261%
26	5.321	1222	1238	1256	rBV2	86584	196491	22.75%	3.009%
27	5.729	1341	1365	1385	rBV2	321077	863706	100.00%	13.229%
28	5.925	1421	1426	1431	rVB3	352	330	0.04%	0.005%
29	5.947	1431	1433	1436	rBV2	271	172	0.02%	0.003%
30	5.964	1436	1438	1442	rVB2	263	190	0.02%	0.003%
31	6.083	1469	1475	1477	rBV2	191	179	0.02%	0.003%
32	6.111	1481	1484	1488	rVB3	301	236	0.03%	0.004%
33	6.153	1493	1497	1500	rBV2	276	200	0.02%	0.003%
34	6.250	1513	1527	1544	rBV	150927	288821	33.44%	4.424%
35	6.430	1580	1583	1586	rBV2	259	174	0.02%	0.003%
36	6.546	1611	1619	1627	rVV6	3287	6002	0.69%	0.092%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047669.D
 Acq On : 25 Mar 2022 12:57
 Operator : SY/MD
 Sample : N2081-05DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.603	1633	1637	1643	rVB2	393	396	0.05%	0.006%
38	6.693	1649	1665	1685	rBV	195834	385113	44.59%	5.898%
39	6.931	1737	1739	1744	rVB2	220	177	0.02%	0.003%
40	6.970	1749	1751	1755	rBV2	232	170	0.02%	0.003%
41	7.041	1770	1773	1774	rBV2	317	187	0.02%	0.003%
42	7.192	1810	1820	1833	rVB5	1275	2625	0.30%	0.040%
43	7.298	1850	1853	1859	rVB2	319	287	0.03%	0.004%
44	7.369	1870	1875	1878	rBV2	248	216	0.03%	0.003%
45	7.459	1896	1903	1905	rBV2	263	253	0.03%	0.004%
46	7.510	1916	1919	1921	rBV2	256	214	0.02%	0.003%
47	7.568	1924	1937	1957	rBV	107931	190923	22.11%	2.924%
48	7.690	1968	1975	1976	rBV4	659	630	0.07%	0.010%
49	7.796	2005	2008	2010	rBV3	365	274	0.03%	0.004%
50	7.899	2026	2040	2057	rBV	392461	690669	79.97%	10.578%
51	8.182	2116	2128	2147	rBV	77576	132305	15.32%	2.026%
52	8.468	2207	2217	2218	rBV4	1116	1153	0.13%	0.018%
53	8.555	2235	2244	2253	rBV3	9954	15696	1.82%	0.240%
54	8.639	2257	2270	2304	rBV	288778	559493	64.78%	8.569%
55	9.015	2384	2387	2390	rVB2	280	173	0.02%	0.003%
56	9.044	2390	2396	2397	rBV	306	223	0.03%	0.003%
57	9.079	2403	2407	2410	rVB2	382	310	0.04%	0.005%
58	9.105	2412	2415	2422	rVB2	440	509	0.06%	0.008%
59	9.172	2434	2436	2442	rVB	260	179	0.02%	0.003%
60	9.259	2461	2463	2468	rVB2	342	280	0.03%	0.004%
61	9.298	2471	2475	2479	rBV2	502	501	0.06%	0.008%
62	9.417	2498	2512	2539	rBV	227546	391877	45.37%	6.002%
63	9.661	2583	2588	2589	rBV2	245	190	0.02%	0.003%
64	9.697	2593	2599	2605	rBV3	862	1125	0.13%	0.017%
65	9.774	2617	2623	2628	rVB2	358	450	0.05%	0.007%
66	9.819	2633	2637	2641	rBV2	227	214	0.02%	0.003%
67	9.870	2647	2653	2656	rBV2	212	265	0.03%	0.004%
68	9.951	2674	2678	2684	rBV3	273	314	0.04%	0.005%
69	10.095	2720	2723	2729	rVV3	386	358	0.04%	0.005%
70	10.256	2769	2773	2775	rBV	249	224	0.03%	0.003%
71	10.394	2810	2816	2819	rBV2	301	263	0.03%	0.004%
72	10.536	2855	2860	2866	rBV	234	214	0.02%	0.003%
73	10.626	2884	2888	2892	rBV	268	237	0.03%	0.004%
74	10.674	2896	2903	2907	rVV2	1834	2163	0.25%	0.033%
75	10.758	2915	2929	2949	rVB	302435	487119	56.40%	7.461%
76	10.896	2955	2972	2983	rBV5	2333	5001	0.58%	0.077%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047669.D
 Acq On : 25 Mar 2022 12:57
 Operator : SY/MD
 Sample : N2081-05DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.963	2988	2993	2998	rVB2	322	329	0.04%	0.005%
78	10.989	2998	3001	3004	rBV2	303	191	0.02%	0.003%
79	11.169	3054	3057	3066	rVB2	265	305	0.04%	0.005%
80	11.414	3128	3133	3136	rBV2	380	343	0.04%	0.005%
81	11.452	3142	3145	3147	rBV2	935	668	0.08%	0.010%
82	11.619	3193	3197	3200	rBV	258	176	0.02%	0.003%
83	11.693	3215	3220	3223	rBV3	702	702	0.08%	0.011%
84	11.745	3231	3236	3241	rVB4	523	522	0.06%	0.008%
85	11.812	3245	3257	3275	rBV	254165	401717	46.51%	6.153%
86	11.938	3292	3296	3299	rBV3	714	562	0.07%	0.009%
87	11.973	3305	3307	3315	rVB3	955	911	0.11%	0.014%
88	12.195	3362	3376	3393	rBV	406796	666531	77.17%	10.209%
89	12.288	3402	3405	3407	rBV	361	203	0.02%	0.003%
90	12.327	3414	3417	3418	rBV	354	192	0.02%	0.003%
91	12.478	3461	3464	3467	rBV	281	194	0.02%	0.003%
92	12.780	3552	3558	3561	rBV3	499	496	0.06%	0.008%
93	12.860	3581	3583	3586	rVB2	347	204	0.02%	0.003%
94	12.889	3586	3592	3593	rBV2	365	441	0.05%	0.007%
95	13.111	3658	3661	3662	rBV2	371	200	0.02%	0.003%
96	13.214	3688	3693	3695	rBV2	401	349	0.04%	0.005%
97	13.539	3788	3794	3798	rBV2	505	588	0.07%	0.009%
98	13.796	3870	3874	3878	rBV2	300	316	0.04%	0.005%
99	13.851	3886	3891	3894	rBV2	419	446	0.05%	0.007%
100	15.243	4321	4324	4329	rBV2	794	780	0.09%	0.012%




Sum of corrected areas: 6529036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047669.D
Acq On : 25 Mar 2022 12:57
Operator : SY/MD
Sample : N2081-05DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

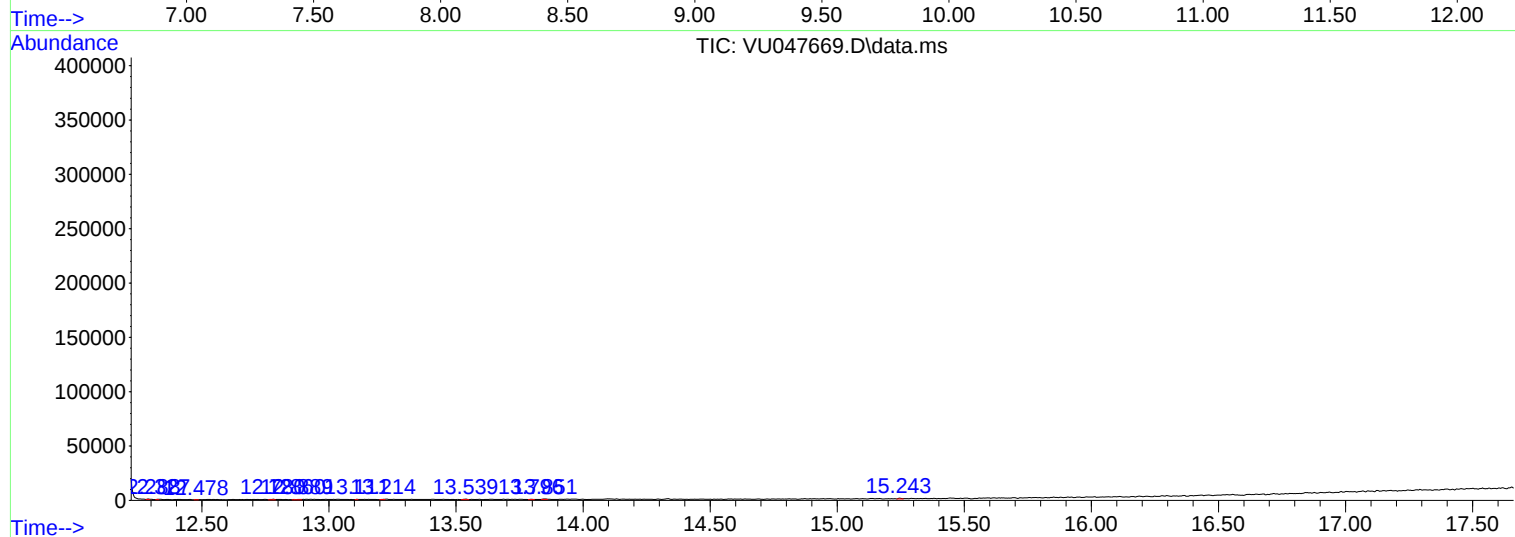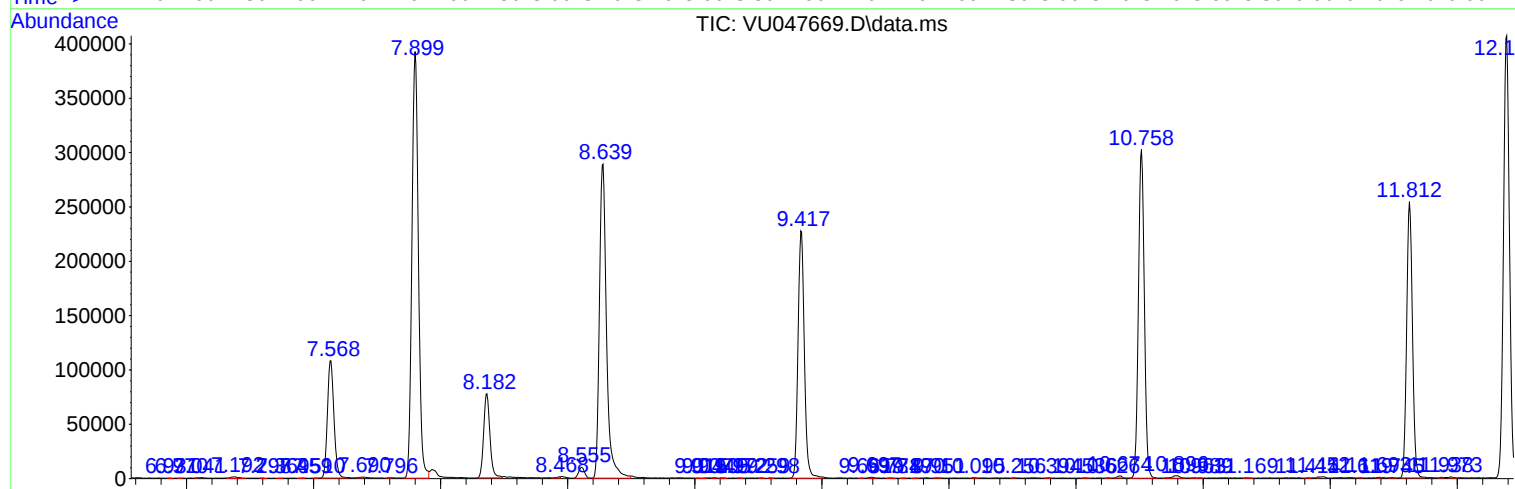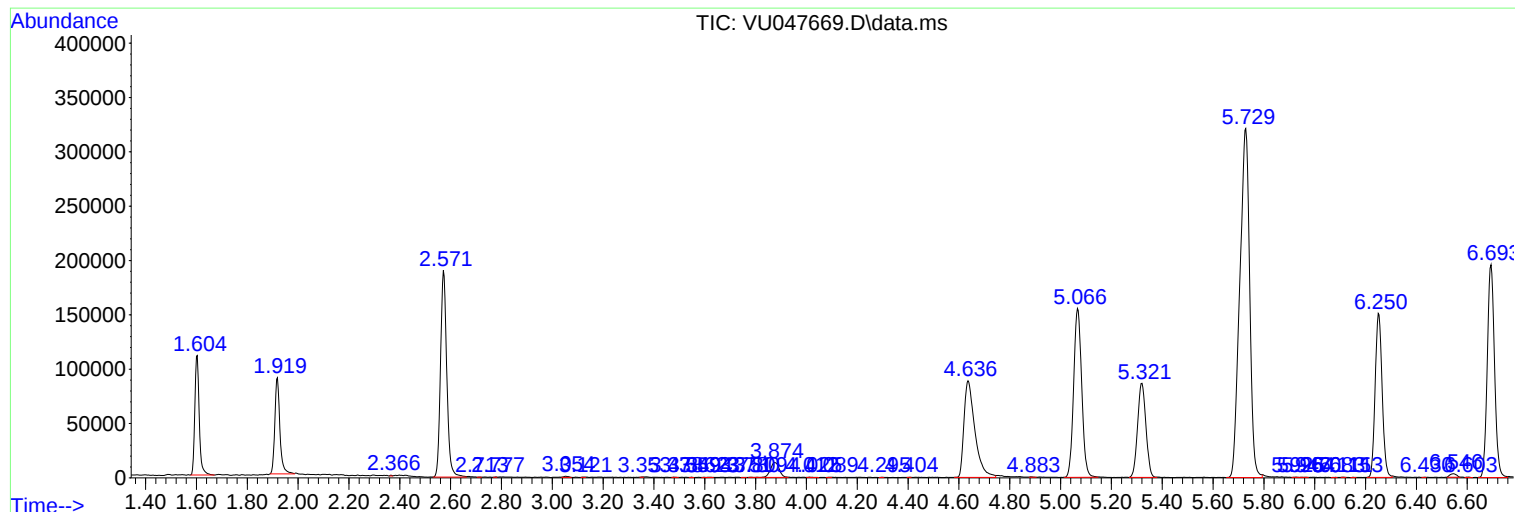

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047669.D
Acq On : 25 Mar 2022 12:57
Operator : SY/MD
Sample : N2081-05DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047669.D
Acq On : 25 Mar 2022 12:57
Operator : SY/MD
Sample : N2081-05DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------