

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047673.D
 Acq On : 25 Mar 2022 15:07
 Operator : SY/MD
 Sample : N2081-10DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047673.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	105	rVB	162516	192842	12.04%	1.548%
2	1.915	171	179	200	rVB	135861	185508	11.58%	1.489%
3	2.491	356	358	363	rBV3	271	224	0.01%	0.002%
4	2.571	371	383	404	rBV	281418	473868	29.58%	3.805%
5	3.015	515	521	526	rBV2	269	350	0.02%	0.003%
6	3.047	526	531	539	rVB2	1116	1793	0.11%	0.014%
7	3.166	563	568	573	rVV2	264	327	0.02%	0.003%
8	3.218	581	584	588	rVB2	431	356	0.02%	0.003%
9	3.247	588	593	597	rBV2	161	203	0.01%	0.002%
10	3.356	614	627	641	rBV4	3256	6678	0.42%	0.054%
11	3.478	657	665	671	rBV3	302	484	0.03%	0.004%
12	3.706	732	736	739	rBV2	235	221	0.01%	0.002%
13	3.874	770	788	811	rBV	113281	267021	16.67%	2.144%
14	4.054	839	844	846	rBV	248	219	0.01%	0.002%
15	4.298	912	920	927	rBV2	309	418	0.03%	0.003%
16	4.330	927	930	932	rBV	273	213	0.01%	0.002%
17	4.501	980	983	987	rVB2	264	201	0.01%	0.002%
18	4.668	1010	1035	1069	rBV2	565498	1601975	100.00%	12.862%
19	4.999	1135	1138	1141	rVB3	441	308	0.02%	0.002%
20	5.066	1141	1159	1180	rBV	232097	508270	31.73%	4.081%
21	5.321	1221	1238	1255	rBV	111673	254191	15.87%	2.041%
22	5.616	1325	1330	1332	rBV	344	331	0.02%	0.003%
23	5.726	1340	1364	1399	rBV2	474388	1291392	80.61%	10.368%
24	6.038	1456	1461	1464	rVV2	360	423	0.03%	0.003%
25	6.115	1481	1485	1488	rBV2	390	304	0.02%	0.002%
26	6.182	1503	1506	1512	rVB3	199	211	0.01%	0.002%
27	6.250	1512	1527	1551	rBV	339544	645501	40.29%	5.183%
28	6.398	1568	1573	1580	rBV2	345	488	0.03%	0.004%
29	6.539	1607	1617	1618	rBV4	1329	1525	0.10%	0.012%
30	6.597	1633	1635	1638	rVB	762	425	0.03%	0.003%
31	6.619	1638	1642	1644	rBV2	288	219	0.01%	0.002%
32	6.693	1650	1665	1692	rBV	295348	575704	35.94%	4.622%
33	6.886	1720	1725	1729	rBV	325	362	0.02%	0.003%
34	6.980	1750	1754	1756	rBV2	308	242	0.02%	0.002%
35	7.041	1768	1773	1780	rVV3	450	634	0.04%	0.005%
36	7.115	1793	1796	1801	rBV2	189	200	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047673.D
 Acq On : 25 Mar 2022 15:07
 Operator : SY/MD
 Sample : N2081-10DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.189	1809	1819	1833	rVB6	1953	4139	0.26%	0.033%
38	7.314	1855	1858	1862	rVB	307	211	0.01%	0.002%
39	7.340	1862	1866	1869	rBV	323	252	0.02%	0.002%
40	7.446	1895	1899	1903	rBV3	254	280	0.02%	0.002%
41	7.500	1911	1916	1920	rBV2	293	339	0.02%	0.003%
42	7.568	1920	1937	1960	rBV	164595	291891	18.22%	2.344%
43	7.687	1969	1974	1984	rBV5	1404	2164	0.14%	0.017%
44	7.796	1998	2008	2012	rBV4	1940	2636	0.16%	0.021%
45	7.899	2021	2040	2054	rBV	602289	1043498	65.14%	8.378%
46	7.970	2056	2062	2076	rVB	34993	58089	3.63%	0.466%
47	8.179	2115	2127	2146	rBV	117471	201011	12.55%	1.614%
48	8.359	2177	2183	2189	rVB4	452	669	0.04%	0.005%
49	8.391	2189	2193	2194	rBV2	418	278	0.02%	0.002%
50	8.558	2239	2245	2246	rBV3	545	493	0.03%	0.004%
51	8.635	2256	2269	2305	rBV	472459	866883	54.11%	6.960%
52	9.066	2399	2403	2408	rVB2	341	298	0.02%	0.002%
53	9.176	2434	2437	2440	rVB3	318	229	0.01%	0.002%
54	9.279	2465	2469	2474	rBV3	243	328	0.02%	0.003%
55	9.417	2499	2512	2550	rVB	510919	849168	53.01%	6.818%
56	9.571	2551	2560	2574	rVB2	11842	18626	1.16%	0.150%
57	9.693	2585	2598	2610	rBV	35607	58232	3.64%	0.468%
58	9.915	2663	2667	2671	rBV2	351	397	0.02%	0.003%
59	10.066	2707	2714	2715	rBV2	307	313	0.02%	0.003%
60	10.102	2715	2725	2738	rVV	21734	35574	2.22%	0.286%
61	10.205	2755	2757	2763	rVV3	306	229	0.01%	0.002%
62	10.250	2768	2771	2776	rVB3	296	289	0.02%	0.002%
63	10.487	2836	2845	2852	rVB3	1521	2433	0.15%	0.020%
64	10.639	2887	2892	2895	rVB2	264	242	0.02%	0.002%
65	10.671	2895	2902	2910	rVB3	2561	3564	0.22%	0.029%
66	10.758	2910	2929	2950	rBV	462013	735814	45.93%	5.908%
67	10.832	2950	2952	2957	rVB3	519	345	0.02%	0.003%
68	10.870	2957	2964	2965	rBV3	722	777	0.05%	0.006%
69	10.905	2968	2975	2988	rVB2	6219	9706	0.61%	0.078%
70	10.999	2994	3004	3010	rBV	23037	38525	2.40%	0.309%
71	11.086	3023	3031	3047	rVB	14721	23046	1.44%	0.185%
72	11.153	3050	3052	3055	rBV2	362	260	0.02%	0.002%
73	11.201	3063	3067	3074	rBV3	348	437	0.03%	0.004%
74	11.295	3085	3096	3107	rBV	16943	25708	1.60%	0.206%
75	11.468	3139	3150	3165	rBV	69637	107747	6.73%	0.865%
76	11.613	3191	3195	3197	rBV3	522	417	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047673.D
 Acq On : 25 Mar 2022 15:07
 Operator : SY/MD
 Sample : N2081-10DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.645	3201	3205	3214	rVB3	1080	1203	0.08%	0.010%
78	11.696	3214	3221	3229	rBV4	1269	1830	0.11%	0.015%
79	11.745	3230	3236	3244	rBV3	1463	2027	0.13%	0.016%
80	11.812	3244	3257	3273	rBV	578678	913363	57.01%	7.333%
81	11.896	3273	3283	3293	rVB	25396	37903	2.37%	0.304%
82	12.092	3336	3344	3362	rBV6	9628	19419	1.21%	0.156%
83	12.195	3362	3376	3393	rVV	637805	1036883	64.73%	8.325%
84	12.317	3412	3414	3416	rBV2	454	252	0.02%	0.002%
85	12.333	3417	3419	3423	rVB3	887	547	0.03%	0.004%
86	12.381	3429	3434	3438	rBV2	867	675	0.04%	0.005%
87	12.487	3451	3467	3479	rBV3	8405	19042	1.19%	0.153%
88	12.571	3486	3493	3502	rBV3	2975	3801	0.24%	0.031%
89	12.684	3521	3528	3531	rBV2	859	991	0.06%	0.008%
90	12.880	3582	3589	3597	rBV4	912	1331	0.08%	0.011%
91	12.947	3608	3610	3612	rBV	369	250	0.02%	0.002%
92	13.028	3628	3635	3643	rVB5	2297	3064	0.19%	0.025%
93	13.449	3763	3766	3781	rVB5	2312	3634	0.23%	0.029%
94	13.507	3781	3784	3786	rBV2	367	293	0.02%	0.002%
95	14.092	3959	3966	3978	rBV2	3865	5526	0.34%	0.044%
96	14.638	4132	4136	4139	rBV2	422	463	0.03%	0.004%
97	15.044	4260	4262	4267	rBV3	736	521	0.03%	0.004%
98	15.105	4278	4281	4283	rBV2	855	628	0.04%	0.005%
99	15.272	4326	4333	4338	rBV2	1234	1650	0.10%	0.013%
100	15.372	4361	4364	4368	rBV3	692	541	0.03%	0.004%




Sum of corrected areas: 12455005

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047673.D
Acq On : 25 Mar 2022 15:07
Operator : SY/MD
Sample : N2081-10DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

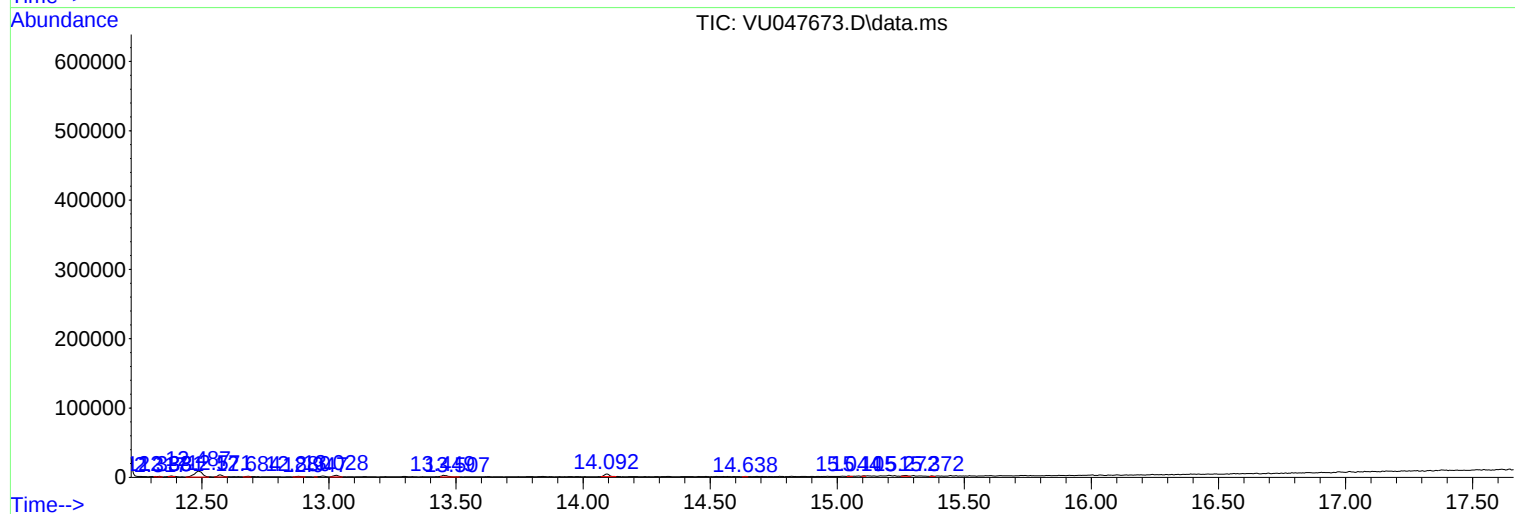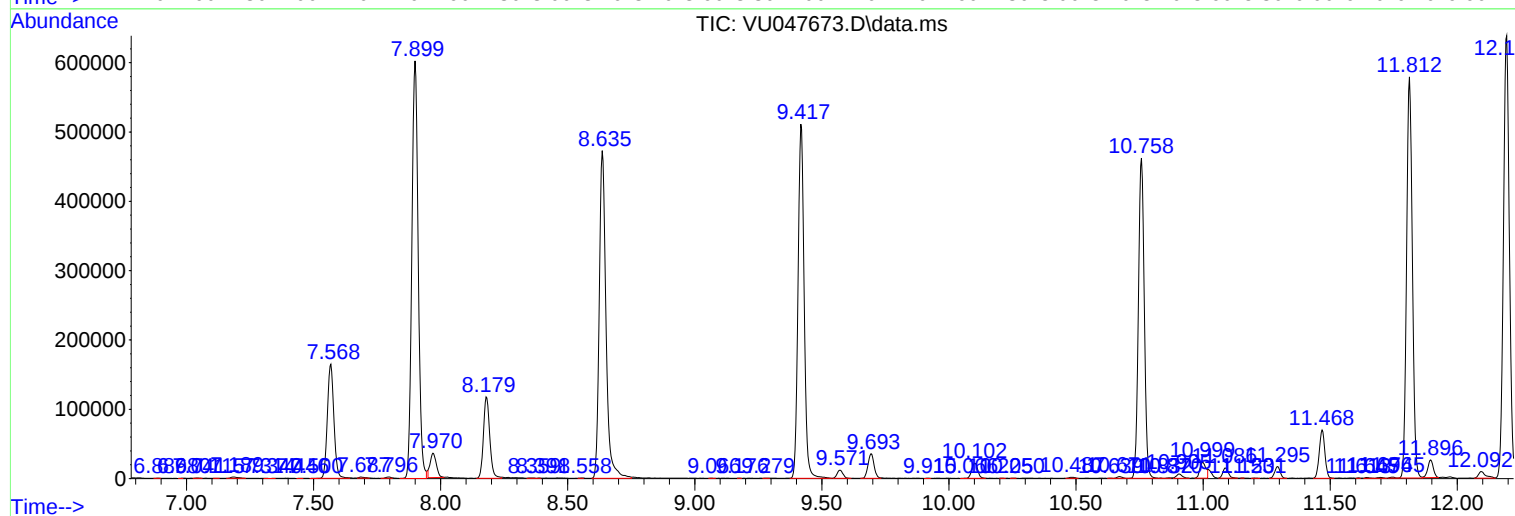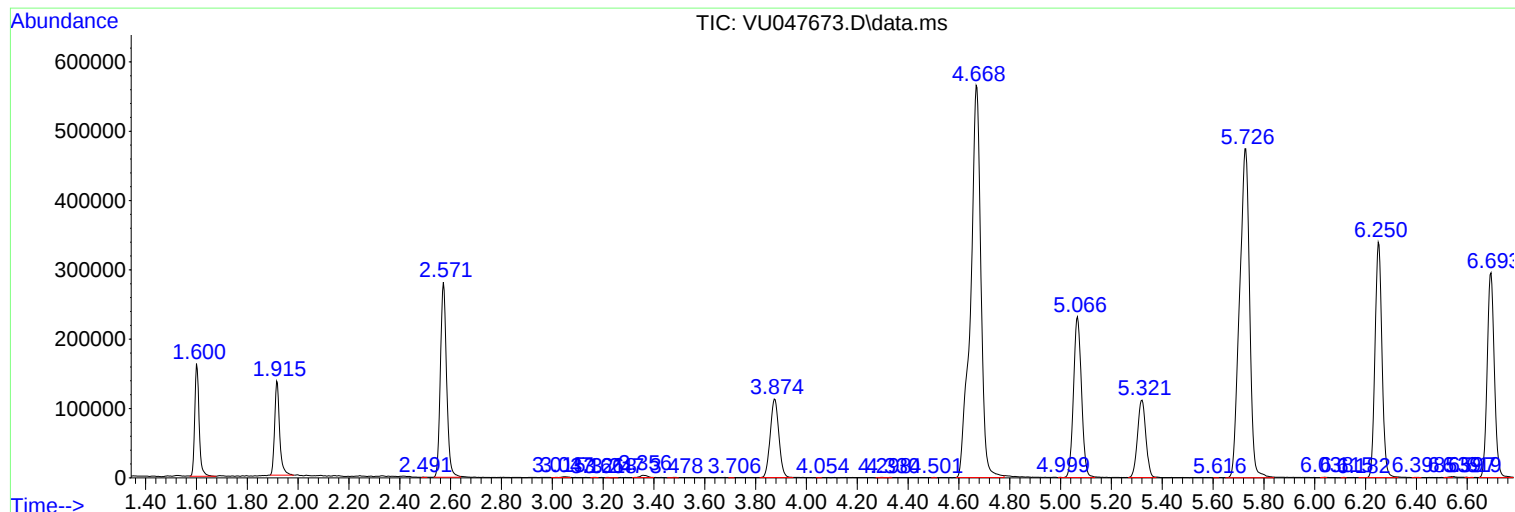

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047673.D
Acq On : 25 Mar 2022 15:07
Operator : SY/MD
Sample : N2081-10DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047673.D
Acq On : 25 Mar 2022 15:07
Operator : SY/MD
Sample : N2081-10DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------