

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047674.D
 Acq On : 25 Mar 2022 15:30
 Operator : SY/MD
 Sample : N2081-11DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047674.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rBV	145420	171387	14.50%	1.835%
2	1.916	171	179	198	rBV	114723	160038	13.54%	1.713%
3	2.572	370	383	405	rBV	252265	427854	36.19%	4.580%
4	2.732	431	433	437	rBV2	267	190	0.02%	0.002%
5	2.800	450	454	463	rVB3	477	649	0.05%	0.007%
6	2.861	469	473	478	rBV2	271	277	0.02%	0.003%
7	3.051	526	532	539	rVV5	944	1352	0.11%	0.014%
8	3.137	556	559	563	rBV3	238	220	0.02%	0.002%
9	3.292	600	607	608	rBV	296	233	0.02%	0.002%
10	3.311	610	613	619	rVB2	344	295	0.02%	0.003%
11	3.353	619	626	630	rBV5	1573	2447	0.21%	0.026%
12	3.552	684	688	692	rVB2	221	180	0.02%	0.002%
13	3.584	694	698	704	rBV	181	239	0.02%	0.003%
14	3.668	721	724	728	rBV	242	222	0.02%	0.002%
15	3.739	742	746	748	rVB3	292	220	0.02%	0.002%
16	3.761	748	753	756	rBV	241	272	0.02%	0.003%
17	3.790	758	762	764	rVV3	212	202	0.02%	0.002%
18	3.874	772	788	808	rVB	27630	64834	5.48%	0.694%
19	4.063	843	847	850	rBV	284	253	0.02%	0.003%
20	4.269	908	911	914	rVB2	309	193	0.02%	0.002%
21	4.379	942	945	954	rVB2	222	245	0.02%	0.003%
22	4.430	954	961	965	rVB	299	394	0.03%	0.004%
23	4.507	981	985	989	rBV3	207	194	0.02%	0.002%
24	4.568	1000	1004	1005	rBV	273	184	0.02%	0.002%
25	4.662	1012	1033	1068	rBV2	142358	563980	47.71%	6.037%
26	5.006	1137	1140	1143	rVB2	402	247	0.02%	0.003%
27	5.067	1143	1159	1178	rBV	211030	467224	39.52%	5.001%
28	5.208	1201	1203	1211	rVB2	220	236	0.02%	0.003%
29	5.321	1220	1238	1257	rBV2	154375	346355	29.30%	3.707%
30	5.452	1277	1279	1283	rVB	316	179	0.02%	0.002%
31	5.726	1342	1364	1387	rBV2	438594	1182114	100.00%	12.654%
32	5.996	1446	1448	1451	rVB3	359	217	0.02%	0.002%
33	6.031	1456	1459	1461	rBV2	259	210	0.02%	0.002%
34	6.250	1513	1527	1549	rBV	221519	420210	35.55%	4.498%
35	6.542	1610	1618	1629	rVV5	4158	7644	0.65%	0.082%
36	6.594	1629	1634	1637	rBV4	343	365	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047674.D
 Acq On : 25 Mar 2022 15:30
 Operator : SY/MD
 Sample : N2081-11DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1650	1665	1691	rBV	268306	525775	44.48%	5.628%
38	6.803	1695	1699	1701	rBV3	762	583	0.05%	0.006%
39	7.038	1769	1772	1774	rVV	392	229	0.02%	0.002%
40	7.060	1777	1779	1785	rVB3	490	407	0.03%	0.004%
41	7.189	1810	1819	1825	rBV4	2240	3000	0.25%	0.032%
42	7.356	1868	1871	1875	rVB2	341	231	0.02%	0.002%
43	7.443	1895	1898	1902	rVB2	324	194	0.02%	0.002%
44	7.568	1923	1937	1955	rBV	151163	263807	22.32%	2.824%
45	7.687	1970	1974	1983	rVB6	1500	1951	0.17%	0.021%
46	7.729	1985	1987	1992	rVB4	384	226	0.02%	0.002%
47	7.761	1992	1997	1999	rBV3	342	278	0.02%	0.003%
48	7.806	2008	2011	2016	rBV2	301	304	0.03%	0.003%
49	7.899	2026	2040	2056	rBV	543439	943693	79.83%	10.101%
50	8.179	2113	2127	2152	rBV	107370	189285	16.01%	2.026%
51	8.446	2206	2210	2214	rBV2	352	392	0.03%	0.004%
52	8.475	2215	2219	2224	rVB2	599	641	0.05%	0.007%
53	8.555	2235	2244	2257	rVB3	10171	16930	1.43%	0.181%
54	8.636	2257	2269	2317	rBV	425550	800077	67.68%	8.564%
55	8.803	2317	2321	2325	rVB3	369	323	0.03%	0.003%
56	8.919	2354	2357	2360	rVB2	326	188	0.02%	0.002%
57	9.166	2431	2434	2437	rBV2	272	198	0.02%	0.002%
58	9.182	2437	2439	2443	rVB3	313	179	0.02%	0.002%
59	9.372	2491	2498	2500	rBV2	339	411	0.03%	0.004%
60	9.417	2500	2512	2541	rVV	324875	559214	47.31%	5.986%
61	9.565	2555	2558	2559	rBV	385	216	0.02%	0.002%
62	9.620	2569	2575	2577	rBV2	370	299	0.03%	0.003%
63	9.693	2590	2598	2606	rBV5	1175	1774	0.15%	0.019%
64	9.854	2644	2648	2652	rVB	300	243	0.02%	0.003%
65	9.992	2686	2691	2695	rBV2	195	241	0.02%	0.003%
66	10.047	2706	2708	2714	rVB2	341	185	0.02%	0.002%
67	10.102	2719	2725	2730	rBV2	497	574	0.05%	0.006%
68	10.221	2759	2762	2768	rBV	254	212	0.02%	0.002%
69	10.382	2808	2812	2815	rBV2	308	236	0.02%	0.003%
70	10.404	2815	2819	2821	rVV	255	211	0.02%	0.002%
71	10.594	2873	2878	2881	rBV2	294	283	0.02%	0.003%
72	10.668	2895	2901	2911	rBV6	2134	3374	0.29%	0.036%
73	10.758	2915	2929	2947	rBV	424761	677764	57.33%	7.255%
74	10.870	2959	2964	2965	rBV	393	349	0.03%	0.004%
75	10.896	2969	2972	2977	rVV4	856	852	0.07%	0.009%
76	10.922	2977	2980	2986	rVB3	682	543	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047674.D
 Acq On : 25 Mar 2022 15:30
 Operator : SY/MD
 Sample : N2081-11DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.092	3030	3033	3037	rVB2	437	362	0.03%	0.004%
78	11.221	3069	3073	3077	rBV2	323	288	0.02%	0.003%
79	11.417	3132	3134	3139	rVB2	256	188	0.02%	0.002%
80	11.462	3139	3148	3158	rVB6	2281	3803	0.32%	0.041%
81	11.671	3209	3213	3215	rBV2	248	238	0.02%	0.003%
82	11.693	3215	3220	3227	rVB3	1149	1373	0.12%	0.015%
83	11.748	3234	3237	3239	rBV	368	185	0.02%	0.002%
84	11.812	3245	3257	3278	rBV	365972	585928	49.57%	6.272%
85	11.976	3303	3308	3318	rVB6	1365	1652	0.14%	0.018%
86	12.095	3342	3345	3347	rBV2	375	264	0.02%	0.003%
87	12.195	3363	3376	3394	rBV	572444	925343	78.28%	9.905%
88	12.285	3402	3404	3408	rVB5	453	269	0.02%	0.003%
89	12.327	3414	3417	3420	rVB3	484	348	0.03%	0.004%
90	12.362	3425	3428	3432	rBV2	252	272	0.02%	0.003%
91	12.417	3441	3445	3447	rBV2	374	256	0.02%	0.003%
92	12.459	3455	3458	3461	rBV	240	213	0.02%	0.002%
93	12.484	3462	3466	3471	rVV2	447	466	0.04%	0.005%
94	12.594	3495	3500	3501	rBV2	259	252	0.02%	0.003%
95	12.745	3544	3547	3552	rBV3	379	277	0.02%	0.003%
96	12.771	3552	3555	3558	rBV	415	375	0.03%	0.004%
97	13.446	3762	3765	3768	rBV	326	236	0.02%	0.003%
98	14.095	3961	3967	3972	rBV2	842	1335	0.11%	0.014%
99	15.163	4296	4299	4304	rBV	454	467	0.04%	0.005%
100	15.372	4362	4364	4367	rBV2	476	331	0.03%	0.004%




Sum of corrected areas: 9342148

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047674.D
Acq On : 25 Mar 2022 15:30
Operator : SY/MD
Sample : N2081-11DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

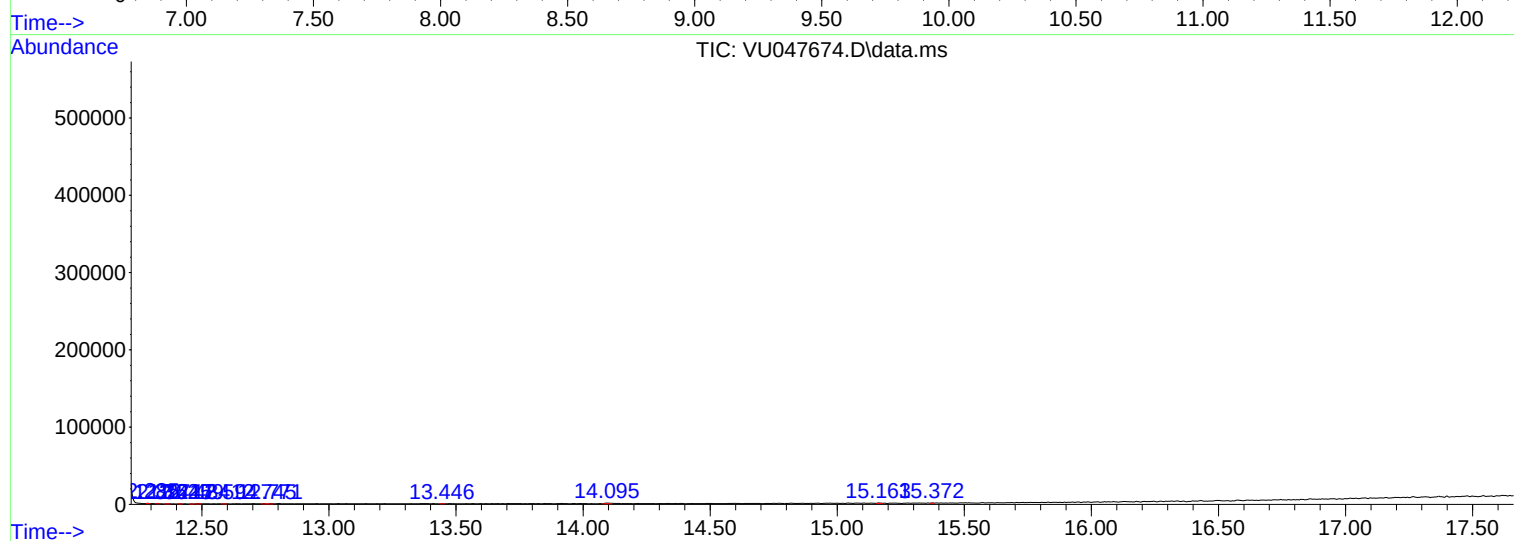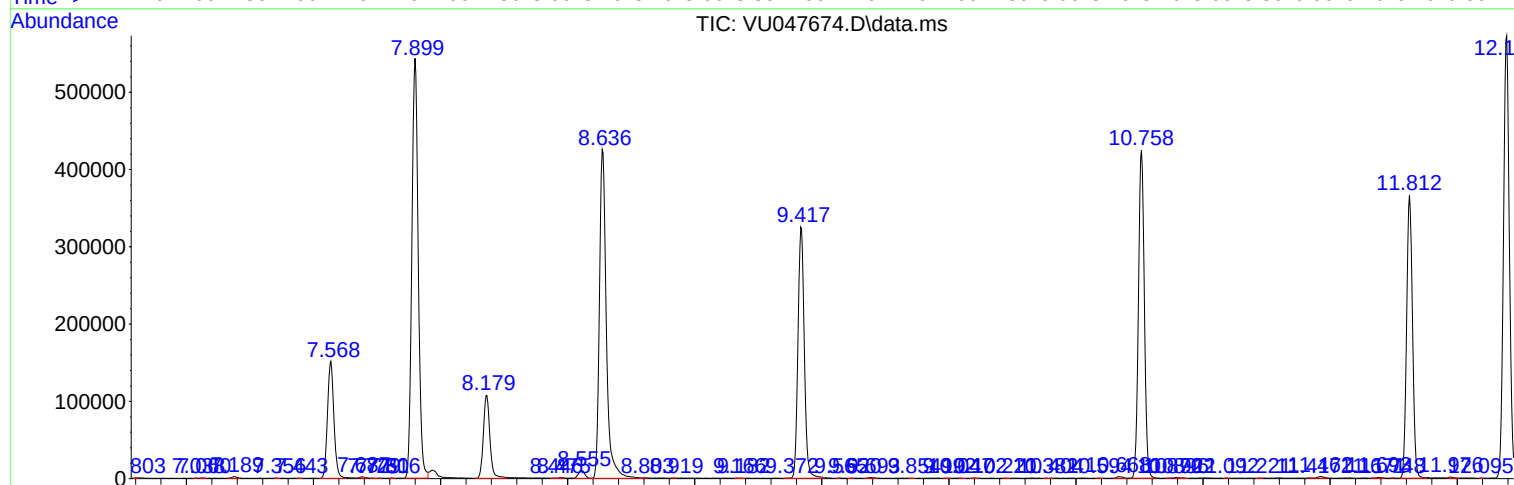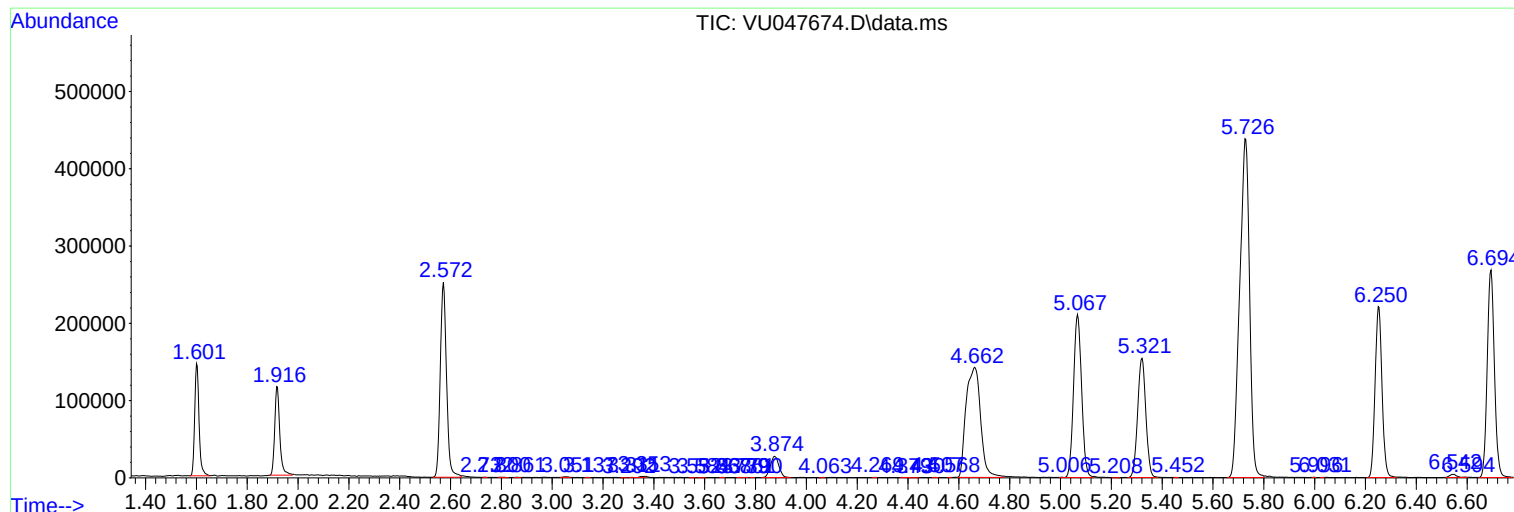

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047674.D
Acq On : 25 Mar 2022 15:30
Operator : SY/MD
Sample : N2081-11DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047674.D
Acq On : 25 Mar 2022 15:30
Operator : SY/MD
Sample : N2081-11DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------