

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047677.D
 Acq On : 25 Mar 2022 17:16
 Operator : SY/MD
 Sample : N2081-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047677.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rBV	123632	145082	3.67%	0.743%
2	1.681	104	106	107	rBV2	872	409	0.01%	0.002%
3	1.916	171	179	194	rBV	97454	133959	3.39%	0.686%
4	2.086	227	232	240	rVB	5898	7581	0.19%	0.039%
5	2.141	241	249	256	rBV	11536	17519	0.44%	0.090%
6	2.456	344	347	352	rVB3	356	260	0.01%	0.001%
7	2.514	363	365	370	rBV2	277	227	0.01%	0.001%
8	2.581	370	386	407	rBV4	832757	1530849	38.76%	7.840%
9	2.784	446	449	450	rBV	728	361	0.01%	0.002%
10	2.957	495	503	505	rBV2	388	409	0.01%	0.002%
11	3.051	526	532	533	rBV3	773	735	0.02%	0.004%
12	3.170	563	569	570	rBV3	340	292	0.01%	0.001%
13	3.234	586	589	597	rVB2	181	211	0.01%	0.001%
14	3.359	616	628	642	rVB2	15432	29770	0.75%	0.152%
15	3.604	701	704	706	rBV2	256	207	0.01%	0.001%
16	3.874	769	788	814	rBV2	389808	921965	23.35%	4.722%
17	4.237	896	901	905	rBV2	214	245	0.01%	0.001%
18	4.523	984	990	995	rBV2	271	337	0.01%	0.002%
19	4.668	1012	1035	1067	rBV2	627311	1623988	41.12%	8.317%
20	4.967	1126	1128	1132	rVB2	402	285	0.01%	0.001%
21	5.067	1139	1159	1183	rBV	197317	474364	12.01%	2.430%
22	5.321	1218	1238	1262	rBV	1768337	3949275	100.00%	20.227%
23	5.533	1297	1304	1314	rVB6	2773	5221	0.13%	0.027%
24	5.607	1325	1327	1332	rBV2	303	277	0.01%	0.001%
25	5.729	1343	1365	1384	rBV2	394716	1052530	26.65%	5.391%
26	5.848	1400	1402	1406	rVB3	521	302	0.01%	0.002%
27	5.980	1434	1443	1445	rVV4	495	581	0.01%	0.003%
28	6.012	1450	1453	1456	rBV2	306	270	0.01%	0.001%
29	6.170	1496	1502	1504	rBV2	319	263	0.01%	0.001%
30	6.250	1512	1527	1552	rBV	398628	765817	19.39%	3.922%
31	6.362	1560	1562	1567	rVB2	454	278	0.01%	0.001%
32	6.546	1603	1619	1647	rBV	860645	1636112	41.43%	8.380%
33	6.694	1652	1665	1689	rVB	245791	472995	11.98%	2.422%
34	6.912	1729	1733	1739	rVB3	225	282	0.01%	0.001%
35	6.999	1755	1760	1762	rBV3	371	345	0.01%	0.002%
36	7.034	1768	1771	1774	rBV2	425	342	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047677.D
 Acq On : 25 Mar 2022 17:16
 Operator : SY/MD
 Sample : N2081-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.105	1790	1793	1801	rVB4	488	598	0.02%	0.003%
38	7.189	1809	1819	1822	rBV5	996	1498	0.04%	0.008%
39	7.231	1829	1832	1837	rVB	487	405	0.01%	0.002%
40	7.260	1837	1841	1846	rBV3	592	536	0.01%	0.003%
41	7.375	1871	1877	1878	rBV2	294	242	0.01%	0.001%
42	7.417	1886	1890	1892	rBV	352	309	0.01%	0.002%
43	7.501	1914	1916	1922	rVB	270	206	0.01%	0.001%
44	7.568	1922	1937	1959	rBV	130476	229858	5.82%	1.177%
45	7.681	1971	1972	1974	rBV2	541	230	0.01%	0.001%
46	7.787	2000	2005	2006	rBV2	567	409	0.01%	0.002%
47	7.796	2006	2008	2010	rBV2	460	314	0.01%	0.002%
48	7.899	2026	2040	2056	rBV	498377	867051	21.95%	4.441%
49	8.118	2105	2108	2114	rBV2	234	263	0.01%	0.001%
50	8.182	2116	2128	2147	rBV	90766	157115	3.98%	0.805%
51	8.404	2185	2197	2208	rBV3	21496	36653	0.93%	0.188%
52	8.475	2209	2219	2230	rVB	6403	11333	0.29%	0.058%
53	8.555	2230	2244	2259	rBV	685686	1160472	29.38%	5.943%
54	8.639	2259	2270	2308	rVB	354529	672926	17.04%	3.446%
55	8.838	2330	2332	2335	rVB2	603	332	0.01%	0.002%
56	8.864	2335	2340	2344	rBV4	459	473	0.01%	0.002%
57	8.883	2344	2346	2351	rBV2	345	301	0.01%	0.002%
58	8.973	2371	2374	2379	rBV	560	494	0.01%	0.003%
59	9.041	2392	2395	2399	rBV2	274	252	0.01%	0.001%
60	9.420	2498	2513	2549	rVB	596684	1009448	25.56%	5.170%
61	9.571	2555	2560	2569	rVB2	1023	1594	0.04%	0.008%
62	9.655	2584	2586	2590	rVB2	410	282	0.01%	0.001%
63	9.694	2590	2598	2608	rBV6	1633	2751	0.07%	0.014%
64	9.941	2674	2675	2682	rVB3	267	223	0.01%	0.001%
65	10.086	2716	2720	2721	rBV2	350	215	0.01%	0.001%
66	10.105	2721	2726	2735	rVB7	1156	1957	0.05%	0.010%
67	10.449	2829	2833	2837	rBV2	429	325	0.01%	0.002%
68	10.484	2838	2844	2845	rBV	700	514	0.01%	0.003%
69	10.562	2866	2868	2873	rVB3	285	225	0.01%	0.001%
70	10.629	2887	2889	2895	rVB2	382	308	0.01%	0.002%
71	10.674	2895	2903	2910	rBV4	1822	2440	0.06%	0.012%
72	10.758	2916	2929	2948	rBV	373685	601685	15.24%	3.082%
73	10.825	2948	2950	2957	rVB5	571	603	0.02%	0.003%
74	10.893	2961	2971	2981	rBV3	10193	17406	0.44%	0.089%
75	11.086	3026	3031	3034	rVV3	641	743	0.02%	0.004%
76	11.115	3038	3040	3044	rVB3	598	372	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047677.D
 Acq On : 25 Mar 2022 17:16
 Operator : SY/MD
 Sample : N2081-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.333	3102	3108	3110	rBV2	236	220	0.01%	0.001%
78	11.404	3125	3130	3135	rBV2	282	303	0.01%	0.002%
79	11.433	3135	3139	3141	rVV2	285	215	0.01%	0.001%
80	11.472	3141	3151	3161	rVB7	2825	4620	0.12%	0.024%
81	11.523	3163	3167	3172	rVB2	336	313	0.01%	0.002%
82	11.697	3214	3221	3227	rVB4	689	1059	0.03%	0.005%
83	11.748	3227	3237	3243	rBV5	1340	2167	0.05%	0.011%
84	11.812	3244	3257	3280	rVV	679929	1073974	27.19%	5.500%
85	11.899	3280	3284	3287	rVV5	401	326	0.01%	0.002%
86	11.973	3303	3307	3314	rVB6	1088	1257	0.03%	0.006%
87	12.195	3362	3376	3394	rBV	527631	850328	21.53%	4.355%
88	12.327	3414	3417	3423	rVB3	828	547	0.01%	0.003%
89	12.465	3457	3460	3462	rBV2	323	206	0.01%	0.001%
90	12.533	3478	3481	3486	rBV2	386	349	0.01%	0.002%
91	12.732	3539	3543	3545	rVB2	371	234	0.01%	0.001%
92	12.777	3545	3557	3568	rBV4	2244	4007	0.10%	0.021%
93	13.227	3690	3697	3709	rVB4	1907	3011	0.08%	0.015%
94	13.607	3811	3815	3823	rVB4	479	600	0.02%	0.003%
95	13.848	3883	3890	3898	rVB2	2921	3661	0.09%	0.019%
96	14.012	3937	3941	3943	rBV2	438	432	0.01%	0.002%
97	14.092	3957	3966	3981	rVB	8517	13630	0.35%	0.070%
98	14.234	4006	4010	4014	rBV2	322	338	0.01%	0.002%
99	14.333	4034	4041	4051	rBV3	4230	5730	0.15%	0.029%
100	14.394	4057	4060	4062	rBV	435	289	0.01%	0.001%




Sum of corrected areas: 19525122

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047677.D
Acq On : 25 Mar 2022 17:16
Operator : SY/MD
Sample : N2081-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

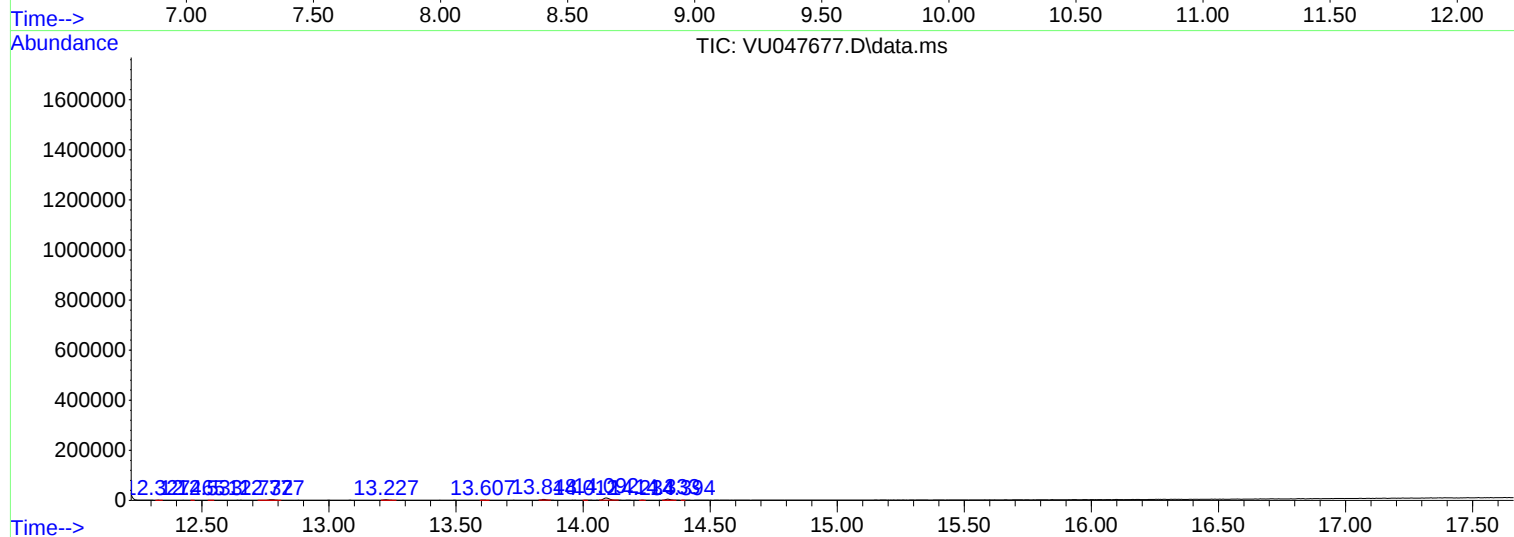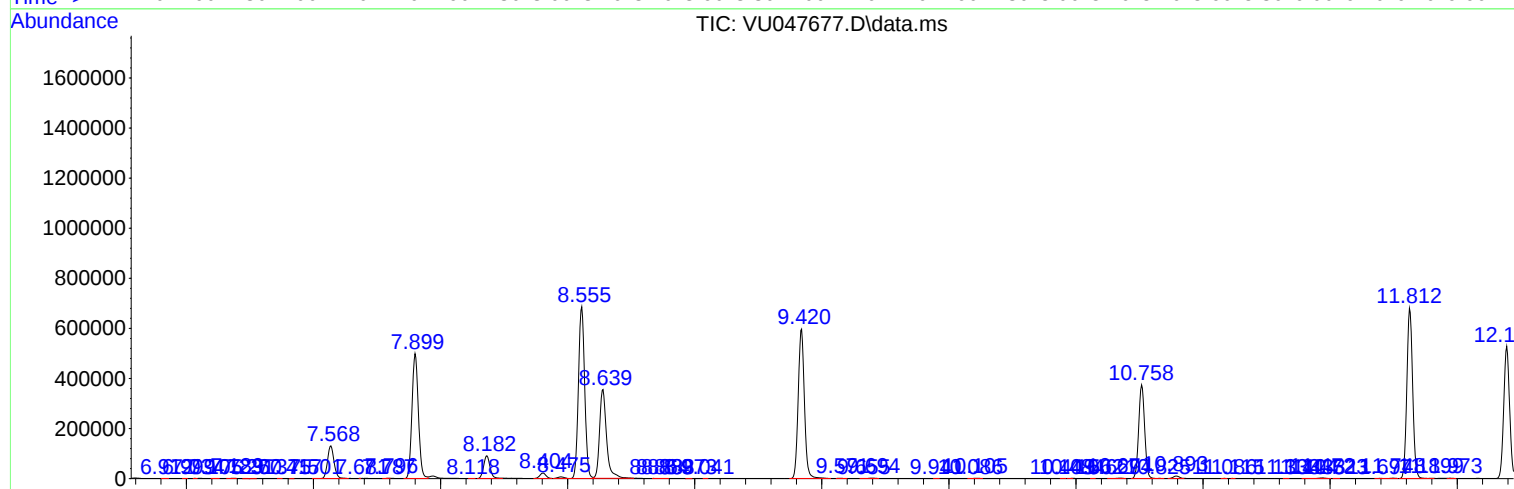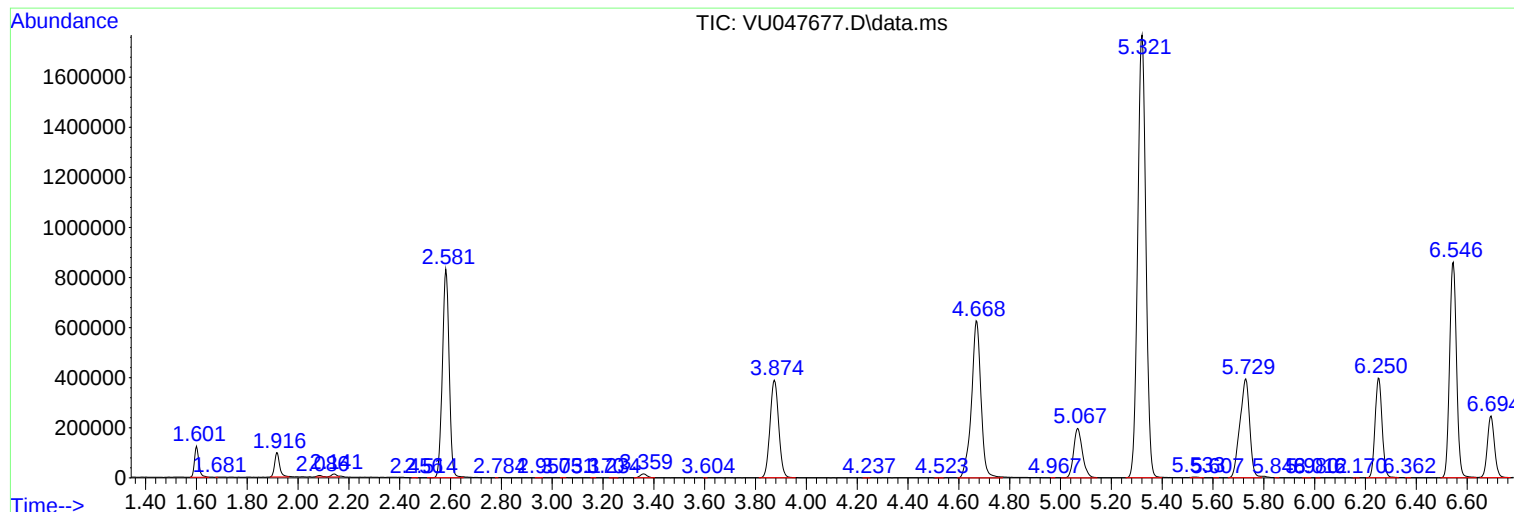

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047677.D
Acq On : 25 Mar 2022 17:16
Operator : SY/MD
Sample : N2081-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047677.D
Acq On : 25 Mar 2022 17:16
Operator : SY/MD
Sample : N2081-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------