

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047680.D
 Acq On : 25 Mar 2022 18:24
 Operator : SY/MD
 Sample : N2082-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW618

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rBV	121515	142639	7.31%	1.144%
2	1.916	170	179	196	rBV	97992	136694	7.01%	1.096%
3	2.507	361	363	367	rVB	434	213	0.01%	0.002%
4	2.572	370	383	409	rBV2	246198	441989	22.65%	3.544%
5	2.732	430	433	441	rVB4	637	688	0.04%	0.006%
6	2.768	441	444	448	rBV3	331	311	0.02%	0.002%
7	2.797	448	453	457	rVV	724	813	0.04%	0.007%
8	2.835	461	465	469	rBV	261	217	0.01%	0.002%
9	2.996	510	515	522	rBV2	403	461	0.02%	0.004%
10	3.047	527	531	538	rVB4	701	930	0.05%	0.007%
11	3.102	544	548	553	rVB2	247	210	0.01%	0.002%
12	3.157	560	565	566	rBV	304	240	0.01%	0.002%
13	3.228	583	587	594	rBV3	304	362	0.02%	0.003%
14	3.359	615	628	645	rBV2	18921	38039	1.95%	0.305%
15	3.874	771	788	808	rBV	151603	352419	18.06%	2.826%
16	3.996	823	826	830	rVB2	277	232	0.01%	0.002%
17	4.121	863	865	870	rVB	418	286	0.01%	0.002%
18	4.154	870	875	880	rBV2	255	394	0.02%	0.003%
19	4.186	880	885	888	rBV2	195	240	0.01%	0.002%
20	4.317	923	926	931	rBV2	362	348	0.02%	0.003%
21	4.353	935	937	941	rVV	365	255	0.01%	0.002%
22	4.549	995	998	1005	rVB	236	275	0.01%	0.002%
23	4.668	1011	1035	1069	rBV2	770370	1950973	100.00%	15.646%
24	5.067	1141	1159	1180	rVV	194249	425148	21.79%	3.409%
25	5.321	1220	1238	1262	rBV	454346	1032342	52.91%	8.279%
26	5.446	1273	1277	1278	rBV2	240	191	0.01%	0.002%
27	5.520	1298	1300	1305	rVB2	398	315	0.02%	0.003%
28	5.552	1305	1310	1315	rBV2	336	376	0.02%	0.003%
29	5.726	1343	1364	1398	rBV2	392742	1059604	54.31%	8.497%
30	5.948	1431	1433	1437	rVB3	350	214	0.01%	0.002%
31	5.973	1437	1441	1445	rVB2	262	262	0.01%	0.002%
32	5.999	1446	1449	1453	rVB2	282	191	0.01%	0.002%
33	6.047	1461	1464	1467	rBV2	580	352	0.02%	0.003%
34	6.108	1479	1483	1486	rBV2	272	253	0.01%	0.002%
35	6.250	1511	1527	1553	rBV	400521	759548	38.93%	6.091%
36	6.542	1608	1618	1632	rBV2	17241	33086	1.70%	0.265%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047680.D
 Acq On : 25 Mar 2022 18:24
 Operator : SY/MD
 Sample : N2082-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW618

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1649	1665	1685	rBV	236870	471712	24.18%	3.783%
38	6.896	1724	1728	1730	rBV2	397	308	0.02%	0.002%
39	7.047	1770	1775	1776	rBV2	266	211	0.01%	0.002%
40	7.134	1798	1802	1806	rVB2	245	243	0.01%	0.002%
41	7.189	1812	1819	1827	rBV4	783	1140	0.06%	0.009%
42	7.568	1924	1937	1958	rVV	126012	224051	11.48%	1.797%
43	7.690	1970	1975	1982	rVB5	840	1031	0.05%	0.008%
44	7.742	1987	1991	1995	rVB2	377	326	0.02%	0.003%
45	7.793	2003	2007	2008	rBV	312	208	0.01%	0.002%
46	7.845	2020	2023	2026	rVB2	325	231	0.01%	0.002%
47	7.899	2026	2040	2056	rBV	490864	861752	44.17%	6.911%
48	8.179	2116	2127	2141	rBV	90344	152203	7.80%	1.221%
49	8.359	2180	2183	2187	rBV4	275	236	0.01%	0.002%
50	8.404	2189	2197	2204	rVB5	2129	3407	0.17%	0.027%
51	8.475	2204	2219	2228	rBV3	2331	4622	0.24%	0.037%
52	8.555	2232	2244	2257	rBV	105122	178749	9.16%	1.433%
53	8.636	2257	2269	2302	rBV	355781	668249	34.25%	5.359%
54	8.883	2344	2346	2351	rVB3	426	349	0.02%	0.003%
55	8.915	2351	2356	2360	rBV2	253	317	0.02%	0.003%
56	9.044	2391	2396	2399	rVB3	195	222	0.01%	0.002%
57	9.185	2437	2440	2443	rBV3	341	234	0.01%	0.002%
58	9.250	2454	2460	2462	rBV2	211	239	0.01%	0.002%
59	9.359	2491	2494	2496	rBV2	263	190	0.01%	0.002%
60	9.417	2499	2512	2549	rBV	586631	996394	51.07%	7.990%
61	9.565	2553	2558	2559	rBV3	531	358	0.02%	0.003%
62	9.693	2593	2598	2606	rBV5	802	1195	0.06%	0.010%
63	9.874	2650	2654	2657	rVB2	296	205	0.01%	0.002%
64	9.989	2688	2690	2698	rVB2	280	272	0.01%	0.002%
65	10.099	2721	2724	2725	rBV	326	189	0.01%	0.002%
66	10.282	2779	2781	2785	rBV	259	196	0.01%	0.002%
67	10.362	2803	2806	2808	rVV2	326	210	0.01%	0.002%
68	10.388	2811	2814	2819	rVB3	335	280	0.01%	0.002%
69	10.449	2830	2833	2836	rBV2	316	214	0.01%	0.002%
70	10.504	2848	2850	2856	rVB3	267	285	0.01%	0.002%
71	10.671	2896	2902	2912	rVB4	1551	2170	0.11%	0.017%
72	10.758	2916	2929	2949	rVV	373573	601479	30.83%	4.823%
73	10.893	2961	2971	2983	rVB2	4324	7364	0.38%	0.059%
74	10.951	2984	2989	2991	rVB2	372	255	0.01%	0.002%
75	10.967	2991	2994	3000	rVB2	293	314	0.02%	0.003%
76	11.066	3021	3025	3028	rBV3	229	239	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047680.D
 Acq On : 25 Mar 2022 18:24
 Operator : SY/MD
 Sample : N2082-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW618

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.092	3029	3033	3036	rVV4	429	340	0.02%	0.003%
78	11.462	3140	3148	3157	rBV5	1883	3310	0.17%	0.027%
79	11.539	3169	3172	3176	rBV3	247	210	0.01%	0.002%
80	11.571	3180	3182	3184	rVV	349	196	0.01%	0.002%
81	11.703	3217	3223	3230	rVB4	771	1041	0.05%	0.008%
82	11.745	3232	3236	3238	rBV2	421	333	0.02%	0.003%
83	11.812	3243	3257	3273	rBV	659449	1046320	53.63%	8.391%
84	11.967	3301	3305	3315	rVB4	1290	2011	0.10%	0.016%
85	12.034	3323	3326	3331	rVB3	399	403	0.02%	0.003%
86	12.086	3337	3342	3345	rBV3	499	505	0.03%	0.004%
87	12.192	3361	3375	3401	rBV	517218	841295	43.12%	6.747%
88	12.282	3401	3403	3408	rVB3	447	324	0.02%	0.003%
89	12.330	3414	3418	3424	rBV3	502	515	0.03%	0.004%
90	12.378	3427	3433	3440	rBV3	514	661	0.03%	0.005%
91	12.494	3466	3469	3471	rBV	376	259	0.01%	0.002%
92	12.629	3509	3511	3515	rBV2	266	210	0.01%	0.002%
93	12.719	3533	3539	3542	rBV2	323	458	0.02%	0.004%
94	12.774	3548	3556	3562	rBV2	922	1454	0.07%	0.012%
95	13.028	3632	3635	3637	rBV2	312	244	0.01%	0.002%
96	13.844	3884	3889	3891	rBV2	718	681	0.03%	0.005%
97	14.092	3959	3966	3978	rBV2	3031	4602	0.24%	0.037%
98	14.336	4036	4042	4046	rVB3	930	937	0.05%	0.008%
99	14.542	4103	4106	4112	rVB4	382	278	0.01%	0.002%
100	14.668	4142	4145	4147	rBV	338	237	0.01%	0.002%




Sum of corrected areas: 12469783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047680.D
Acq On : 25 Mar 2022 18:24
Operator : SY/MD
Sample : N2082-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW618

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

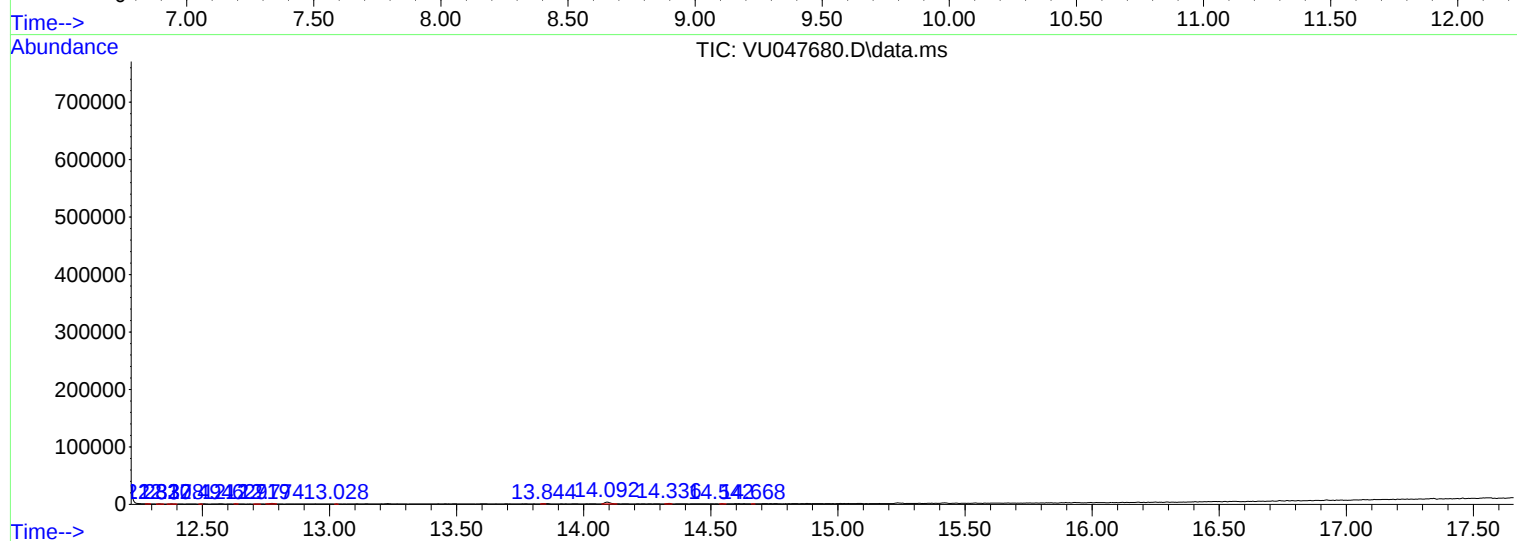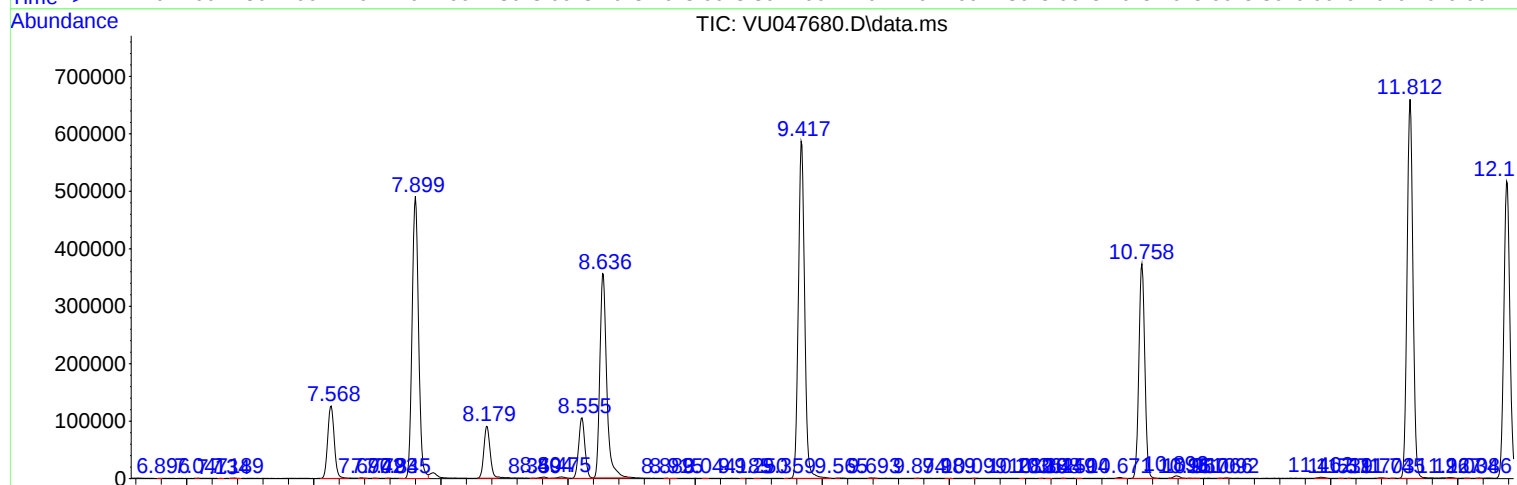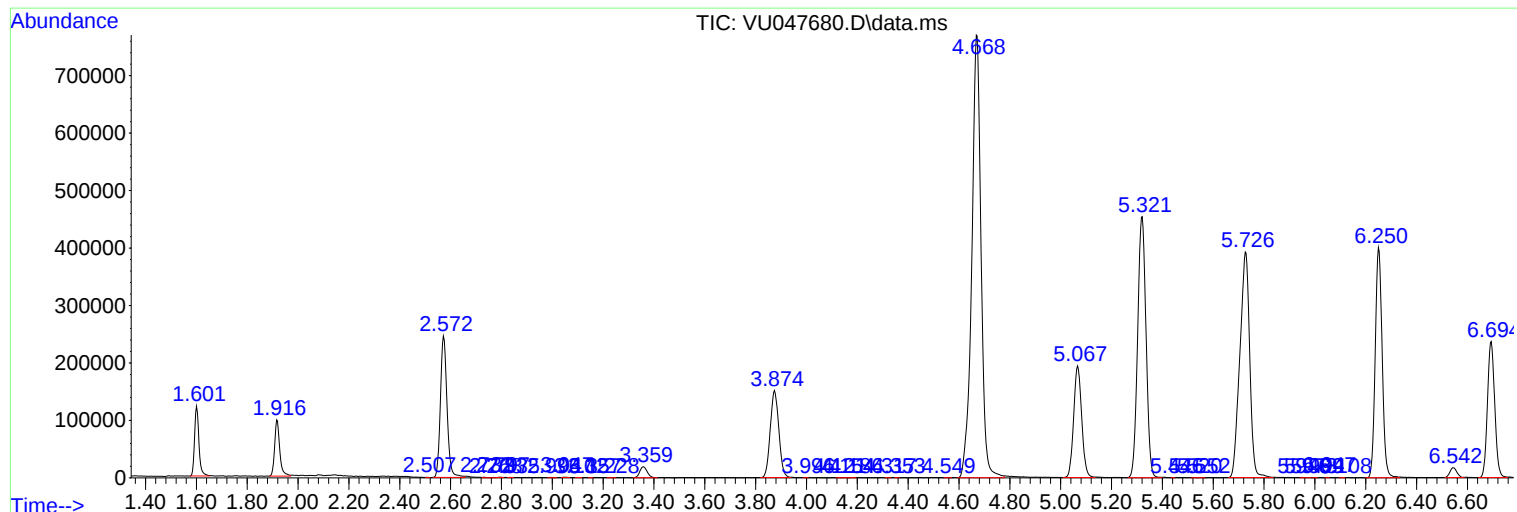

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047680.D
Acq On : 25 Mar 2022 18:24
Operator : SY/MD
Sample : N2082-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW618

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047680.D
Acq On : 25 Mar 2022 18:24
Operator : SY/MD
Sample : N2082-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW618

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------