

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047681.D
 Acq On : 25 Mar 2022 18:47
 Operator : SY/MD
 Sample : N2082-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Z0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047681.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rBV2	137452	166280	15.77%	1.630%
2	1.916	171	179	198	rBV	93125	129073	12.24%	1.265%
3	2.572	370	383	404	rBV	225067	378014	35.84%	3.705%
4	2.839	463	466	470	rVB	287	265	0.03%	0.003%
5	2.877	474	478	481	rBV2	359	297	0.03%	0.003%
6	2.941	492	498	502	rBV2	412	496	0.05%	0.005%
7	2.967	502	506	508	rBV2	338	263	0.02%	0.003%
8	3.147	559	562	565	rBV3	321	240	0.02%	0.002%
9	3.170	565	569	572	rBV2	392	330	0.03%	0.003%
10	3.318	613	615	618	rVV	280	212	0.02%	0.002%
11	3.359	618	628	642	rVB	7796	14340	1.36%	0.141%
12	3.552	684	688	690	rVB2	312	258	0.02%	0.003%
13	3.578	690	696	698	rBV2	197	196	0.02%	0.002%
14	3.633	710	713	716	rBV2	186	190	0.02%	0.002%
15	3.874	768	788	810	rBV	142219	339375	32.18%	3.326%
16	3.980	818	821	825	rVB2	352	264	0.03%	0.003%
17	4.051	839	843	846	rBV2	410	332	0.03%	0.003%
18	4.154	870	875	879	rBV2	282	219	0.02%	0.002%
19	4.176	879	882	884	rVV	317	208	0.02%	0.002%
20	4.231	895	899	904	rVB2	313	318	0.03%	0.003%
21	4.514	982	987	988	rBV	254	214	0.02%	0.002%
22	4.668	1010	1035	1071	rBV2	279031	826035	78.32%	8.096%
23	4.861	1093	1095	1097	rBV	442	212	0.02%	0.002%
24	4.967	1126	1128	1136	rVB2	280	248	0.02%	0.002%
25	5.067	1143	1159	1185	rBV	188859	414903	39.34%	4.066%
26	5.317	1222	1237	1256	rBV2	73174	165624	15.70%	1.623%
27	5.385	1256	1258	1263	rVB2	407	304	0.03%	0.003%
28	5.424	1263	1270	1273	rVB2	280	204	0.02%	0.002%
29	5.604	1320	1326	1329	rVB2	264	278	0.03%	0.003%
30	5.639	1329	1337	1339	rBV	347	395	0.04%	0.004%
31	5.729	1342	1365	1400	rBV2	387961	1044141	99.01%	10.233%
32	5.977	1437	1442	1444	rVB4	318	285	0.03%	0.003%
33	6.134	1487	1491	1495	rVB3	360	278	0.03%	0.003%
34	6.160	1495	1499	1504	rBV2	235	185	0.02%	0.002%
35	6.250	1513	1527	1557	rBV	401710	763510	72.40%	7.483%
36	6.543	1606	1618	1632	rBV	27287	50926	4.83%	0.499%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047681.D
 Acq On : 25 Mar 2022 18:47
 Operator : SY/MD
 Sample : N2082-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Z0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1651	1665	1687	rBV	235115	464885	44.08%	4.556%
38	7.015	1760	1765	1768	rBV2	497	435	0.04%	0.004%
39	7.041	1768	1773	1775	rBV3	614	647	0.06%	0.006%
40	7.186	1814	1818	1826	rVB3	863	1056	0.10%	0.010%
41	7.382	1876	1879	1884	rVB2	267	266	0.03%	0.003%
42	7.436	1892	1896	1899	rBV2	250	231	0.02%	0.002%
43	7.494	1911	1914	1921	rBV3	189	226	0.02%	0.002%
44	7.568	1924	1937	1957	rBV	122102	220100	20.87%	2.157%
45	7.758	1993	1996	2001	rVB2	278	221	0.02%	0.002%
46	7.800	2005	2009	2012	rBV3	458	441	0.04%	0.004%
47	7.899	2024	2040	2056	rBV	487191	848178	80.42%	8.313%
48	8.112	2103	2106	2114	rBV3	425	591	0.06%	0.006%
49	8.182	2115	2128	2146	rBV	87176	152807	14.49%	1.498%
50	8.314	2167	2169	2176	rVB2	392	365	0.03%	0.004%
51	8.395	2191	2194	2196	rBV2	575	435	0.04%	0.004%
52	8.475	2210	2219	2231	rVB3	3456	5603	0.53%	0.055%
53	8.555	2234	2244	2257	rVB3	16026	26128	2.48%	0.256%
54	8.639	2257	2270	2313	rBV	345742	673838	63.89%	6.604%
55	8.838	2327	2332	2334	rBV4	262	223	0.02%	0.002%
56	8.899	2348	2351	2355	rBV2	420	316	0.03%	0.003%
57	8.973	2370	2374	2379	rBV3	224	247	0.02%	0.002%
58	9.417	2496	2512	2549	rBV	587160	1000778	94.89%	9.808%
59	9.642	2579	2582	2585	rBV	244	186	0.02%	0.002%
60	9.697	2590	2599	2604	rVV3	871	1324	0.13%	0.013%
61	9.722	2604	2607	2612	rVB2	421	373	0.04%	0.004%
62	9.755	2612	2617	2620	rBV3	293	376	0.04%	0.004%
63	9.793	2626	2629	2632	rVB2	275	186	0.02%	0.002%
64	9.861	2646	2650	2655	rVV2	350	319	0.03%	0.003%
65	10.198	2751	2755	2758	rVV3	247	200	0.02%	0.002%
66	10.308	2786	2789	2794	rVB3	299	301	0.03%	0.003%
67	10.414	2818	2822	2825	rVB	253	190	0.02%	0.002%
68	10.623	2883	2887	2890	rBV2	423	390	0.04%	0.004%
69	10.645	2890	2894	2896	rVV2	298	249	0.02%	0.002%
70	10.674	2897	2903	2910	rVV6	1596	1872	0.18%	0.018%
71	10.758	2916	2929	2946	rVV	364862	594701	56.39%	5.829%
72	10.893	2962	2971	2983	rVB	5179	8432	0.80%	0.083%
73	10.957	2989	2991	2996	rVB2	339	252	0.02%	0.002%
74	11.028	3009	3013	3017	rVB2	450	360	0.03%	0.004%
75	11.050	3017	3020	3024	rBV3	248	196	0.02%	0.002%
76	11.092	3032	3033	3037	rVV2	354	246	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047681.D
 Acq On : 25 Mar 2022 18:47
 Operator : SY/MD
 Sample : N2082-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Z0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.404	3126	3130	3134	rVB	381	304	0.03%	0.003%
78	11.430	3134	3138	3140	rBV	344	241	0.02%	0.002%
79	11.462	3140	3148	3159	rVB5	1606	3246	0.31%	0.032%
80	11.616	3193	3196	3199	rBV2	329	259	0.02%	0.003%
81	11.687	3215	3218	3219	rBV2	589	360	0.03%	0.004%
82	11.697	3219	3221	3224	rVB3	912	539	0.05%	0.005%
83	11.742	3229	3235	3236	rBV2	552	427	0.04%	0.004%
84	11.812	3244	3257	3281	rBV	666187	1054626	100.00%	10.336%
85	11.970	3303	3306	3314	rVB5	1142	1243	0.12%	0.012%
86	12.060	3331	3334	3337	rBV2	360	212	0.02%	0.002%
87	12.195	3361	3376	3393	rBV	503982	827282	78.44%	8.108%
88	12.330	3415	3418	3421	rVB3	362	213	0.02%	0.002%
89	12.616	3503	3507	3509	rBV	347	266	0.03%	0.003%
90	12.632	3509	3512	3514	rVV2	359	236	0.02%	0.002%
91	12.774	3549	3556	3564	rVB4	1075	1725	0.16%	0.017%
92	12.896	3592	3594	3598	rBV2	266	194	0.02%	0.002%
93	13.761	3859	3863	3866	rBV2	398	324	0.03%	0.003%
94	14.050	3950	3953	3958	rBV	342	348	0.03%	0.003%
95	14.099	3960	3968	3976	rVV	1379	2313	0.22%	0.023%
96	14.555	4107	4110	4112	rBV2	352	243	0.02%	0.002%
97	14.906	4216	4219	4222	rBV	475	354	0.03%	0.003%
98	15.131	4287	4289	4295	rBV2	416	427	0.04%	0.004%
99	15.430	4380	4382	4385	rBV2	561	344	0.03%	0.003%
100	15.571	4424	4426	4429	rBV3	558	397	0.04%	0.004%




Sum of corrected areas: 10203205

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047681.D
Acq On : 25 Mar 2022 18:47
Operator : SY/MD
Sample : N2082-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW520

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

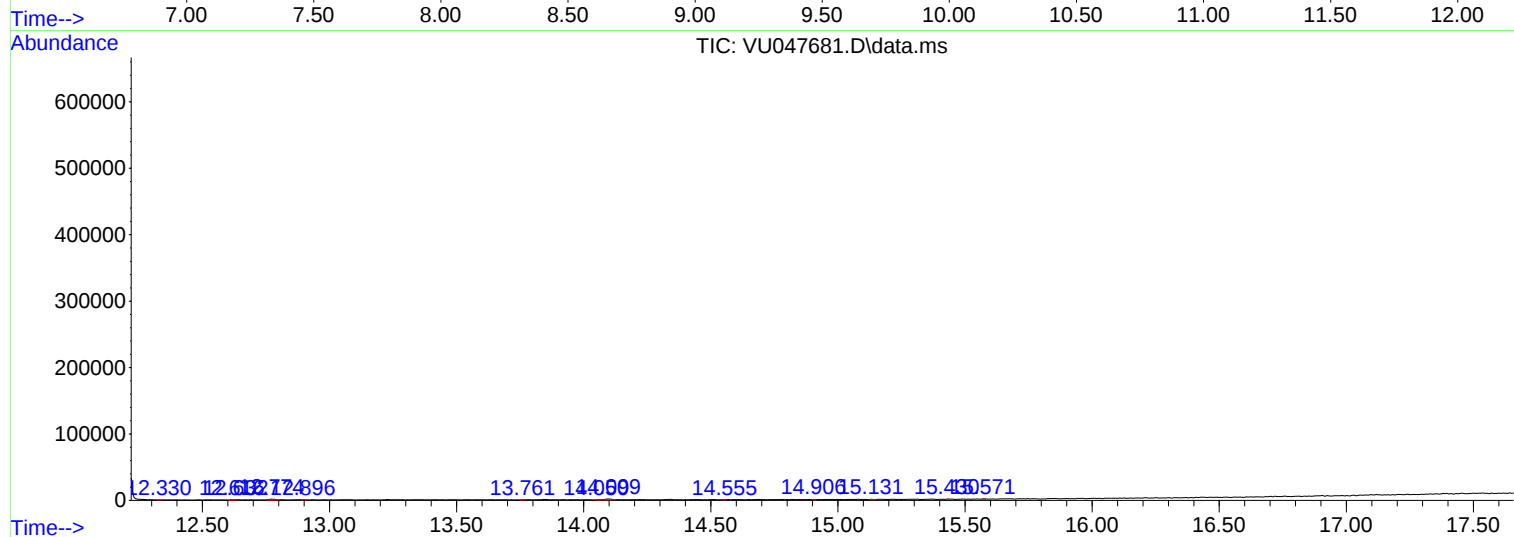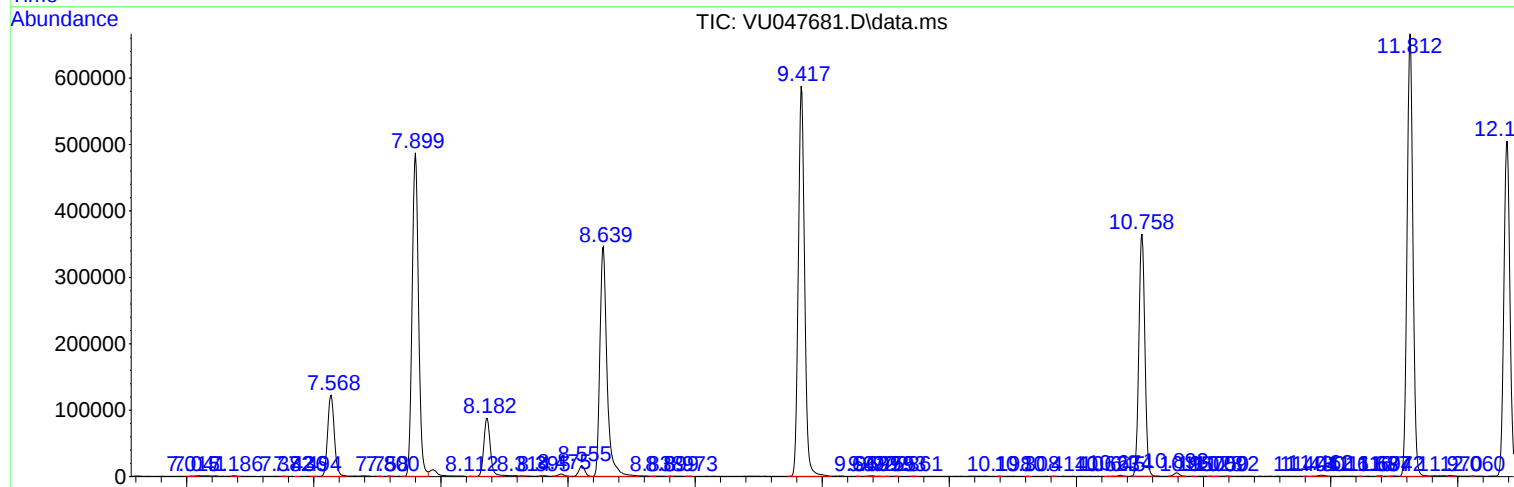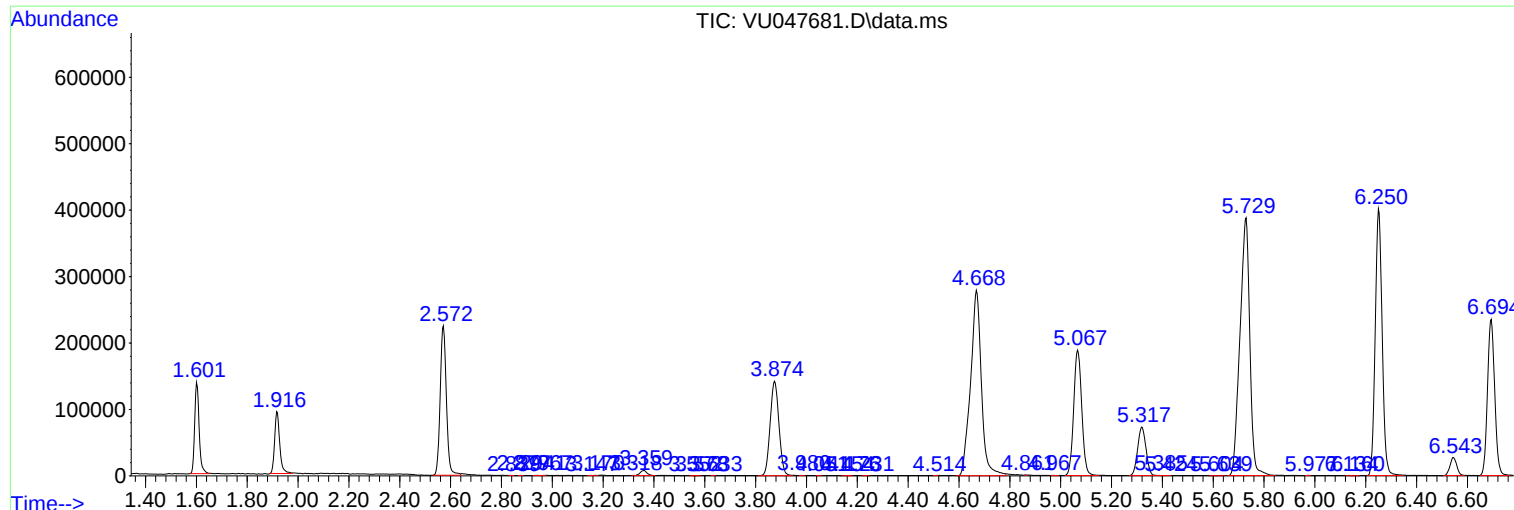

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047681.D
Acq On : 25 Mar 2022 18:47
Operator : SY/MD
Sample : N2082-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047681.D
Acq On : 25 Mar 2022 18:47
Operator : SY/MD
Sample : N2082-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc