

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047685.D
 Acq On : 25 Mar 2022 20:18
 Operator : SY/MD
 Sample : N2082-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW601

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	97	rVB	124365	149219	14.34%	1.419%
2	1.919	172	180	195	rBV	93083	127231	12.23%	1.210%
3	2.572	370	383	408	rBV	221840	381642	36.68%	3.630%
4	3.054	527	533	539	rVB3	725	889	0.09%	0.008%
5	3.224	583	586	589	rBV	230	117	0.01%	0.001%
6	3.240	589	591	594	rVV2	161	103	0.01%	0.001%
7	3.359	619	628	643	rVB3	7986	14953	1.44%	0.142%
8	3.514	673	676	677	rBV	170	90	0.01%	0.001%
9	3.588	694	699	700	rBV2	195	140	0.01%	0.001%
10	3.623	706	710	712	rBV2	214	169	0.02%	0.002%
11	3.774	755	757	764	rVB2	262	159	0.02%	0.002%
12	3.813	764	769	770	rBV	137	93	0.01%	0.001%
13	3.874	770	788	809	rBV	156922	370951	35.66%	3.529%
14	4.035	835	838	841	rBV2	231	112	0.01%	0.001%
15	4.051	841	843	846	rBV	162	102	0.01%	0.001%
16	4.096	852	857	861	rVB2	226	246	0.02%	0.002%
17	4.118	861	864	867	rBV2	252	176	0.02%	0.002%
18	4.234	895	900	902	rBV	263	216	0.02%	0.002%
19	4.269	909	911	914	rVB	281	119	0.01%	0.001%
20	4.292	915	918	921	rVV	140	94	0.01%	0.001%
21	4.311	921	924	929	rVB3	273	249	0.02%	0.002%
22	4.382	942	946	951	rBV2	151	159	0.02%	0.002%
23	4.568	1001	1004	1006	rBV	210	144	0.01%	0.001%
24	4.668	1012	1035	1065	rBV2	149995	542527	52.15%	5.161%
25	4.996	1132	1137	1140	rBV2	239	244	0.02%	0.002%
26	5.067	1141	1159	1184	rVV2	189764	414460	39.84%	3.942%
27	5.205	1200	1202	1205	rBV	311	183	0.02%	0.002%
28	5.237	1209	1212	1215	rVB2	334	215	0.02%	0.002%
29	5.256	1215	1218	1220	rBV2	164	109	0.01%	0.001%
30	5.321	1220	1238	1262	rBV	320377	723241	69.52%	6.880%
31	5.436	1272	1274	1277	rBV2	185	107	0.01%	0.001%
32	5.453	1277	1279	1281	rVB	262	108	0.01%	0.001%
33	5.469	1281	1284	1286	rBV	150	112	0.01%	0.001%
34	5.510	1294	1297	1304	rVB2	295	243	0.02%	0.002%
35	5.549	1304	1309	1312	rBV2	103	120	0.01%	0.001%
36	5.578	1316	1318	1321	rVB3	152	86	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047685.D
 Acq On : 25 Mar 2022 20:18
 Operator : SY/MD
 Sample : N2082-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW601

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.600	1321	1325	1329	rBV2	207	138	0.01%	0.001%
38	5.649	1337	1340	1342	rVB	237	120	0.01%	0.001%
39	5.726	1342	1364	1398	rBV2	384725	1040326	100.00%	9.896%
40	5.916	1418	1423	1431	rBV2	313	543	0.05%	0.005%
41	6.076	1471	1473	1477	rVB2	185	91	0.01%	0.001%
42	6.163	1497	1500	1504	rVB2	259	145	0.01%	0.001%
43	6.250	1513	1527	1548	rBV	391392	739920	71.12%	7.038%
44	6.494	1599	1603	1605	rBV2	184	163	0.02%	0.002%
45	6.543	1608	1618	1631	rVB3	15935	29450	2.83%	0.280%
46	6.694	1649	1665	1683	rBV	235997	464877	44.69%	4.422%
47	6.838	1707	1710	1714	rBV2	202	178	0.02%	0.002%
48	6.893	1724	1727	1729	rBV2	263	200	0.02%	0.002%
49	6.954	1745	1746	1751	rVB2	222	103	0.01%	0.001%
50	7.018	1764	1766	1767	rBV	231	107	0.01%	0.001%
51	7.141	1802	1804	1807	rVB2	332	198	0.02%	0.002%
52	7.186	1812	1818	1821	rBV3	792	900	0.09%	0.009%
53	7.314	1852	1858	1862	rBV2	289	330	0.03%	0.003%
54	7.356	1868	1871	1873	rBV2	187	124	0.01%	0.001%
55	7.420	1888	1891	1893	rBV	150	110	0.01%	0.001%
56	7.452	1898	1901	1904	rBV2	166	95	0.01%	0.001%
57	7.494	1909	1914	1916	rBB3	284	200	0.02%	0.002%
58	7.523	1919	1923	1924	rBV2	234	163	0.02%	0.002%
59	7.568	1924	1937	1955	rBV	124332	220176	21.16%	2.094%
60	7.735	1986	1989	1992	rBV2	190	115	0.01%	0.001%
61	7.748	1992	1993	1997	rVB	264	151	0.01%	0.001%
62	7.899	2022	2040	2056	rBV	486177	847590	81.47%	8.062%
63	8.115	2104	2107	2113	rBV3	334	393	0.04%	0.004%
64	8.179	2113	2127	2147	rBV	88247	152521	14.66%	1.451%
65	8.475	2209	2219	2230	rBV3	1610	3048	0.29%	0.029%
66	8.555	2232	2244	2256	rBV	50980	85340	8.20%	0.812%
67	8.636	2257	2269	2304	rBV	352916	665667	63.99%	6.332%
68	8.854	2333	2337	2340	rBV5	450	302	0.03%	0.003%
69	8.964	2369	2371	2376	rBV3	226	177	0.02%	0.002%
70	9.121	2417	2420	2422	rBV2	323	194	0.02%	0.002%
71	9.276	2462	2468	2471	rBV3	245	213	0.02%	0.002%
72	9.292	2471	2473	2479	rBV3	182	216	0.02%	0.002%
73	9.359	2491	2494	2496	rBV2	167	85	0.01%	0.001%
74	9.417	2498	2512	2551	rVV	569371	977687	93.98%	9.300%
75	9.549	2551	2553	2555	rVV2	357	204	0.02%	0.002%
76	9.568	2555	2559	2568	rVB3	1560	2196	0.21%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047685.D
 Acq On : 25 Mar 2022 20:18
 Operator : SY/MD
 Sample : N2082-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW601

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.697	2592	2599	2606	rBV2	1927	2458	0.24%	0.023%
78	9.822	2636	2638	2643	rVB2	251	178	0.02%	0.002%
79	10.105	2714	2726	2728	rBV5	1830	2383	0.23%	0.023%
80	10.250	2767	2771	2773	rBV	215	178	0.02%	0.002%
81	10.276	2776	2779	2781	rVV2	216	132	0.01%	0.001%
82	10.610	2880	2883	2886	rBV3	273	225	0.02%	0.002%
83	10.671	2894	2902	2908	rBV3	1484	1923	0.18%	0.018%
84	10.758	2916	2929	2949	rVB	372602	594851	57.18%	5.658%
85	10.999	2997	3004	3009	rBV3	816	1153	0.11%	0.011%
86	11.108	3036	3038	3042	rBV2	397	309	0.03%	0.003%
87	11.205	3067	3068	3072	rBV2	241	137	0.01%	0.001%
88	11.243	3078	3080	3083	rBV2	241	149	0.01%	0.001%
89	11.295	3090	3096	3103	rBV3	1021	1375	0.13%	0.013%
90	11.465	3139	3149	3158	rBV7	2369	4338	0.42%	0.041%
91	11.558	3175	3178	3181	rBV	177	109	0.01%	0.001%
92	11.693	3217	3220	3225	rVB4	699	526	0.05%	0.005%
93	11.812	3244	3257	3277	rBV	657996	1035513	99.54%	9.850%
94	12.192	3362	3375	3395	rBV	506834	832967	80.07%	7.923%
95	12.382	3431	3434	3436	rBV2	388	218	0.02%	0.002%
96	12.484	3457	3466	3481	rVB3	13088	21283	2.05%	0.202%
97	13.173	3677	3680	3681	rBV	322	222	0.02%	0.002%
98	14.015	3935	3942	3951	rVB3	5712	7996	0.77%	0.076%
99	14.089	3956	3965	3975	rVV4	15778	25429	2.44%	0.242%
100	14.150	3978	3984	3997	rVB4	9191	15041	1.45%	0.143%


Sum of corrected areas: 10512977

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047685.D
Acq On : 25 Mar 2022 20:18
Operator : SY/MD
Sample : N2082-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

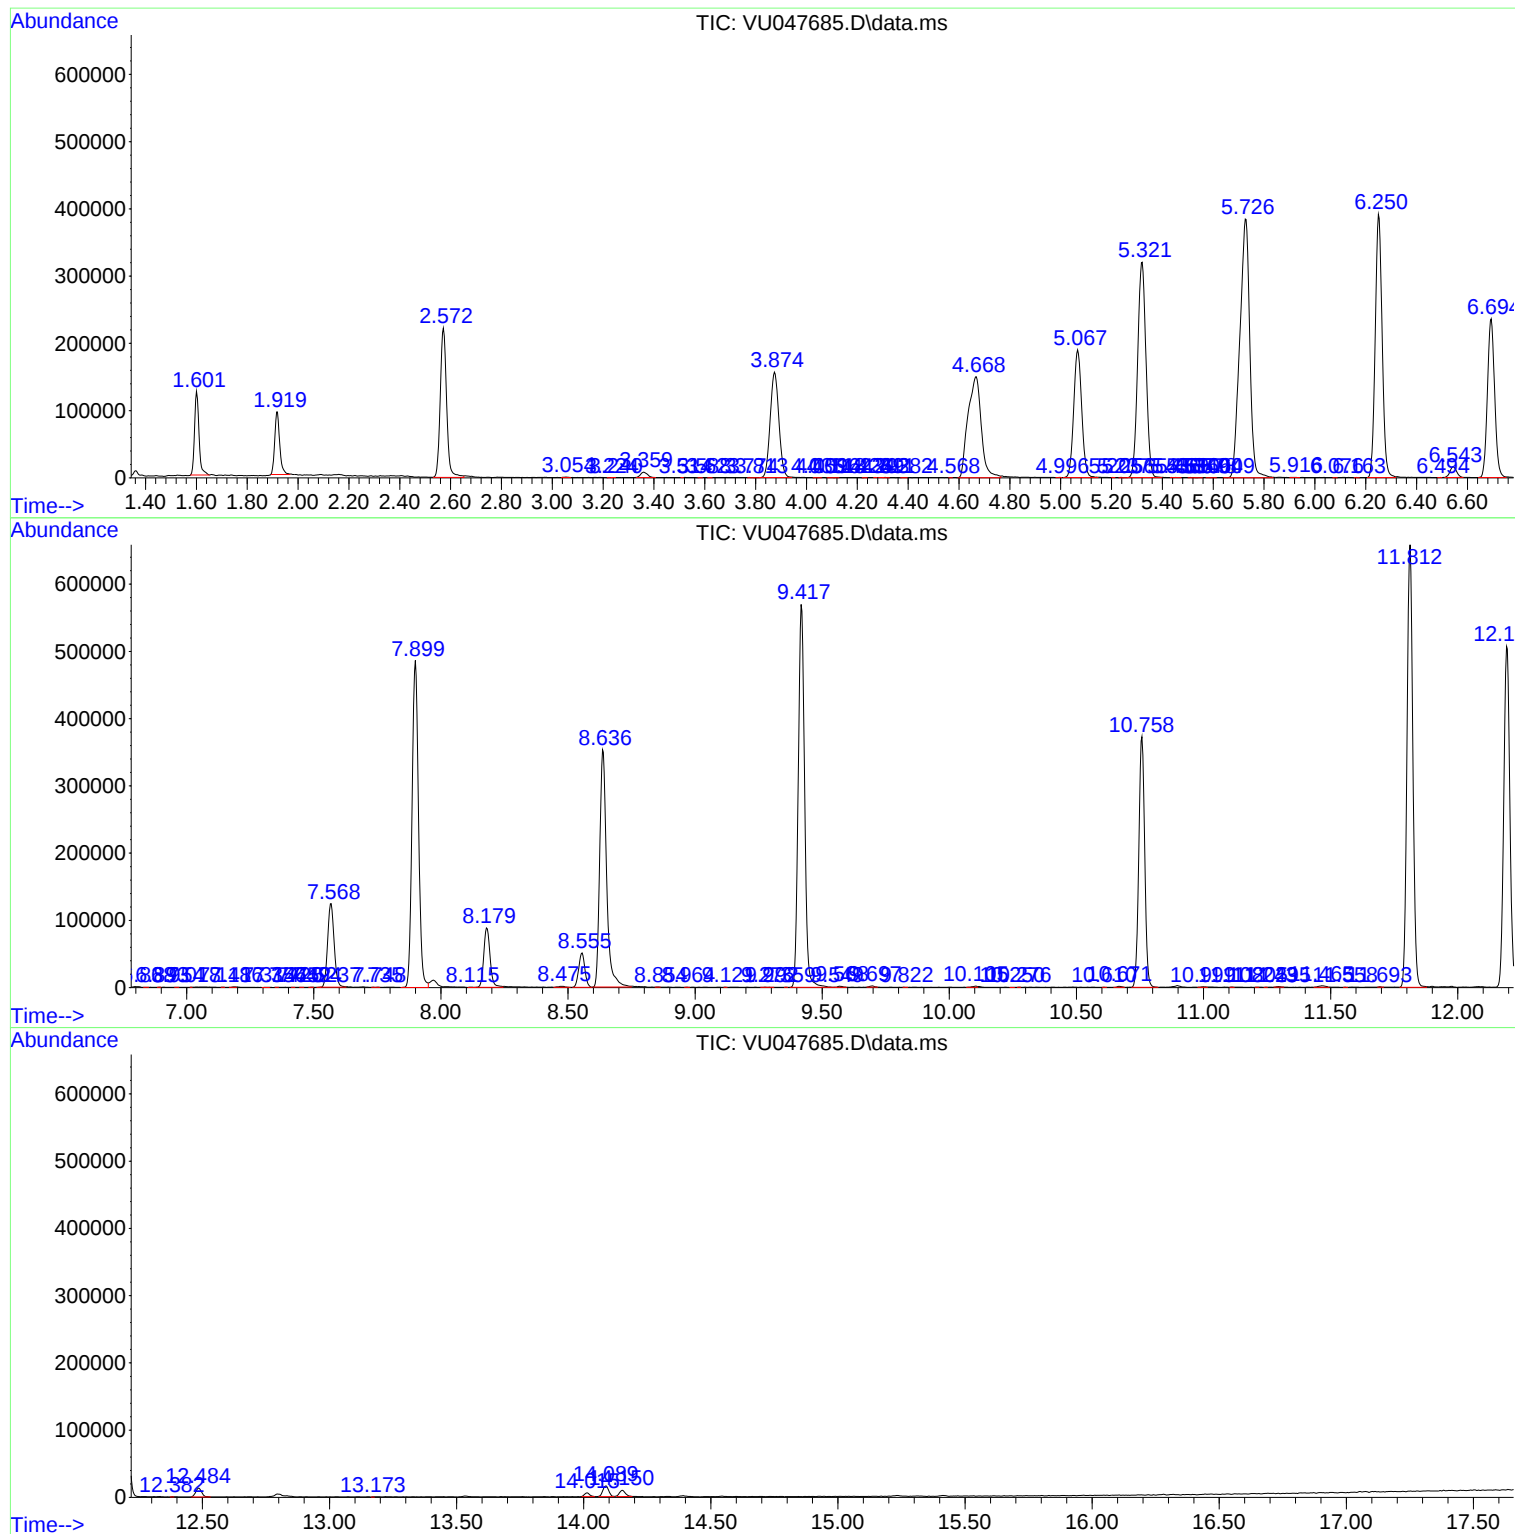

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047685.D
Acq On : 25 Mar 2022 20:18
Operator : SY/MD
Sample : N2082-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047685.D
Acq On : 25 Mar 2022 20:18
Operator : SY/MD
Sample : N2082-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------