

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047686.D
 Acq On : 25 Mar 2022 20:41
 Operator : SY/MD
 Sample : N2082-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW602

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	17	rVB2	16413	16325	1.57%	0.170%
2	1.600	74	81	97	rBV	122935	149117	14.34%	1.551%
3	1.919	172	180	196	rBV	95690	133482	12.83%	1.388%
4	2.572	371	383	420	rBV2	235298	419896	40.37%	4.366%
5	2.829	461	463	465	rBV	316	179	0.02%	0.002%
6	2.941	491	498	502	rBV3	378	538	0.05%	0.006%
7	3.054	524	533	539	rBV3	592	897	0.09%	0.009%
8	3.179	569	572	575	rBV2	508	351	0.03%	0.004%
9	3.199	575	578	582	rVB4	534	369	0.04%	0.004%
10	3.260	592	597	601	rVB2	439	455	0.04%	0.005%
11	3.295	601	608	615	rBV2	395	612	0.06%	0.006%
12	3.359	618	628	640	rBV5	2784	5740	0.55%	0.060%
13	3.475	661	664	667	rBV3	242	181	0.02%	0.002%
14	3.526	676	680	684	rBV2	344	294	0.03%	0.003%
15	3.549	684	687	693	rVV2	326	340	0.03%	0.004%
16	3.732	742	744	746	rBV2	150	79	0.01%	0.001%
17	3.803	763	766	770	rVB3	207	176	0.02%	0.002%
18	3.874	771	788	813	rBV	92694	220229	21.17%	2.290%
19	4.009	828	830	833	rBV2	194	108	0.01%	0.001%
20	4.086	852	854	858	rVB3	187	117	0.01%	0.001%
21	4.112	860	862	865	rBV2	121	84	0.01%	0.001%
22	4.131	865	868	872	rVB	240	177	0.02%	0.002%
23	4.170	878	880	883	rBV2	186	93	0.01%	0.001%
24	4.353	934	937	940	rBV2	236	164	0.02%	0.002%
25	4.407	949	954	957	rBV2	231	183	0.02%	0.002%
26	4.436	960	963	964	rBV2	143	82	0.01%	0.001%
27	4.485	973	978	985	rVB3	221	300	0.03%	0.003%
28	4.520	985	989	991	rBV2	177	142	0.01%	0.001%
29	4.642	1011	1027	1060	rBV2	99946	365960	35.18%	3.805%
30	4.999	1133	1138	1140	rBV2	336	284	0.03%	0.003%
31	5.067	1143	1159	1191	rVV	189370	416014	40.00%	4.326%
32	5.218	1204	1206	1211	rVB	450	251	0.02%	0.003%
33	5.243	1211	1214	1216	rBV	210	160	0.02%	0.002%
34	5.317	1223	1237	1258	rVB3	69079	158560	15.24%	1.649%
35	5.423	1264	1270	1271	rBV2	251	271	0.03%	0.003%
36	5.469	1276	1284	1287	rBV2	144	175	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047686.D
 Acq On : 25 Mar 2022 20:41
 Operator : SY/MD
 Sample : N2082-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW602

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.488	1287	1290	1292	rBV2	139	112	0.01%	0.001%
38	5.520	1297	1300	1302	rBV	346	262	0.03%	0.003%
39	5.562	1310	1313	1317	rBV2	260	173	0.02%	0.002%
40	5.729	1343	1365	1380	rBV2	387392	1040124	100.00%	10.815%
41	6.012	1449	1453	1454	rBV2	245	160	0.02%	0.002%
42	6.041	1458	1462	1464	rBV2	160	121	0.01%	0.001%
43	6.105	1478	1482	1486	rBV	471	382	0.04%	0.004%
44	6.250	1512	1527	1557	rBV	386355	742044	71.34%	7.716%
45	6.452	1586	1590	1592	rBV3	322	205	0.02%	0.002%
46	6.468	1593	1595	1597	rBV	155	85	0.01%	0.001%
47	6.494	1602	1603	1607	rVB2	436	232	0.02%	0.002%
48	6.542	1607	1618	1637	rVB3	31092	61021	5.87%	0.634%
49	6.616	1637	1641	1643	rVB2	298	172	0.02%	0.002%
50	6.694	1647	1665	1686	rBV	239027	466089	44.81%	4.846%
51	6.845	1710	1712	1714	rBV2	269	96	0.01%	0.001%
52	6.973	1748	1752	1757	rBV2	167	133	0.01%	0.001%
53	7.179	1811	1816	1817	rBV	427	395	0.04%	0.004%
54	7.240	1833	1835	1837	rBV	221	105	0.01%	0.001%
55	7.253	1837	1839	1843	rVB2	216	135	0.01%	0.001%
56	7.301	1850	1854	1858	rBV3	400	336	0.03%	0.003%
57	7.366	1871	1874	1876	rBV	221	147	0.01%	0.002%
58	7.494	1913	1914	1917	rVB	173	72	0.01%	0.001%
59	7.517	1917	1921	1924	rBV	154	125	0.01%	0.001%
60	7.568	1924	1937	1960	rBV	121478	220478	21.20%	2.293%
61	7.687	1969	1974	1982	rBV5	833	1371	0.13%	0.014%
62	7.774	1998	2001	2003	rBV2	300	175	0.02%	0.002%
63	7.899	2026	2040	2056	rBV	493126	853113	82.02%	8.871%
64	8.179	2115	2127	2143	rBV	86438	149703	14.39%	1.557%
65	8.555	2233	2244	2257	rBV2	43824	73811	7.10%	0.767%
66	8.636	2257	2269	2300	rBV	357097	672614	64.67%	6.994%
67	8.874	2339	2343	2346	rBV2	238	242	0.02%	0.003%
68	8.922	2355	2358	2366	rBV4	333	414	0.04%	0.004%
69	9.021	2386	2389	2394	rBV2	188	195	0.02%	0.002%
70	9.102	2411	2414	2416	rBV2	241	141	0.01%	0.001%
71	9.176	2435	2437	2440	rVB2	204	97	0.01%	0.001%
72	9.292	2470	2473	2476	rBV2	197	137	0.01%	0.001%
73	9.417	2499	2512	2549	rBV	571953	975761	93.81%	10.146%
74	9.652	2581	2585	2586	rBV2	209	136	0.01%	0.001%
75	9.693	2591	2598	2607	rVV4	1274	1940	0.19%	0.020%
76	9.809	2630	2634	2639	rBV3	235	294	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047686.D
 Acq On : 25 Mar 2022 20:41
 Operator : SY/MD
 Sample : N2082-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW602

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.906	2662	2664	2669	rBV	234	173	0.02%	0.002%
78	10.066	2712	2714	2717	rVB3	329	186	0.02%	0.002%
79	10.108	2718	2727	2730	rBV5	1086	1455	0.14%	0.015%
80	10.259	2770	2774	2777	rVB2	247	198	0.02%	0.002%
81	10.513	2848	2853	2856	rBV	227	237	0.02%	0.002%
82	10.542	2860	2862	2863	rBV	171	89	0.01%	0.001%
83	10.600	2876	2880	2881	rBV	196	125	0.01%	0.001%
84	10.671	2899	2902	2905	rBV2	493	320	0.03%	0.003%
85	10.758	2916	2929	2949	rVB	369294	592872	57.00%	6.165%
86	10.935	2982	2984	2986	rBV	239	138	0.01%	0.001%
87	10.986	2998	3000	3002	rBV	148	78	0.01%	0.001%
88	11.182	3057	3061	3065	rBV3	252	210	0.02%	0.002%
89	11.243	3075	3080	3086	rBV3	401	576	0.06%	0.006%
90	11.320	3102	3104	3106	rBV	212	79	0.01%	0.001%
91	11.423	3133	3136	3138	rBV	106	94	0.01%	0.001%
92	11.439	3138	3141	3143	rBV2	350	241	0.02%	0.003%
93	11.471	3143	3151	3152	rBV3	1229	1305	0.13%	0.014%
94	11.555	3174	3177	3179	rBV	256	156	0.01%	0.002%
95	11.742	3230	3235	3240	rBV3	590	753	0.07%	0.008%
96	11.812	3244	3257	3279	rVV	645347	1026065	98.65%	10.669%
97	12.195	3363	3376	3392	rBV	512591	831783	79.97%	8.649%
98	12.423	3443	3447	3449	rBV2	336	242	0.02%	0.003%
99	12.484	3460	3466	3473	rBV6	2095	3331	0.32%	0.035%
100	14.150	3981	3984	3986	rBV3	1058	869	0.08%	0.009%




Sum of corrected areas: 9617308

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047686.D
Acq On : 25 Mar 2022 20:41
Operator : SY/MD
Sample : N2082-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW602

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

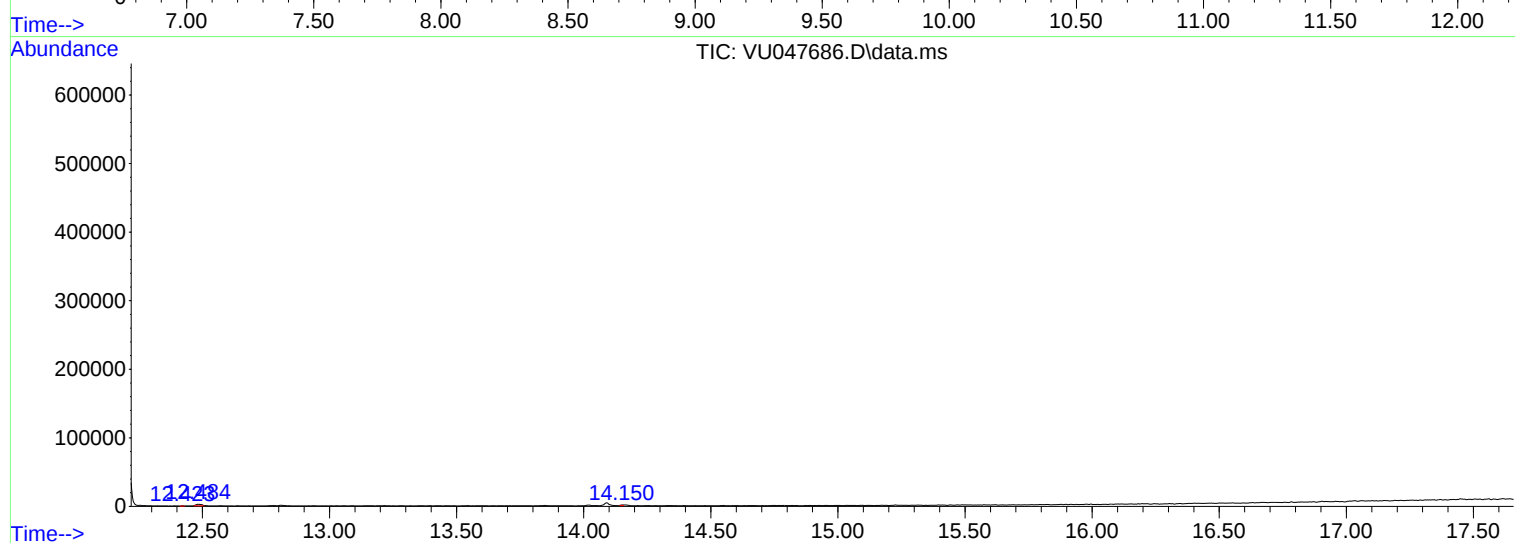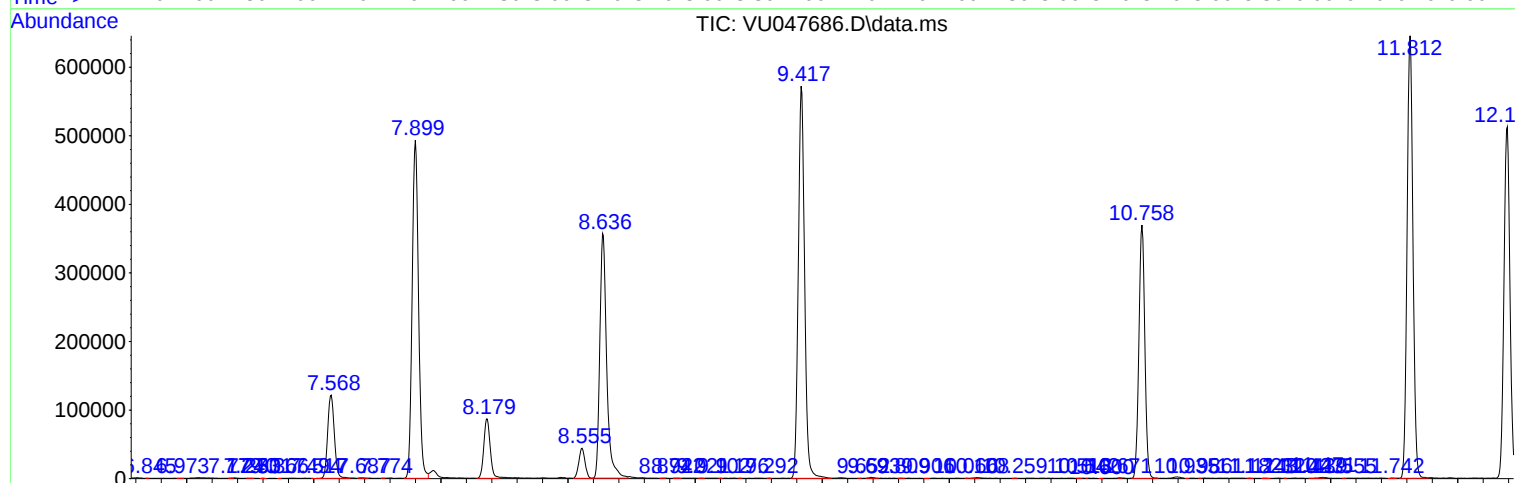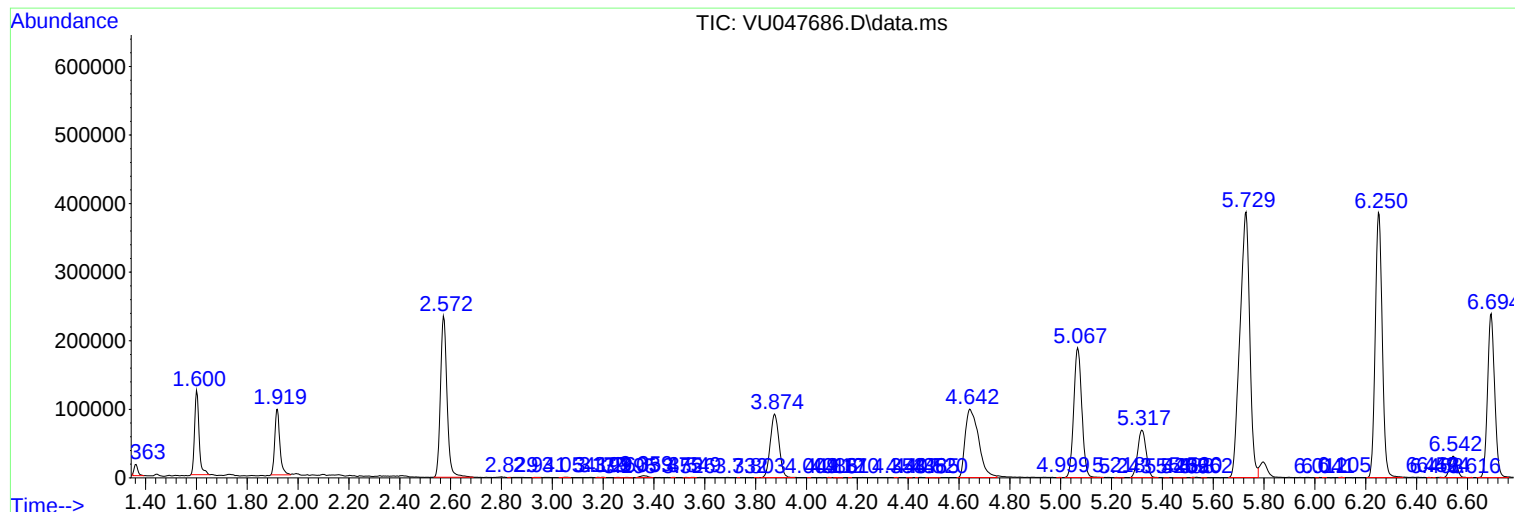

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047686.D
Acq On : 25 Mar 2022 20:41
Operator : SY/MD
Sample : N2082-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW602

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047686.D
Acq On : 25 Mar 2022 20:41
Operator : SY/MD
Sample : N2082-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW602

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------