

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047687.D
 Acq On : 25 Mar 2022 21:04
 Operator : SY/MD
 Sample : N2082-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rBV	119137	139497	13.48%	1.428%
2	1.916	172	179	205	rVB	92797	129488	12.51%	1.325%
3	2.572	371	383	401	rBV	215267	362097	34.98%	3.706%
4	2.864	471	474	477	rBV	180	144	0.01%	0.001%
5	2.990	509	513	520	rBV3	497	459	0.04%	0.005%
6	3.019	520	522	525	rBV	242	149	0.01%	0.002%
7	3.109	548	550	553	rVB2	238	134	0.01%	0.001%
8	3.192	571	576	586	rBV3	530	561	0.05%	0.006%
9	3.285	602	605	608	rBV3	313	191	0.02%	0.002%
10	3.359	613	628	643	rBV2	20961	40650	3.93%	0.416%
11	3.420	644	647	648	rBV	216	110	0.01%	0.001%
12	3.514	673	676	678	rBV	199	120	0.01%	0.001%
13	3.588	695	699	702	rBV3	276	231	0.02%	0.002%
14	3.607	702	705	709	rBV	338	281	0.03%	0.003%
15	3.700	732	734	736	rBV2	198	97	0.01%	0.001%
16	3.713	736	738	740	rVV	160	67	0.01%	0.001%
17	3.732	742	744	748	rBV	199	113	0.01%	0.001%
18	3.874	770	788	812	rBV3	30873	72945	7.05%	0.747%
19	3.980	818	821	828	rVB3	327	286	0.03%	0.003%
20	4.018	829	833	836	rBV3	233	189	0.02%	0.002%
21	4.076	847	851	856	rVB2	263	244	0.02%	0.002%
22	4.112	858	862	865	rBV	187	154	0.01%	0.002%
23	4.221	894	896	898	rVB	129	50	0.00%	0.001%
24	4.247	901	904	906	rBV	245	139	0.01%	0.001%
25	4.298	918	920	921	rBV	102	49	0.00%	0.001%
26	4.308	921	923	925	rBV	194	89	0.01%	0.001%
27	4.388	946	948	950	rBV	166	115	0.01%	0.001%
28	4.459	968	970	971	rBV	118	51	0.00%	0.001%
29	4.504	981	984	987	rVB3	203	126	0.01%	0.001%
30	4.530	989	992	994	rBV	164	103	0.01%	0.001%
31	4.568	1002	1004	1005	rBV	83	40	0.00%	0.000%
32	4.665	1013	1034	1069	rBV3	124435	472851	45.68%	4.840%
33	5.067	1142	1159	1186	rBV	188269	415857	40.17%	4.256%
34	5.202	1198	1201	1203	rBV2	90	62	0.01%	0.001%
35	5.321	1221	1238	1256	rBV2	97638	217187	20.98%	2.223%
36	5.488	1286	1290	1294	rBV3	185	154	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047687.D
 Acq On : 25 Mar 2022 21:04
 Operator : SY/MD
 Sample : N2082-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.536	1302	1305	1308	rVB2	457	289	0.03%	0.003%
38	5.584	1319	1320	1324	rVB2	156	45	0.00%	0.000%
39	5.729	1343	1365	1390	rBV2	384583	1035144	100.00%	10.595%
40	6.099	1477	1480	1482	rBV2	239	174	0.02%	0.002%
41	6.189	1502	1508	1510	rBV2	175	174	0.02%	0.002%
42	6.250	1513	1527	1553	rVV	392074	740156	71.50%	7.576%
43	6.546	1605	1619	1640	rBV	87019	168280	16.26%	1.722%
44	6.623	1641	1643	1646	rBV	270	142	0.01%	0.001%
45	6.639	1646	1648	1651	rBV2	311	228	0.02%	0.002%
46	6.694	1651	1665	1685	rBV	233415	459032	44.34%	4.698%
47	6.848	1710	1713	1716	rBV3	340	256	0.02%	0.003%
48	6.887	1719	1725	1729	rVV3	297	370	0.04%	0.004%
49	6.909	1729	1732	1734	rVB	324	197	0.02%	0.002%
50	6.951	1743	1745	1748	rVB2	296	101	0.01%	0.001%
51	7.002	1759	1761	1763	rBV	149	68	0.01%	0.001%
52	7.041	1770	1773	1775	rBV2	190	115	0.01%	0.001%
53	7.079	1783	1785	1786	rBV2	80	36	0.00%	0.000%
54	7.099	1786	1791	1797	rVV3	401	587	0.06%	0.006%
55	7.150	1805	1807	1808	rBV	235	133	0.01%	0.001%
56	7.189	1812	1819	1823	rBV4	987	1213	0.12%	0.012%
57	7.346	1861	1868	1872	rBV2	354	388	0.04%	0.004%
58	7.433	1892	1895	1902	rBV2	262	317	0.03%	0.003%
59	7.504	1913	1917	1920	rBV4	280	210	0.02%	0.002%
60	7.568	1924	1937	1954	rBV	121527	214031	20.68%	2.191%
61	7.758	1994	1996	1998	rVB	320	132	0.01%	0.001%
62	7.899	2026	2040	2056	rBV	478186	833272	80.50%	8.529%
63	8.179	2112	2127	2149	rBV3	96006	186188	17.99%	1.906%
64	8.555	2232	2244	2257	rBV	111931	188875	18.25%	1.933%
65	8.636	2258	2269	2304	rVV	348791	660808	63.84%	6.764%
66	9.067	2401	2403	2406	rBV2	200	120	0.01%	0.001%
67	9.115	2414	2418	2420	rBV2	211	163	0.02%	0.002%
68	9.198	2441	2444	2445	rBV	162	82	0.01%	0.001%
69	9.266	2461	2465	2469	rBV2	204	175	0.02%	0.002%
70	9.292	2471	2473	2475	rBV	171	110	0.01%	0.001%
71	9.317	2479	2481	2485	rVV2	240	169	0.02%	0.002%
72	9.349	2488	2491	2494	rBV2	203	132	0.01%	0.001%
73	9.417	2499	2512	2540	rBV	578492	975065	94.20%	9.980%
74	9.568	2555	2559	2567	rVB3	632	723	0.07%	0.007%
75	9.626	2575	2577	2581	rBV2	188	93	0.01%	0.001%
76	9.648	2581	2584	2591	rVB2	362	315	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047687.D
 Acq On : 25 Mar 2022 21:04
 Operator : SY/MD
 Sample : N2082-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.694	2591	2598	2603	rBV4	804	1273	0.12%	0.013%
78	9.758	2614	2618	2623	rBV2	414	494	0.05%	0.005%
79	9.857	2647	2649	2652	rBV2	251	150	0.01%	0.002%
80	10.070	2711	2715	2718	rBV2	197	170	0.02%	0.002%
81	10.092	2718	2722	2724	rBV2	410	339	0.03%	0.003%
82	10.298	2783	2786	2790	rVB2	276	211	0.02%	0.002%
83	10.340	2794	2799	2802	rVB2	257	206	0.02%	0.002%
84	10.362	2802	2806	2807	rBV2	209	145	0.01%	0.001%
85	10.452	2831	2834	2838	rBV3	388	413	0.04%	0.004%
86	10.671	2895	2902	2909	rVB5	1480	1954	0.19%	0.020%
87	10.758	2916	2929	2947	rBV	367248	593786	57.36%	6.078%
88	11.050	3015	3020	3022	rBV	305	303	0.03%	0.003%
89	11.089	3030	3032	3038	rVB	461	349	0.03%	0.004%
90	11.156	3049	3053	3057	rBV3	210	218	0.02%	0.002%
91	11.227	3073	3075	3076	rBV	231	120	0.01%	0.001%
92	11.446	3139	3143	3144	rBV2	699	454	0.04%	0.005%
93	11.546	3169	3174	3177	rBV2	224	253	0.02%	0.003%
94	11.693	3217	3220	3225	rBV3	579	470	0.05%	0.005%
95	11.742	3230	3235	3237	rBV4	346	271	0.03%	0.003%
96	11.812	3244	3257	3278	rBV	639959	1026641	99.18%	10.508%
97	12.073	3335	3338	3343	rBV3	504	462	0.04%	0.005%
98	12.137	3356	3358	3360	rBV2	276	135	0.01%	0.001%
99	12.192	3363	3375	3393	rVV	504584	816239	78.85%	8.354%
100	12.484	3459	3466	3473	rVB7	1300	1865	0.18%	0.019%




Sum of corrected areas: 9770109

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047687.D
Acq On : 25 Mar 2022 21:04
Operator : SY/MD
Sample : N2082-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

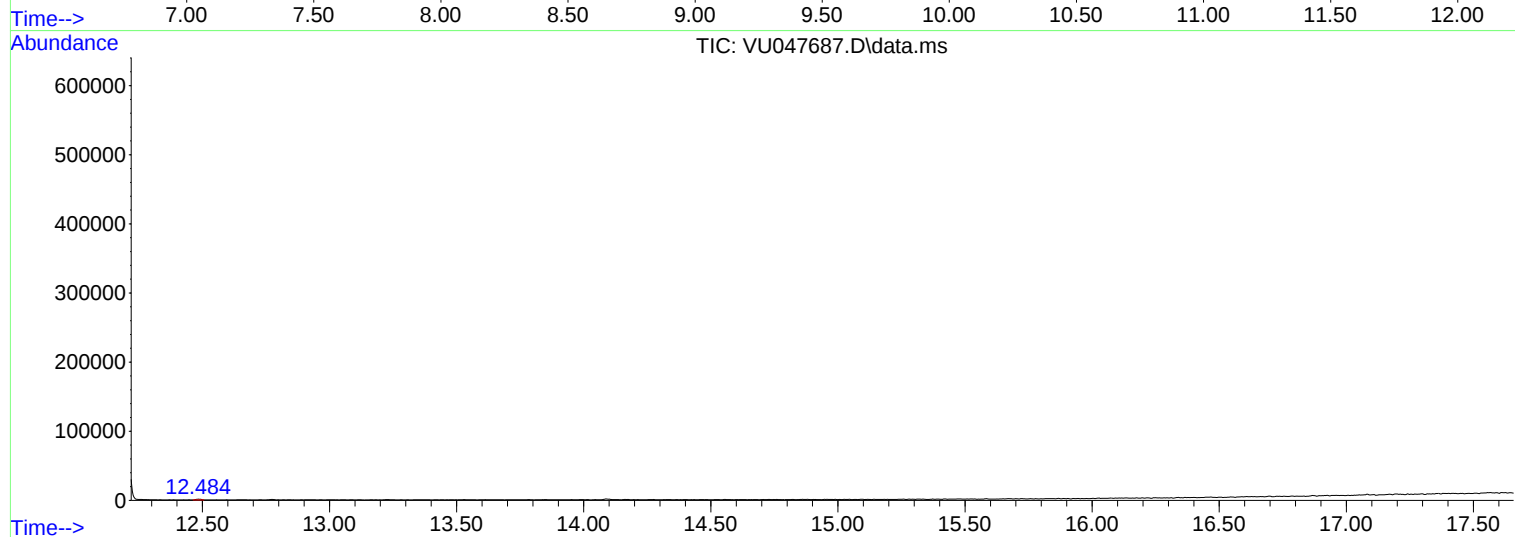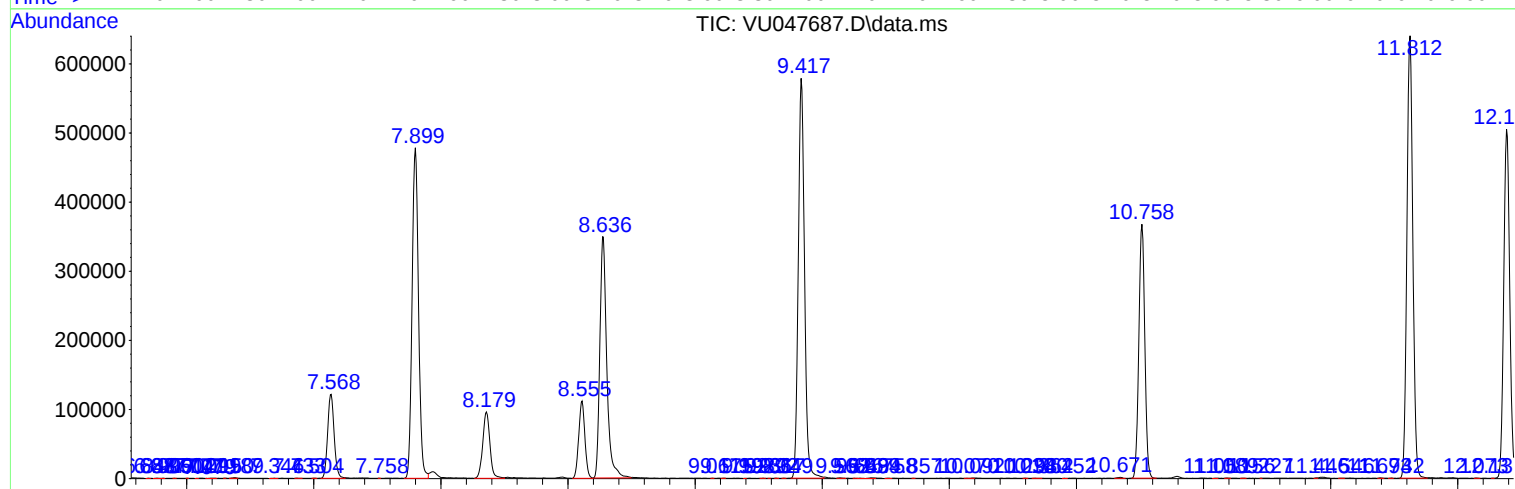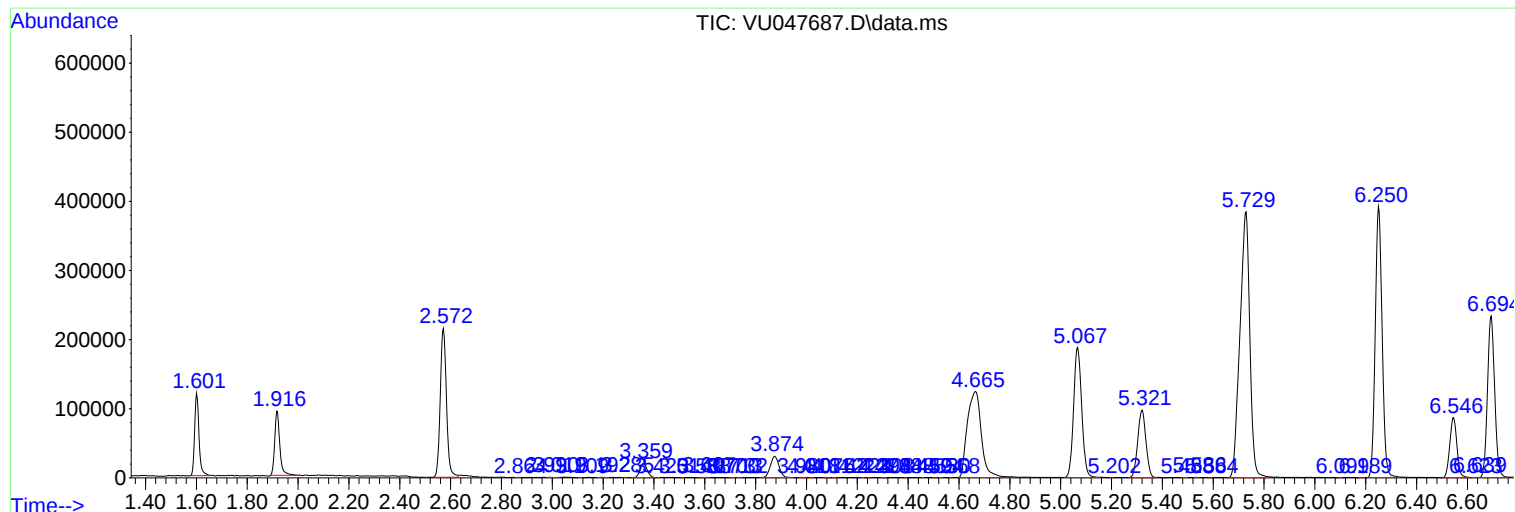

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047687.D
Acq On : 25 Mar 2022 21:04
Operator : SY/MD
Sample : N2082-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047687.D
Acq On : 25 Mar 2022 21:04
Operator : SY/MD
Sample : N2082-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------