

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047690.D
 Acq On : 25 Mar 2022 22:12
 Operator : SY/MD
 Sample : N2082-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.494	41	48	63	rBV	28121	32422	3.22%	0.371%
2	1.600	74	81	102	rVB	118318	138935	13.79%	1.589%
3	1.916	171	179	200	rVB	101143	138192	13.71%	1.580%
4	2.263	284	287	290	rVB2	941	656	0.07%	0.008%
5	2.514	360	365	367	rBV3	438	342	0.03%	0.004%
6	2.571	370	383	401	rBV	213885	355972	35.32%	4.071%
7	2.761	440	442	446	rVB2	278	211	0.02%	0.002%
8	2.941	492	498	500	rBV	286	265	0.03%	0.003%
9	2.970	504	507	510	rBV3	309	208	0.02%	0.002%
10	3.057	529	534	540	rVV5	506	585	0.06%	0.007%
11	3.198	569	578	581	rBV4	551	859	0.09%	0.010%
12	3.317	611	615	619	rBV2	257	266	0.03%	0.003%
13	3.494	668	670	676	rVB3	217	232	0.02%	0.003%
14	3.790	759	762	764	rBV	276	211	0.02%	0.002%
15	3.806	764	767	768	rBV	300	176	0.02%	0.002%
16	3.842	774	778	783	rVB3	337	352	0.03%	0.004%
17	3.883	788	791	795	rVB3	295	212	0.02%	0.002%
18	3.909	795	799	803	rBV2	253	323	0.03%	0.004%
19	3.948	809	811	816	rVB2	179	152	0.02%	0.002%
20	4.118	860	864	869	rBV2	222	287	0.03%	0.003%
21	4.176	879	882	886	rVB	283	210	0.02%	0.002%
22	4.350	932	936	939	rBV2	206	210	0.02%	0.002%
23	4.468	971	973	977	rVV	338	208	0.02%	0.002%
24	4.546	993	997	999	rBV2	219	205	0.02%	0.002%
25	4.571	1002	1005	1010	rVB2	264	245	0.02%	0.003%
26	4.632	1010	1024	1063	rBV	99132	288121	28.59%	3.295%
27	4.938	1116	1119	1122	rBV3	298	200	0.02%	0.002%
28	5.067	1143	1159	1186	rVV2	182869	404568	40.14%	4.627%
29	5.295	1225	1230	1235	rVV4	465	570	0.06%	0.007%
30	5.729	1343	1365	1385	rBV2	377583	1007865	100.00%	11.526%
31	6.118	1481	1486	1491	rBV	363	476	0.05%	0.005%
32	6.150	1492	1496	1501	rVB3	373	301	0.03%	0.003%
33	6.250	1513	1527	1566	rBV	381252	726960	72.13%	8.313%
34	6.385	1566	1569	1572	rBV3	411	334	0.03%	0.004%
35	6.539	1607	1617	1621	rBV4	1301	1855	0.18%	0.021%
36	6.558	1621	1623	1627	rVV3	712	447	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047690.D
 Acq On : 25 Mar 2022 22:12
 Operator : SY/MD
 Sample : N2082-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.581	1627	1630	1633	rVB2	435	264	0.03%	0.003%
38	6.603	1633	1637	1638	rBV2	260	161	0.02%	0.002%
39	6.693	1651	1665	1687	rBV	234736	454604	45.11%	5.199%
40	6.806	1697	1700	1710	rVB4	829	1090	0.11%	0.012%
41	6.874	1717	1721	1725	rBV	198	164	0.02%	0.002%
42	7.108	1788	1794	1803	rVB3	578	908	0.09%	0.010%
43	7.192	1815	1820	1828	rVB5	778	1104	0.11%	0.013%
44	7.269	1842	1844	1847	rBV2	226	153	0.02%	0.002%
45	7.568	1922	1937	1954	rBV	117129	209071	20.74%	2.391%
46	7.722	1982	1985	1990	rVB3	330	300	0.03%	0.003%
47	7.748	1990	1993	1997	rBV	351	262	0.03%	0.003%
48	7.800	2004	2009	2014	rBV3	397	457	0.05%	0.005%
49	7.899	2026	2040	2056	rBV	473295	821962	81.55%	9.400%
50	8.182	2116	2128	2142	rBV	84954	144619	14.35%	1.654%
51	8.430	2202	2205	2208	rVB	275	188	0.02%	0.002%
52	8.472	2208	2218	2232	rVB5	1950	3807	0.38%	0.044%
53	8.552	2239	2243	2247	rBV2	653	540	0.05%	0.006%
54	8.574	2247	2250	2256	rVB2	402	430	0.04%	0.005%
55	8.636	2256	2269	2303	rBV	343250	643646	63.86%	7.361%
56	8.902	2346	2352	2355	rVB3	240	287	0.03%	0.003%
57	8.922	2355	2358	2362	rBV3	312	303	0.03%	0.003%
58	8.954	2366	2368	2372	rVB	266	161	0.02%	0.002%
59	9.041	2392	2395	2399	rVB	201	177	0.02%	0.002%
60	9.066	2399	2403	2405	rBV3	224	181	0.02%	0.002%
61	9.124	2417	2421	2426	rBV3	262	283	0.03%	0.003%
62	9.172	2433	2436	2440	rVB	241	177	0.02%	0.002%
63	9.246	2456	2459	2463	rBV2	173	190	0.02%	0.002%
64	9.320	2479	2482	2485	rBV	285	219	0.02%	0.003%
65	9.417	2499	2512	2547	rBV	561939	956812	94.93%	10.942%
66	9.565	2555	2558	2560	rBV2	404	242	0.02%	0.003%
67	9.697	2592	2599	2605	rVB6	1121	1530	0.15%	0.017%
68	9.735	2605	2611	2620	rBV3	324	542	0.05%	0.006%
69	9.825	2636	2639	2640	rBV	260	152	0.02%	0.002%
70	9.899	2658	2662	2667	rBV2	262	210	0.02%	0.002%
71	10.018	2695	2699	2705	rBV3	265	373	0.04%	0.004%
72	10.098	2720	2724	2727	rBV4	510	473	0.05%	0.005%
73	10.115	2727	2729	2733	rVV2	396	341	0.03%	0.004%
74	10.150	2736	2740	2746	rVV2	310	327	0.03%	0.004%
75	10.269	2771	2777	2780	rVB2	362	363	0.04%	0.004%
76	10.307	2783	2789	2791	rBV2	313	306	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047690.D
 Acq On : 25 Mar 2022 22:12
 Operator : SY/MD
 Sample : N2082-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.320	2791	2793	2796	rBV	235	182	0.02%	0.002%
78	10.491	2841	2846	2849	rBV2	473	440	0.04%	0.005%
79	10.552	2862	2865	2869	rVB	228	179	0.02%	0.002%
80	10.671	2896	2902	2912	rVB6	1359	1966	0.20%	0.022%
81	10.758	2916	2929	2948	rBV	355287	576300	57.18%	6.590%
82	10.893	2962	2971	2982	rVB3	3190	4752	0.47%	0.054%
83	11.208	3066	3069	3073	rVB2	259	206	0.02%	0.002%
84	11.256	3081	3084	3087	rBV2	338	189	0.02%	0.002%
85	11.311	3099	3101	3105	rBV2	249	193	0.02%	0.002%
86	11.439	3138	3141	3142	rBV2	363	184	0.02%	0.002%
87	11.478	3144	3153	3166	rVB5	2071	3636	0.36%	0.042%
88	11.700	3216	3222	3227	rVB4	545	547	0.05%	0.006%
89	11.812	3244	3257	3276	rBV	632014	997287	98.95%	11.405%
90	11.973	3302	3307	3316	rVB5	1387	1846	0.18%	0.021%
91	12.195	3362	3376	3398	rBV	501525	802312	79.61%	9.175%
92	12.436	3449	3451	3455	rVB2	350	183	0.02%	0.002%
93	12.462	3455	3459	3462	rBV3	232	193	0.02%	0.002%
94	12.764	3549	3553	3563	rVB3	561	886	0.09%	0.010%
95	13.028	3632	3635	3639	rBV3	289	295	0.03%	0.003%
96	13.388	3744	3747	3750	rBV2	309	196	0.02%	0.002%
97	13.973	3926	3929	3931	rBV	245	165	0.02%	0.002%
98	15.121	4283	4286	4290	rBV4	514	445	0.04%	0.005%
99	15.169	4299	4301	4304	rVB3	695	337	0.03%	0.004%
100	15.333	4350	4352	4357	rVB3	679	486	0.05%	0.006%




Sum of corrected areas: 8744417

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047690.D
Acq On : 25 Mar 2022 22:12
Operator : SY/MD
Sample : N2082-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

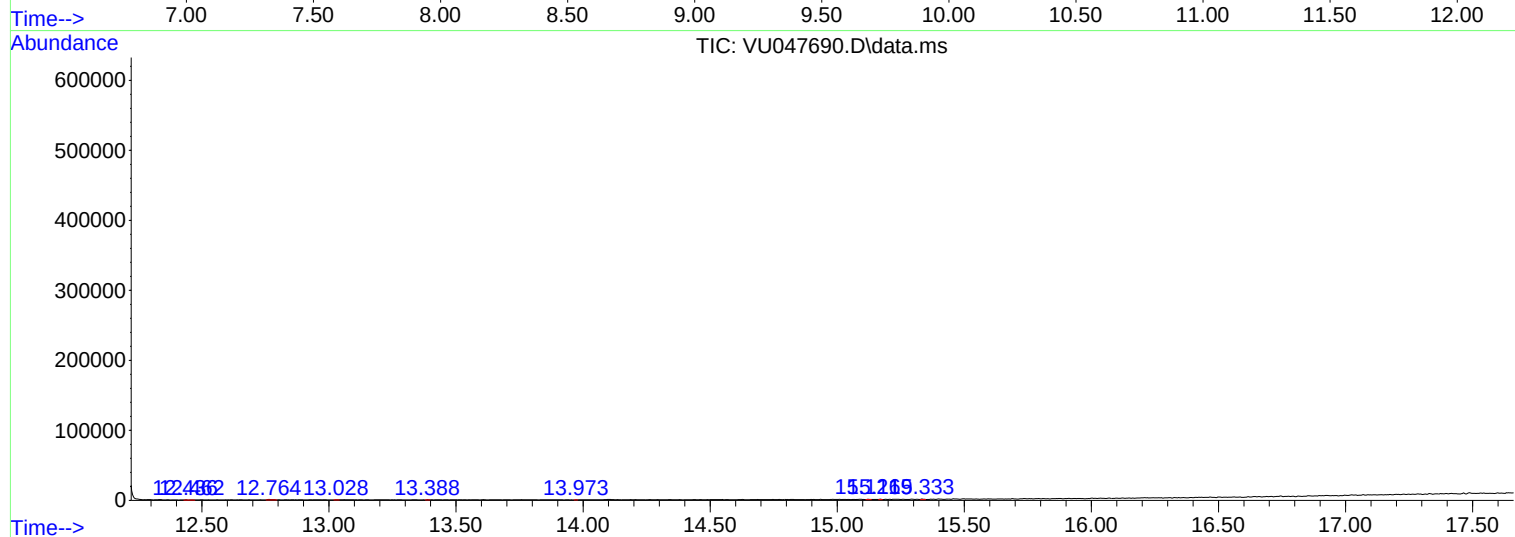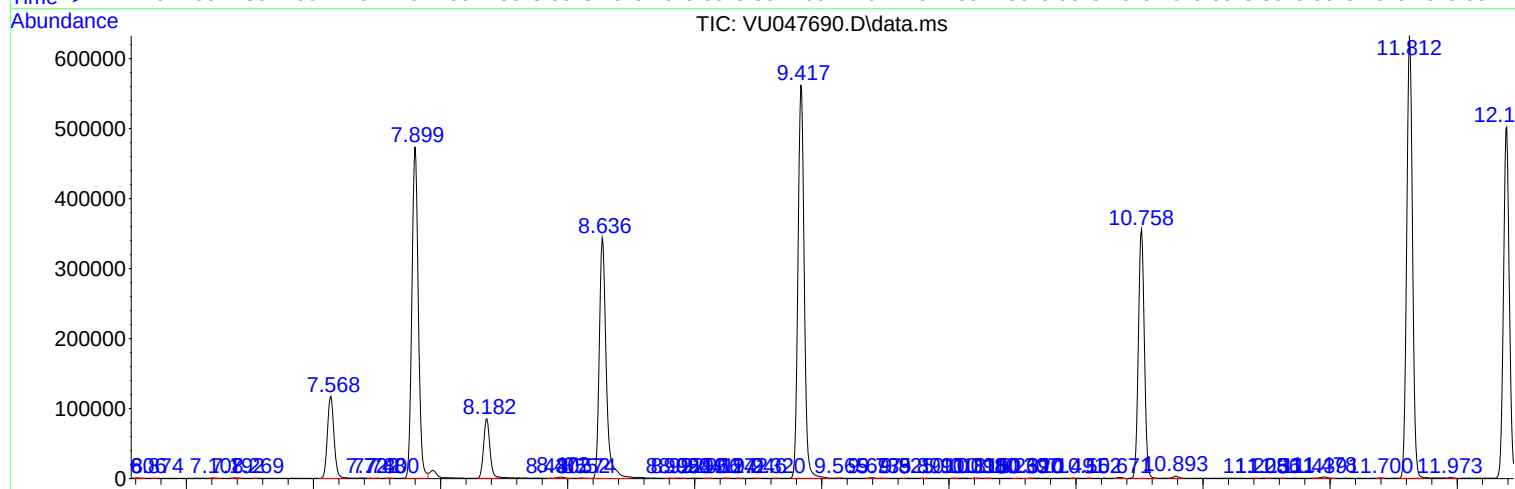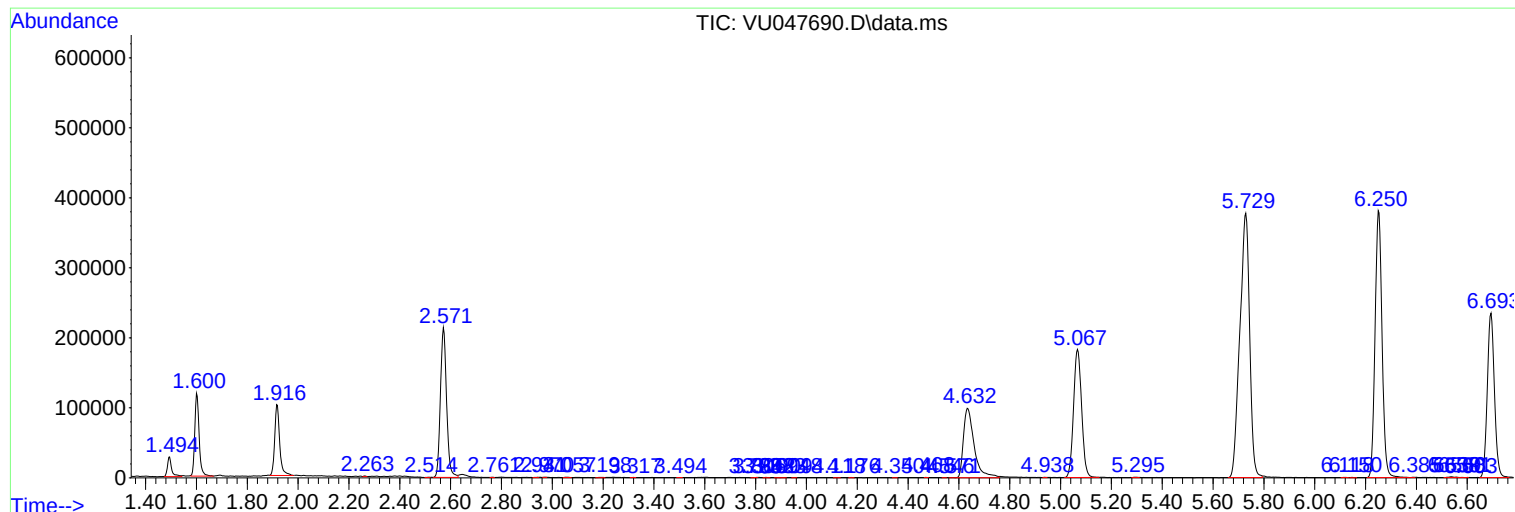

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047690.D
Acq On : 25 Mar 2022 22:12
Operator : SY/MD
Sample : N2082-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047690.D
Acq On : 25 Mar 2022 22:12
Operator : SY/MD
Sample : N2082-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------