

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047691.D
 Acq On : 25 Mar 2022 22:35
 Operator : SY/MD
 Sample : N2082-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW615

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047691.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	40	47	56	rBV	30211	32243	3.19%	0.370%
2	1.601	73	81	101	rBV	118504	139597	13.80%	1.600%
3	1.916	171	179	202	rBV	90777	128360	12.69%	1.471%
4	2.572	370	383	398	rBV	210523	349087	34.51%	4.002%
5	2.787	448	450	451	rBV	494	184	0.02%	0.002%
6	2.932	492	495	498	rBV2	482	375	0.04%	0.004%
7	2.967	503	506	508	rVV2	366	265	0.03%	0.003%
8	2.980	508	510	515	rVB2	612	527	0.05%	0.006%
9	3.189	568	575	580	rBV3	524	714	0.07%	0.008%
10	3.250	590	594	596	rBV	375	275	0.03%	0.003%
11	3.363	625	629	632	rVB4	327	245	0.02%	0.003%
12	3.382	632	635	641	rVB3	363	390	0.04%	0.004%
13	3.411	641	644	647	rBV	364	289	0.03%	0.003%
14	3.584	695	698	699	rVV2	409	273	0.03%	0.003%
15	3.684	726	729	732	rBV2	278	181	0.02%	0.002%
16	3.716	735	739	741	rBV2	279	212	0.02%	0.002%
17	3.752	748	750	754	rVB3	237	172	0.02%	0.002%
18	3.826	768	773	777	rVB2	309	317	0.03%	0.004%
19	4.025	831	835	838	rBV3	388	275	0.03%	0.003%
20	4.047	838	842	846	rBV2	258	190	0.02%	0.002%
21	4.105	853	860	862	rBV2	378	354	0.04%	0.004%
22	4.227	895	898	901	rBV2	291	179	0.02%	0.002%
23	4.552	996	999	1004	rBV2	310	234	0.02%	0.003%
24	4.642	1011	1027	1067	rBV	90027	303068	29.96%	3.474%
25	5.012	1139	1142	1143	rBV2	384	195	0.02%	0.002%
26	5.067	1143	1159	1184	rVV	184317	404683	40.01%	4.639%
27	5.295	1222	1230	1236	rVV3	492	731	0.07%	0.008%
28	5.375	1251	1255	1257	rBV	367	260	0.03%	0.003%
29	5.565	1308	1314	1317	rBV2	172	221	0.02%	0.003%
30	5.729	1343	1365	1391	rBV2	375263	1011421	100.00%	11.594%
31	5.851	1401	1403	1406	rVB2	530	225	0.02%	0.003%
32	5.983	1442	1444	1449	rVB2	433	278	0.03%	0.003%
33	6.118	1481	1486	1489	rBV2	231	265	0.03%	0.003%
34	6.250	1513	1527	1545	rBV	374675	712442	70.44%	8.167%
35	6.481	1597	1599	1604	rVB	302	192	0.02%	0.002%
36	6.526	1605	1613	1615	rBV3	1131	1077	0.11%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047691.D
 Acq On : 25 Mar 2022 22:35
 Operator : SY/MD
 Sample : N2082-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW615

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.562	1622	1624	1629	rVB3	565	403	0.04%	0.005%
38	6.584	1629	1631	1638	rVB3	507	517	0.05%	0.006%
39	6.694	1647	1665	1688	rBV	232495	452546	44.74%	5.188%
40	6.851	1711	1714	1717	rBV3	240	188	0.02%	0.002%
41	7.009	1759	1763	1768	rVV3	201	199	0.02%	0.002%
42	7.063	1776	1780	1785	rVB2	359	310	0.03%	0.004%
43	7.189	1815	1819	1822	rBV3	757	610	0.06%	0.007%
44	7.243	1834	1836	1841	rVV2	292	266	0.03%	0.003%
45	7.340	1861	1866	1869	rBV2	254	262	0.03%	0.003%
46	7.369	1872	1875	1879	rBV	327	282	0.03%	0.003%
47	7.411	1885	1888	1892	rVB2	259	175	0.02%	0.002%
48	7.443	1892	1898	1902	rVB2	289	327	0.03%	0.004%
49	7.497	1912	1915	1918	rBV3	312	234	0.02%	0.003%
50	7.568	1924	1937	1954	rBV	117511	207666	20.53%	2.381%
51	7.687	1969	1974	1986	rVB5	833	1452	0.14%	0.017%
52	7.803	1999	2010	2013	rBV3	620	1026	0.10%	0.012%
53	7.899	2021	2040	2055	rBV	475507	818078	80.88%	9.378%
54	8.182	2115	2128	2148	rBV	82549	146160	14.45%	1.676%
55	8.472	2212	2218	2220	rBV3	1526	1634	0.16%	0.019%
56	8.639	2257	2270	2307	rBV	338576	662669	65.52%	7.596%
57	8.909	2352	2354	2356	rBV2	339	193	0.02%	0.002%
58	9.009	2381	2385	2388	rBV2	268	207	0.02%	0.002%
59	9.034	2388	2393	2395	rBV2	245	212	0.02%	0.002%
60	9.173	2433	2436	2439	rBV	281	226	0.02%	0.003%
61	9.301	2473	2476	2478	rBV2	262	209	0.02%	0.002%
62	9.314	2478	2480	2487	rVB2	235	272	0.03%	0.003%
63	9.417	2499	2512	2548	rBV	561880	950353	93.96%	10.894%
64	9.661	2584	2588	2592	rBV2	237	265	0.03%	0.003%
65	9.697	2592	2599	2609	rVB3	1107	1470	0.15%	0.017%
66	9.796	2627	2630	2634	rVB2	219	189	0.02%	0.002%
67	9.861	2647	2650	2654	rVB2	324	233	0.02%	0.003%
68	9.886	2654	2658	2660	rBV2	286	187	0.02%	0.002%
69	9.989	2687	2690	2692	rBV	219	170	0.02%	0.002%
70	10.201	2752	2756	2762	rVB2	282	250	0.02%	0.003%
71	10.240	2762	2768	2774	rBV	444	458	0.05%	0.005%
72	10.298	2780	2786	2792	rVB3	387	583	0.06%	0.007%
73	10.333	2793	2797	2800	rBV3	337	291	0.03%	0.003%
74	10.362	2800	2806	2809	rVB2	217	204	0.02%	0.002%
75	10.481	2840	2843	2852	rVB3	424	422	0.04%	0.005%
76	10.523	2852	2856	2860	rBV2	225	232	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047691.D
 Acq On : 25 Mar 2022 22:35
 Operator : SY/MD
 Sample : N2082-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW615

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.594	2875	2878	2882	rBV2	305	221	0.02%	0.003%
78	10.674	2894	2903	2911	rVB5	1553	2306	0.23%	0.026%
79	10.758	2915	2929	2947	rBV	362822	584039	57.74%	6.695%
80	10.896	2964	2972	2981	rVB3	2805	4420	0.44%	0.051%
81	11.111	3037	3039	3042	rVB	282	174	0.02%	0.002%
82	11.221	3070	3073	3077	rBV3	246	206	0.02%	0.002%
83	11.298	3095	3097	3100	rVB3	298	220	0.02%	0.003%
84	11.452	3141	3145	3146	rBV2	1061	613	0.06%	0.007%
85	11.587	3183	3187	3191	rBV3	204	217	0.02%	0.002%
86	11.693	3217	3220	3225	rBV3	636	570	0.06%	0.007%
87	11.767	3240	3243	3245	rBV2	297	199	0.02%	0.002%
88	11.812	3245	3257	3276	rVV	625692	985213	97.41%	11.294%
89	11.938	3294	3296	3299	rVB3	560	286	0.03%	0.003%
90	11.970	3304	3306	3307	rBV	400	170	0.02%	0.002%
91	12.034	3323	3326	3328	rBV	250	193	0.02%	0.002%
92	12.076	3336	3339	3342	rVB3	449	292	0.03%	0.003%
93	12.121	3348	3353	3354	rBV	280	210	0.02%	0.002%
94	12.134	3355	3357	3361	rVB	400	254	0.03%	0.003%
95	12.195	3361	3376	3394	rBV	494799	798762	78.97%	9.157%
96	12.510	3472	3474	3479	rVB2	241	195	0.02%	0.002%
97	12.671	3518	3524	3525	rBV	203	237	0.02%	0.003%
98	12.774	3546	3556	3563	rBV5	1014	1988	0.20%	0.023%
99	14.340	4040	4043	4047	rVB3	479	328	0.03%	0.004%
100	15.365	4359	4362	4364	rBV2	763	427	0.04%	0.005%




Sum of corrected areas: 8723366

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047691.D
Acq On : 25 Mar 2022 22:35
Operator : SY/MD
Sample : N2082-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

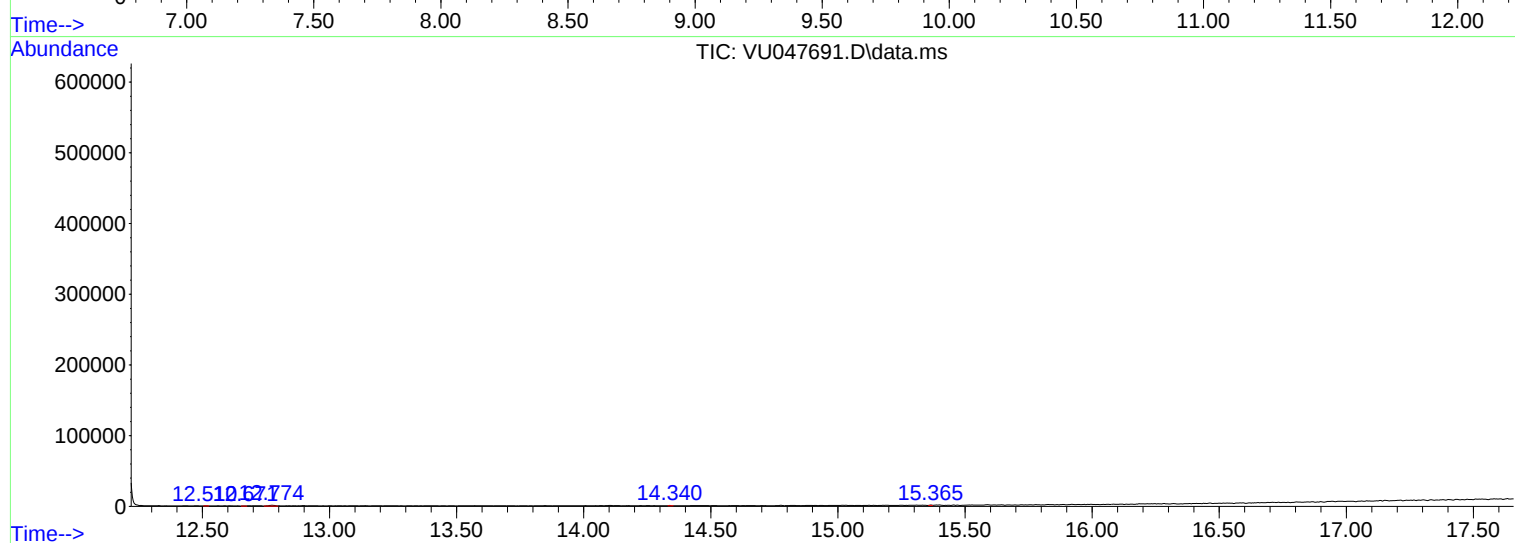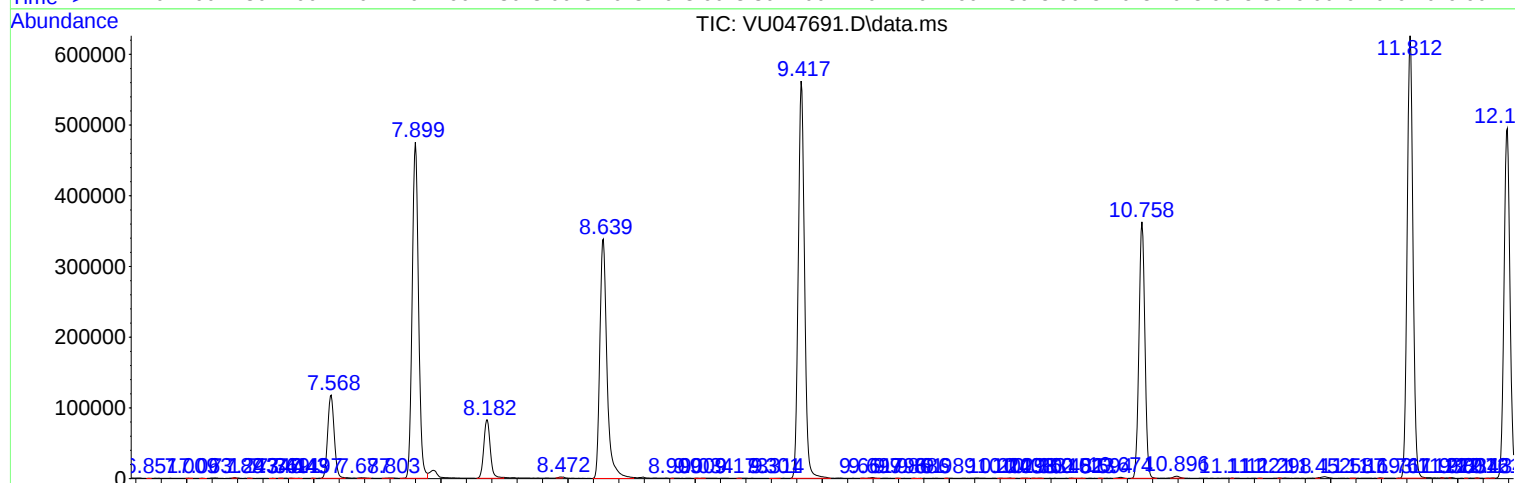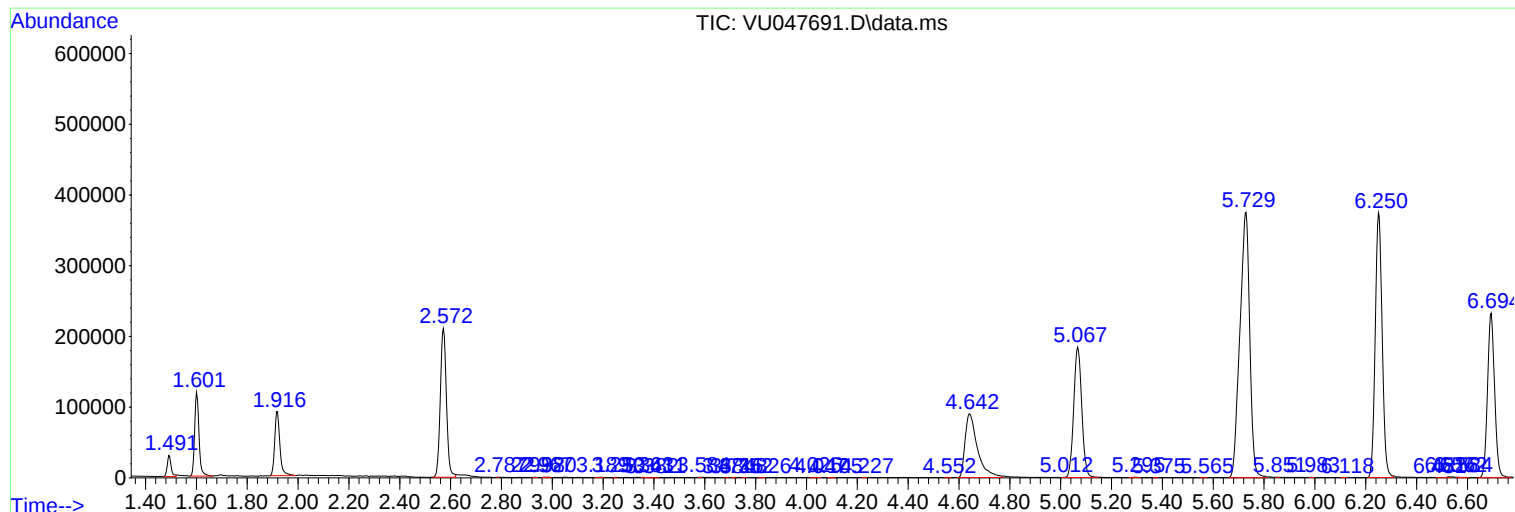

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047691.D
Acq On : 25 Mar 2022 22:35
Operator : SY/MD
Sample : N2082-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
Data File : VU047691.D
Acq On : 25 Mar 2022 22:35
Operator : SY/MD
Sample : N2082-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------