


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032522\
 Data File : VU047663.D
 Acq On : 25 Mar 2022 09:08
 Operator : SY/MD
 Sample : BFB054
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB054

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U031822DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Mar 18 13:19:37 2022

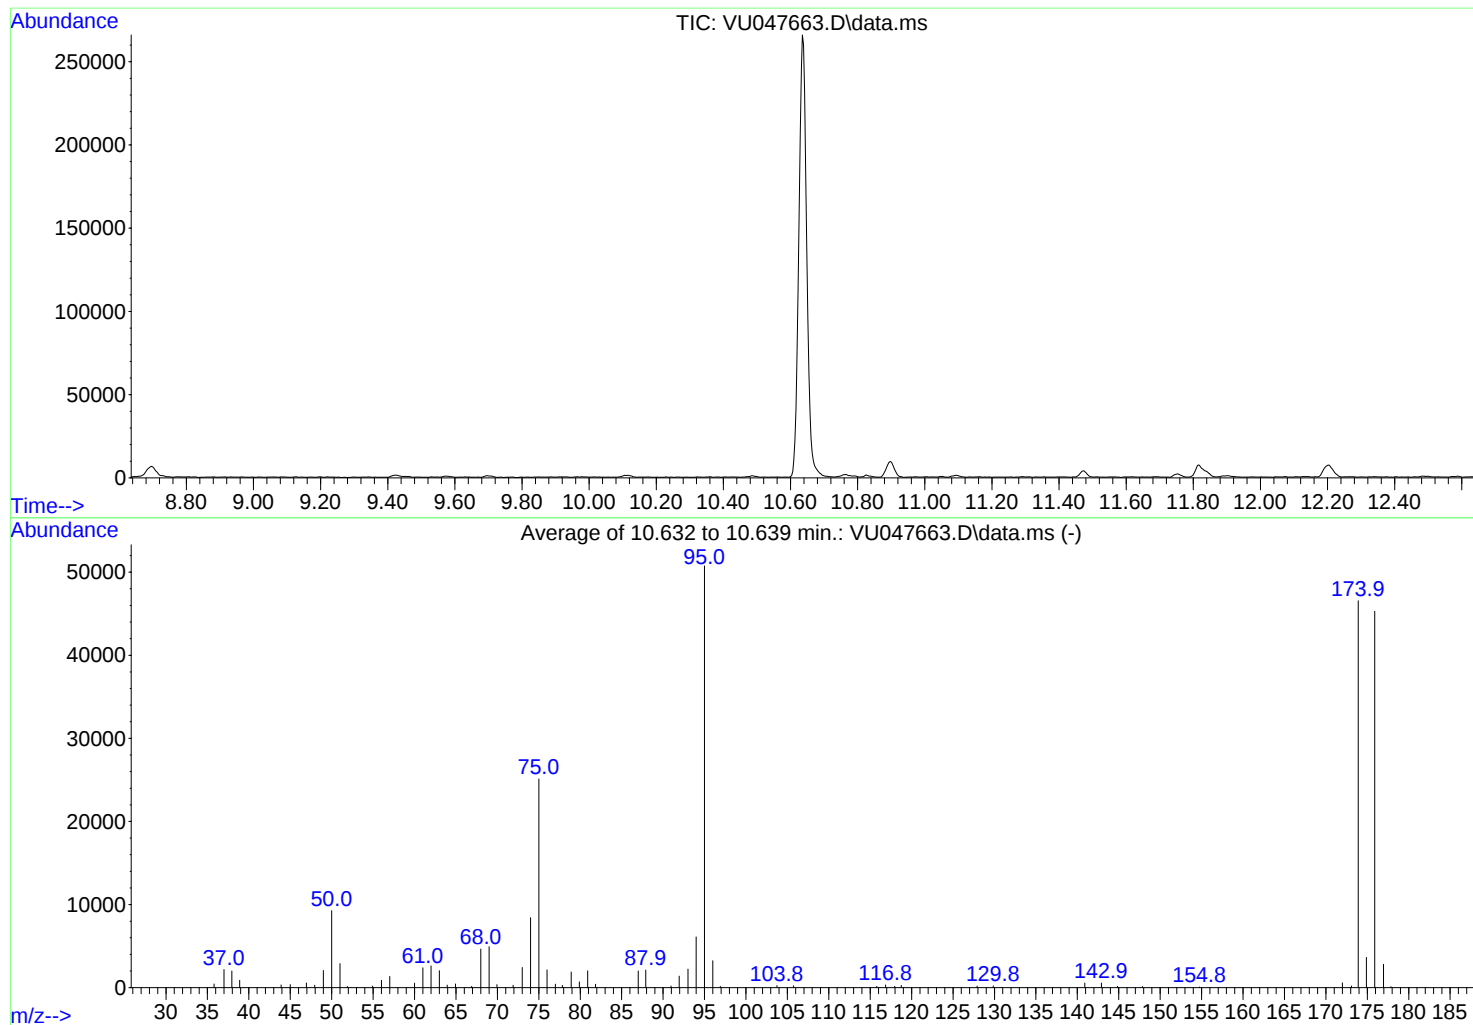

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	9267	PASS
75	95	30	60	49.5	25107	PASS
95	95	100	100	100.0	50763	PASS
96	95	5	9	6.4	3235	PASS
173	174	0.00	2	0.4	190	PASS
174	95	50	100	91.7	46563	PASS
175	174	5	9	7.8	3639	PASS
176	174	95	101	97.3	45291	PASS
177	176	5	9	6.2	2807	PASS

m/z	Abundance
39.80	162.0
43.90	301.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.80	475.0
37.00	2113.0
37.90	2034.0
38.90	936.0
40.00	150.0
43.90	533.0
45.00	400.0
46.90	596.0
47.90	264.0
49.00	2167.0
50.00	8949.0
51.00	3015.0
51.90	132.0
54.90	194.0
56.00	843.0
57.00	1215.0
60.00	516.0
61.00	2348.0
62.00	2576.0
63.00	1963.0
63.90	266.0
64.90	447.0
66.90	140.0
68.00	4702.0
69.00	4528.0
70.00	411.0
71.90	262.0
73.00	2305.0
74.00	8169.0
75.00	24248.0
76.00	2058.0
77.00	385.0
77.80	259.0
78.90	1838.0
79.90	601.0
80.90	1965.0
81.80	388.0
87.00	1895.0
87.90	2003.0
90.90	184.0
91.90	1253.0
93.00	2076.0
94.00	5863.0
95.00	49432.0
96.00	3246.0
96.90	192.0
103.70	240.0
105.80	220.0
115.70	144.0
116.90	324.0
118.00	163.0
118.80	284.0
127.90	156.0
129.80	229.0
140.90	542.0
142.90	538.0
144.90	137.0
147.80	112.0
154.70	109.0
172.00	480.0
173.90	43768.0
174.90	3383.0
175.90	42312.0
176.90	2499.0
177.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.80	467.0
37.00	2235.0
37.90	2081.0
38.90	910.0
40.00	152.0
43.90	637.0
45.00	376.0
46.00	113.0
47.00	591.0
47.90	290.0
49.00	2115.0
50.00	9588.0
51.00	2970.0
51.90	143.0
54.90	199.0
56.00	912.0
57.00	1405.0
60.00	539.0
61.00	2445.0
62.00	2740.0
63.00	2108.0
64.00	322.0
64.90	459.0
66.90	163.0
68.00	4718.0
69.00	5091.0
69.90	375.0
71.90	293.0
73.00	2516.0
74.00	8624.0
75.00	25912.0
76.00	2218.0
77.00	463.0
77.80	273.0
78.90	1962.0
79.90	724.0
80.90	2085.0
81.80	408.0
86.00	106.0
87.00	2095.0
87.90	2180.0
91.00	197.0
91.90	1433.0
93.00	2322.0
94.00	6345.0
95.00	52544.0
96.00	3317.0
96.90	150.0
103.80	269.0
105.80	231.0
115.80	165.0
116.80	343.0
117.90	162.0
118.80	280.0
127.90	205.0
129.80	210.0
130.80	109.0
140.90	576.0
142.90	560.0
144.90	158.0
147.80	147.0
154.80	100.0
172.00	602.0
173.90	48232.0
174.90	3772.0
175.90	46576.0
176.90	2874.0
177.90	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.80	414.0
37.00	2193.0
38.00	1899.0
38.90	810.0
40.00	133.0
43.90	693.0
45.00	351.0
47.00	521.0
48.00	285.0
49.00	1902.0
50.00	9265.0
51.00	2661.0
51.90	134.0
55.00	193.0
56.00	890.0
57.00	1409.0
60.00	558.0
61.00	2361.0
62.00	2536.0
63.00	2039.0
64.00	331.0
65.00	396.0
66.90	156.0
68.00	4482.0
69.00	5175.0
69.90	343.0
71.90	285.0
73.00	2484.0
74.00	8468.0
75.00	25160.0
76.00	2143.0
77.00	417.0
77.90	261.0
78.90	1883.0
79.90	733.0
80.90	2010.0
81.90	397.0
87.00	2019.0
87.90	2164.0
91.00	189.0
92.00	1499.0
93.00	2310.0
94.00	6094.0
95.00	50312.0
96.00	3142.0
96.90	103.0
103.80	265.0
105.70	227.0
115.90	161.0
116.80	331.0
117.90	169.0
118.70	267.0
127.90	209.0
129.90	216.0
140.90	534.0
142.90	561.0
144.80	150.0
147.90	134.0
172.00	638.0
173.10	571.0
173.90	47688.0
174.90	3763.0
175.90	46984.0
177.00	3048.0
177.80	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054