

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032524\
 Data File : VU058214.D
 Acq On : 25 Mar 2024 17:02
 Operator : MD/SY
 Sample : P1841-01DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU058214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	108	rVB	37923	41404	15.13%	1.692%
2	1.910	184	193	204	rBV	34831	44071	16.11%	1.801%
3	2.563	385	396	411	rBV	56263	94124	34.40%	3.847%
4	3.039	533	544	555	rBV	3289	5958	2.18%	0.244%
5	4.627	1025	1038	1071	rBV3	32500	110828	40.50%	4.530%
6	5.055	1155	1171	1193	rBV	53754	121331	44.34%	4.959%
7	5.717	1358	1377	1396	rBV2	107294	273628	100.00%	11.183%
8	6.241	1526	1540	1560	rBV	86454	165793	60.59%	6.776%
9	6.534	1617	1631	1658	rBV	136360	264081	96.51%	10.793%
10	6.682	1665	1677	1698	rVB	66755	129254	47.24%	5.283%
11	7.560	1940	1950	1966	rBV	28300	50193	18.34%	2.051%
12	7.891	2042	2053	2079	rBV	125914	223543	81.70%	9.136%
13	8.177	2132	2142	2161	rBV2	15143	26864	9.82%	1.098%
14	8.550	2248	2258	2271	rVB2	13320	22315	8.16%	0.912%
15	8.630	2271	2283	2318	rBV2	113386	239017	87.35%	9.769%
16	9.412	2514	2526	2550	rBV	121028	207251	75.74%	8.470%
17	10.749	2932	2942	2961	rBV2	40478	67164	24.55%	2.745%
18	11.807	3259	3271	3294	rBV	111116	182622	66.74%	7.464%
19	12.187	3376	3389	3412	rBV	106821	177311	64.80%	7.247%




Sum of corrected areas: 2446752

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032524\
Data File : VU058214.D
Acq On : 25 Mar 2024 17:02
Operator : MD/SY
Sample : P1841-01DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

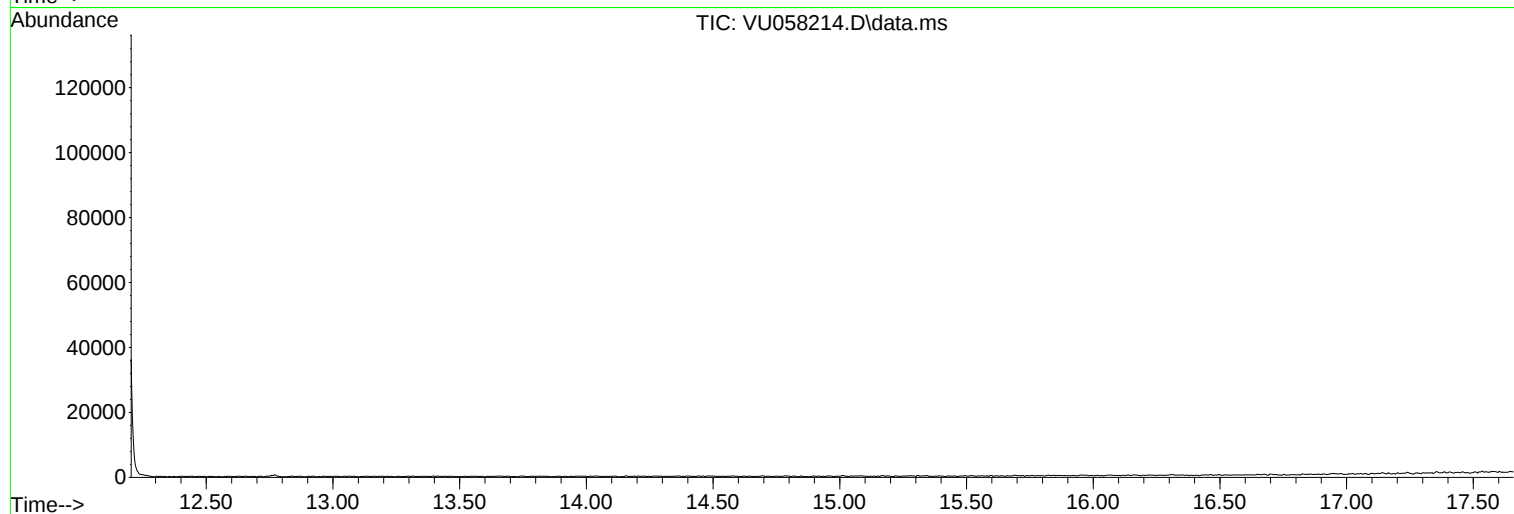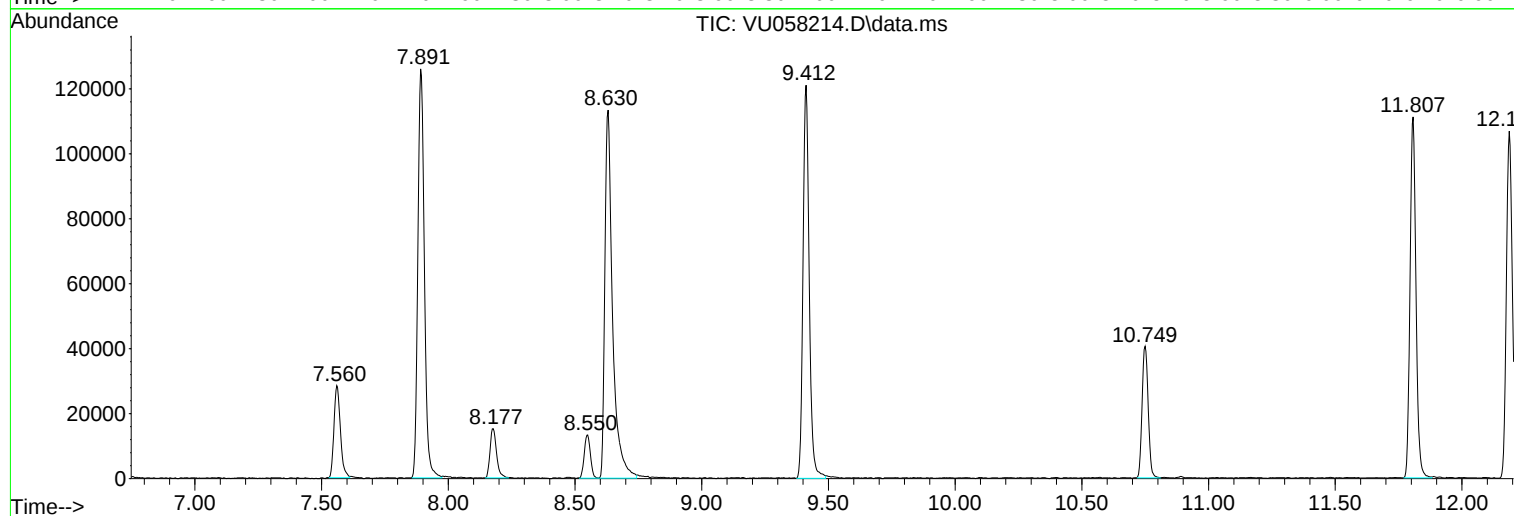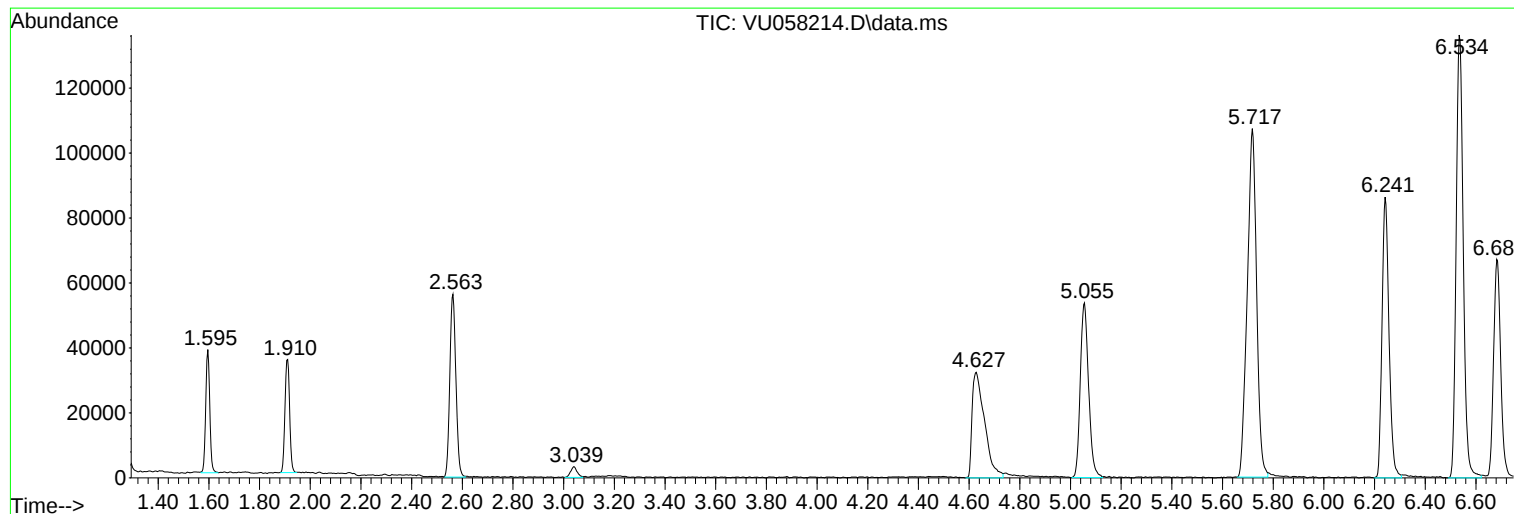

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032524\
Data File : VU058214.D
Acq On : 25 Mar 2024 17:02
Operator : MD/SY
Sample : P1841-01DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032524\
Data File : VU058214.D
Acq On : 25 Mar 2024 17:02
Operator : MD/SY
Sample : P1841-01DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc