

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032524\
 Data File : VU058215.D
 Acq On : 25 Mar 2024 17:26
 Operator : MD/SY
 Sample : P1841-02DL 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU058215.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	108	rVB	38363	42611	15.11%	1.713%
2	1.908	184	192	203	rVB	35513	43882	15.56%	1.764%
3	2.560	384	395	414	rVB2	58781	98367	34.88%	3.954%
4	3.039	535	544	555	rBV4	3108	5828	2.07%	0.234%
5	4.628	1027	1038	1076	rBV3	32964	110740	39.26%	4.451%
6	5.055	1157	1171	1196	rVB	55157	122693	43.50%	4.931%
7	5.718	1357	1377	1397	rBV2	109271	282033	100.00%	11.336%
8	6.242	1525	1540	1562	rBV	87779	169452	60.08%	6.811%
9	6.534	1616	1631	1656	rBV	132597	254984	90.41%	10.249%
10	6.682	1665	1677	1697	rVB	66707	130976	46.44%	5.264%
11	7.560	1939	1950	1965	rBV	28490	51470	18.25%	2.069%
12	7.891	2041	2053	2089	rBV	129495	228194	80.91%	9.172%
13	8.174	2132	2141	2155	rBV	15733	26621	9.44%	1.070%
14	8.547	2244	2257	2269	rBV2	13997	23217	8.23%	0.933%
15	8.631	2272	2283	2322	rBV2	116097	245044	86.88%	9.849%
16	9.412	2514	2526	2554	rBV	121928	211828	75.11%	8.514%
17	10.750	2929	2942	2959	rBV	41434	68765	24.38%	2.764%
18	11.804	3260	3270	3289	rBV	111651	187322	66.42%	7.529%
19	12.187	3378	3389	3415	rBV	109399	183927	65.21%	7.393%




Sum of corrected areas: 2487954

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032524\
Data File : VU058215.D
Acq On : 25 Mar 2024 17:26
Operator : MD/SY
Sample : P1841-02DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

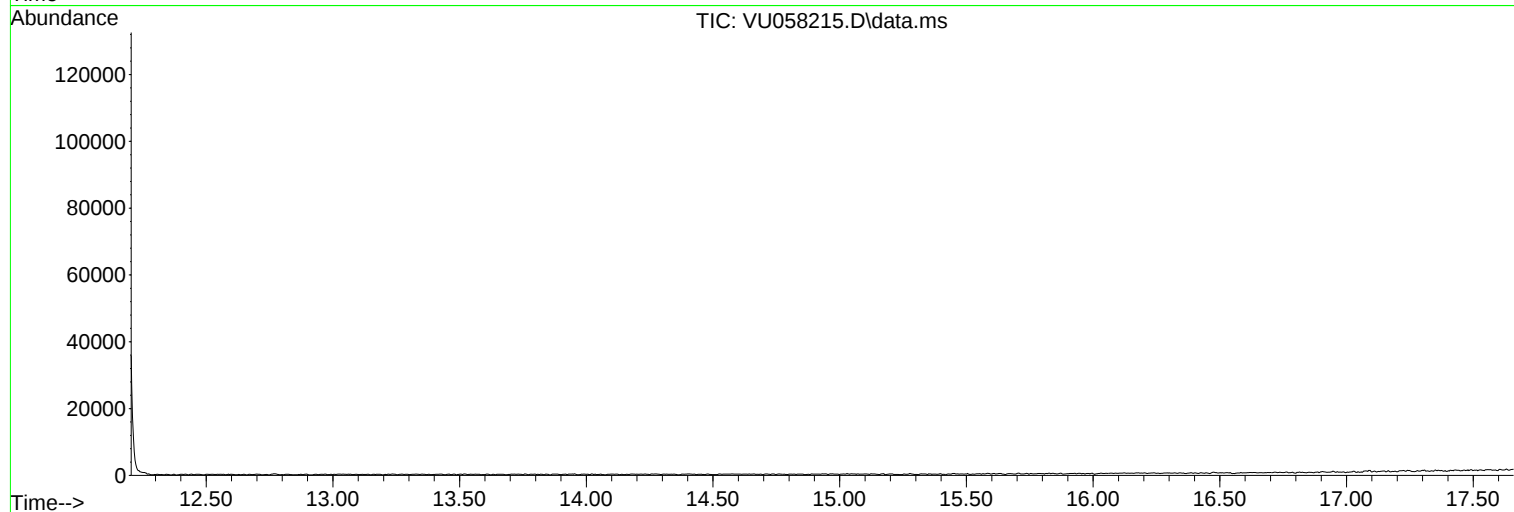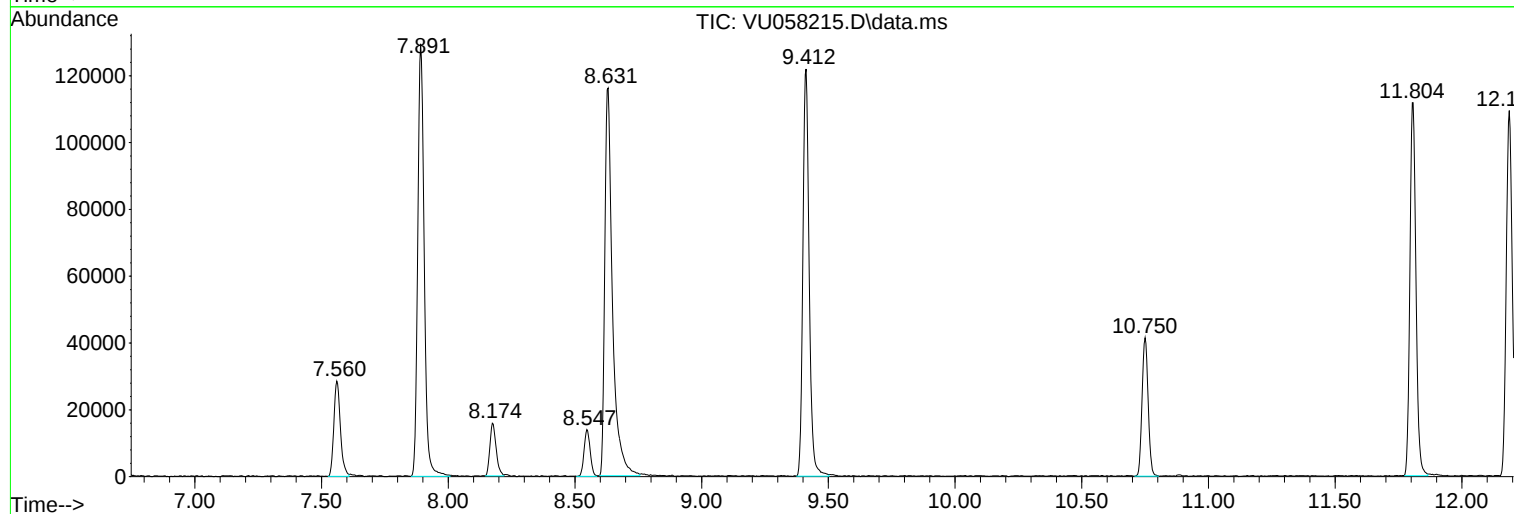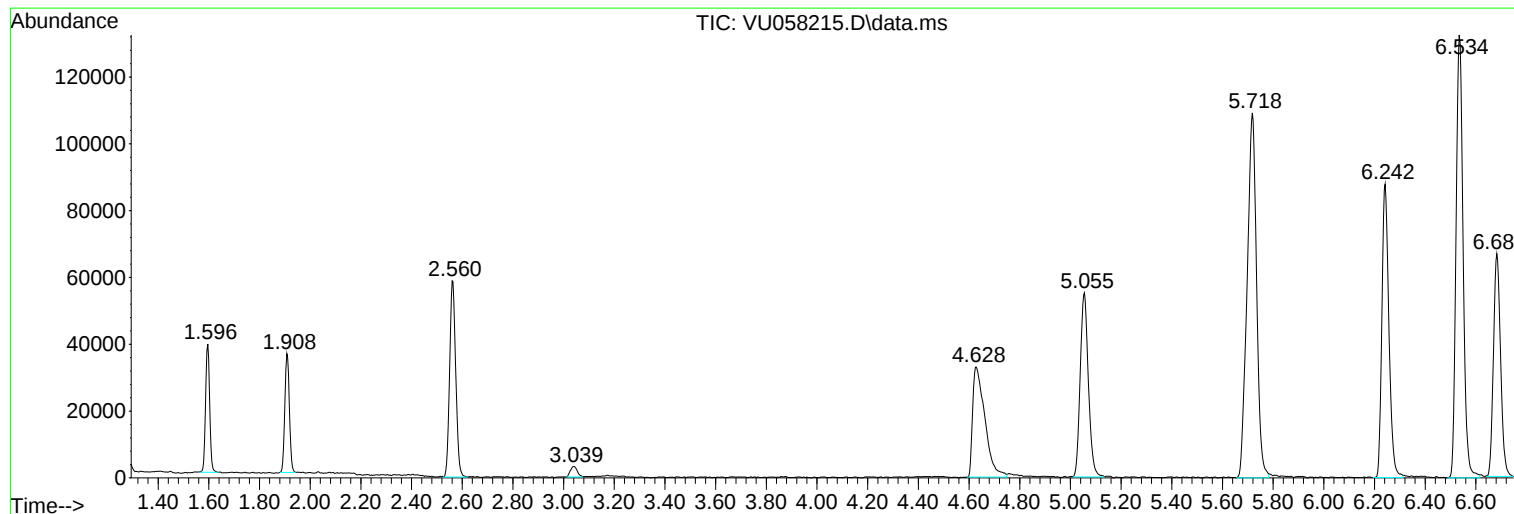

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032524\
Data File : VU058215.D
Acq On : 25 Mar 2024 17:26
Operator : MD/SY
Sample : P1841-02DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032524\
Data File : VU058215.D
Acq On : 25 Mar 2024 17:26
Operator : MD/SY
Sample : P1841-02DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc