


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032524\
Data File : VU058209.D
Acq On : 25 Mar 2024 13:57
Operator : MD/SY
Sample : BFB129
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB129

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Mar 26 01:41:16 2024

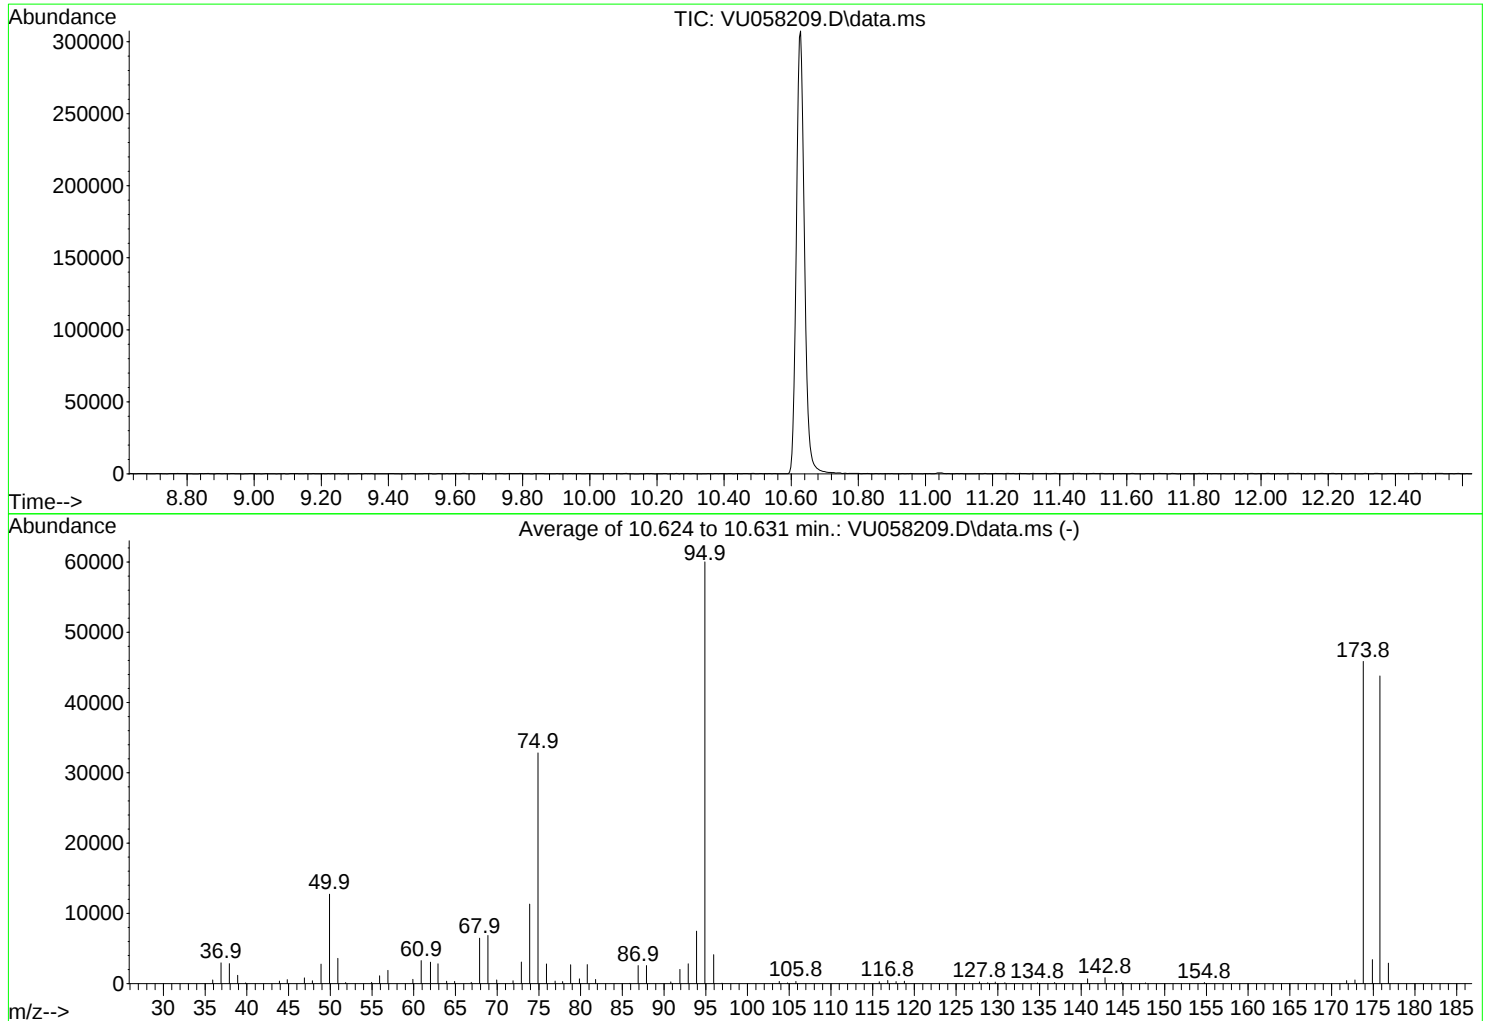

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	12737	PASS
75	95	30	80	54.7	32832	PASS
95	95	100	100	100.0	60024	PASS
96	95	5	9	6.9	4128	PASS
173	174	0.00	2	1.1	518	PASS
174	95	50	120	76.4	45856	PASS
175	174	5	9	7.5	3427	PASS
176	174	95	101	95.5	43784	PASS
177	176	5	9	6.7	2916	PASS

m/z	Abundance
43.80	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB129

m/z	Abundance
35.90	514.0
36.90	3065.0
37.90	2914.0
38.90	1313.0
39.80	140.0
43.90	555.0
44.90	540.0
46.90	833.0
47.90	472.0
48.90	2854.0
49.90	13232.0
50.90	3707.0
51.90	167.0
54.90	172.0
55.90	1123.0
56.90	1903.0
59.90	612.0
60.90	3396.0
62.00	3115.0
62.90	2758.0
64.00	367.0
64.90	356.0
66.90	161.0
67.90	6880.0
68.90	7166.0
70.00	507.0
71.90	405.0
72.90	2990.0
73.90	11427.0
74.90	33744.0
75.90	2734.0
77.00	430.0
77.80	322.0
78.80	2798.0
79.90	695.0
80.80	2722.0
81.80	600.0
86.90	2624.0
87.90	2628.0
90.80	251.0
91.90	2128.0
92.90	2840.0
93.90	7563.0
94.90	61232.0
96.00	4387.0
97.00	117.0
103.80	297.0
104.80	102.0
105.80	370.0
115.80	280.0
116.80	468.0
117.80	262.0
118.80	384.0
127.80	266.0
128.80	154.0
129.60	232.0
130.90	131.0
134.70	125.0
136.80	146.0
140.80	696.0
142.80	911.0
144.90	171.0
147.70	124.0
154.80	155.0
171.80	438.0
172.90	526.0
173.80	45336.0
174.90	3508.0
175.80	43472.0
176.80	2911.0

Instrument :
MSVOA_U
ClientSampleId :
BFB129

m/z	Abundance
35.90	547.0
36.90	3000.0
37.90	2917.0
38.90	1201.0
39.90	119.0
44.00	539.0
44.80	583.0
46.90	867.0
47.80	433.0
48.90	2858.0
49.90	13179.0
50.90	3688.0
51.90	170.0
54.90	198.0
55.90	1154.0
56.90	1959.0
59.90	643.0
60.90	3374.0
62.00	3127.0
62.90	2947.0
63.90	340.0
64.90	343.0
66.90	177.0
67.90	6600.0
68.90	7076.0
69.90	527.0
71.90	429.0
72.90	3154.0
73.90	11530.0
74.90	33712.0
75.90	2909.0
77.00	371.0
77.80	307.0
78.80	2762.0
79.80	701.0
80.80	2810.0
81.80	625.0
85.90	111.0
86.90	2645.0
87.90	2651.0
90.80	260.0
91.90	2087.0
92.90	2913.0
93.90	7624.0
94.90	61888.0
95.90	4223.0
103.80	322.0
104.80	123.0
105.80	326.0
115.80	289.0
116.80	463.0
117.80	316.0
118.80	348.0
127.80	248.0
128.80	135.0
129.70	244.0
130.80	131.0
134.70	108.0
136.80	178.0
140.80	688.0
142.80	879.0
144.80	177.0
147.70	120.0
154.70	175.0
171.80	466.0
172.80	528.0
173.80	47320.0
174.90	3527.0
175.80	44984.0
176.80	3017.0

Instrument :
MSVOA_U
ClientSampleId :
BFB129

m/z	Abundance
35.90	525.0
36.90	2837.0
37.90	2718.0
38.90	1043.0
39.90	102.0
43.90	508.0
44.80	603.0
46.90	780.0
47.80	336.0
48.90	2616.0
49.90	11799.0
50.90	3382.0
51.80	170.0
55.00	192.0
55.90	1074.0
56.90	1831.0
59.90	610.0
60.90	3089.0
62.00	2888.0
62.90	2785.0
63.90	298.0
64.90	281.0
66.90	185.0
67.90	5924.0
68.90	6335.0
69.90	531.0
71.90	384.0
72.90	3094.0
73.90	10973.0
74.90	31040.0
75.90	2781.0
76.90	314.0
77.90	283.0
78.80	2506.0
79.80	674.0
80.80	2621.0
81.80	559.0
86.90	2484.0
87.90	2464.0
90.80	243.0
91.90	1859.0
92.90	2726.0
93.90	7235.0
94.90	56952.0
95.90	3775.0
96.90	100.0
103.80	329.0
104.80	106.0
105.80	276.0
115.80	252.0
116.80	426.0
117.80	325.0
118.80	303.0
127.80	209.0
128.80	109.0
129.80	242.0
130.80	117.0
134.80	102.0
136.80	162.0
140.70	658.0
142.90	751.0
144.80	157.0
147.70	102.0
154.70	161.0
171.80	426.0
172.70	500.0
173.80	44912.0
174.90	3246.0
175.80	42896.0
176.80	2820.0

Instrument :
MSVOA_U
ClientSampleId :
BFB129