

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Quantitation Report (QT Reviewed)


Data File : VU030435.D
Acq On : 26 Mar 2019 11:37
Operator : JC/SP
Sample : K2070-15DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09E1DL

Manual Integrations
APPROVED

MMDadoda
3/27/2019 9:55:24 AM

Quant Time: Mar 27 05:07:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 04:29:49 2019
Response via : Initial Calibration

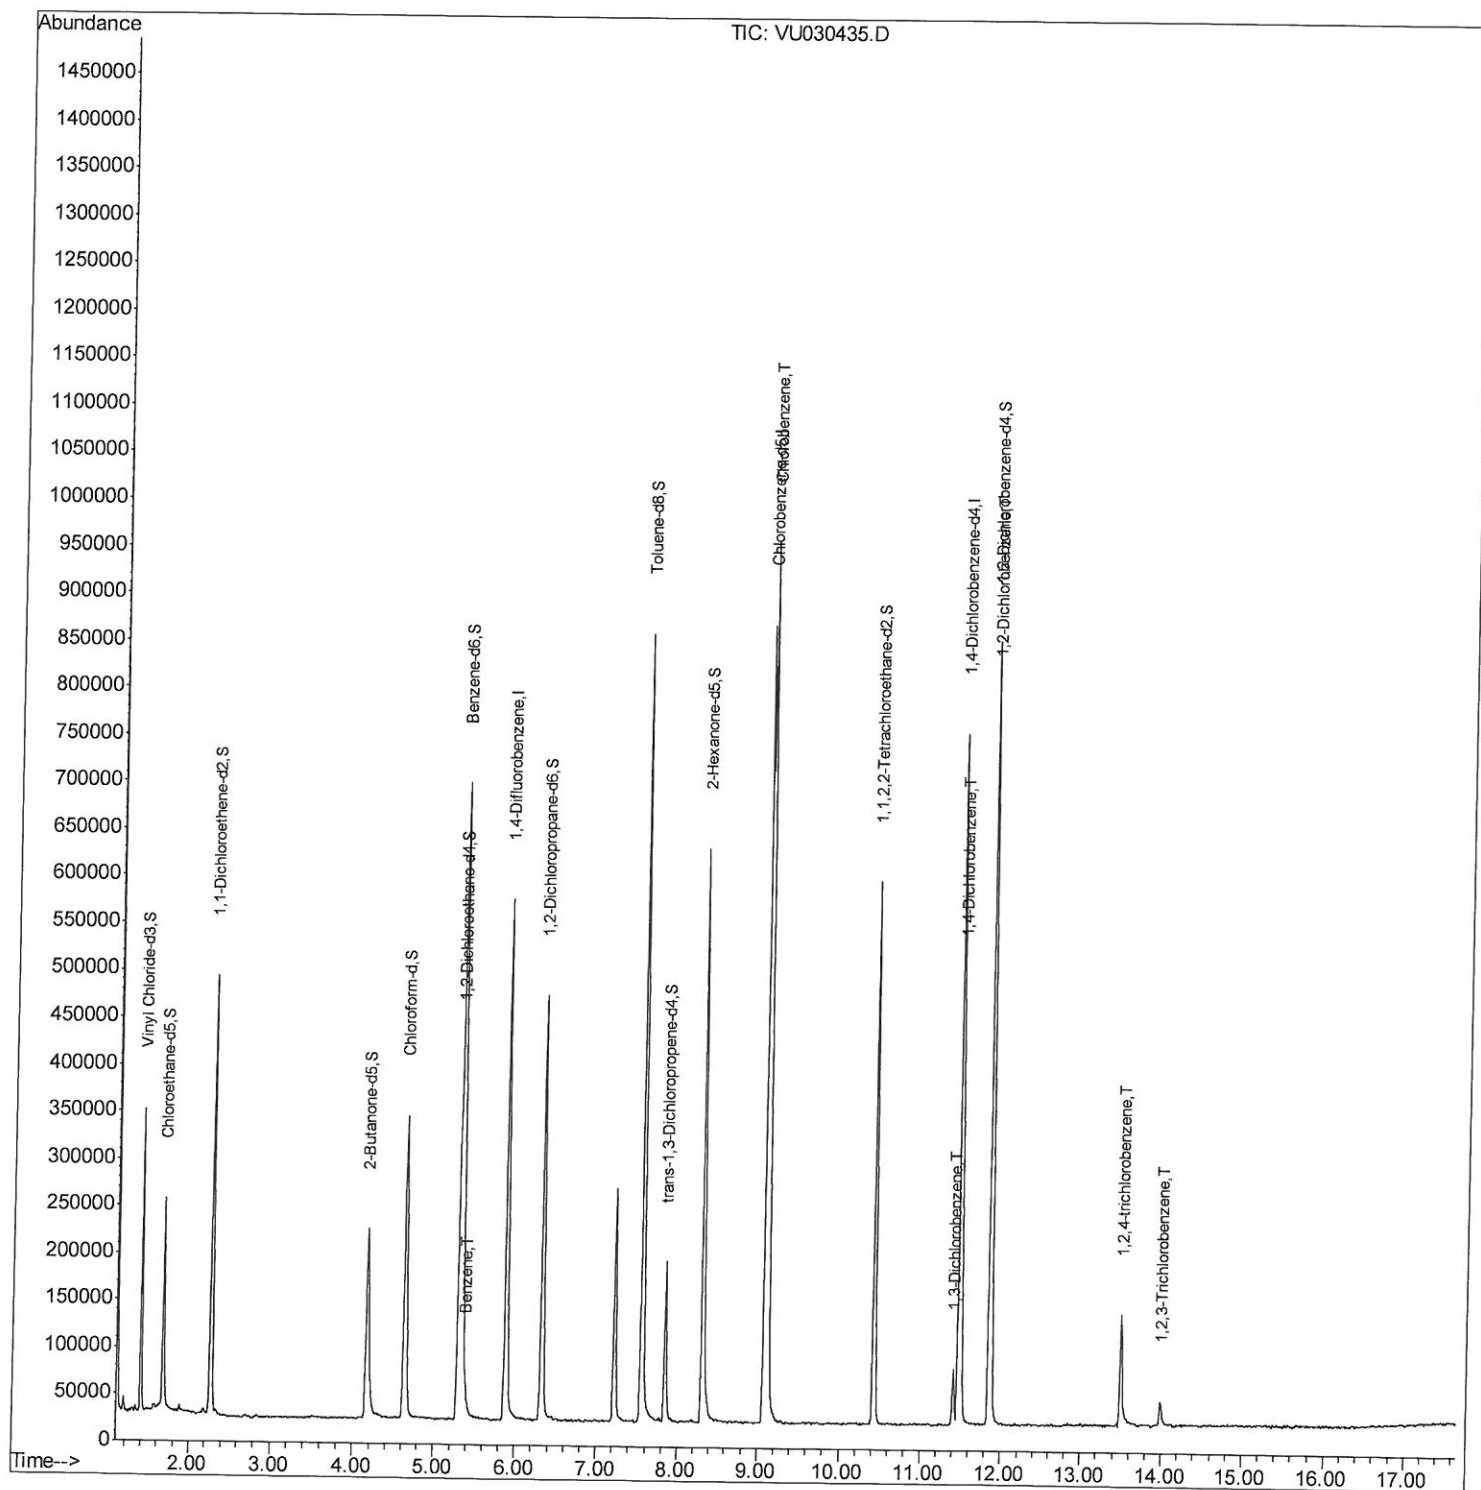

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Quantitation Report (Qedit)




Data File : VU030435.D
Acq On : 26 Mar 2019 11:37
Operator : JC/SP
Sample : K2070-15DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09E1DL

Manual Integrations
APPROVED

MMDadoda
3/27/2019 9:55:24 AM

Quant Time: Mar 27 04:33:25 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 04:29:49 2019
Response via : Initial Calibration

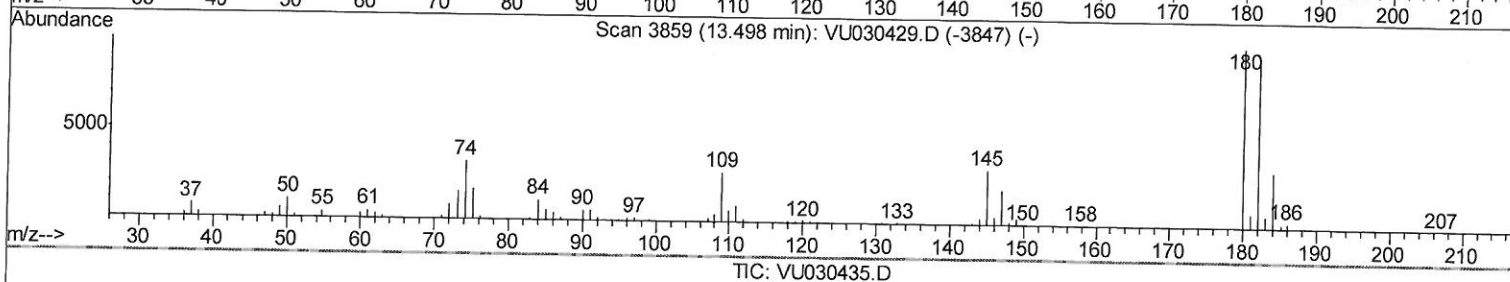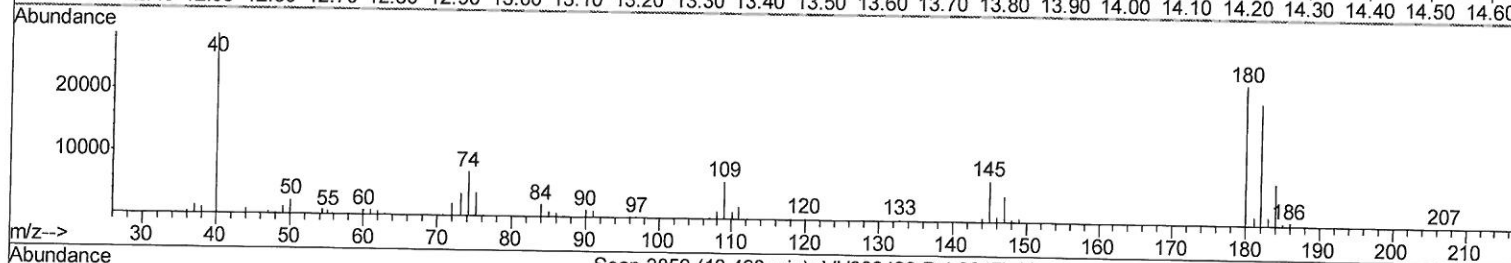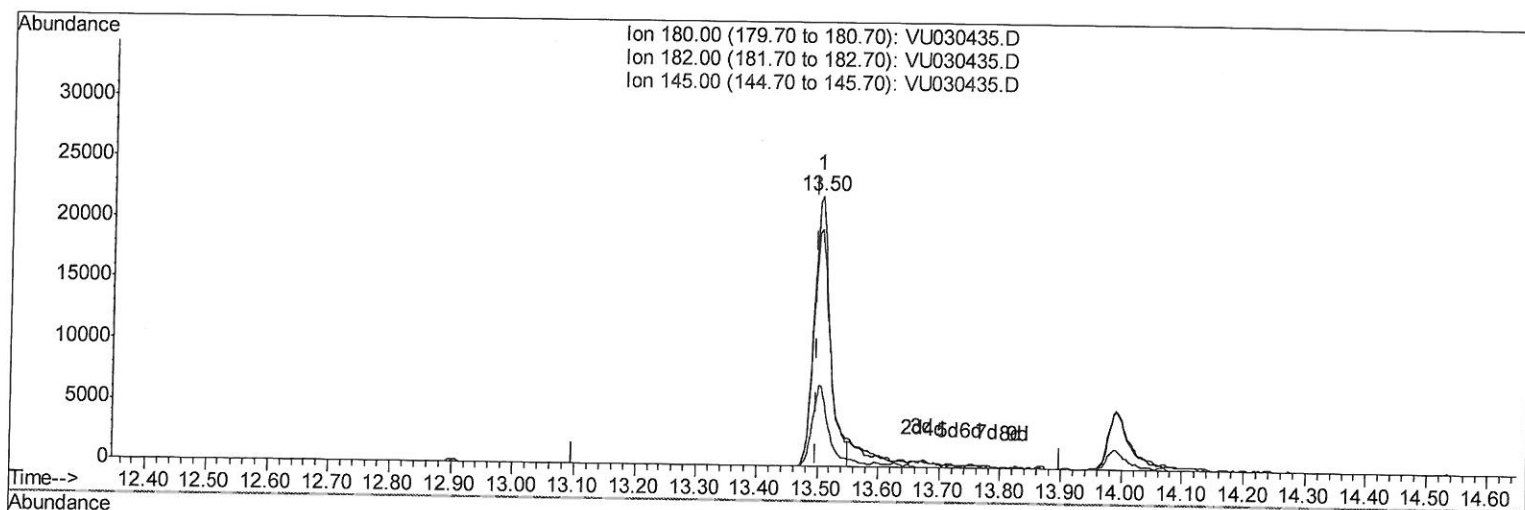

(68) 1,2,4-trichlorobenzene (T)

13.504min (+0.006) 10.75ug/L

response 41198

Ion	Exp%	Act%
180.00	100	100
182.00	95.10	92.56
145.00	30.60	32.03
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Quantitation Report (Qedit)




Data File : VU030435.D
Acq On : 26 Mar 2019 11:37
Operator : JC/SP
Sample : K2070-15DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09E1DL

Manual Integrations
APPROVED

MMDadoda
3/27/2019 9:55:24 AM

Quant Time: Mar 27 04:33:25 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 04:29:49 2019
Response via : Initial Calibration

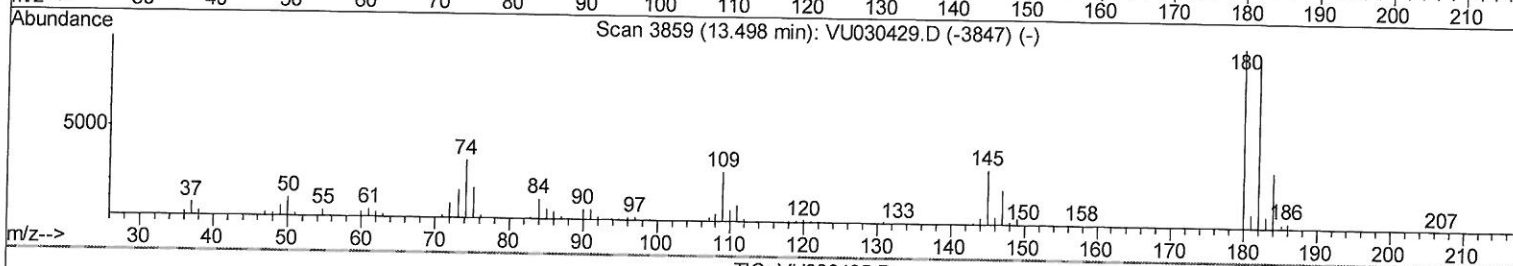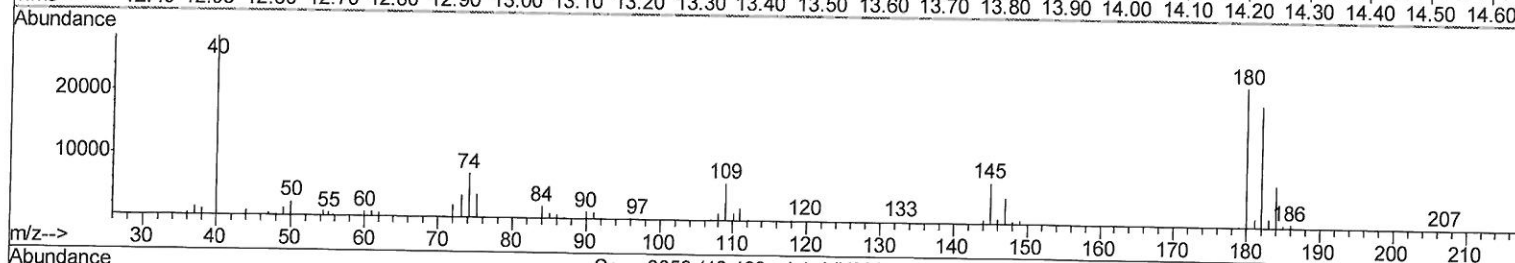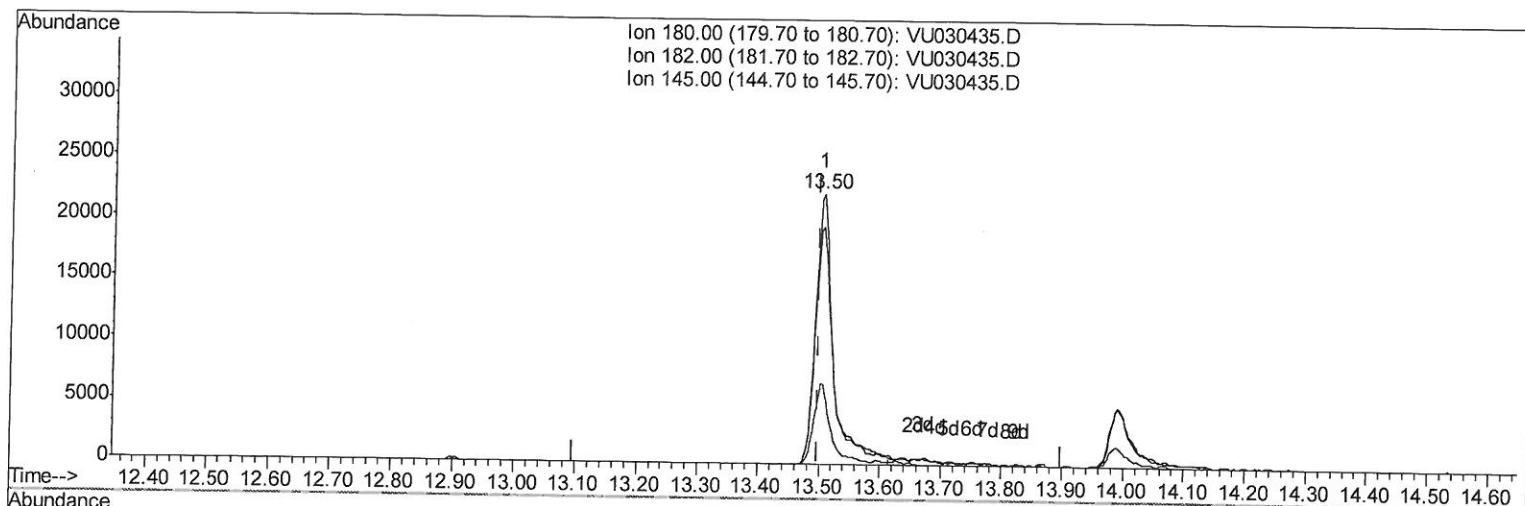

TIC: VU030435.D

(68) 1,2,4-trichlorobenzene (T)

13.504min (+0.006) 12.03ug/L m

response 46103

Ion	Exp%	Act%
180.00	100	100
182.00	95.10	82.71
145.00	30.60	28.63
0.00	0.00	0.00

7 mg
3/27/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032619\

Quantitation Report (QT Reviewed)

Data File : VU030435.D

Acq On : 26 Mar 2019 11:37

Operator : JC/SP

Sample : K2070-15DL 400X

Misc : 5.0mL/MSVOA_U/WATER

ALS Vial : 8 Sample Multiplier: 1

Instrument :

MSVOA_U

ClientSampleId :

C09E1DL

Manual Integrations

APPROVED

MMDadoda

3/27/2019 9:55:24 AM

Quant Time: Mar 27 05:07:33 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M

Quant Title : VOC Analysis

QLast Update : Wed Mar 27 04:29:49 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	448087	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	438738	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	180206	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	198873	55.15	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	110.30%
7) Chloroethane-d5	1.68	69	156990	54.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	109.84%
11) 1,1-Dichloroethene-d2	2.27	63	274370	40.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.22%
21) 2-Butanone-d5	4.17	46	343633	101.37	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.37%
24) Chloroform-d	4.64	84	319635	51.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.88%
26) 1,2-Dichloroethane-d4	5.31	65	215689	53.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.10%
32) Benzene-d6	5.34	84	661289	52.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.12%
36) 1,2-Dichloropropane-d6	6.33	67	231169	53.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.40%
41) Toluene-d8	7.56	98	568183	50.28	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.56%
43) trans-1,3-Dichloropropene-	7.85	79	98093	48.46	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.92%
47) 2-Hexanone-d5	8.31	63	213627	91.58	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.58%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	299804	48.67	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.34%
64) 1,2-Dichlorobenzene-d4	11.86	152	190616	52.79	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.58%

Target Compounds

					Qvalue
33) Benzene	5.39	78	26981	1.807	ug/L 100
51) Chlorobenzene	9.12	112	470969	50.135	ug/L 99
62) 1,3-Dichlorobenzene	11.42	146	23934	4.061	ug/L 98
63) 1,4-Dichlorobenzene	11.50	146	105071	17.319	ug/L 98
65) 1,2-Dichlorobenzene	11.87	146	137382	23.055	ug/L 99
68) 1,2,4-trichlorobenzene	13.50	180	46103m	12.027	ug/L 99
70) 1,2,3-Trichlorobenzene	13.99	180	11626	2.872	ug/L 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

71 m0
3/27/19