

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030432.D
 Acq On : 26 Mar 2019 10:26
 Operator : JC/SP
 Sample : K2062-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	39	rVB2	15288	14757	0.85%	0.112%
2	1.399	89	96	107	rBV	256971	260725	15.03%	1.979%
3	1.672	173	181	201	rVB	190006	251290	14.49%	1.907%
4	2.267	356	366	380	rBV	378872	580750	33.49%	4.408%
5	3.383	710	713	717	rBV	2776	1965	0.11%	0.015%
6	4.174	948	959	982	rBV	197655	508830	29.34%	3.862%
7	4.643	1090	1105	1124	rBV	282739	659139	38.01%	5.003%
8	5.334	1298	1320	1346	rBV2	586326	1734130	100.00%	13.162%
9	5.601	1400	1403	1407	rBV	1269	1205	0.07%	0.009%
10	5.701	1428	1434	1442	rBV	2471	3626	0.21%	0.028%
11	5.881	1478	1490	1513	rBV	478032	964097	55.60%	7.318%
12	6.096	1552	1557	1563	rVB	1942	2393	0.14%	0.018%
13	6.125	1563	1566	1571	rVB	2114	1770	0.10%	0.013%
14	6.174	1576	1581	1587	rBV3	1961	2743	0.16%	0.021%
15	6.328	1614	1629	1657	rBV	394574	819779	47.27%	6.222%
16	6.444	1661	1665	1668	rBV	2995	2608	0.15%	0.020%
17	6.527	1688	1691	1694	rVB	1988	1157	0.07%	0.009%
18	6.553	1694	1699	1702	rBV	1900	2166	0.12%	0.016%
19	6.743	1752	1758	1762	rVB	1458	1694	0.10%	0.013%
20	6.781	1765	1770	1773	rBV	2163	2134	0.12%	0.016%
21	6.875	1796	1799	1803	rBV	1414	1201	0.07%	0.009%
22	6.903	1803	1808	1811	rBV	1550	1766	0.10%	0.013%
23	7.048	1850	1853	1856	rVV2	2091	1712	0.10%	0.013%
24	7.122	1873	1876	1882	rVB	1685	2070	0.12%	0.016%
25	7.177	1889	1893	1896	rBV2	1915	1794	0.10%	0.014%
26	7.225	1896	1908	1931	rVV	214385	396085	22.84%	3.006%
27	7.424	1967	1970	1974	rBV	1650	1334	0.08%	0.010%
28	7.563	1999	2013	2040	rBV	704668	1291798	74.49%	9.805%
29	7.759	2071	2074	2079	rBV2	1522	1560	0.09%	0.012%
30	7.849	2091	2102	2119	rBV	150769	266106	15.35%	2.020%
31	8.006	2147	2151	2154	rBV2	1529	1565	0.09%	0.012%
32	8.199	2208	2211	2214	rBV	1822	1338	0.08%	0.010%
33	8.309	2234	2245	2281	rVV	627760	1163763	67.11%	8.833%
34	8.546	2315	2319	2323	rVB	1884	1578	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030432.D
 Acq On : 26 Mar 2019 10:26
 Operator : JC/SP
 Sample : K2062-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	8.604	2333	2337	2340	rBV	1776	1330	0.08%	0.010%
36	8.662	2352	2355	2360	rVB	1603	1288	0.07%	0.010%
37	8.698	2361	2366	2374	rVB2	1975	3105	0.18%	0.024%
38	8.739	2374	2379	2382	rBV	1615	1562	0.09%	0.012%
39	8.762	2383	2386	2391	rVB	1696	1371	0.08%	0.010%
40	8.820	2396	2404	2407	rVB	1588	1919	0.11%	0.015%
41	8.862	2412	2417	2421	rVB	2131	2281	0.13%	0.017%
42	8.890	2421	2426	2427	rBV	2096	1793	0.10%	0.014%
43	9.003	2457	2461	2465	rBV2	1469	1550	0.09%	0.012%
44	9.087	2475	2487	2511	rBV	699383	1204994	69.49%	9.146%
45	9.225	2528	2530	2534	rVB2	1915	1132	0.07%	0.009%
46	9.325	2559	2561	2569	rVB	1764	1469	0.08%	0.011%
47	9.421	2587	2591	2598	rBV	1455	1707	0.10%	0.013%
48	9.556	2629	2633	2640	rVB2	2031	2007	0.12%	0.015%
49	9.595	2640	2645	2651	rBV2	2143	2822	0.16%	0.021%
50	9.688	2669	2674	2677	rBV	2060	1631	0.09%	0.012%
51	9.707	2677	2680	2684	rBV	1679	1145	0.07%	0.009%
52	9.739	2684	2690	2696	rBV	1822	2591	0.15%	0.020%
53	9.775	2696	2701	2708	rVB2	2249	2583	0.15%	0.020%
54	9.810	2708	2712	2714	rBV	1580	1250	0.07%	0.009%
55	9.939	2747	2752	2755	rBV2	1675	1803	0.10%	0.014%
56	9.993	2766	2769	2775	rVB2	2085	2000	0.12%	0.015%
57	10.029	2775	2780	2785	rBV	1836	1818	0.10%	0.014%
58	10.090	2793	2799	2802	rBV2	1091	1285	0.07%	0.010%
59	10.167	2815	2823	2826	rBV2	2791	3218	0.19%	0.024%
60	10.247	2843	2848	2852	rVV	1495	1612	0.09%	0.012%
61	10.427	2889	2904	2925	rBV	545375	892464	51.46%	6.774%
62	10.527	2932	2935	2939	rBV	2019	1489	0.09%	0.011%
63	10.624	2962	2965	2969	rVB	1655	1294	0.07%	0.010%
64	10.659	2969	2976	2979	rVB2	1992	1982	0.11%	0.015%
65	10.704	2986	2990	2997	rBV	1635	2111	0.12%	0.016%
66	10.752	3002	3005	3010	rVB	1538	1240	0.07%	0.009%
67	10.800	3017	3020	3025	rVB	1755	1315	0.08%	0.010%
68	10.958	3066	3069	3073	rVV	1728	1432	0.08%	0.011%
69	10.980	3074	3076	3082	rVB	2168	1874	0.11%	0.014%
70	11.025	3086	3090	3092	rBV	1883	1160	0.07%	0.009%
71	11.061	3092	3101	3106	rVB	2929	4264	0.25%	0.032%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030432.D
 Acq On : 26 Mar 2019 10:26
 Operator : JC/SP
 Sample : K2062-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.096	3106	3112	3115	rBV	2223	1877	0.11%	0.014%
73	11.270	3160	3166	3172	rVV	1893	2565	0.15%	0.019%
74	11.357	3191	3193	3196	rBV2	1713	1300	0.07%	0.010%
75	11.431	3207	3216	3220	rVV3	2570	3523	0.20%	0.027%
76	11.482	3220	3232	3251	rBV	592882	976328	56.30%	7.410%
77	11.665	3287	3289	3294	rVB	1914	1220	0.07%	0.009%
78	11.736	3306	3311	3316	rBV2	1636	1964	0.11%	0.015%
79	11.771	3319	3322	3328	rVB	1934	1579	0.09%	0.012%
80	11.858	3337	3349	3366	rBV	612989	1032747	59.55%	7.839%
81	12.167	3442	3445	3449	rBV	1475	1371	0.08%	0.010%
82	12.572	3568	3571	3579	rBV2	1720	1909	0.11%	0.014%
83	12.720	3613	3617	3623	rBV	2347	3046	0.18%	0.023%
84	12.829	3647	3651	3654	rBV2	1745	1325	0.08%	0.010%
85	12.855	3654	3659	3663	rVV	2433	2232	0.13%	0.017%
86	12.964	3690	3693	3697	rVB	2221	1427	0.08%	0.011%
87	13.013	3705	3708	3711	rBV	1655	1243	0.07%	0.009%
88	13.360	3813	3816	3819	rBV	1954	1536	0.09%	0.012%
89	13.402	3826	3829	3832	rVB2	2289	1514	0.09%	0.011%
90	13.421	3832	3835	3840	rBV	1349	1137	0.07%	0.009%
91	13.678	3911	3915	3919	rBV2	1572	1783	0.10%	0.014%
92	13.713	3924	3926	3929	rVB	2277	1213	0.07%	0.009%
93	13.884	3975	3979	3984	rBV2	1379	1705	0.10%	0.013%
94	13.948	3996	3999	4002	rBV	2173	1528	0.09%	0.012%
95	14.119	4048	4052	4058	rBV	1968	2471	0.14%	0.019%
96	14.270	4096	4099	4102	rBV2	2368	1402	0.08%	0.011%
97	14.656	4215	4219	4229	rVB	2871	4780	0.28%	0.036%
98	15.295	4416	4418	4425	rVB	1853	1530	0.09%	0.012%
99	16.077	4658	4661	4668	rBV	2927	3668	0.21%	0.028%
100	16.189	4693	4696	4700	rBV	3182	2592	0.15%	0.020%


Sum of corrected areas: 13175034

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030432.D
Acq On : 26 Mar 2019 10:26
Operator : JC/SP
Sample : K2062-14
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

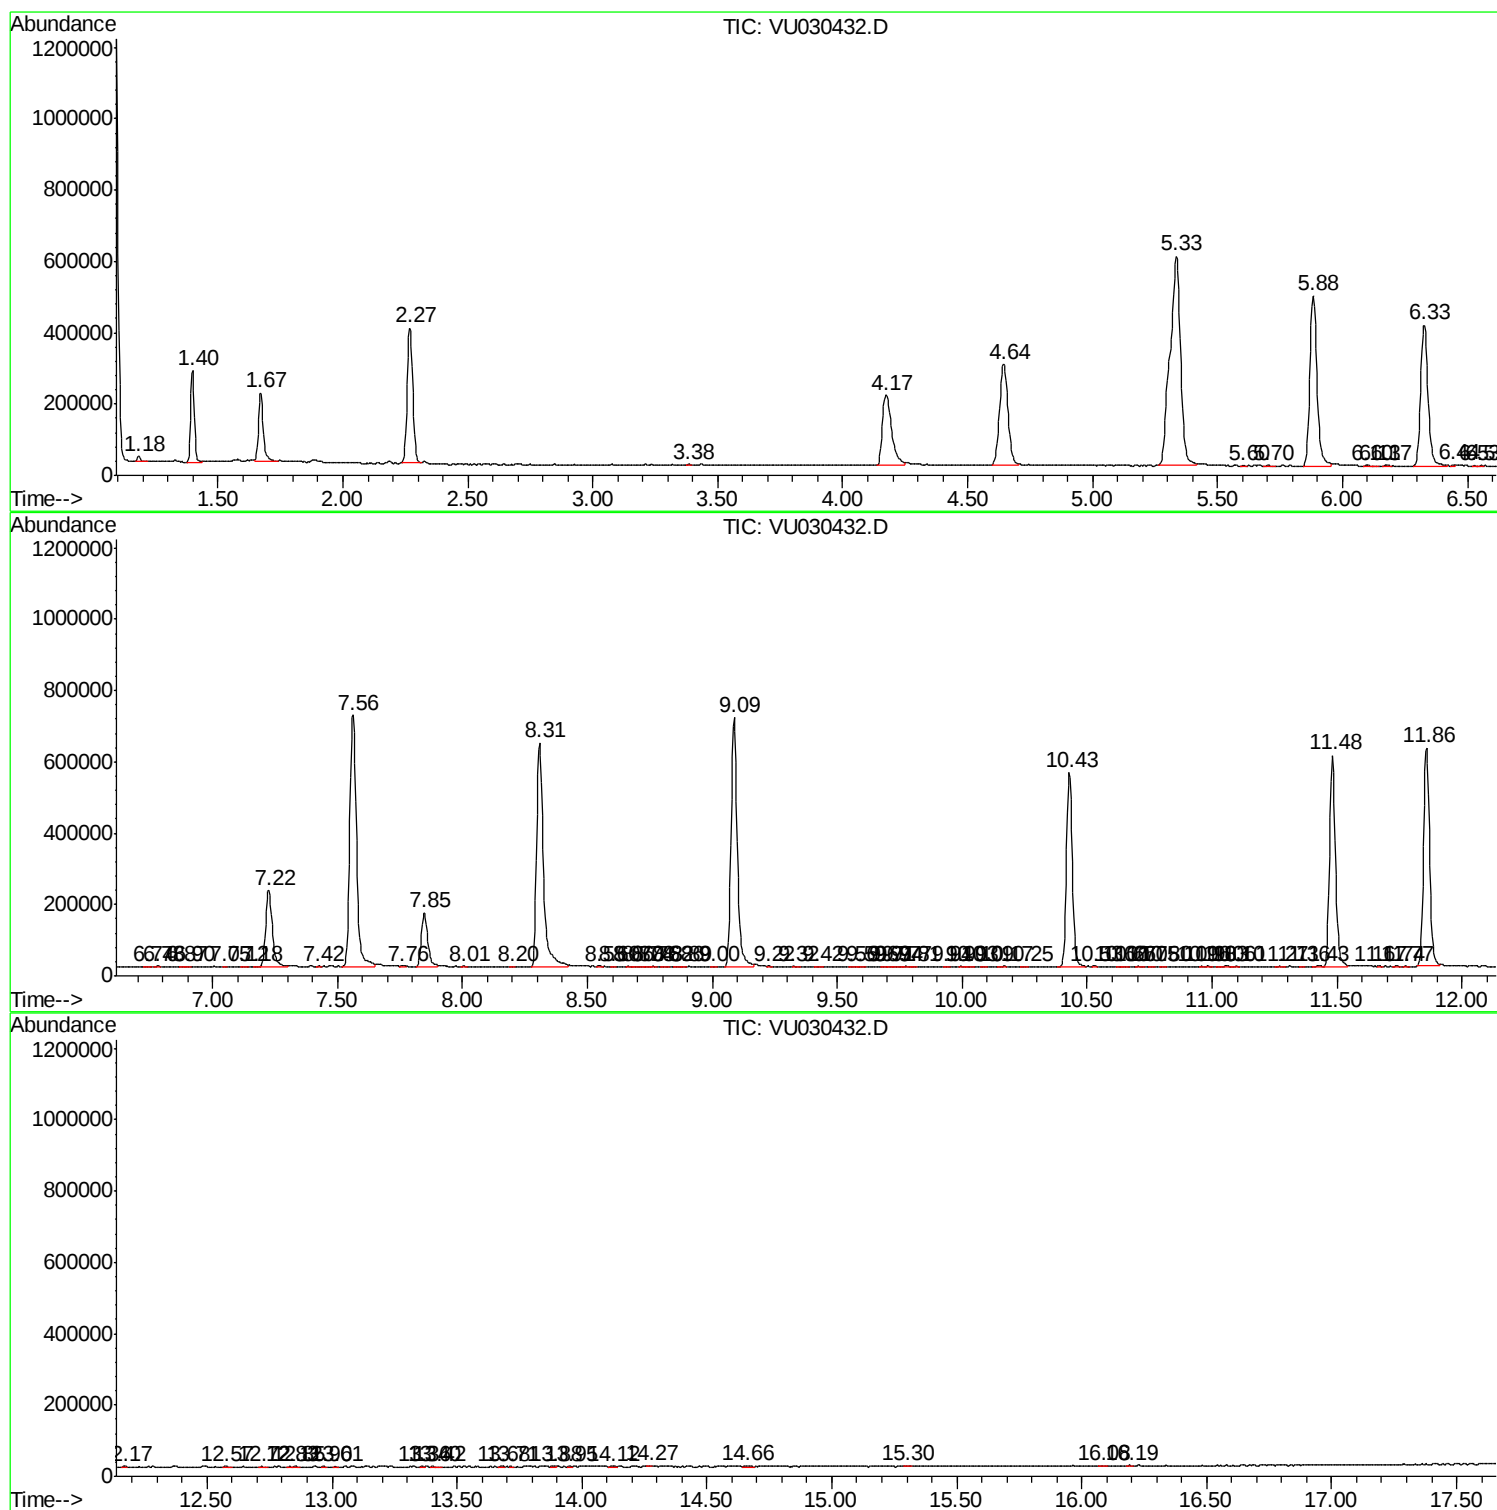

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030432.D
Acq On : 26 Mar 2019 10:26
Operator : JC/SP
Sample : K2062-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030432.D
Acq On : 26 Mar 2019 10:26
Operator : JC/SP
Sample : K2062-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc