

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030434.D
 Acq On : 26 Mar 2019 11:13
 Operator : JC/SP
 Sample : K2022-20
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09J4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	35	rBV	15155	13755	0.70%	0.095%
2	1.399	89	96	109	rBV	307780	307741	15.76%	2.116%
3	1.669	173	180	198	rVB	222841	292396	14.97%	2.011%
4	2.267	356	366	378	rBV	450679	687340	35.19%	4.726%
5	2.322	378	383	397	rVB3	26138	42135	2.16%	0.290%
6	2.450	411	423	439	rBV	20443	39180	2.01%	0.269%
7	2.553	453	455	456	rBV2	1088	441	0.02%	0.003%
8	2.630	471	479	483	rVB3	2318	2869	0.15%	0.020%
9	2.656	485	487	489	rVB	961	433	0.02%	0.003%
10	2.672	489	492	497	rBV2	699	578	0.03%	0.004%
11	2.704	498	502	506	rBV2	1657	1362	0.07%	0.009%
12	2.746	512	515	517	rBV2	590	398	0.02%	0.003%
13	2.759	517	519	522	rVB	1303	723	0.04%	0.005%
14	2.781	522	526	532	rBV	1426	1753	0.09%	0.012%
15	2.839	532	544	550	rBV5	3362	6003	0.31%	0.041%
16	2.884	555	558	561	rVB	1043	703	0.04%	0.005%
17	2.904	561	564	567	rVB	943	558	0.03%	0.004%
18	2.929	567	572	575	rBV3	1610	1603	0.08%	0.011%
19	2.949	575	578	581	rVV	1088	819	0.04%	0.006%
20	2.968	581	584	588	rVV	1174	1144	0.06%	0.008%
21	2.987	588	590	593	rVB	1295	693	0.04%	0.005%
22	3.006	593	596	601	rBV2	1090	840	0.04%	0.006%
23	3.032	601	604	607	rVB	910	568	0.03%	0.004%
24	3.051	607	610	612	rBV	592	431	0.02%	0.003%
25	3.096	621	624	627	rBV	446	268	0.01%	0.002%
26	3.125	630	633	636	rVV	518	329	0.02%	0.002%
27	3.167	644	646	649	rVB	786	390	0.02%	0.003%
28	3.228	657	665	668	rBV	2155	2930	0.15%	0.020%
29	3.283	680	682	686	rBV	896	538	0.03%	0.004%
30	3.334	695	698	700	rBV	821	515	0.03%	0.004%
31	3.392	711	716	718	rBV2	1043	913	0.05%	0.006%
32	3.405	718	720	723	rVV	1093	666	0.03%	0.005%
33	3.428	723	727	732	rVV	1676	1810	0.09%	0.012%
34	3.453	732	735	738	rVV	1043	779	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030434.D
 Acq On : 26 Mar 2019 11:13
 Operator : JC/SP
 Sample : K2022-20
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09J4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	3.473	738	741	744	rVV	668	609	0.03%	0.004%
36	3.489	744	746	749	rVV	787	450	0.02%	0.003%
37	3.508	749	752	754	rVV	802	466	0.02%	0.003%
38	3.524	754	757	760	rVV2	640	508	0.03%	0.003%
39	3.543	760	763	766	rVV2	523	499	0.03%	0.003%
40	3.569	767	771	775	rVB	1521	1424	0.07%	0.010%
41	3.588	775	777	779	rBV	580	396	0.02%	0.003%
42	3.640	789	793	797	rBV	829	774	0.04%	0.005%
43	3.666	797	801	804	rBV	1020	1041	0.05%	0.007%
44	3.698	808	811	814	rBV	1032	878	0.04%	0.006%
45	3.775	831	835	838	rBV	1427	1426	0.07%	0.010%
46	3.823	844	850	853	rBV	2098	2045	0.10%	0.014%
47	3.846	853	857	860	rVV	867	662	0.03%	0.005%
48	3.868	860	864	865	rBV2	489	328	0.02%	0.002%
49	3.881	866	868	871	rVV2	526	377	0.02%	0.003%
50	3.900	871	874	876	rVB	635	391	0.02%	0.003%
51	3.942	882	887	890	rVB	1660	1669	0.09%	0.011%
52	3.965	890	894	897	rBV2	1118	938	0.05%	0.006%
53	3.981	897	899	903	rVV2	851	598	0.03%	0.004%
54	4.013	906	909	914	rVB	1958	1575	0.08%	0.011%
55	4.039	914	917	920	rBV2	1097	715	0.04%	0.005%
56	4.061	920	924	927	rBV	1307	1363	0.07%	0.009%
57	4.087	927	932	934	rBV	919	845	0.04%	0.006%
58	4.116	939	941	945	rVB	740	513	0.03%	0.004%
59	4.174	945	959	984	rBV	197910	518297	26.54%	3.564%
60	4.521	1063	1067	1073	rBV	1764	1951	0.10%	0.013%
61	4.566	1079	1081	1084	rBV	883	455	0.02%	0.003%
62	4.643	1088	1105	1125	rBV	313269	743918	38.09%	5.115%
63	4.820	1155	1160	1161	rBV2	1415	1177	0.06%	0.008%
64	4.862	1171	1173	1175	rBV	801	407	0.02%	0.003%
65	4.932	1193	1195	1197	rBV2	617	280	0.01%	0.002%
66	4.948	1197	1200	1202	rVV2	1205	695	0.04%	0.005%
67	4.968	1203	1206	1210	rVV	1553	1147	0.06%	0.008%
68	4.987	1210	1212	1217	rVB	1513	1147	0.06%	0.008%
69	5.026	1220	1224	1225	rBV	1294	970	0.05%	0.007%
70	5.039	1225	1228	1231	rBV2	977	703	0.04%	0.005%
71	5.096	1244	1246	1249	rVB2	1049	535	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030434.D
 Acq On : 26 Mar 2019 11:13
 Operator : JC/SP
 Sample : K2022-20
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09J4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	5.125	1252	1255	1260	rVB2	1432	1340	0.07%	0.009%
73	5.154	1260	1264	1265	rBV	1414	1057	0.05%	0.007%
74	5.190	1272	1275	1278	rVB	1539	847	0.04%	0.006%
75	5.215	1278	1283	1288	rBV2	1349	1631	0.08%	0.011%
76	5.334	1296	1320	1343	rBV2	670825	1953203	100.00%	13.430%
77	5.762	1451	1453	1455	rBV	1025	579	0.03%	0.004%
78	5.833	1472	1475	1477	rBV	1271	910	0.05%	0.006%
79	5.884	1478	1491	1512	rBV	555168	1105426	56.60%	7.601%
80	6.186	1581	1585	1587	rBV	1385	996	0.05%	0.007%
81	6.222	1594	1596	1599	rBV	1241	819	0.04%	0.006%
82	6.328	1615	1629	1650	rBV	434769	887111	45.42%	6.100%
83	6.588	1708	1710	1713	rBV2	1204	537	0.03%	0.004%
84	6.701	1742	1745	1748	rBV2	1386	1153	0.06%	0.008%
85	6.746	1756	1759	1764	rVB2	1194	915	0.05%	0.006%
86	6.974	1828	1830	1833	rBV	1389	917	0.05%	0.006%
87	7.080	1860	1863	1865	rBV	1257	905	0.05%	0.006%
88	7.225	1897	1908	1926	rBV	241334	433332	22.19%	2.980%
89	7.366	1949	1952	1955	rBV	1743	1561	0.08%	0.011%
90	7.563	2000	2013	2054	rBV	816153	1503497	76.98%	10.338%
91	7.845	2091	2101	2120	rBV	168175	290515	14.87%	1.998%
92	8.144	2191	2194	2196	rBV	1099	779	0.04%	0.005%
93	8.177	2201	2204	2208	rBV2	2079	1797	0.09%	0.012%
94	8.308	2234	2245	2280	rBV	593202	1101034	56.37%	7.571%
95	9.087	2475	2487	2517	rBV	786609	1371651	70.23%	9.432%
96	10.334	2873	2875	2880	rBV	1441	1213	0.06%	0.008%
97	10.427	2893	2904	2930	rVB	564529	920586	47.13%	6.330%
98	11.482	3220	3232	3253	rBV	668023	1104088	56.53%	7.592%
99	11.858	3337	3349	3374	rBV	687085	1147912	58.77%	7.893%
100	13.125	3741	3743	3746	rBV	1930	1093	0.06%	0.008%


Sum of corrected areas: 14543180

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030434.D
Acq On : 26 Mar 2019 11:13
Operator : JC/SP
Sample : K2022-20
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09J4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

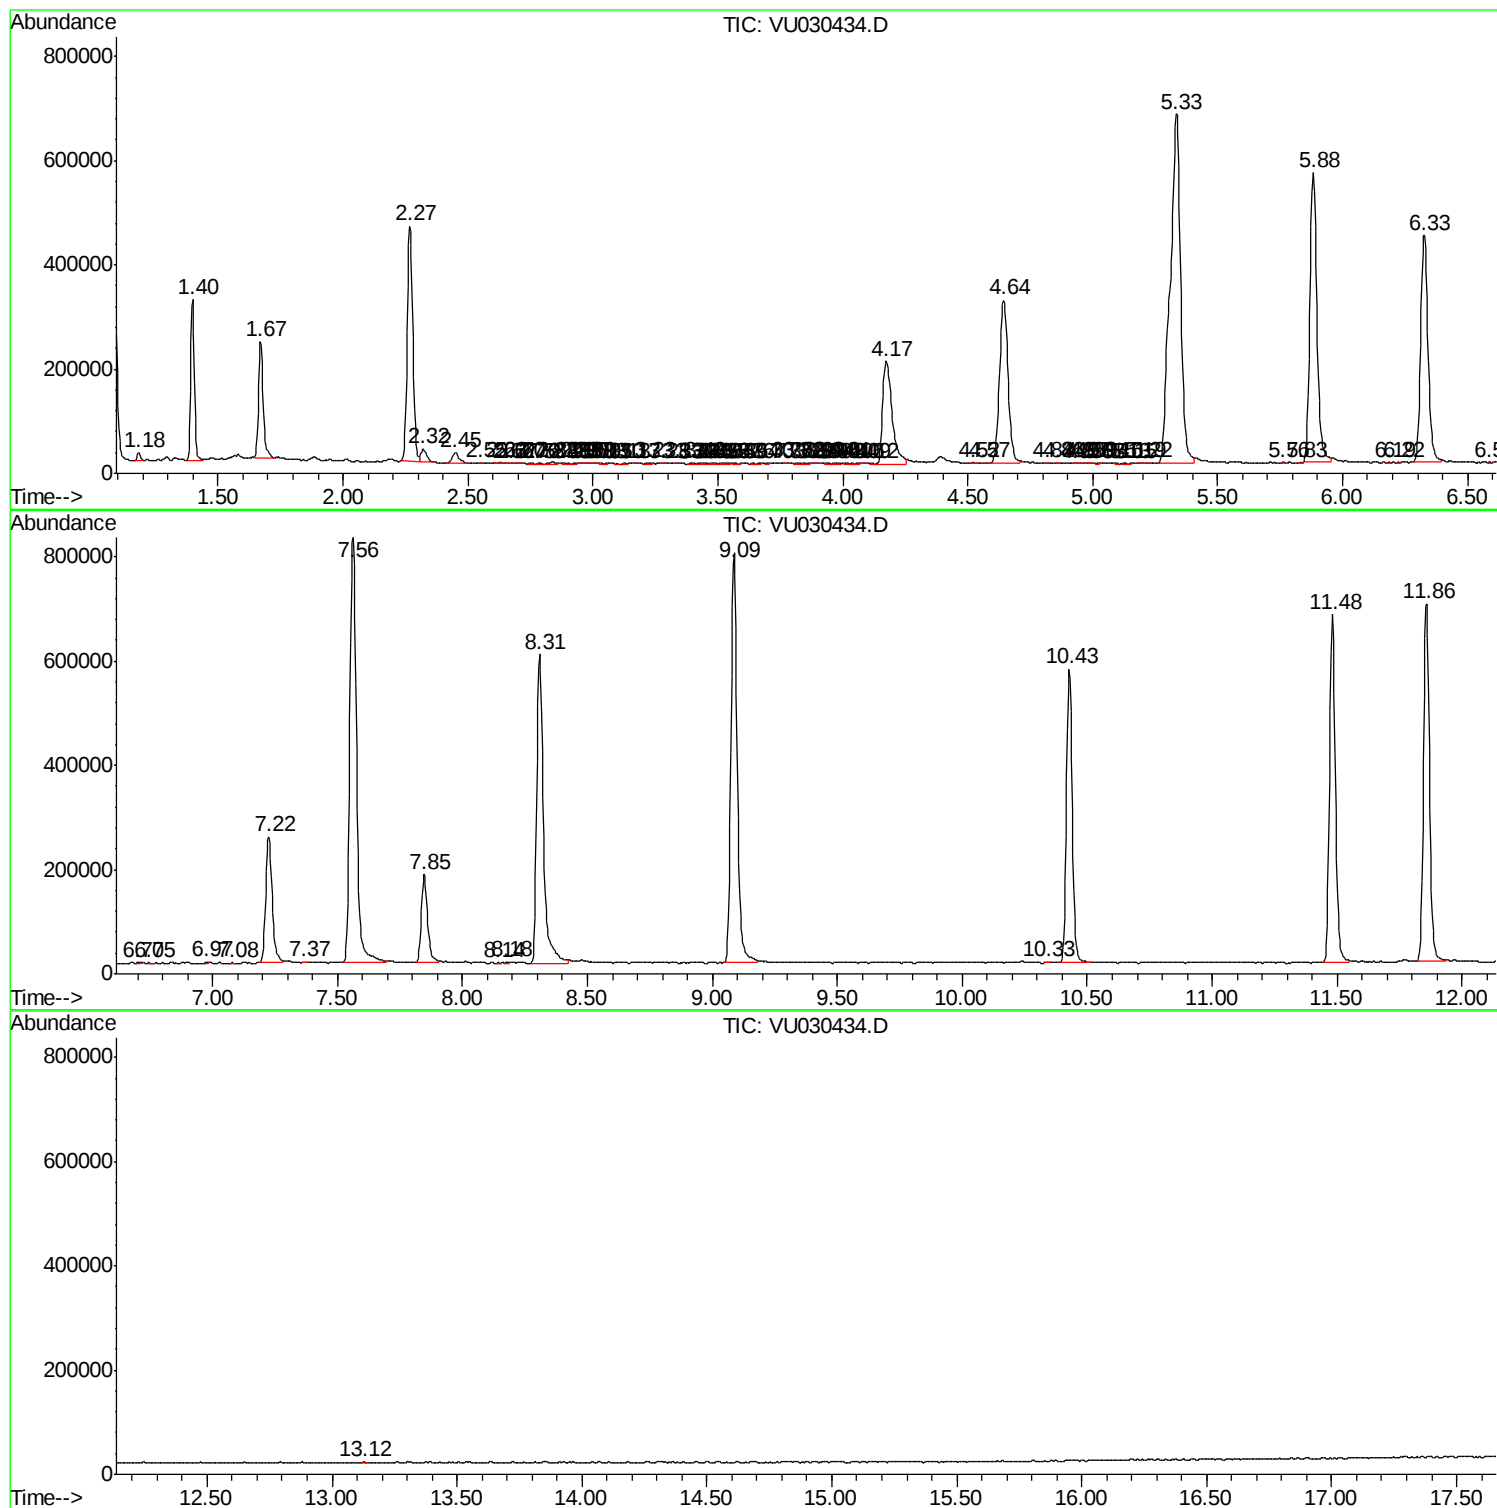

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030434.D
Acq On : 26 Mar 2019 11:13
Operator : JC/SP
Sample : K2022-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09J4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030434.D
Acq On : 26 Mar 2019 11:13
Operator : JC/SP
Sample : K2022-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09J4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc