

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030435.D
 Acq On : 26 Mar 2019 11:37
 Operator : JC/SP
 Sample : K2070-15DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09E1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	39	rVB2	15128	16988	0.82%	0.105%
2	1.254	48	51	57	rBV	3094	3670	0.18%	0.023%
3	1.331	71	75	81	rVB	5453	4929	0.24%	0.030%
4	1.399	89	96	108	rVB	320626	314624	15.25%	1.938%
5	1.672	174	181	197	rVB	220465	289803	14.04%	1.786%
6	2.154	328	331	335	rBV	2302	2015	0.10%	0.012%
7	2.187	336	341	349	rVB4	5793	8745	0.42%	0.054%
8	2.270	356	367	380	rBV	463816	706046	34.22%	4.350%
9	2.479	429	432	435	rVB2	1613	1117	0.05%	0.007%
10	2.547	450	453	457	rVB	1884	1409	0.07%	0.009%
11	2.572	457	461	465	rBV	2077	2065	0.10%	0.013%
12	2.675	490	493	497	rBV	2043	1818	0.09%	0.011%
13	2.701	497	501	506	rVV2	1820	2035	0.10%	0.013%
14	2.807	530	534	538	rBV	2225	2463	0.12%	0.015%
15	2.842	541	545	553	rVB3	2564	3348	0.16%	0.021%
16	2.878	553	556	562	rVB	1448	1158	0.06%	0.007%
17	3.090	617	622	624	rBV	1997	1993	0.10%	0.012%
18	3.260	672	675	681	rVB	1669	1745	0.08%	0.011%
19	3.450	730	734	736	rBV	1763	1193	0.06%	0.007%
20	3.756	825	829	834	rVV	1654	1552	0.08%	0.010%
21	3.904	871	875	877	rBV	1443	1320	0.06%	0.008%
22	3.968	892	895	899	rVB	1623	1202	0.06%	0.007%
23	3.994	899	903	905	rBV	2129	1572	0.08%	0.010%
24	4.026	909	913	919	rVB	1490	1595	0.08%	0.010%
25	4.174	947	959	987	rBV	201674	528707	25.62%	3.257%
26	4.643	1090	1105	1128	rVV	320042	753724	36.53%	4.644%
27	4.968	1201	1206	1212	rBV	1632	2058	0.10%	0.013%
28	5.167	1263	1268	1273	rVB2	1753	1763	0.09%	0.011%
29	5.199	1273	1278	1281	rBV	2168	2261	0.11%	0.014%
30	5.338	1297	1321	1351	rBV2	675228	2063452	100.00%	12.713%
31	5.617	1405	1408	1413	rVB	1696	1115	0.05%	0.007%
32	5.646	1414	1417	1421	rVB	1957	1440	0.07%	0.009%
33	5.675	1421	1426	1430	rBV	1425	1492	0.07%	0.009%
34	5.781	1456	1459	1461	rBV	1436	1002	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030435.D
 Acq On : 26 Mar 2019 11:37
 Operator : JC/SP
 Sample : K2070-15DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09E1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	5.884	1475	1491	1518	rBV	551445	1123264	54.44%	6.921%
36	6.122	1562	1565	1570	rBV2	1313	1509	0.07%	0.009%
37	6.199	1585	1589	1597	rVB	2839	3484	0.17%	0.021%
38	6.328	1615	1629	1657	rBV	449698	915140	44.35%	5.638%
39	6.546	1693	1697	1700	rBV	1512	1152	0.06%	0.007%
40	6.585	1704	1709	1712	rVB	1302	1313	0.06%	0.008%
41	6.710	1745	1748	1752	rVB	2604	2088	0.10%	0.013%
42	6.743	1752	1758	1765	rBV	2112	3143	0.15%	0.019%
43	6.784	1765	1771	1773	rBV	2028	1963	0.10%	0.012%
44	6.871	1794	1798	1800	rBV	2669	2113	0.10%	0.013%
45	6.936	1812	1818	1824	rVB	2001	2274	0.11%	0.014%
46	6.990	1832	1835	1838	rVV	1765	1297	0.06%	0.008%
47	7.061	1853	1857	1860	rBV	1796	1467	0.07%	0.009%
48	7.087	1862	1865	1870	rVB	1621	1194	0.06%	0.007%
49	7.225	1897	1908	1930	rBV	246973	450554	21.83%	2.776%
50	7.498	1989	1993	1996	rBV	1549	1309	0.06%	0.008%
51	7.563	2000	2013	2034	rBV	835070	1501466	72.76%	9.251%
52	7.778	2077	2080	2086	rVB	3124	3048	0.15%	0.019%
53	7.849	2092	2102	2121	rBV	168894	294138	14.25%	1.812%
54	8.308	2233	2245	2278	rBV	608257	1137557	55.13%	7.009%
55	8.585	2329	2331	2334	rBV	2036	1286	0.06%	0.008%
56	8.659	2348	2354	2358	rBV	2109	2989	0.14%	0.018%
57	8.733	2374	2377	2380	rBV	1819	1239	0.06%	0.008%
58	8.849	2408	2413	2416	rBV	2154	1940	0.09%	0.012%
59	8.974	2449	2452	2455	rBV	1430	1108	0.05%	0.007%
60	9.000	2455	2460	2463	rBV2	1061	1223	0.06%	0.008%
61	9.087	2475	2487	2491	rBV	844248	1327605	64.34%	8.180%
62	9.350	2566	2569	2571	rBV	1787	1296	0.06%	0.008%
63	9.437	2593	2596	2601	rBV	2337	2130	0.10%	0.013%
64	9.585	2639	2642	2647	rVB	1938	1289	0.06%	0.008%
65	9.611	2647	2650	2652	rBV	1619	1036	0.05%	0.006%
66	9.688	2670	2674	2678	rBV	2466	2538	0.12%	0.016%
67	9.787	2701	2705	2709	rBV	2410	2644	0.13%	0.016%
68	9.813	2709	2713	2716	rVB	1420	1289	0.06%	0.008%
69	9.833	2716	2719	2722	rBV	1527	1028	0.05%	0.006%
70	9.919	2741	2746	2748	rBV	1149	1040	0.05%	0.006%
71	9.942	2750	2753	2756	rVB	1846	1155	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030435.D
 Acq On : 26 Mar 2019 11:37
 Operator : JC/SP
 Sample : K2070-15DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09E1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.064	2787	2791	2794	rBV	1369	1181	0.06%	0.007%
73	10.141	2812	2815	2818	rBV	1734	1034	0.05%	0.006%
74	10.209	2833	2836	2838	rBV	1461	1016	0.05%	0.006%
75	10.270	2852	2855	2860	rVB	2210	1473	0.07%	0.009%
76	10.302	2860	2865	2868	rBV	2026	1799	0.09%	0.011%
77	10.427	2890	2904	2923	rBV	574761	940711	45.59%	5.796%
78	10.643	2967	2971	2981	rVB	2127	3042	0.15%	0.019%
79	10.733	2994	2999	3001	rBV2	1211	1228	0.06%	0.008%
80	10.778	3009	3013	3015	rBV	1723	1450	0.07%	0.009%
81	10.935	3058	3062	3069	rBV	1916	2516	0.12%	0.016%
82	11.051	3093	3098	3101	rBV	1492	1431	0.07%	0.009%
83	11.196	3137	3143	3148	rBV	1525	2023	0.10%	0.012%
84	11.241	3152	3157	3158	rBV	2001	1729	0.08%	0.011%
85	11.418	3202	3212	3221	rBV	59333	95033	4.61%	0.586%
86	11.482	3221	3232	3259	rVB2	729087	1567650	75.97%	9.659%
87	11.710	3300	3303	3305	rBV2	1818	1264	0.06%	0.008%
88	11.858	3337	3349	3375	rBV2	828148	1772653	85.91%	10.922%
89	12.103	3421	3425	3428	rBV	1671	1682	0.08%	0.010%
90	12.180	3446	3449	3456	rBV2	1704	1770	0.09%	0.011%
91	12.218	3458	3461	3465	rVV	1217	1051	0.05%	0.006%
92	12.411	3518	3521	3528	rBV	1869	2770	0.13%	0.017%
93	12.720	3614	3617	3621	rBV	1404	1247	0.06%	0.008%
94	13.205	3766	3768	3772	rVB	1939	1292	0.06%	0.008%
95	13.228	3772	3775	3777	rBV2	1951	1163	0.06%	0.007%
96	13.299	3793	3797	3801	rVB	2642	2660	0.13%	0.016%
97	13.504	3850	3861	3878	rBV	118688	231564	11.22%	1.427%
98	13.990	4004	4012	4033	rVB3	24310	49692	2.41%	0.306%
99	14.266	4095	4098	4104	rBV2	1853	1995	0.10%	0.012%
100	15.382	4441	4445	4449	rBV2	3122	2617	0.13%	0.016%


Sum of corrected areas: 16230463

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030435.D
Acq On : 26 Mar 2019 11:37
Operator : JC/SP
Sample : K2070-15DL 400X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C09E1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

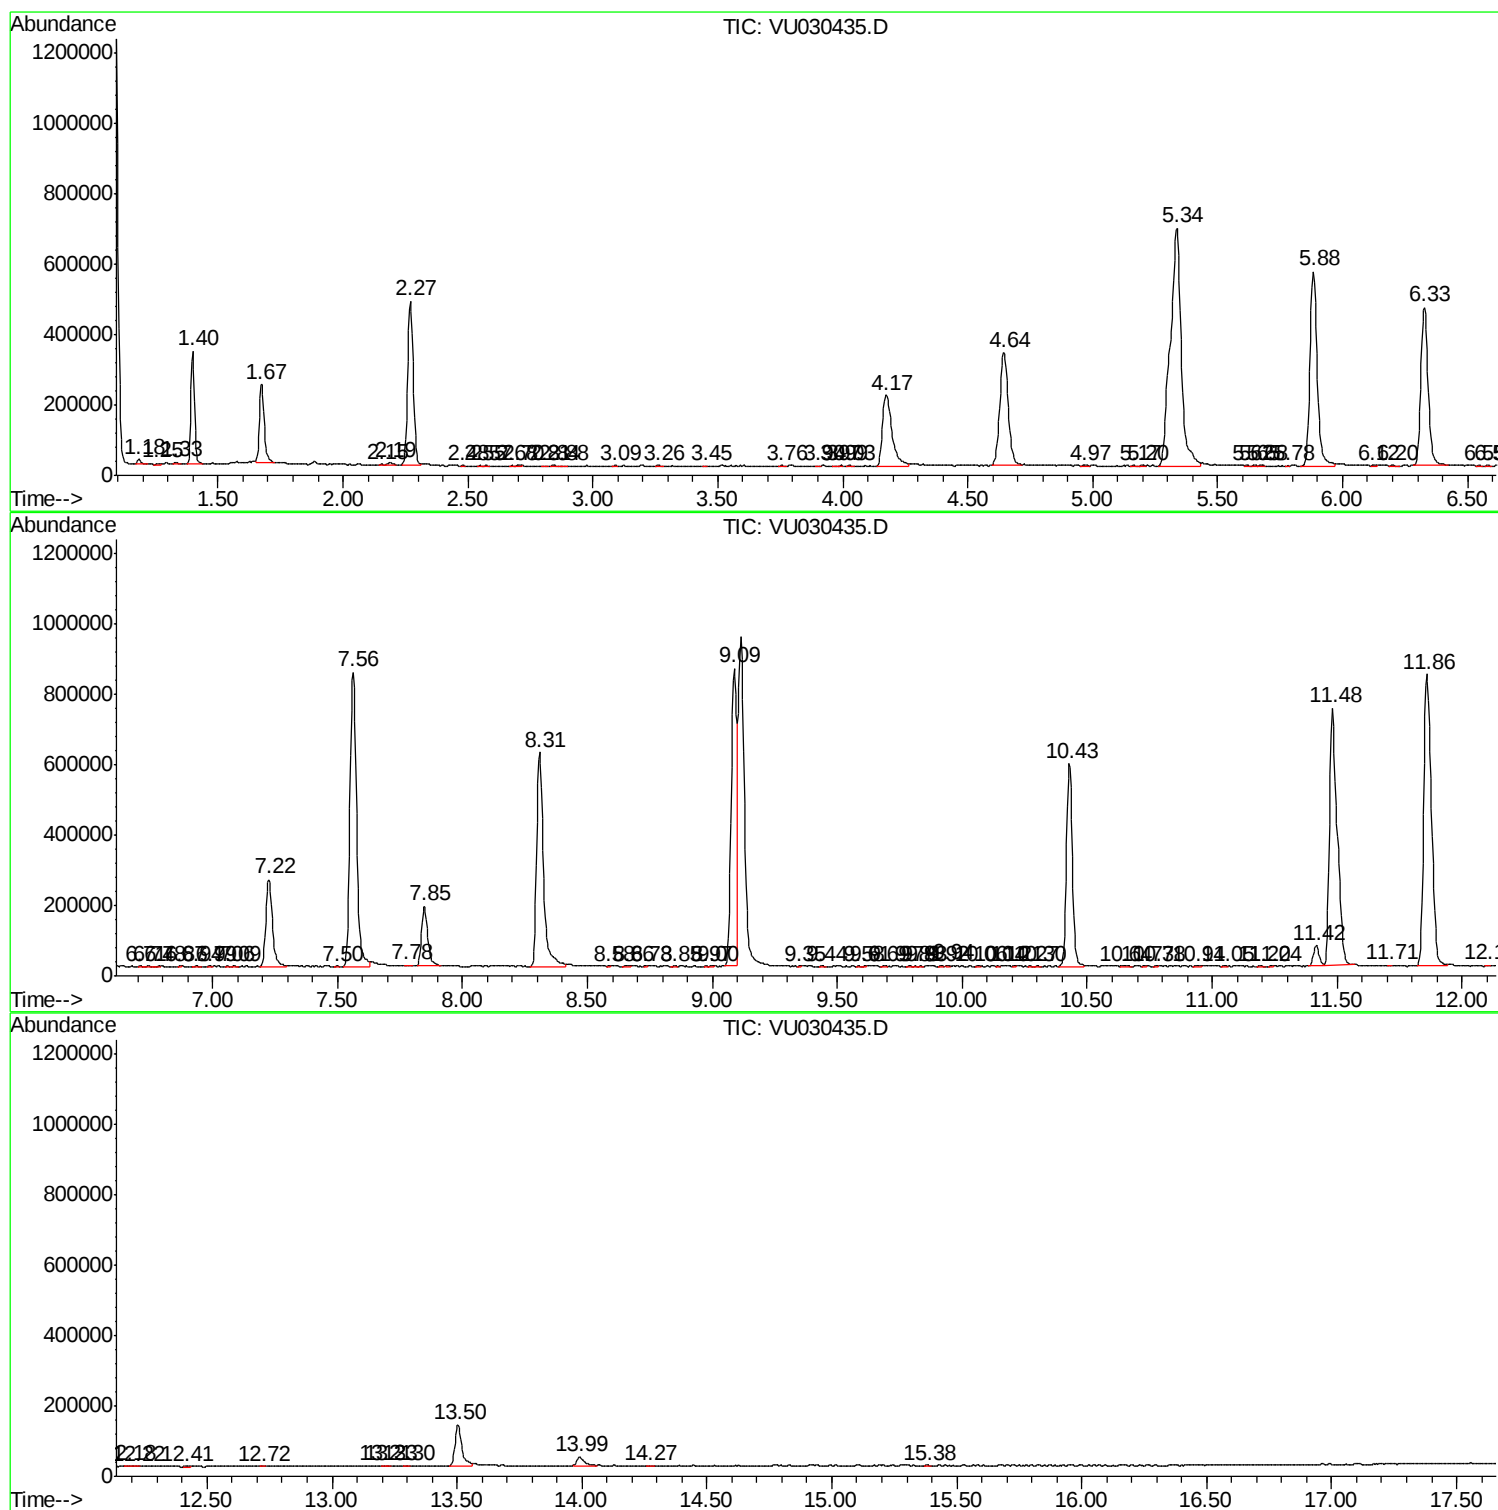

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030435.D
Acq On : 26 Mar 2019 11:37
Operator : JC/SP
Sample : K2070-15DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09E1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030435.D
Acq On : 26 Mar 2019 11:37
Operator : JC/SP
Sample : K2070-15DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09E1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc