

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030436.D
 Acq On : 26 Mar 2019 12:00
 Operator : JC/SP
 Sample : K2016-12DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0989DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	35	rVB3	14947	14686	0.43%	0.085%
2	1.399	88	96	112	rBV	302929	308642	9.02%	1.779%
3	1.675	174	182	198	rVB	212851	281380	8.22%	1.622%
4	2.270	356	367	380	rVB	444137	676831	19.77%	3.901%
5	2.537	447	450	454	rBV	1635	1299	0.04%	0.007%
6	2.646	479	484	491	rVB2	1234	1842	0.05%	0.011%
7	2.682	491	495	498	rBV	1850	1799	0.05%	0.010%
8	2.797	528	531	535	rVB	2715	2137	0.06%	0.012%
9	2.875	552	555	559	rBV	1972	1221	0.04%	0.007%
10	3.064	610	614	616	rBV	1568	1376	0.04%	0.008%
11	3.161	640	644	647	rBV2	1692	1256	0.04%	0.007%
12	3.341	697	700	706	rVB	1315	1385	0.04%	0.008%
13	3.434	722	729	733	rBV	2392	2839	0.08%	0.016%
14	3.466	735	739	746	rVB	2330	2836	0.08%	0.016%
15	3.518	746	755	757	rBV	1684	2205	0.06%	0.013%
16	3.550	762	765	767	rBV	1822	1283	0.04%	0.007%
17	3.592	772	778	780	rBV	1311	1316	0.04%	0.008%
18	3.633	787	791	794	rBV	1813	1206	0.04%	0.007%
19	3.666	797	801	804	rBV	1699	1452	0.04%	0.008%
20	3.711	812	815	821	rVB2	1871	1917	0.06%	0.011%
21	3.920	877	880	884	rVB	2420	1933	0.06%	0.011%
22	3.984	897	900	903	rBV	1591	1124	0.03%	0.006%
23	4.122	940	943	947	rVB	2327	1731	0.05%	0.010%
24	4.174	947	959	985	rBV	198182	524623	15.33%	3.024%
25	4.547	1072	1075	1079	rVB	1931	1656	0.05%	0.010%
26	4.582	1079	1086	1089	rBV	2439	2783	0.08%	0.016%
27	4.643	1089	1105	1129	rVV	308052	731940	21.38%	4.219%
28	4.807	1153	1156	1159	rBV	2087	1454	0.04%	0.008%
29	5.106	1247	1249	1253	rBV2	1348	1125	0.03%	0.006%
30	5.209	1277	1281	1287	rVB2	1414	1614	0.05%	0.009%
31	5.338	1298	1321	1331	rBV2	660354	1925357	56.25%	11.097%
32	5.682	1426	1428	1432	rVB	2494	1348	0.04%	0.008%
33	5.884	1477	1491	1515	rBV	541023	1108924	32.40%	6.391%
34	6.055	1541	1544	1548	rBV	1721	1277	0.04%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030436.D
 Acq On : 26 Mar 2019 12:00
 Operator : JC/SP
 Sample : K2016-12DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0989DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.132	1566	1568	1574	rBV	1691	1523	0.04%	0.009%
36	6.193	1585	1587	1594	rVB	2419	1995	0.06%	0.011%
37	6.328	1613	1629	1649	rBV	436735	897988	26.24%	5.176%
38	6.592	1709	1711	1715	rVB	2126	1297	0.04%	0.007%
39	6.614	1715	1718	1721	rBV	2116	1637	0.05%	0.009%
40	6.875	1793	1799	1802	rVV	1144	1270	0.04%	0.007%
41	6.916	1809	1812	1817	rVB	1773	1420	0.04%	0.008%
42	6.948	1817	1822	1824	rBV2	1470	1431	0.04%	0.008%
43	6.990	1829	1835	1838	rBV	3208	3373	0.10%	0.019%
44	7.093	1859	1867	1871	rVB	1844	2529	0.07%	0.015%
45	7.116	1871	1874	1877	rBV	1866	1610	0.05%	0.009%
46	7.225	1893	1908	1928	rBV	242710	443272	12.95%	2.555%
47	7.440	1971	1975	1977	rBV	2927	2212	0.06%	0.013%
48	7.489	1984	1990	1996	rVB	2190	3161	0.09%	0.018%
49	7.563	1996	2013	2038	rBV	824920	1490159	43.54%	8.589%
50	7.846	2091	2101	2122	rBV	163629	289413	8.46%	1.668%
51	7.987	2142	2145	2150	rVB	1465	1197	0.03%	0.007%
52	8.022	2150	2156	2163	rVB	1831	2507	0.07%	0.014%
53	8.119	2184	2186	2192	rVB	1877	1481	0.04%	0.009%
54	8.177	2201	2204	2209	rVB	1434	1299	0.04%	0.007%
55	8.309	2230	2245	2275	rBV	603140	1119205	32.70%	6.451%
56	8.672	2355	2358	2361	rBV	1798	1376	0.04%	0.008%
57	8.903	2427	2430	2432	rBV	1936	1133	0.03%	0.007%
58	8.948	2439	2444	2447	rVB	1499	1403	0.04%	0.008%
59	8.977	2449	2453	2456	rBV	1609	1289	0.04%	0.007%
60	9.035	2466	2471	2474	rBV	1349	1339	0.04%	0.008%
61	9.087	2474	2487	2493	rBV	821121	1459534	42.64%	8.412%
62	9.244	2534	2536	2541	rVB	1409	1161	0.03%	0.007%
63	9.302	2552	2554	2559	rVB	1604	1322	0.04%	0.008%
64	9.331	2559	2563	2567	rVB	1203	1213	0.04%	0.007%
65	9.370	2567	2575	2576	rBV	1695	2210	0.06%	0.013%
66	9.440	2594	2597	2600	rVV	1951	1243	0.04%	0.007%
67	9.511	2615	2619	2622	rBV	2090	1507	0.04%	0.009%
68	9.562	2631	2635	2641	rVB	1505	1600	0.05%	0.009%
69	9.607	2646	2649	2654	rVV	1284	1200	0.04%	0.007%
70	9.691	2672	2675	2678	rBV	1697	1227	0.04%	0.007%
71	9.849	2720	2724	2732	rVB	1883	2476	0.07%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030436.D
 Acq On : 26 Mar 2019 12:00
 Operator : JC/SP
 Sample : K2016-12DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0989DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	9.980	2760	2765	2771	rBV	1831	2426	0.07%	0.014%
73	10.013	2771	2775	2778	rBV	2199	1789	0.05%	0.010%
74	10.241	2840	2846	2851	rBV	2650	3064	0.09%	0.018%
75	10.312	2863	2868	2876	rVB2	2102	3580	0.10%	0.021%
76	10.347	2876	2879	2881	rBV	1951	1428	0.04%	0.008%
77	10.363	2881	2884	2887	rVV	2020	1611	0.05%	0.009%
78	10.427	2889	2904	2930	rVB	552739	915221	26.74%	5.275%
79	10.527	2930	2935	2938	rBV	2585	2189	0.06%	0.013%
80	10.556	2941	2944	2948	rBV	1292	1272	0.04%	0.007%
81	11.180	3135	3138	3143	rVB2	1270	1141	0.03%	0.007%
82	11.357	3188	3193	3202	rVB	2084	2910	0.09%	0.017%
83	11.418	3202	3212	3221	rBV	55870	93655	2.74%	0.540%
84	11.482	3221	3232	3235	rBV	789592	1166617	34.08%	6.724%
85	11.775	3320	3323	3326	rBV	1817	1236	0.04%	0.007%
86	11.871	3334	3353	3385	rBV2	1531301	3422724	100.00%	19.727%
87	12.080	3415	3418	3423	rVB	1887	1789	0.05%	0.010%
88	12.447	3529	3532	3537	rBV2	1564	1645	0.05%	0.009%
89	12.623	3582	3587	3590	rBV	2008	1849	0.05%	0.011%
90	12.656	3590	3597	3601	rBV	2801	2860	0.08%	0.016%
91	12.771	3629	3633	3636	rBV	2409	1893	0.06%	0.011%
92	13.128	3740	3744	3746	rBV	1546	1276	0.04%	0.007%
93	13.501	3849	3860	3885	rBV	139676	274610	8.02%	1.583%
94	13.887	3975	3980	3983	rVB2	1689	1743	0.05%	0.010%
95	13.990	4002	4012	4026	rBV4	31398	65640	1.92%	0.378%
96	14.199	4074	4077	4080	rBV2	1681	1340	0.04%	0.008%
97	14.572	4190	4193	4196	rBV	1796	1173	0.03%	0.007%
98	14.697	4225	4232	4238	rBV3	2413	3501	0.10%	0.020%
99	14.906	4293	4297	4300	rBV	1517	1539	0.04%	0.009%
100	15.964	4623	4626	4628	rBV	2554	1435	0.04%	0.008%


Sum of corrected areas: 17350165

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030436.D
Acq On : 26 Mar 2019 12:00
Operator : JC/SP
Sample : K2016-12DL 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0989DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

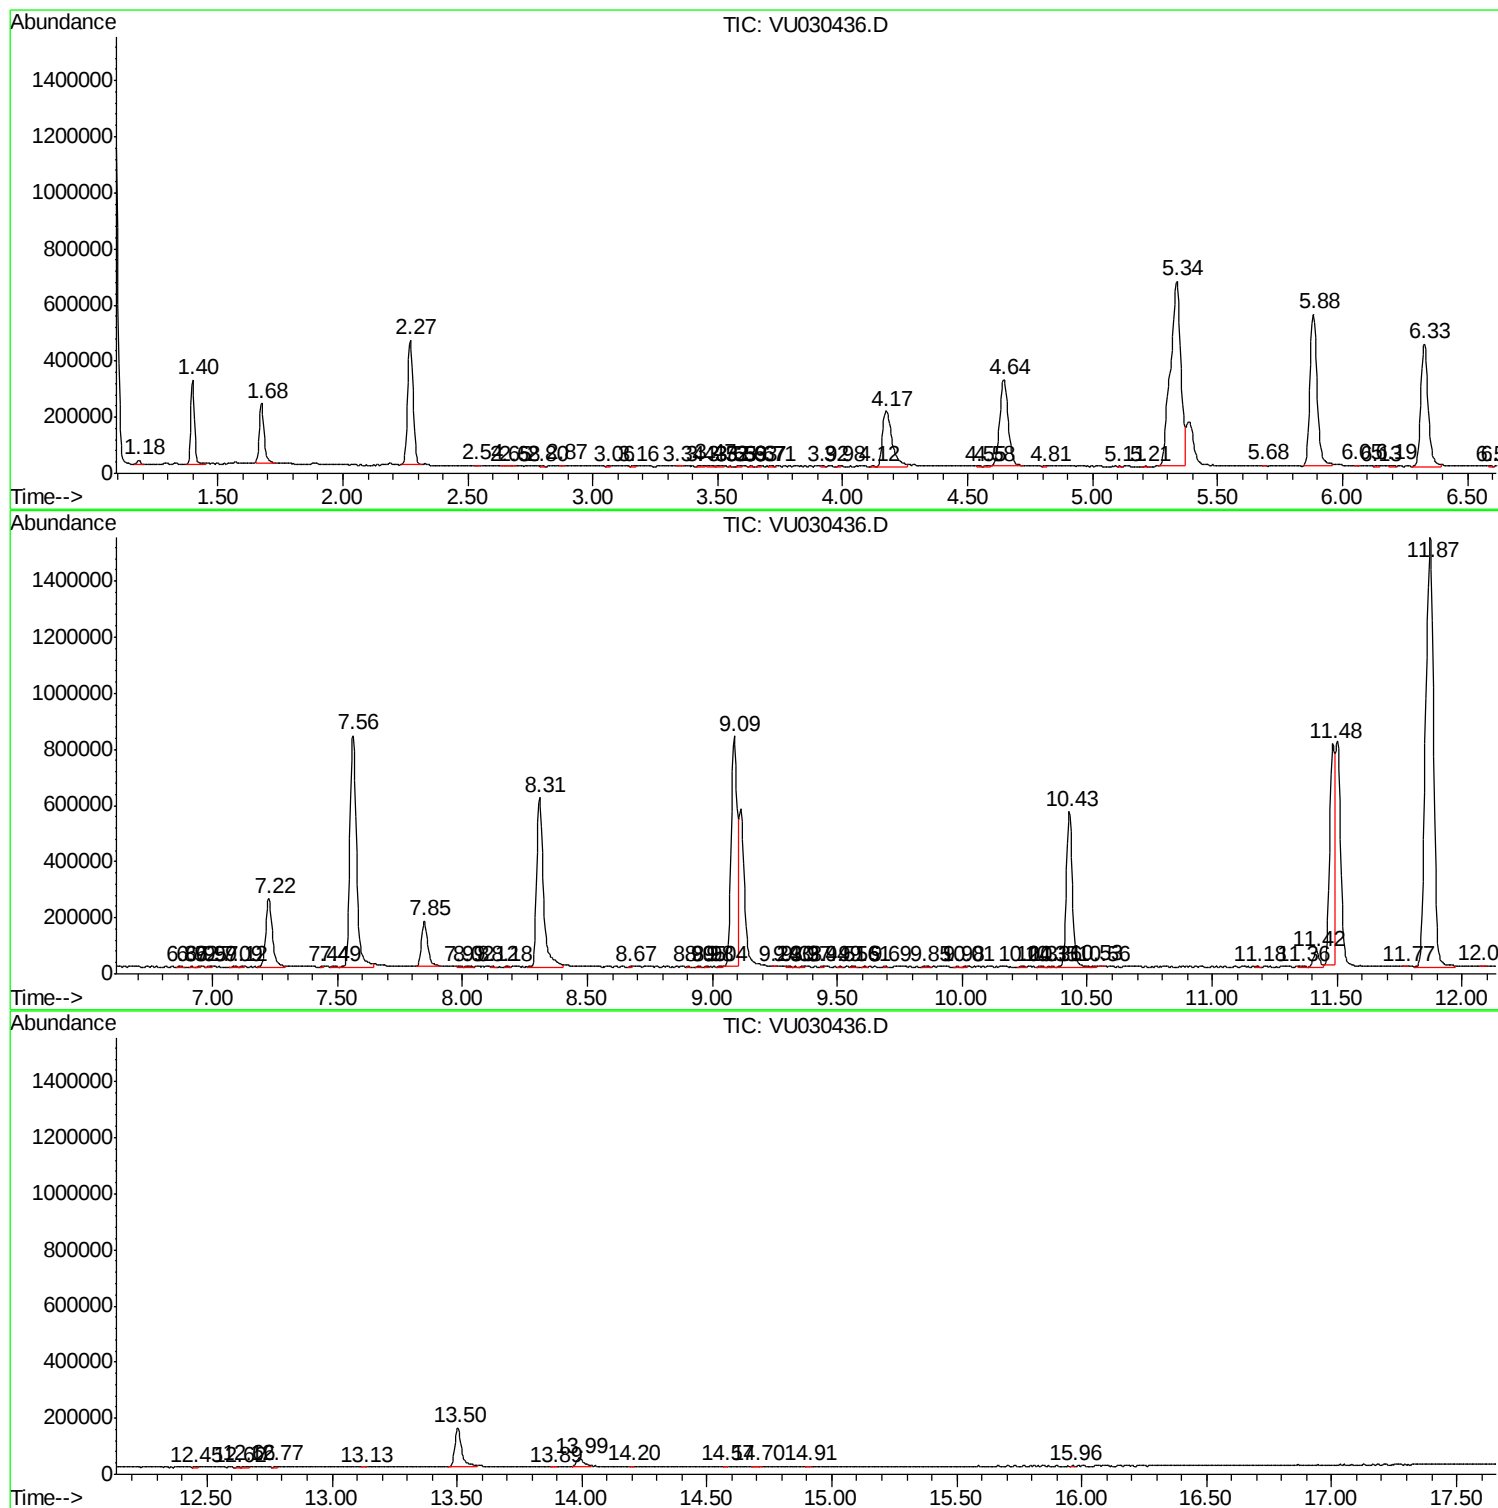

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030436.D
Acq On : 26 Mar 2019 12:00
Operator : JC/SP
Sample : K2016-12DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0989DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030436.D
Acq On : 26 Mar 2019 12:00
Operator : JC/SP
Sample : K2016-12DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0989DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc