

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030439.D
 Acq On : 26 Mar 2019 13:11
 Operator : JC/SP
 Sample : K2070-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09E3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	37	rVB3	14127	13185	0.32%	0.064%
2	1.399	89	96	111	rVB	307892	308458	7.52%	1.505%
3	1.672	174	181	203	rVB	218758	284010	6.93%	1.386%
4	2.270	356	367	381	rBV	451202	687625	16.77%	3.356%
5	4.173	948	959	986	rBV	205197	530465	12.94%	2.589%
6	4.643	1090	1105	1131	rBV	312790	740264	18.05%	3.613%
7	4.884	1177	1180	1186	rBV2	1904	1967	0.05%	0.010%
8	4.926	1190	1193	1194	rBV	1675	1031	0.03%	0.005%
9	5.337	1298	1321	1331	rBV2	661377	1946523	47.47%	9.500%
10	5.881	1477	1490	1516	rBV	548523	1111253	27.10%	5.424%
11	6.183	1582	1584	1587	rBV	1277	790	0.02%	0.004%
12	6.328	1615	1629	1649	rBV	437673	887187	21.63%	4.330%
13	6.447	1663	1666	1673	rBV	2538	3024	0.07%	0.015%
14	6.559	1699	1701	1707	rVB2	2104	1668	0.04%	0.008%
15	6.585	1707	1709	1711	rBV	1082	650	0.02%	0.003%
16	6.598	1711	1713	1715	rVV	1710	1145	0.03%	0.006%
17	6.636	1719	1725	1731	rVB	1769	2172	0.05%	0.011%
18	6.714	1746	1749	1752	rBV	1329	739	0.02%	0.004%
19	6.810	1776	1779	1783	rVB	1483	1157	0.03%	0.006%
20	6.833	1783	1786	1792	rBV	1788	1394	0.03%	0.007%
21	6.964	1820	1827	1831	rBV	1400	1758	0.04%	0.009%
22	6.987	1831	1834	1840	rVV	1576	1368	0.03%	0.007%
23	7.022	1840	1845	1850	rVB	1220	1328	0.03%	0.006%
24	7.077	1857	1862	1864	rBV2	1512	1378	0.03%	0.007%
25	7.141	1879	1882	1886	rBV	1497	1354	0.03%	0.007%
26	7.177	1890	1893	1896	rBV	1484	1195	0.03%	0.006%
27	7.225	1896	1908	1932	rVV	237559	441427	10.76%	2.154%
28	7.353	1945	1948	1951	rBV	2609	2220	0.05%	0.011%
29	7.472	1982	1985	1988	rBV	1576	1225	0.03%	0.006%
30	7.501	1992	1994	2000	rVB	1328	1313	0.03%	0.006%
31	7.562	2000	2013	2050	rBV	834432	1516102	36.97%	7.399%
32	7.845	2091	2101	2121	rBV	165626	292293	7.13%	1.427%
33	8.000	2144	2149	2152	rBV	1518	1664	0.04%	0.008%
34	8.041	2158	2162	2165	rBV	1365	1246	0.03%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030439.D
 Acq On : 26 Mar 2019 13:11
 Operator : JC/SP
 Sample : K2070-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09E3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	8.061	2165	2168	2171	rVB2	1911	1189	0.03%	0.006%
36	8.112	2182	2184	2190	rVB2	1389	1210	0.03%	0.006%
37	8.151	2190	2196	2200	rBV	3142	3565	0.09%	0.017%
38	8.196	2207	2210	2213	rVV	1124	740	0.02%	0.004%
39	8.215	2213	2216	2223	rVB3	1287	1242	0.03%	0.006%
40	8.308	2234	2245	2278	rBV	621319	1147971	27.99%	5.603%
41	8.617	2335	2341	2344	rBV	1478	1739	0.04%	0.008%
42	8.694	2359	2365	2369	rBV	1895	2117	0.05%	0.010%
43	8.736	2373	2378	2382	rVB	1685	1747	0.04%	0.009%
44	8.762	2382	2386	2389	rBV2	1364	945	0.02%	0.005%
45	8.781	2389	2392	2396	rVB	1661	1479	0.04%	0.007%
46	8.810	2396	2401	2402	rBV2	1211	1021	0.02%	0.005%
47	8.858	2413	2416	2422	rBV	1663	1367	0.03%	0.007%
48	8.897	2424	2428	2429	rBV	1165	815	0.02%	0.004%
49	8.919	2433	2435	2438	rVB	1486	787	0.02%	0.004%
50	8.980	2449	2454	2457	rBV	1240	1315	0.03%	0.006%
51	9.086	2474	2487	2492	rBV	822985	1402871	34.21%	6.847%
52	9.283	2544	2548	2551	rBV	2020	1746	0.04%	0.009%
53	9.508	2611	2618	2620	rBV	1555	1844	0.04%	0.009%
54	9.585	2637	2642	2644	rBV	1216	962	0.02%	0.005%
55	9.601	2644	2647	2649	rVV	1015	688	0.02%	0.003%
56	9.659	2659	2665	2670	rBV	2140	2985	0.07%	0.015%
57	9.688	2670	2674	2677	rVV	1786	1424	0.03%	0.007%
58	9.707	2677	2680	2683	rVV2	929	756	0.02%	0.004%
59	9.775	2698	2701	2704	rVV2	1426	958	0.02%	0.005%
60	9.868	2728	2730	2736	rVB	1387	1435	0.03%	0.007%
61	9.900	2736	2740	2742	rBV	1921	1652	0.04%	0.008%
62	9.951	2753	2756	2760	rVB	1377	861	0.02%	0.004%
63	10.067	2790	2792	2795	rVB	1481	844	0.02%	0.004%
64	10.090	2795	2799	2801	rBV	1053	785	0.02%	0.004%
65	10.167	2819	2823	2826	rBV2	1057	853	0.02%	0.004%
66	10.241	2841	2846	2848	rBV	1384	1425	0.03%	0.007%
67	10.254	2848	2850	2853	rVB	1661	897	0.02%	0.004%
68	10.279	2854	2858	2860	rBV	1383	1259	0.03%	0.006%
69	10.350	2877	2880	2884	rVB2	978	752	0.02%	0.004%
70	10.427	2893	2904	2925	rVV	570855	926990	22.60%	4.524%
71	10.614	2954	2962	2967	rBV2	2668	3667	0.09%	0.018%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030439.D
 Acq On : 26 Mar 2019 13:11
 Operator : JC/SP
 Sample : K2070-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09E3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.659	2973	2976	2978	rBV2	1151	879	0.02%	0.004%
73	10.723	2993	2996	2999	rVB2	1476	938	0.02%	0.005%
74	10.742	2999	3002	3007	rBV	2076	1961	0.05%	0.010%
75	10.771	3008	3011	3014	rVV	1021	677	0.02%	0.003%
76	10.826	3025	3028	3031	rBV	1643	1179	0.03%	0.006%
77	10.874	3039	3043	3045	rBV2	1783	1248	0.03%	0.006%
78	10.903	3050	3052	3054	rBV2	1407	837	0.02%	0.004%
79	10.967	3068	3072	3075	rBV	1341	984	0.02%	0.005%
80	11.000	3079	3082	3084	rBV2	1542	921	0.02%	0.004%
81	11.102	3112	3114	3117	rVB2	1526	905	0.02%	0.004%
82	11.144	3121	3127	3130	rBV2	1739	1802	0.04%	0.009%
83	11.202	3139	3145	3148	rBV	1030	1442	0.04%	0.007%
84	11.295	3170	3174	3179	rBV	1463	1595	0.04%	0.008%
85	11.414	3200	3211	3221	rBV	316900	507294	12.37%	2.476%
86	11.501	3221	3238	3267	rVB2	1068850	2739793	66.81%	13.372%
87	11.778	3322	3324	3329	rBV	1639	1115	0.03%	0.005%
88	11.874	3335	3354	3378	rBV2	1959878	4100873	100.00%	20.015%
89	12.183	3447	3450	3452	rBV2	1448	739	0.02%	0.004%
90	12.199	3452	3455	3457	rBV	1238	725	0.02%	0.004%
91	12.260	3471	3474	3475	rBV	1954	1142	0.03%	0.006%
92	12.299	3481	3486	3487	rBV2	1891	1511	0.04%	0.007%
93	12.337	3495	3498	3499	rBV	1630	930	0.02%	0.005%
94	12.488	3542	3545	3547	rBV	1222	790	0.02%	0.004%
95	12.649	3587	3595	3596	rBV2	1593	2179	0.05%	0.011%
96	12.913	3673	3677	3678	rBV	1859	1400	0.03%	0.007%
97	13.501	3849	3860	3887	rBV	289229	507776	12.38%	2.478%
98	13.987	4000	4011	4034	rBV	149596	288982	7.05%	1.410%
99	14.382	4132	4134	4137	rBV	1543	1300	0.03%	0.006%
100	15.533	4489	4492	4494	rBV	2441	1856	0.05%	0.009%


Sum of corrected areas: 20489254

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030439.D
Acq On : 26 Mar 2019 13:11
Operator : JC/SP
Sample : K2070-17 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09E3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

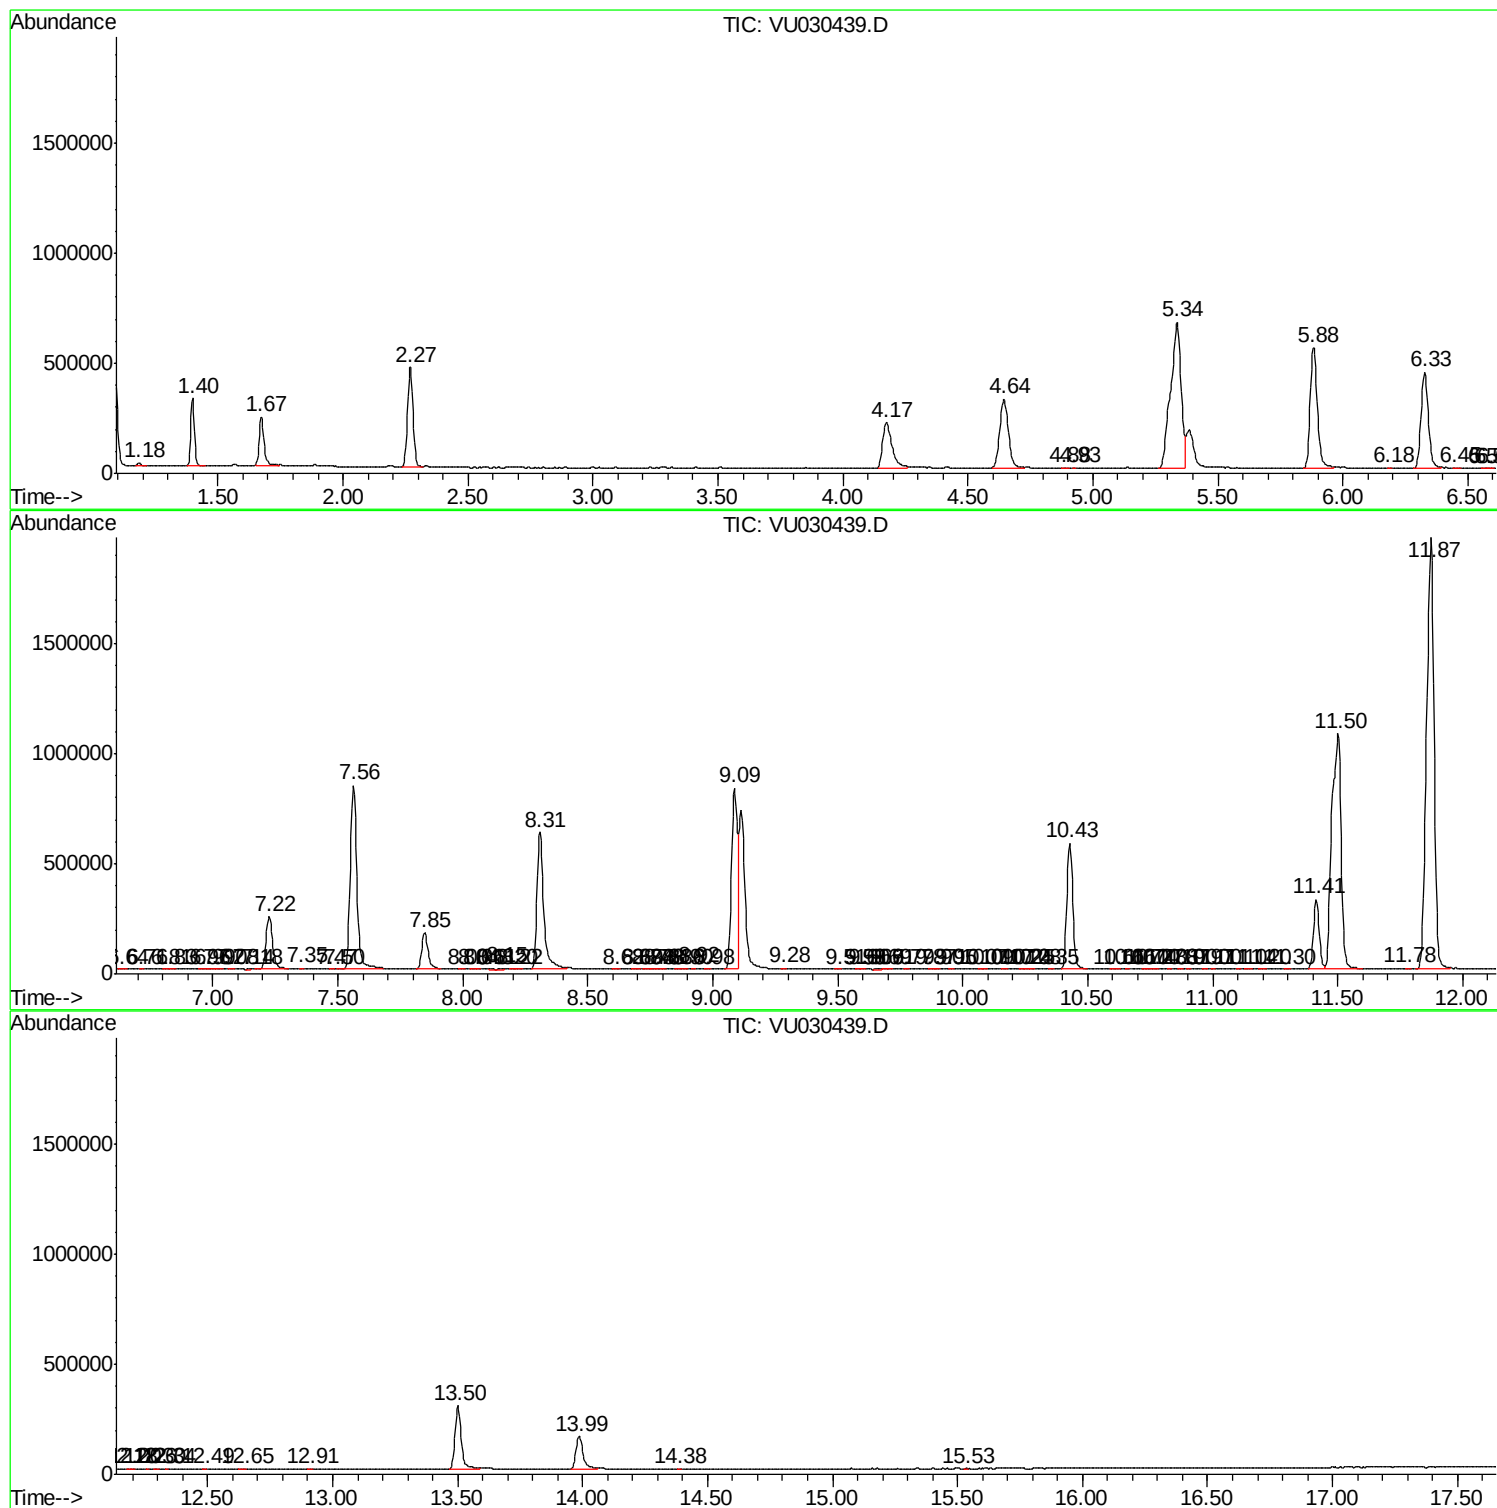

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030439.D
Acq On : 26 Mar 2019 13:11
Operator : JC/SP
Sample : K2070-17 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09E3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030439.D
Acq On : 26 Mar 2019 13:11
Operator : JC/SP
Sample : K2070-17 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09E3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc