

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030443.D
 Acq On : 26 Mar 2019 14:44
 Operator : JC/SP
 Sample : K2016-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	37	rVB	14631	13202	0.78%	0.104%
2	1.399	89	96	108	rBV	263697	265807	15.61%	2.098%
3	1.672	174	181	198	rVB	186843	248656	14.61%	1.962%
4	2.270	356	367	381	rBV	381629	583534	34.28%	4.605%
5	2.444	417	421	426	rBV3	2081	1969	0.12%	0.016%
6	2.492	433	436	438	rBV	1878	1501	0.09%	0.012%
7	2.884	552	558	563	rBV	2726	3586	0.21%	0.028%
8	3.141	634	638	644	rBV	2211	2249	0.13%	0.018%
9	3.212	656	660	664	rBV	1745	1619	0.10%	0.013%
10	3.321	691	694	698	rVB	1966	1452	0.09%	0.011%
11	3.521	750	756	760	rBV	2075	2733	0.16%	0.022%
12	3.723	816	819	822	rBV	1666	1227	0.07%	0.010%
13	4.093	930	934	937	rBV	2072	1704	0.10%	0.013%
14	4.174	947	959	984	rBV	182510	483214	28.38%	3.813%
15	4.489	1054	1057	1061	rBV2	1263	1252	0.07%	0.010%
16	4.547	1072	1075	1079	rBV	1937	1412	0.08%	0.011%
17	4.643	1090	1105	1126	rBV	270917	640006	37.59%	5.051%
18	4.871	1170	1176	1179	rBV2	1463	1767	0.10%	0.014%
19	5.180	1268	1272	1276	rBV	1472	1575	0.09%	0.012%
20	5.337	1297	1321	1351	rBV2	567059	1702383	100.00%	13.435%
21	5.585	1395	1398	1402	rVB2	2113	1609	0.09%	0.013%
22	5.659	1418	1421	1425	rBV	1652	1284	0.08%	0.010%
23	5.727	1439	1442	1445	rBV	1712	1228	0.07%	0.010%
24	5.743	1445	1447	1455	rVB	1808	1350	0.08%	0.011%
25	5.788	1455	1461	1465	rVB	1891	2217	0.13%	0.017%
26	5.884	1478	1491	1509	rBV	471376	942205	55.35%	7.436%
27	6.087	1551	1554	1559	rVB	2629	1951	0.11%	0.015%
28	6.167	1576	1579	1582	rBV	2103	1511	0.09%	0.012%
29	6.190	1584	1586	1593	rVB	2004	1722	0.10%	0.014%
30	6.222	1593	1596	1602	rVB	2709	2879	0.17%	0.023%
31	6.270	1605	1611	1613	rBV	1986	1941	0.11%	0.015%
32	6.328	1615	1629	1651	rBV	385941	780863	45.87%	6.162%
33	6.505	1679	1684	1689	rBV	2597	3197	0.19%	0.025%
34	6.566	1700	1703	1707	rBV	1606	1201	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030443.D
 Acq On : 26 Mar 2019 14:44
 Operator : JC/SP
 Sample : K2016-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.591	1707	1711	1716	rBV	1454	1277	0.08%	0.010%
36	6.726	1750	1753	1755	rBV	1712	1230	0.07%	0.010%
37	6.771	1763	1767	1773	rVB	2412	2470	0.15%	0.019%
38	6.842	1784	1789	1798	rVB	2610	3711	0.22%	0.029%
39	7.103	1867	1870	1874	rBV	1791	1609	0.09%	0.013%
40	7.225	1896	1908	1927	rBV	191583	350893	20.61%	2.769%
41	7.562	1995	2013	2036	rBV	689924	1250148	73.44%	9.866%
42	7.849	2091	2102	2126	rBV	134325	245434	14.42%	1.937%
43	8.009	2145	2152	2156	rBV	1609	1961	0.12%	0.015%
44	8.042	2157	2162	2167	rVB	1684	2014	0.12%	0.016%
45	8.067	2167	2170	2172	rBV	2042	1383	0.08%	0.011%
46	8.135	2188	2191	2195	rBV	1799	1653	0.10%	0.013%
47	8.308	2228	2245	2282	rBV	587328	1109894	65.20%	8.759%
48	8.508	2305	2307	2310	rVB	2583	1464	0.09%	0.012%
49	8.617	2337	2341	2344	rVB	1779	1442	0.08%	0.011%
50	8.659	2349	2354	2359	rBV	1871	1993	0.12%	0.016%
51	8.833	2404	2408	2412	rBV	1510	1376	0.08%	0.011%
52	8.890	2423	2426	2431	rBV	2600	2213	0.13%	0.017%
53	8.951	2442	2445	2451	rVB	2203	2036	0.12%	0.016%
54	9.016	2459	2465	2470	rBV	2016	2703	0.16%	0.021%
55	9.087	2475	2487	2509	rBV	680915	1173809	68.95%	9.263%
56	9.270	2542	2544	2551	rVB	1672	1583	0.09%	0.012%
57	9.312	2552	2557	2561	rBV2	1558	1715	0.10%	0.014%
58	9.408	2581	2587	2589	rBV2	1190	1257	0.07%	0.010%
59	9.472	2602	2607	2609	rBV	1497	1445	0.08%	0.011%
60	9.566	2632	2636	2639	rBV	2326	1625	0.10%	0.013%
61	9.749	2686	2693	2695	rBV	1717	1704	0.10%	0.013%
62	9.858	2719	2727	2729	rBV	1773	1867	0.11%	0.015%
63	9.910	2739	2743	2747	rBV	2021	2168	0.13%	0.017%
64	9.958	2754	2758	2763	rBV	1544	1337	0.08%	0.011%
65	10.035	2776	2782	2786	rBV	2001	2213	0.13%	0.017%
66	10.170	2820	2824	2829	rBV	2136	2204	0.13%	0.017%
67	10.292	2859	2862	2866	rBV	1896	1326	0.08%	0.010%
68	10.427	2891	2904	2921	rBV	510648	832482	48.90%	6.570%
69	10.569	2942	2948	2950	rBV	1604	2034	0.12%	0.016%
70	10.804	3017	3021	3026	rBV	1497	1536	0.09%	0.012%
71	10.932	3056	3061	3063	rBV	1750	1669	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030443.D
 Acq On : 26 Mar 2019 14:44
 Operator : JC/SP
 Sample : K2016-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.035	3089	3093	3095	rBV	1753	1532	0.09%	0.012%
73	11.099	3110	3113	3119	rVB	2153	1780	0.10%	0.014%
74	11.135	3119	3124	3126	rBV	2008	1743	0.10%	0.014%
75	11.421	3209	3213	3218	rVB3	1849	1669	0.10%	0.013%
76	11.482	3219	3232	3252	rBV	563480	926110	54.40%	7.309%
77	11.803	3325	3332	3335	rBV	2140	2713	0.16%	0.021%
78	11.858	3336	3349	3371	rVV	569812	974612	57.25%	7.691%
79	12.173	3444	3447	3449	rVV	1992	1330	0.08%	0.010%
80	12.257	3469	3473	3476	rBV	2278	2433	0.14%	0.019%
81	12.292	3480	3484	3487	rBV	1303	1212	0.07%	0.010%
82	12.318	3490	3492	3497	rVB	2254	1539	0.09%	0.012%
83	12.344	3497	3500	3504	rBV2	1885	1360	0.08%	0.011%
84	12.524	3553	3556	3559	rBV2	1496	1277	0.08%	0.010%
85	12.565	3565	3569	3572	rBV2	1750	1547	0.09%	0.012%
86	12.636	3587	3591	3596	rVB	1838	1585	0.09%	0.013%
87	12.729	3616	3620	3623	rBV	2126	1673	0.10%	0.013%
88	12.823	3646	3649	3652	rBV	1371	1199	0.07%	0.009%
89	13.479	3850	3853	3859	rBV	1936	1887	0.11%	0.015%
90	13.604	3889	3892	3895	rBV	2007	1395	0.08%	0.011%
91	13.736	3929	3933	3935	rBV	1730	1402	0.08%	0.011%
92	13.836	3961	3964	3965	rBV	2294	1284	0.08%	0.010%
93	13.942	3994	3997	4002	rVB2	1671	1570	0.09%	0.012%
94	14.154	4061	4063	4066	rBV	1688	1291	0.08%	0.010%
95	15.099	4354	4357	4360	rVB	2110	1339	0.08%	0.011%
96	15.157	4369	4375	4379	rBV	2345	3199	0.19%	0.025%
97	15.479	4472	4475	4478	rBV	1869	1482	0.09%	0.012%
98	15.565	4500	4502	4506	rBV2	1685	1337	0.08%	0.011%
99	16.176	4687	4692	4694	rBV	2702	3007	0.18%	0.024%
100	16.231	4706	4709	4712	rBV	2657	2265	0.13%	0.018%


Sum of corrected areas: 12671656

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030443.D
Acq On : 26 Mar 2019 14:44
Operator : JC/SP
Sample : K2016-14
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

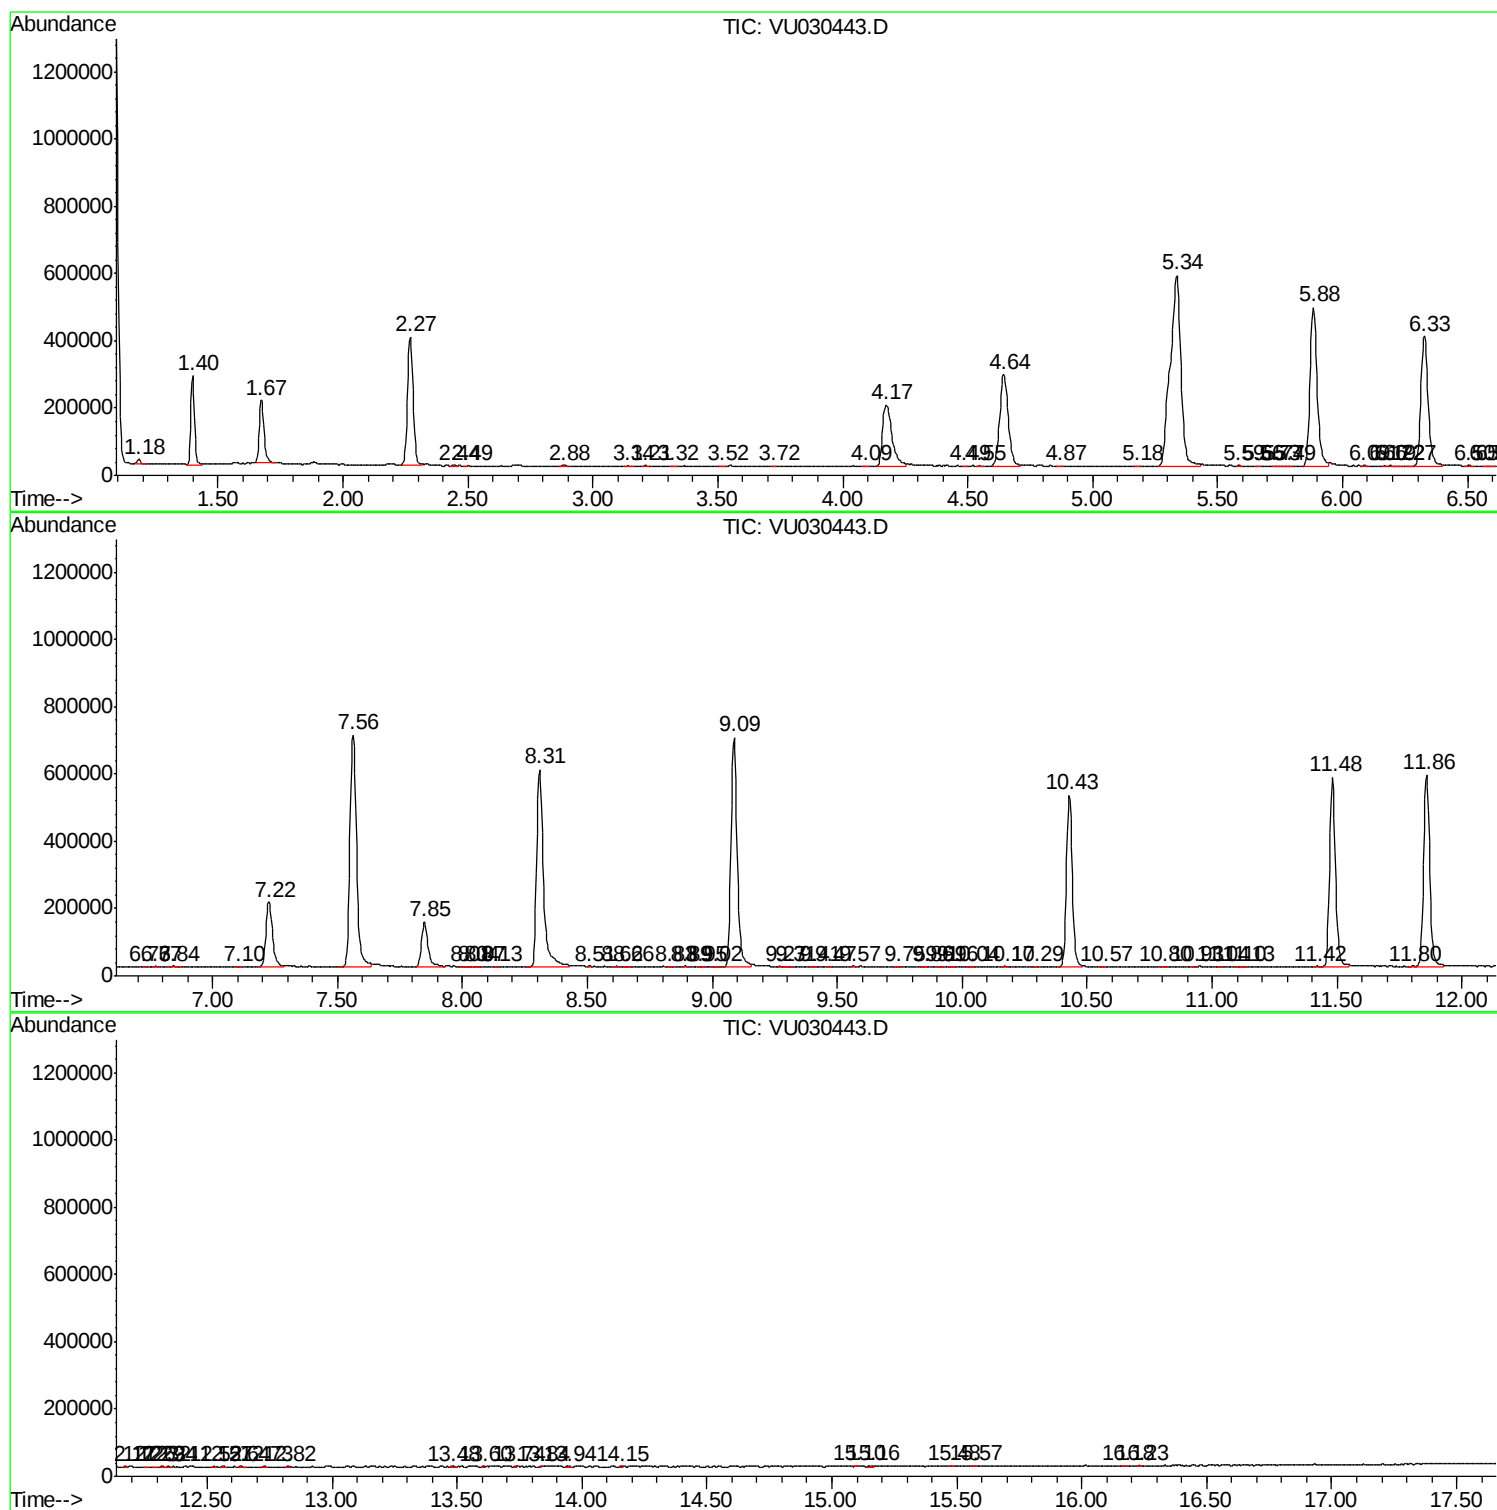

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030443.D
Acq On : 26 Mar 2019 14:44
Operator : JC/SP
Sample : K2016-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030443.D
Acq On : 26 Mar 2019 14:44
Operator : JC/SP
Sample : K2016-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
