

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030447.D
 Acq On : 26 Mar 2019 16:44
 Operator : JC/SP
 Sample : VU0326WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	37	rVB	14726	14280	0.80%	0.106%
2	1.399	89	96	108	rBV	274799	281435	15.78%	2.086%
3	1.672	174	181	198	rVB	201582	261460	14.66%	1.938%
4	2.270	356	367	380	rBV	409532	627845	35.20%	4.654%
5	2.440	416	420	423	rBV2	1629	1723	0.10%	0.013%
6	2.614	470	474	476	rBV	1776	1372	0.08%	0.010%
7	2.694	492	499	502	rBV4	3493	4369	0.24%	0.032%
8	2.813	529	536	540	rBV	1104	1523	0.09%	0.011%
9	2.923	566	570	572	rBV	1546	1226	0.07%	0.009%
10	3.093	620	623	627	rVB	1762	1257	0.07%	0.009%
11	3.186	649	652	656	rVB	2079	1402	0.08%	0.010%
12	3.225	656	664	670	rBV	1886	3040	0.17%	0.023%
13	3.270	674	678	680	rBV	1622	1111	0.06%	0.008%
14	3.357	702	705	709	rBV2	1382	1341	0.08%	0.010%
15	3.405	715	720	726	rBV2	1366	2111	0.12%	0.016%
16	3.556	760	767	773	rVB	1677	2483	0.14%	0.018%
17	3.588	773	777	780	rBV	1544	1334	0.07%	0.010%
18	3.608	780	783	789	rVB	1463	1631	0.09%	0.012%
19	3.649	789	796	799	rBV	1607	1734	0.10%	0.013%
20	3.707	811	814	820	rBV	1279	1058	0.06%	0.008%
21	3.797	837	842	846	rBV2	1317	1278	0.07%	0.009%
22	3.910	873	877	879	rBV	1644	1338	0.08%	0.010%
23	3.961	886	893	896	rBV	1663	1842	0.10%	0.014%
24	4.029	911	914	919	rVB	1479	1181	0.07%	0.009%
25	4.055	919	922	927	rVB	1923	1763	0.10%	0.013%
26	4.173	947	959	996	rBV	182327	485152	27.20%	3.596%
27	4.437	1037	1041	1044	rBV	2363	1788	0.10%	0.013%
28	4.482	1051	1055	1058	rBV	2457	1798	0.10%	0.013%
29	4.582	1083	1086	1088	rBV2	1441	1091	0.06%	0.008%
30	4.643	1090	1105	1129	rVV	280620	670483	37.59%	4.970%
31	4.881	1175	1179	1186	rBV3	1666	2125	0.12%	0.016%
32	5.103	1244	1248	1251	rVV	1494	1126	0.06%	0.008%
33	5.254	1291	1295	1297	rBV	2074	1558	0.09%	0.012%
34	5.337	1297	1321	1346	rVV2	594533	1783823	100.00%	13.222%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030447.D
 Acq On : 26 Mar 2019 16:44
 Operator : JC/SP
 Sample : VU0326WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	5.537	1381	1383	1386	rBV	1725	1265	0.07%	0.009%
36	5.884	1478	1491	1531	rVV	522761	1055728	59.18%	7.825%
37	6.231	1596	1599	1604	rVB	1759	1473	0.08%	0.011%
38	6.328	1615	1629	1652	rBV	401996	817933	45.85%	6.062%
39	6.607	1713	1716	1723	rVB2	1816	1215	0.07%	0.009%
40	6.717	1745	1750	1754	rBV	1558	1293	0.07%	0.010%
41	6.775	1762	1768	1773	rBV	2245	2342	0.13%	0.017%
42	6.820	1778	1782	1786	rVB	1802	1450	0.08%	0.011%
43	6.952	1821	1823	1828	rVV2	1718	1474	0.08%	0.011%
44	7.003	1835	1839	1843	rVV	1603	1479	0.08%	0.011%
45	7.148	1882	1884	1892	rVV2	1253	1263	0.07%	0.009%
46	7.225	1896	1908	1936	rBV	202275	378430	21.21%	2.805%
47	7.434	1968	1973	1976	rVB	1764	1441	0.08%	0.011%
48	7.562	2000	2013	2037	rBV	748079	1331142	74.62%	9.866%
49	7.845	2091	2101	2128	rBV	137546	251359	14.09%	1.863%
50	8.222	2215	2218	2225	rVB	1158	1293	0.07%	0.010%
51	8.308	2234	2245	2284	rBV	600539	1117120	62.63%	8.280%
52	8.585	2328	2331	2335	rVB	1464	1219	0.07%	0.009%
53	8.951	2442	2445	2447	rBV	2474	1749	0.10%	0.013%
54	9.086	2475	2487	2512	rBV	750873	1289099	72.27%	9.555%
55	9.434	2590	2595	2598	rBV	1317	1428	0.08%	0.011%
56	9.633	2653	2657	2666	rVV2	1342	1657	0.09%	0.012%
57	9.697	2674	2677	2682	rVB	1913	1409	0.08%	0.010%
58	9.836	2716	2720	2727	rVB	2073	2144	0.12%	0.016%
59	9.906	2739	2742	2748	rBV	942	1128	0.06%	0.008%
60	9.961	2755	2759	2764	rVB2	1122	1046	0.06%	0.008%
61	10.038	2777	2783	2789	rBV2	1311	2175	0.12%	0.016%
62	10.231	2836	2843	2847	rBV	1887	2125	0.12%	0.016%
63	10.427	2889	2904	2923	rBV	522834	859052	48.16%	6.367%
64	10.614	2959	2962	2970	rVB2	1770	2087	0.12%	0.015%
65	10.659	2970	2976	2978	rBV	1005	1127	0.06%	0.008%
66	10.836	3027	3031	3035	rVB	1578	1325	0.07%	0.010%
67	10.919	3055	3057	3062	rVB2	1402	1096	0.06%	0.008%
68	11.035	3088	3093	3100	rBV	1324	1606	0.09%	0.012%
69	11.209	3143	3147	3150	rBV	1969	1683	0.09%	0.012%
70	11.283	3166	3170	3174	rVB2	1022	1153	0.06%	0.009%
71	11.414	3207	3211	3214	rBV3	2347	2158	0.12%	0.016%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030447.D
 Acq On : 26 Mar 2019 16:44
 Operator : JC/SP
 Sample : VU0326WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.482	3220	3232	3253	rBV	620570	1052821	59.02%	7.803%
73	11.739	3308	3312	3318	rVB	1655	1704	0.10%	0.013%
74	11.858	3334	3349	3370	rBV	632074	1072683	60.13%	7.951%
75	12.192	3449	3453	3456	rBV2	1972	1693	0.09%	0.013%
76	12.212	3456	3459	3463	rVV3	1293	1047	0.06%	0.008%
77	12.311	3484	3490	3493	rBV2	1948	1822	0.10%	0.014%
78	12.334	3493	3497	3500	rBV	1569	1375	0.08%	0.010%
79	12.401	3512	3518	3521	rBV2	1605	1765	0.10%	0.013%
80	12.527	3553	3557	3563	rBV	1306	1219	0.07%	0.009%
81	12.691	3604	3608	3613	rBV	1358	1461	0.08%	0.011%
82	12.887	3666	3669	3672	rBV	1760	1351	0.08%	0.010%
83	13.009	3702	3707	3710	rBV2	1475	1489	0.08%	0.011%
84	13.083	3726	3730	3733	rBV	1658	1365	0.08%	0.010%
85	13.231	3773	3776	3779	rVB	1720	1032	0.06%	0.008%
86	13.263	3779	3786	3788	rBV2	1547	2069	0.12%	0.015%
87	13.279	3788	3791	3794	rVB	1455	1045	0.06%	0.008%
88	13.652	3904	3907	3910	rBV	1347	1031	0.06%	0.008%
89	13.684	3914	3917	3920	rVB2	2583	1780	0.10%	0.013%
90	13.720	3921	3928	3931	rBV	2155	2807	0.16%	0.021%
91	14.003	4006	4016	4023	rBV5	5738	10845	0.61%	0.080%
92	14.099	4043	4046	4052	rVB	1581	1668	0.09%	0.012%
93	14.151	4057	4062	4065	rBV2	2566	2581	0.14%	0.019%
94	14.173	4066	4069	4074	rVB2	1389	1124	0.06%	0.008%
95	14.340	4118	4121	4124	rVB	2017	1121	0.06%	0.008%
96	14.479	4161	4164	4170	rBV	1569	1560	0.09%	0.012%
97	15.337	4428	4431	4433	rBV	1792	1194	0.07%	0.009%
98	15.646	4524	4527	4531	rBV	2156	1805	0.10%	0.013%
99	15.684	4535	4539	4545	rBV3	2502	2960	0.17%	0.022%
100	15.713	4546	4548	4552	rBV2	1521	1135	0.06%	0.008%


Sum of corrected areas: 13491799

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030447.D
Acq On : 26 Mar 2019 16:44
Operator : JC/SP
Sample : VU0326WBL02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

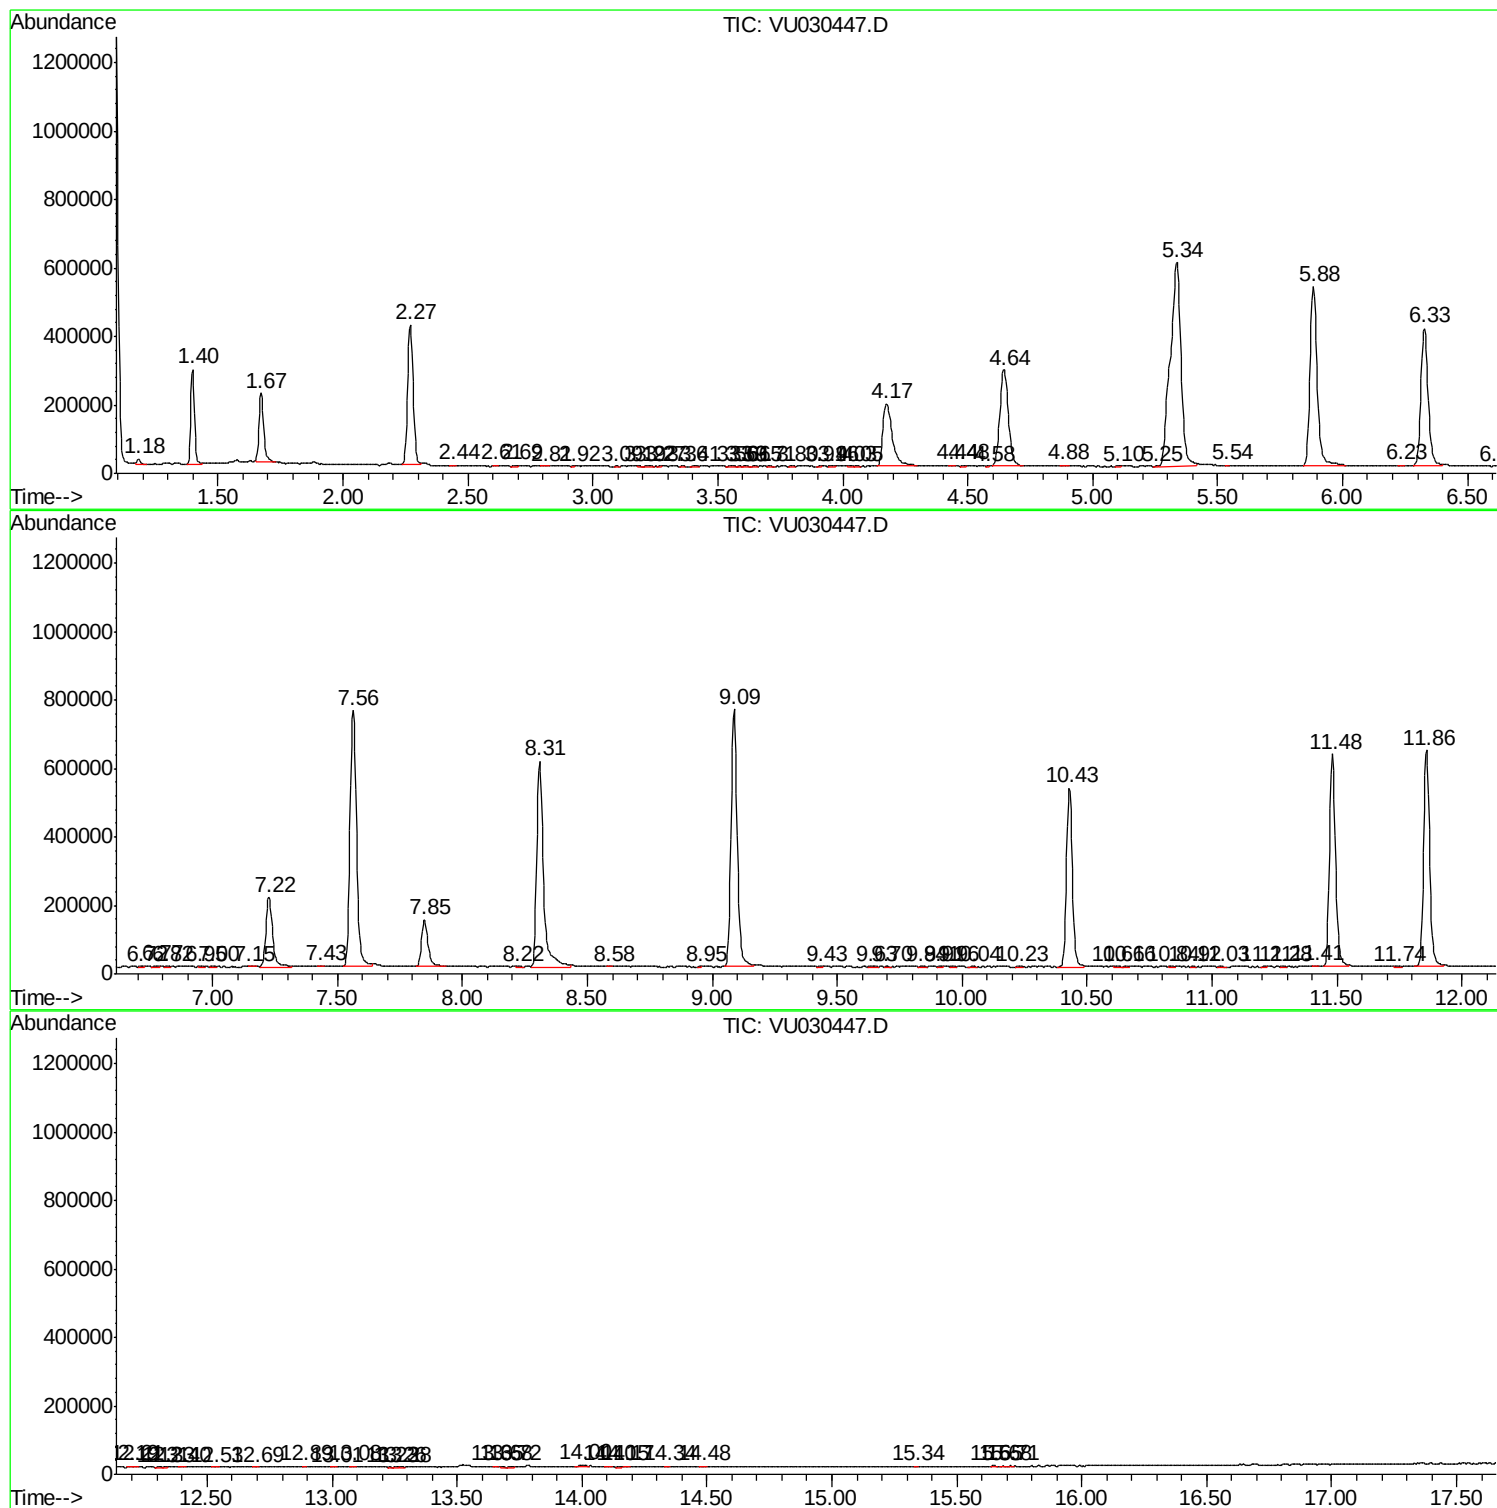

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030447.D
Acq On : 26 Mar 2019 16:44
Operator : JC/SP
Sample : VU0326WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030447.D
Acq On : 26 Mar 2019 16:44
Operator : JC/SP
Sample : VU0326WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc