

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030450.D
 Acq On : 26 Mar 2019 17:55
 Operator : JC/SP
 Sample : K2022-12 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09C7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	34	rVB2	15050	13854	0.73%	0.093%
2	1.399	89	96	107	rBV	271631	276395	14.53%	1.859%
3	1.669	173	180	200	rVB	212369	278496	14.64%	1.873%
4	2.267	355	366	380	rBV	418440	637535	33.51%	4.287%
5	2.431	414	417	419	rBV	1672	1228	0.06%	0.008%
6	2.563	455	458	464	rBV	1317	1296	0.07%	0.009%
7	2.659	483	488	491	rBV2	1216	1255	0.07%	0.008%
8	2.688	494	497	500	rBV2	2098	1793	0.09%	0.012%
9	3.154	639	642	645	rBV	1618	1361	0.07%	0.009%
10	3.322	691	694	701	rVV2	1074	1289	0.07%	0.009%
11	3.373	707	710	714	rVB	2545	1795	0.09%	0.012%
12	3.563	765	769	774	rVV	1700	1854	0.10%	0.012%
13	3.643	791	794	801	rVB2	1522	1687	0.09%	0.011%
14	3.678	801	805	810	rBV	2131	2038	0.11%	0.014%
15	3.707	810	814	818	rBV	2131	2210	0.12%	0.015%
16	3.868	860	864	868	rVB	1960	1842	0.10%	0.012%
17	3.894	868	872	875	rBV2	1515	1414	0.07%	0.010%
18	4.071	923	927	932	rVB	2023	1940	0.10%	0.013%
19	4.116	938	941	947	rBV	1848	1811	0.10%	0.012%
20	4.174	947	959	990	rBV	209735	547166	28.76%	3.680%
21	4.643	1090	1105	1123	rBV	308144	720178	37.85%	4.843%
22	4.878	1174	1178	1185	rVB	1924	2255	0.12%	0.015%
23	4.974	1204	1208	1209	rBV	2523	1945	0.10%	0.013%
24	5.010	1216	1219	1223	rVB	1867	1418	0.07%	0.010%
25	5.203	1275	1279	1285	rVB	1779	1953	0.10%	0.013%
26	5.238	1285	1290	1295	rBV	1528	2056	0.11%	0.014%
27	5.338	1298	1321	1347	rBV2	636892	1902592	100.00%	12.795%
28	5.479	1363	1365	1374	rVB	2820	3321	0.17%	0.022%
29	5.881	1476	1490	1512	rBV	543895	1101709	57.91%	7.409%
30	6.119	1560	1564	1565	rBV2	1717	1245	0.07%	0.008%
31	6.244	1596	1603	1607	rBV	1862	2281	0.12%	0.015%
32	6.325	1613	1628	1656	rBV2	432845	881975	46.36%	5.931%
33	6.482	1675	1677	1682	rVB2	2037	1420	0.07%	0.010%
34	6.553	1697	1699	1705	rVB2	1308	1272	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030450.D
 Acq On : 26 Mar 2019 17:55
 Operator : JC/SP
 Sample : K2022-12 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09C7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.592	1705	1711	1717	rVB	1437	2199	0.12%	0.015%
36	6.691	1735	1742	1746	rBV	1403	1893	0.10%	0.013%
37	6.746	1756	1759	1761	rBV	2036	1263	0.07%	0.008%
38	6.855	1788	1793	1798	rBV	1319	1309	0.07%	0.009%
39	6.910	1808	1810	1815	rBV	1334	1237	0.07%	0.008%
40	7.157	1883	1887	1891	rVB	1764	1525	0.08%	0.010%
41	7.225	1895	1908	1928	rBV	239082	437293	22.98%	2.941%
42	7.347	1943	1946	1950	rVB	2230	1593	0.08%	0.011%
43	7.485	1986	1989	1991	rBV	1693	1098	0.06%	0.007%
44	7.563	2000	2013	2040	rBV	797641	1426599	74.98%	9.594%
45	7.804	2085	2088	2091	rBV	2259	1456	0.08%	0.010%
46	7.845	2091	2101	2125	rVV	163987	294683	15.49%	1.982%
47	7.932	2125	2128	2134	rVB	3062	2683	0.14%	0.018%
48	7.964	2134	2138	2141	rVB	2694	1819	0.10%	0.012%
49	7.990	2141	2146	2148	rBV2	1594	1492	0.08%	0.010%
50	8.157	2193	2198	2200	rBV	1655	1568	0.08%	0.011%
51	8.173	2200	2203	2207	rVB2	1366	1165	0.06%	0.008%
52	8.228	2214	2220	2221	rBV2	1374	1312	0.07%	0.009%
53	8.309	2234	2245	2279	rBV	645247	1190718	62.58%	8.008%
54	8.527	2311	2313	2319	rVB	2008	1830	0.10%	0.012%
55	9.009	2457	2463	2464	rBV	1476	1548	0.08%	0.010%
56	9.087	2475	2487	2522	rVV	820069	1523538	80.08%	10.246%
57	9.363	2570	2573	2581	rBV	1831	1779	0.09%	0.012%
58	9.398	2581	2584	2590	rVB	1496	1246	0.07%	0.008%
59	9.714	2678	2682	2686	rVV	1977	2029	0.11%	0.014%
60	9.733	2686	2688	2693	rVV	1464	1362	0.07%	0.009%
61	9.762	2693	2697	2702	rVB	2527	2482	0.13%	0.017%
62	9.791	2702	2706	2709	rBV	1535	1440	0.08%	0.010%
63	9.845	2719	2723	2726	rBV	1134	1099	0.06%	0.007%
64	10.038	2779	2783	2785	rBV	1737	1402	0.07%	0.009%
65	10.080	2792	2796	2804	rVB	2181	2602	0.14%	0.017%
66	10.263	2847	2853	2857	rVV	1461	2002	0.11%	0.013%
67	10.376	2884	2888	2891	rBV	2331	1939	0.10%	0.013%
68	10.427	2892	2904	2923	rVV	579452	940625	49.44%	6.326%
69	10.620	2961	2964	2970	rVB2	1521	1210	0.06%	0.008%
70	10.707	2985	2991	2994	rBV	1643	1827	0.10%	0.012%
71	10.948	3063	3066	3071	rBV	1493	1448	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030450.D
 Acq On : 26 Mar 2019 17:55
 Operator : JC/SP
 Sample : K2022-12 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09C7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.061	3097	3101	3102	rBV2	2341	1670	0.09%	0.011%
73	11.077	3103	3106	3110	rVV2	1593	1884	0.10%	0.013%
74	11.341	3183	3188	3194	rBV	1762	2716	0.14%	0.018%
75	11.418	3203	3212	3220	rBV2	19317	29977	1.58%	0.202%
76	11.482	3220	3232	3255	rVV2	672461	1244197	65.39%	8.367%
77	11.858	3334	3349	3376	rBV	697026	1269419	66.72%	8.537%
78	12.077	3414	3417	3421	rVB	1605	1152	0.06%	0.008%
79	12.312	3487	3490	3493	rVB	2456	1711	0.09%	0.012%
80	12.344	3496	3500	3504	rBV	2042	1927	0.10%	0.013%
81	12.434	3525	3528	3535	rVB2	2209	2406	0.13%	0.016%
82	12.466	3535	3538	3542	rBV	2798	2471	0.13%	0.017%
83	12.713	3610	3615	3620	rBV	2769	3186	0.17%	0.021%
84	12.897	3666	3672	3675	rBV2	1682	1867	0.10%	0.013%
85	12.967	3688	3694	3698	rBV	2167	3200	0.17%	0.022%
86	13.231	3771	3776	3779	rBV2	1769	1816	0.10%	0.012%
87	13.250	3779	3782	3787	rVV2	1299	1524	0.08%	0.010%
88	13.283	3789	3792	3797	rVB	1551	1751	0.09%	0.012%
89	13.514	3859	3864	3871	rBV4	6472	10360	0.54%	0.070%
90	13.697	3918	3921	3924	rVV	2085	1445	0.08%	0.010%
91	13.794	3948	3951	3953	rBV2	1446	1062	0.06%	0.007%
92	13.951	3997	4000	4003	rVB	1938	1063	0.06%	0.007%
93	14.151	4059	4062	4067	rVB	1730	1303	0.07%	0.009%
94	14.205	4076	4079	4084	rBV	1607	1594	0.08%	0.011%
95	14.411	4140	4143	4146	rBV	1698	1334	0.07%	0.009%
96	14.736	4239	4244	4249	rBV	2582	2968	0.16%	0.020%
97	14.967	4313	4316	4319	rBV	1782	1323	0.07%	0.009%
98	15.061	4342	4345	4349	rVB	2847	2092	0.11%	0.014%
99	15.090	4349	4354	4358	rBV	2414	3041	0.16%	0.020%
100	15.594	4509	4511	4515	rBV2	1321	1055	0.06%	0.007%


Sum of corrected areas: 14869706

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030450.D
Acq On : 26 Mar 2019 17:55
Operator : JC/SP
Sample : K2022-12 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C09C7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

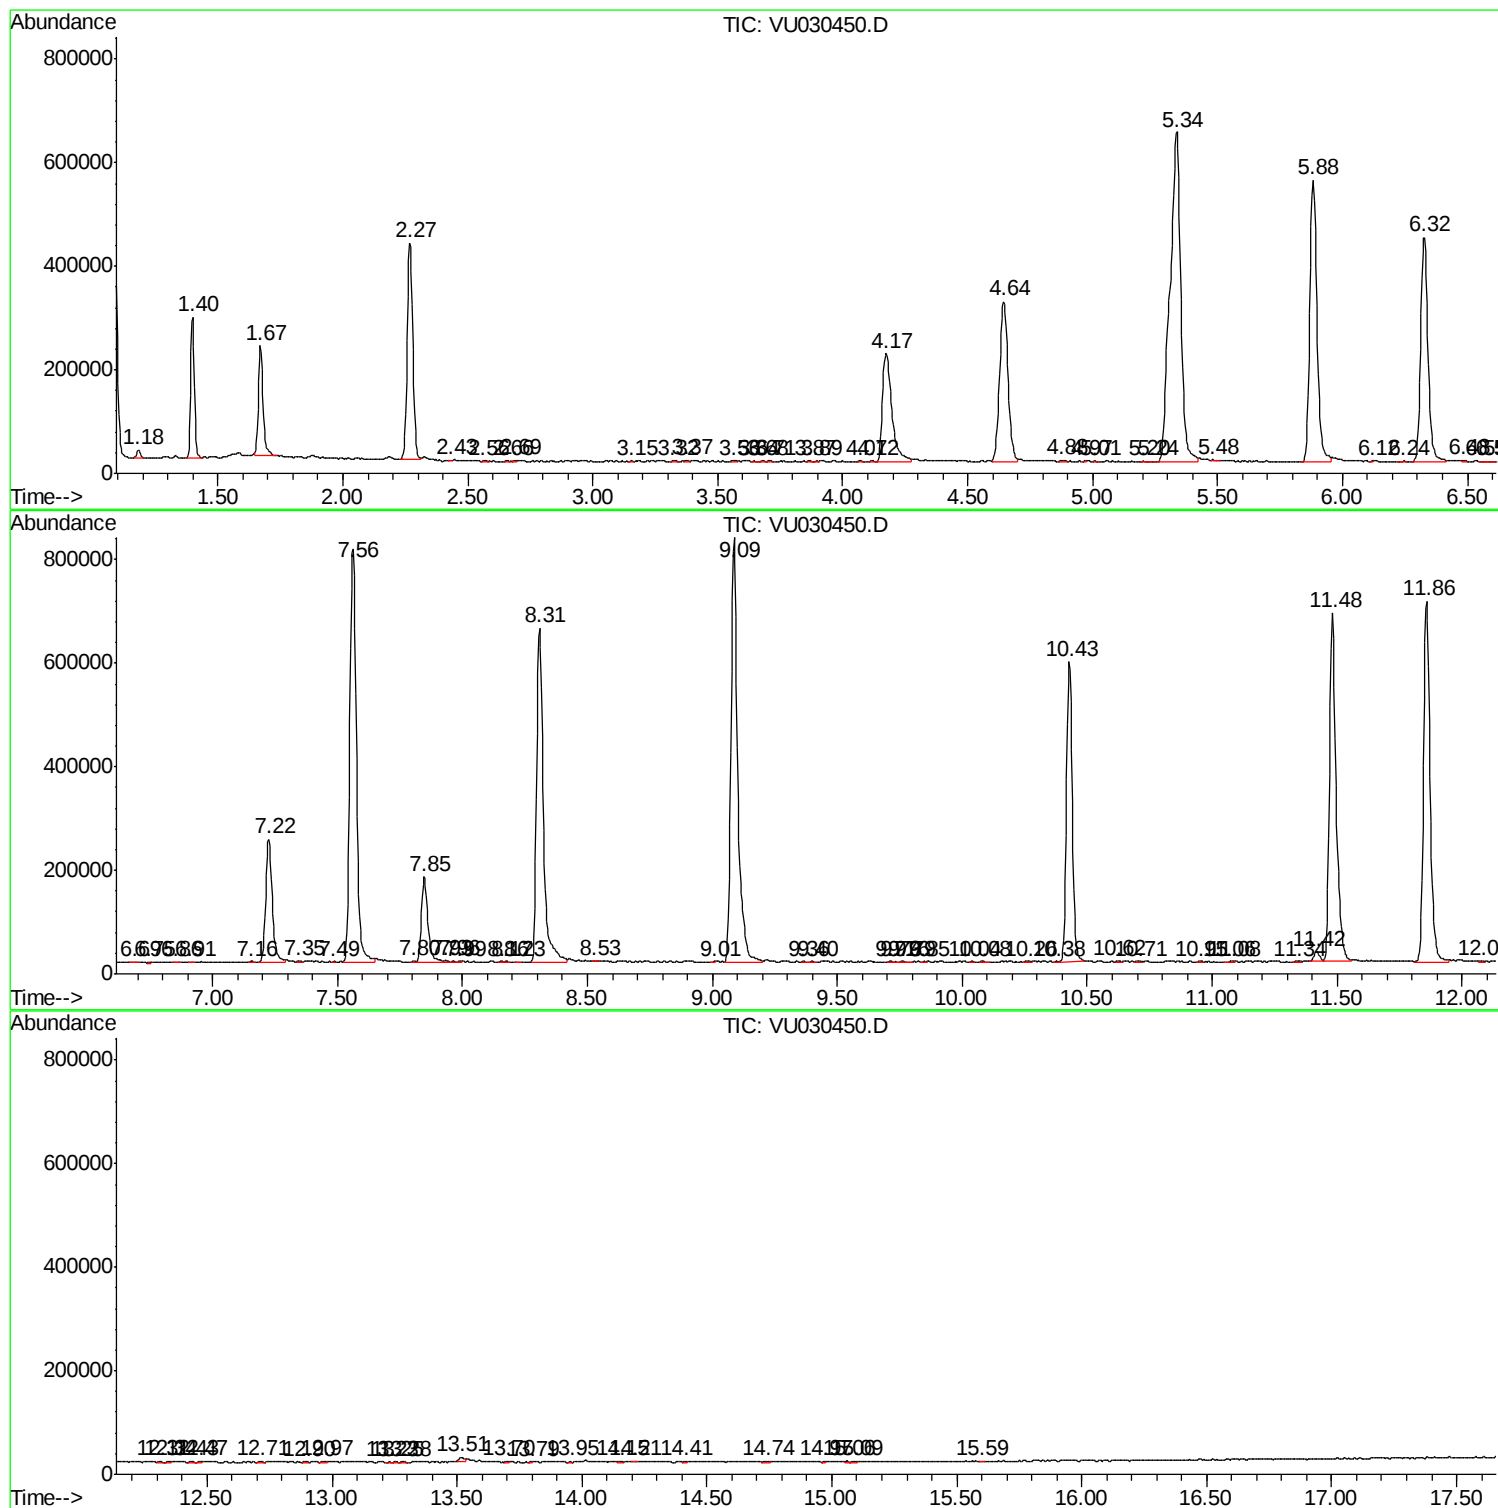

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030450.D
Acq On : 26 Mar 2019 17:55
Operator : JC/SP
Sample : K2022-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09C7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030450.D
Acq On : 26 Mar 2019 17:55
Operator : JC/SP
Sample : K2022-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09C7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc